

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111720\
 Data File : BF122343.D
 Acq On : 17 Nov 2020 13:35
 Operator : JU/CG
 Sample : PB133049BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB133049BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF122343.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.269	27	31	35	rVB	95553	124790	1.18%	0.195%
2	5.492	573	579	582	rBV	7645041	8218391	77.65%	12.810%
3	6.486	742	748	751	rBV	6690852	8516007	80.46%	13.274%
4	6.863	809	812	816	rBV	2247689	1838856	17.37%	2.866%
5	7.428	902	908	911	rBV	5141762	5603531	52.94%	8.734%
6	8.151	1025	1031	1034	rBV	2539191	2389999	22.58%	3.725%
7	9.227	1208	1214	1217	rBV	8859843	9780297	92.41%	15.245%
8	9.904	1323	1329	1338	rBV	3119010	2792793	26.39%	4.353%
9	10.692	1457	1463	1481	rBV	5935428	6409994	60.56%	9.991%
10	11.392	1575	1582	1585	rBV	3109633	2831941	26.76%	4.414%
11	12.980	1845	1852	1855	rBV	9725461	10583839	100.00%	16.497%
12	14.027	2026	2030	2040	rBV	2943175	2696407	25.48%	4.203%
13	15.498	2274	2280	2295	rBV	1705296	2368432	22.38%	3.692%




Sum of corrected areas: 64155277

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111720\
Data File : BF122343.D
Acq On : 17 Nov 2020 13:35
Operator : JU/CG
Sample : PB133049BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB133049BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

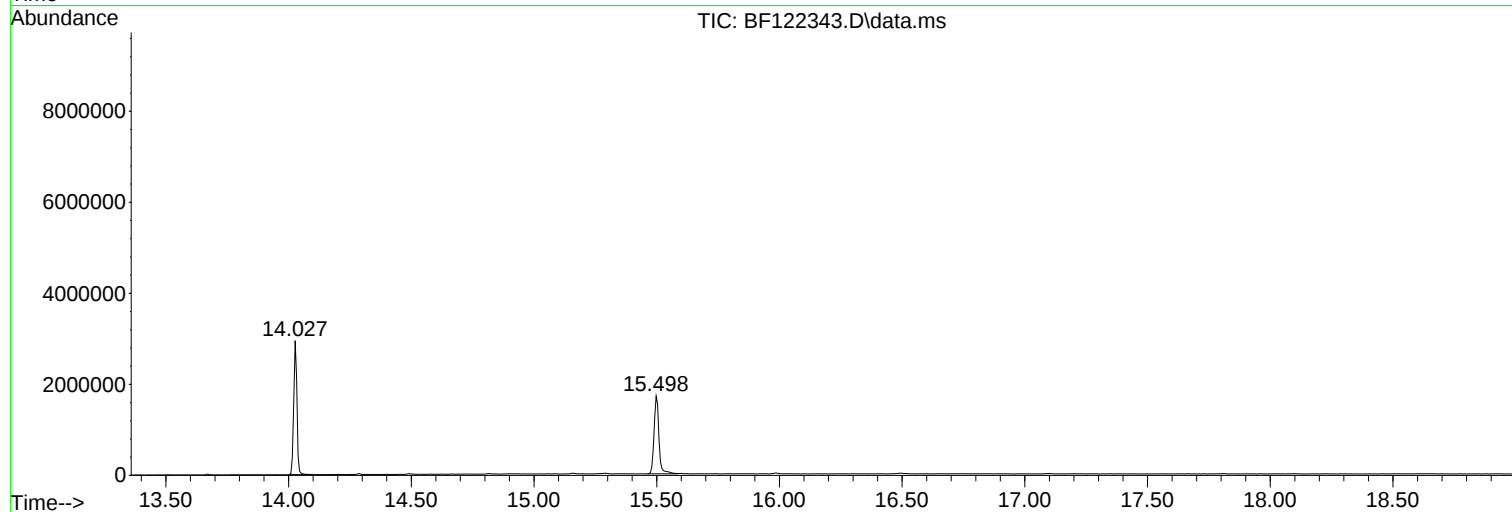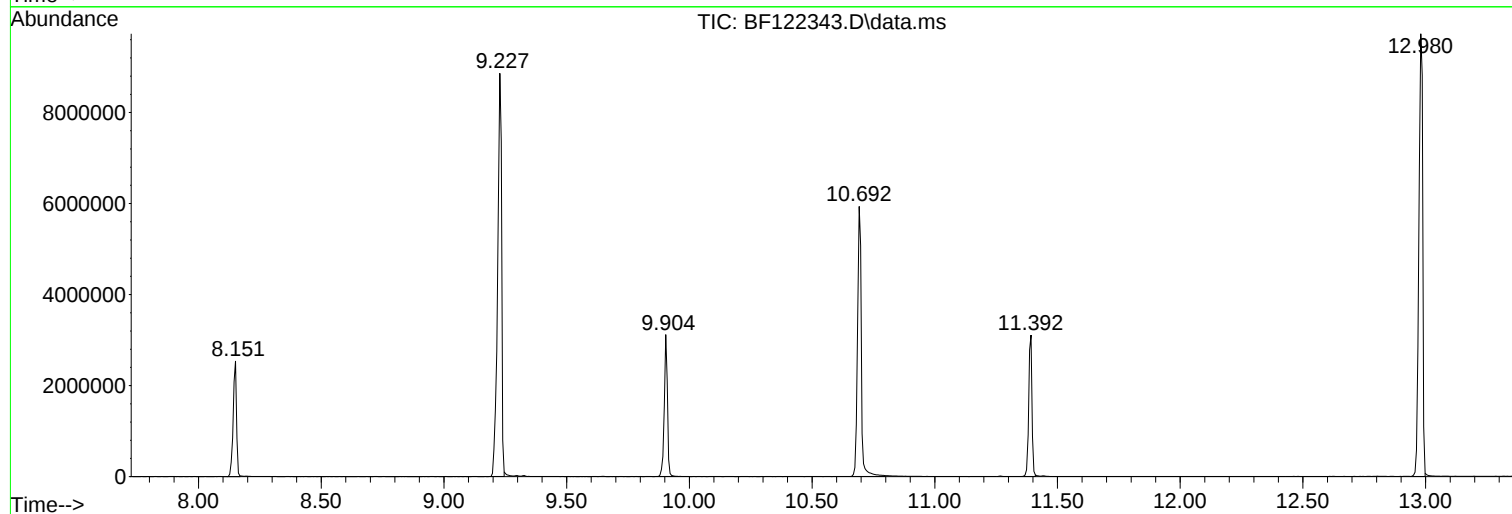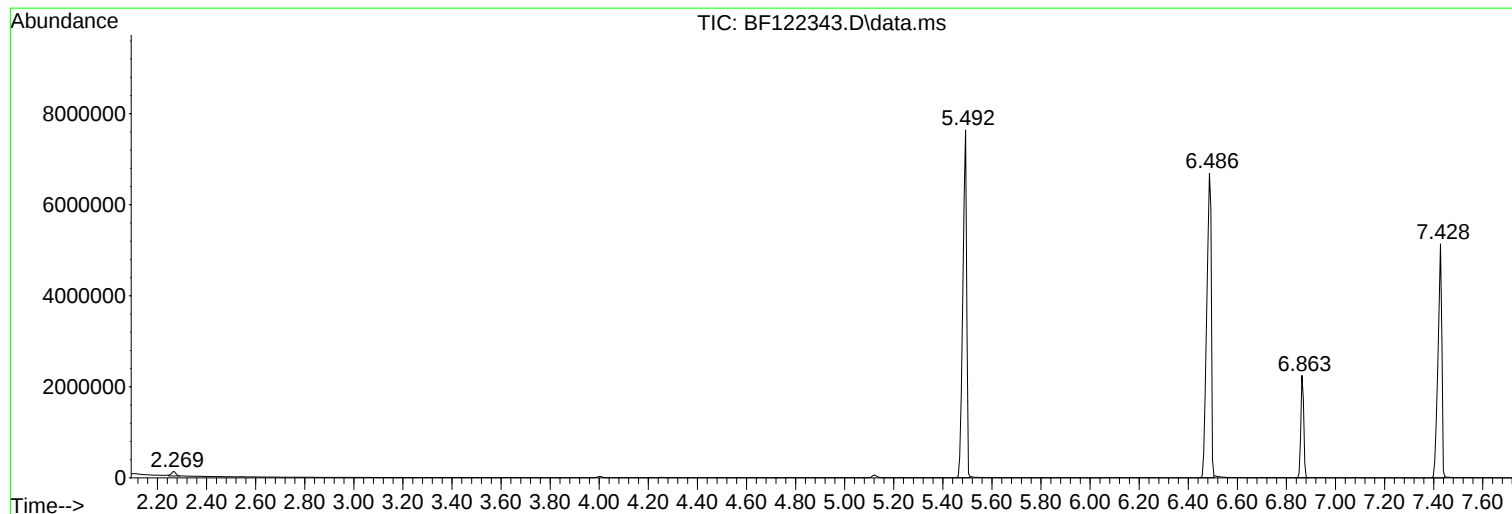

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111720\
Data File : BF122343.D
Acq On : 17 Nov 2020 13:35
Operator : JU/CG
Sample : PB133049BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB133049BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111720\
Data File : BF122343.D
Acq On : 17 Nov 2020 13:35
Operator : JU/CG
Sample : PB133049BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB133049BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------