

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111720\
 Data File : BF122345.D
 Acq On : 17 Nov 2020 14:44
 Operator : JU/CG
 Sample : L4586-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 R-LA-33-4-WC

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF122345.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.163	7	13	19	rVB	1201217	1552758	15.61%	2.117%
2	3.340	208	213	223	rBV	50220	105522	1.06%	0.144%
3	5.481	571	577	580	rBV	6989188	7682981	77.23%	10.477%
4	6.487	742	748	751	rBV	6485098	8093820	81.36%	11.037%
5	6.687	779	782	796	rVB	221422	234327	2.36%	0.320%
6	6.863	809	812	816	rVB	2177224	1686870	16.96%	2.300%
7	7.428	902	908	911	rBV	5252015	5135938	51.63%	7.003%
8	8.151	1026	1031	1034	rBV	2393489	2196852	22.08%	2.996%
9	9.228	1208	1214	1217	rBV	8857618	8671747	87.17%	11.825%
10	9.616	1276	1280	1284	rBV	1857639	1505538	15.13%	2.053%
11	9.904	1324	1329	1332	rBV	3101102	2570100	25.84%	3.505%
12	10.692	1457	1463	1466	rBV	6197366	5950043	59.81%	8.114%
13	11.386	1576	1581	1585	rBV	2976669	2732818	27.47%	3.727%
14	11.921	1666	1672	1687	rBV	1657394	1878673	18.89%	2.562%
15	12.374	1745	1749	1752	rVB	193005	161341	1.62%	0.220%
16	12.627	1785	1792	1800	rBV5	97764	237586	2.39%	0.324%
17	12.704	1800	1805	1816	rBV	783616	973360	9.78%	1.327%
18	12.980	1847	1852	1855	rBV	9699743	9947853	100.00%	13.565%
19	13.168	1872	1884	1887	rBV2	130999	390404	3.92%	0.532%
20	13.821	1990	1995	1998	rBV	94689	139620	1.40%	0.190%
21	13.874	1998	2004	2023	rVB3	1033713	2063082	20.74%	2.813%
22	14.027	2025	2030	2033	rBV	3331391	2889188	29.04%	3.940%
23	14.121	2038	2046	2054	rBV2	133605	357019	3.59%	0.487%
24	14.504	2105	2111	2125	rBV4	180859	366802	3.69%	0.500%
25	14.815	2157	2164	2174	rBV	191183	328997	3.31%	0.449%
26	14.962	2185	2189	2194	rBV	475471	512368	5.15%	0.699%
27	15.157	2218	2222	2224	rBV	242431	263273	2.65%	0.359%
28	15.186	2224	2227	2235	rVV	386267	689528	6.93%	0.940%
29	15.498	2274	2280	2284	rBV	1794902	2315966	23.28%	3.158%
30	15.539	2284	2287	2297	rVB2	116473	229200	2.30%	0.313%
31	15.745	2317	2322	2327	rBV	114415	162488	1.63%	0.222%
32	15.980	2356	2362	2367	rBV	212687	327041	3.29%	0.446%
33	16.039	2367	2372	2380	rBV2	166940	388010	3.90%	0.529%
34	16.492	2445	2449	2459	rVB3	71302	128621	1.29%	0.175%
35	17.092	2545	2551	2558	rBV2	60711	124619	1.25%	0.170%
36	17.333	2587	2592	2599	rVB9	63067	138810	1.40%	0.189%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111720\
Data File : BF122345.D
Acq On : 17 Nov 2020 14:44
Operator : JU/CG
Sample : L4586-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
R-LA-33-4-WC

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	17.580	2628	2634	2644	rBV7	69210	201119	2.02%	0.274%
----	--------	------	------	------	------	-------	--------	-------	--------




Sum of corrected areas: 73334282

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111720\
Data File : BF122345.D
Acq On : 17 Nov 2020 14:44
Operator : JU/CG
Sample : L4586-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
R-LA-33-4-WC

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

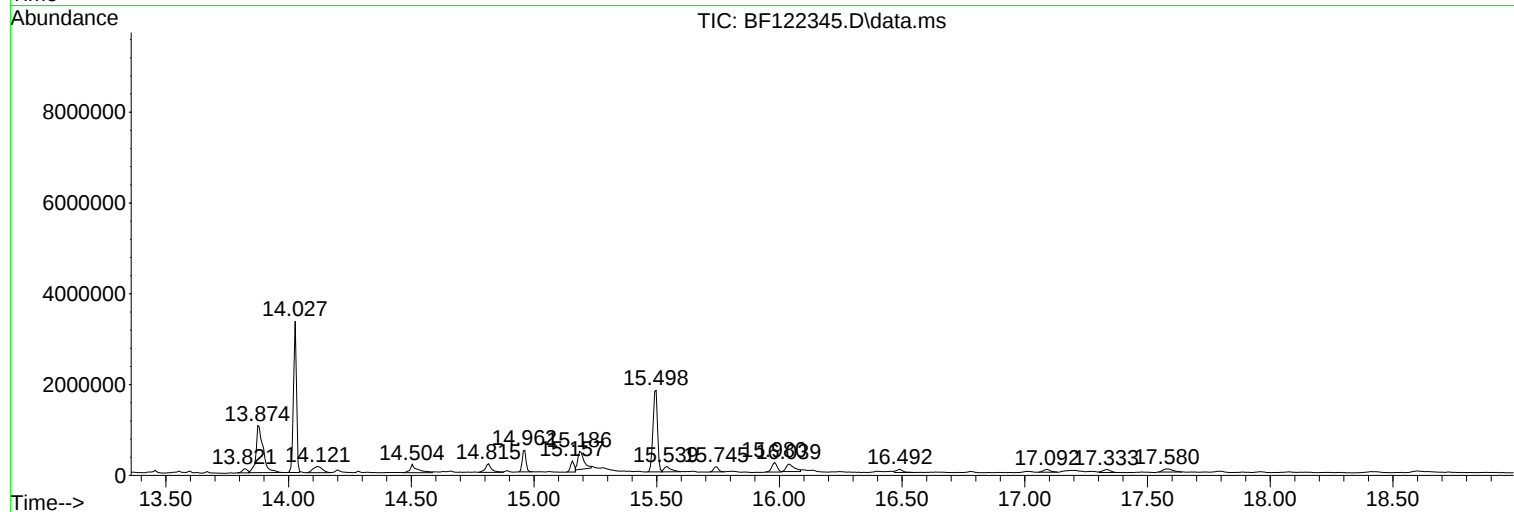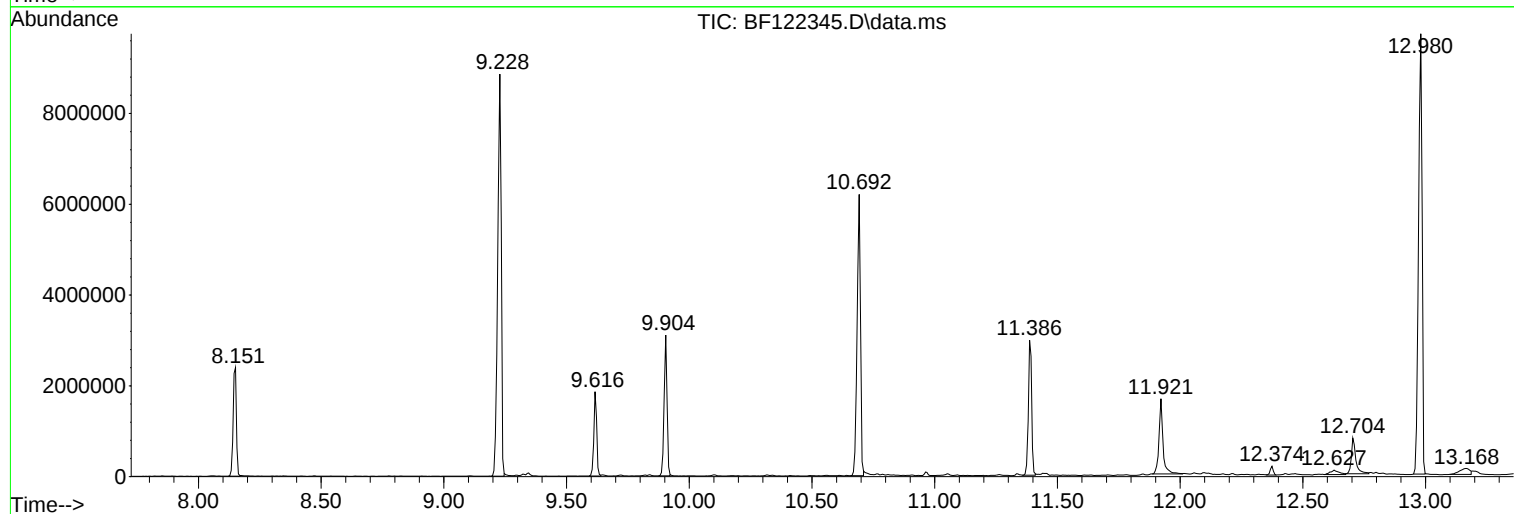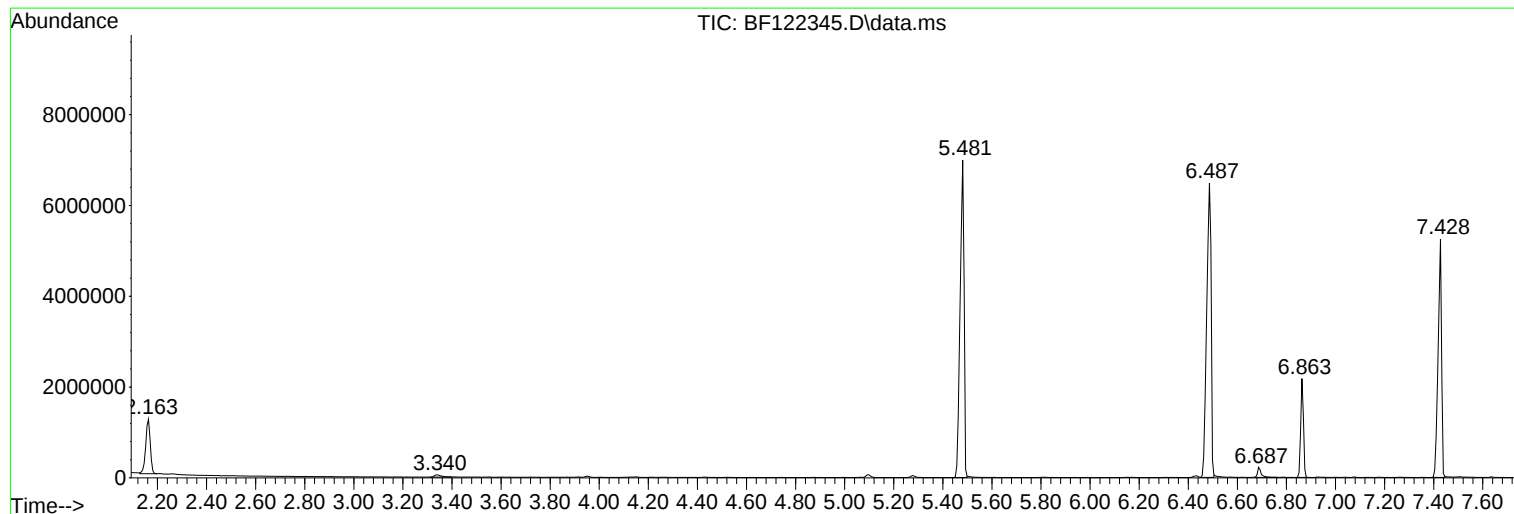

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111720\
Data File : BF122345.D
Acq On : 17 Nov 2020 14:44
Operator : JU/CG
Sample : L4586-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
R-LA-33-4-WC

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111720\
Data File : BF122345.D
Acq On : 17 Nov 2020 14:44
Operator : JU/CG
Sample : L4586-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
R-LA-33-4-WC

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------