
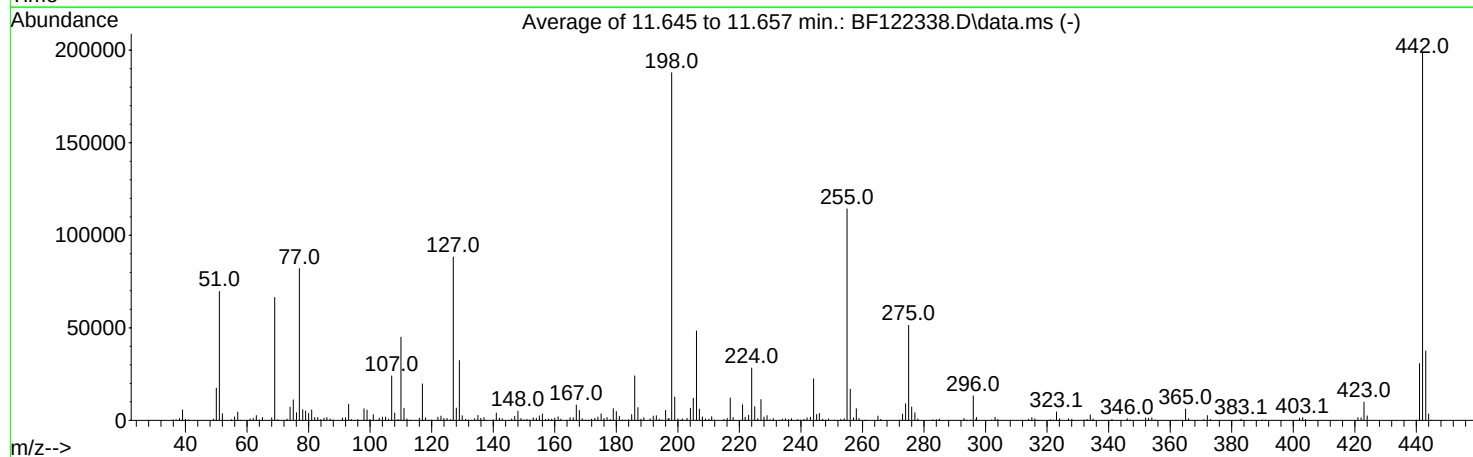


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111720\
Data File : BF122338.D
Acq On : 17 Nov 2020 10:26
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Nov 10 12:25:42 2020

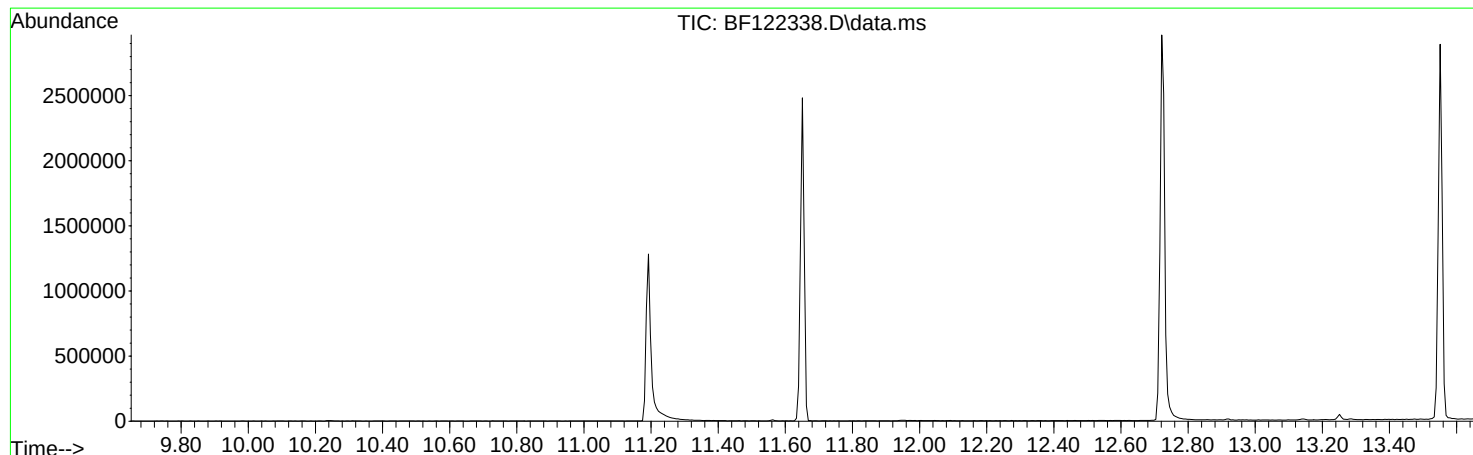

AutoFind: Scans 1625, 1626, 1627; Background Corrected with Scan 1620

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.1	69696	PASS
68	69	0.00	2	1.9	1278	PASS
69	198	0.00	100	35.3	66371	PASS
70	69	0.00	2	0.6	373	PASS
127	198	10	80	47.0	88296	PASS
197	198	0.00	2	0.6	1052	PASS
198	198	100	100	100.0	187819	PASS
199	198	5	9	6.7	12615	PASS
275	198	10	60	27.4	51395	PASS
365	198	1	100	3.3	6126	PASS
441	198	0.01	100	16.4	30710	PASS
442	442	100	100	100.0	198744	PASS
443	442	15	24	18.9	37560	PASS