
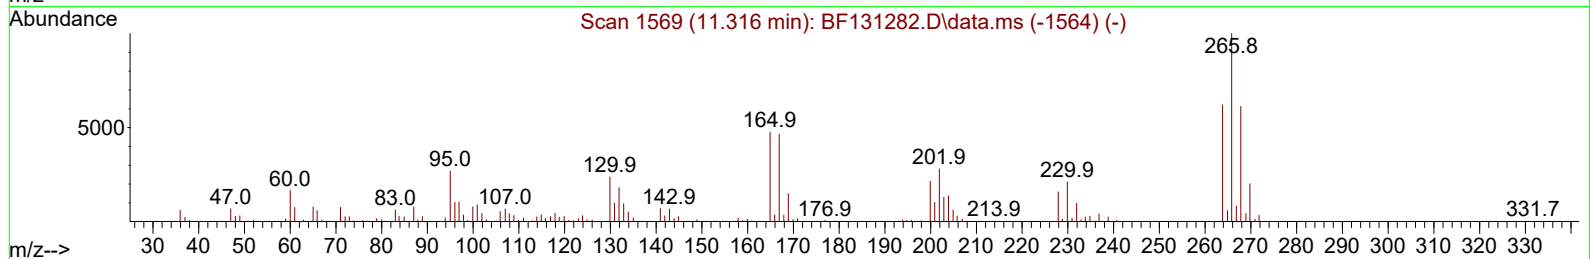
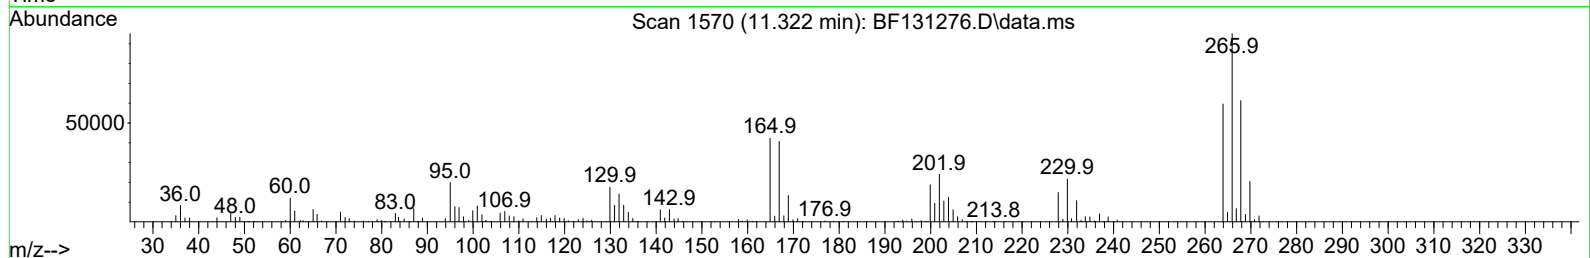


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111722\
Data File : BF131276.D
Acq On : 17 Nov 2022 09:38
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 18 05:25:10 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 18 01:41:28 2022
Response via : Initial Calibration

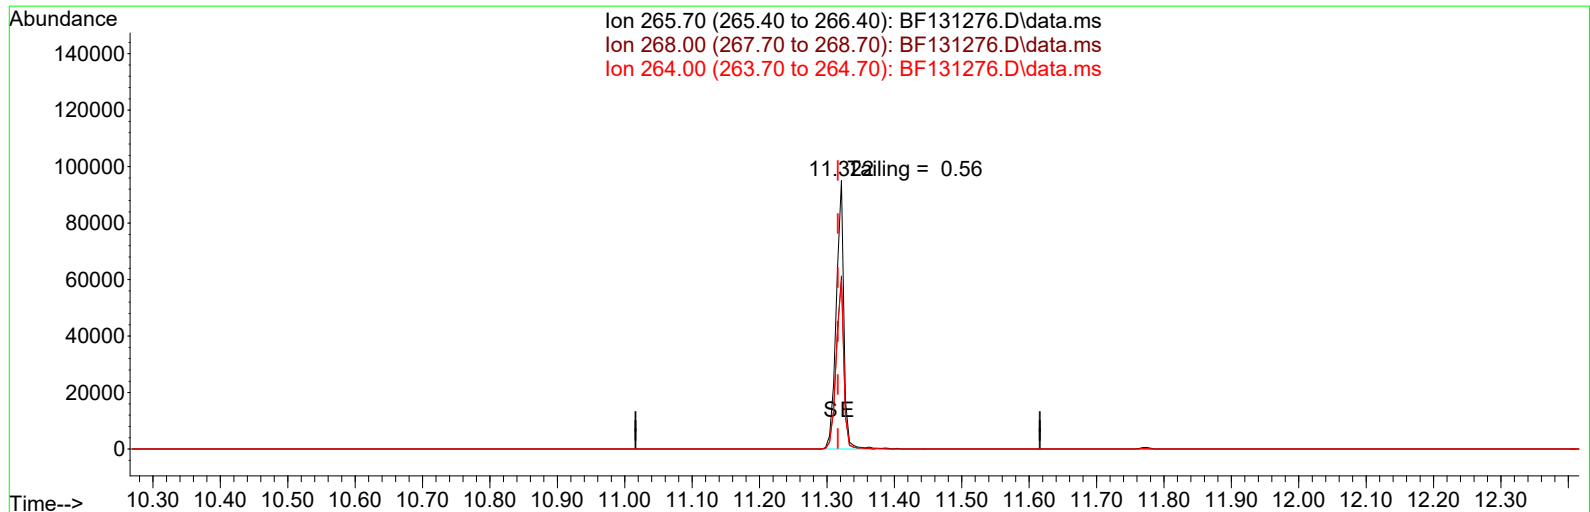

TIC: BF131276.D\data.ms

(70) Pentachlorophenol (C)




11.322min (+ 0.006) 10663.90 ng

response 75060

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	64.45
264.00	62.10	62.72
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111722\
Data File : BF131276.D
Acq On : 17 Nov 2022 09:38
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 18 05:25:10 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 18 01:41:28 2022
Response via : Initial Calibration

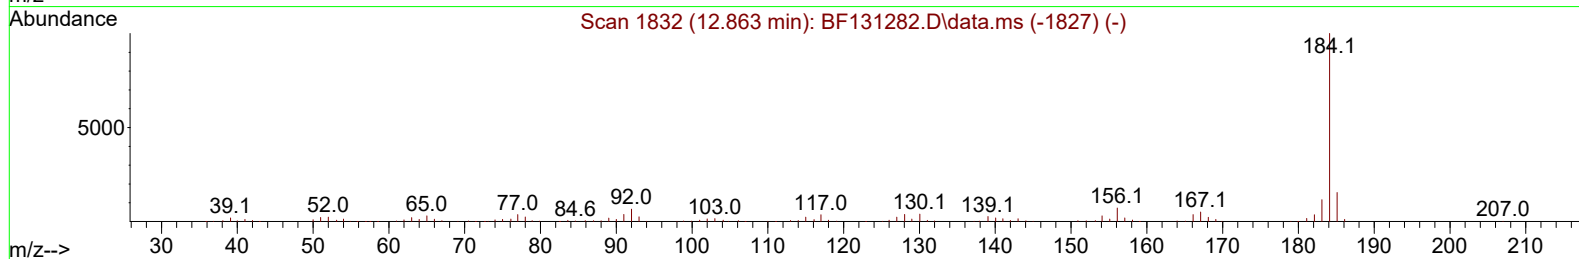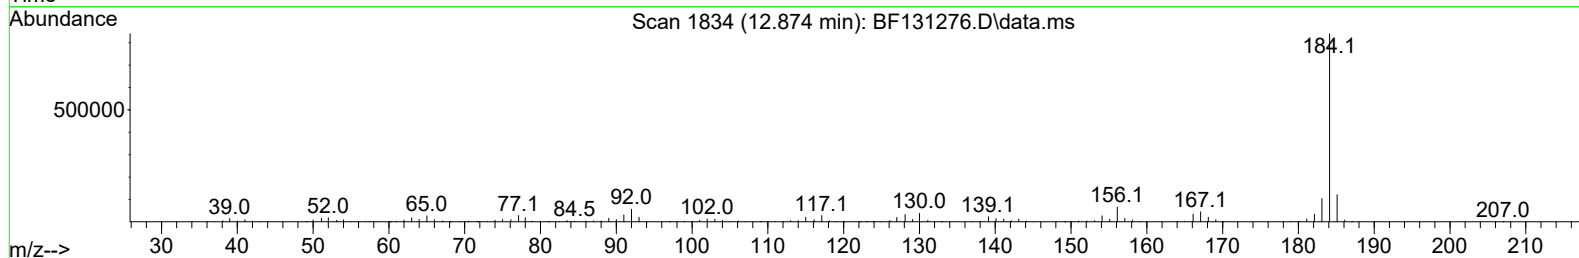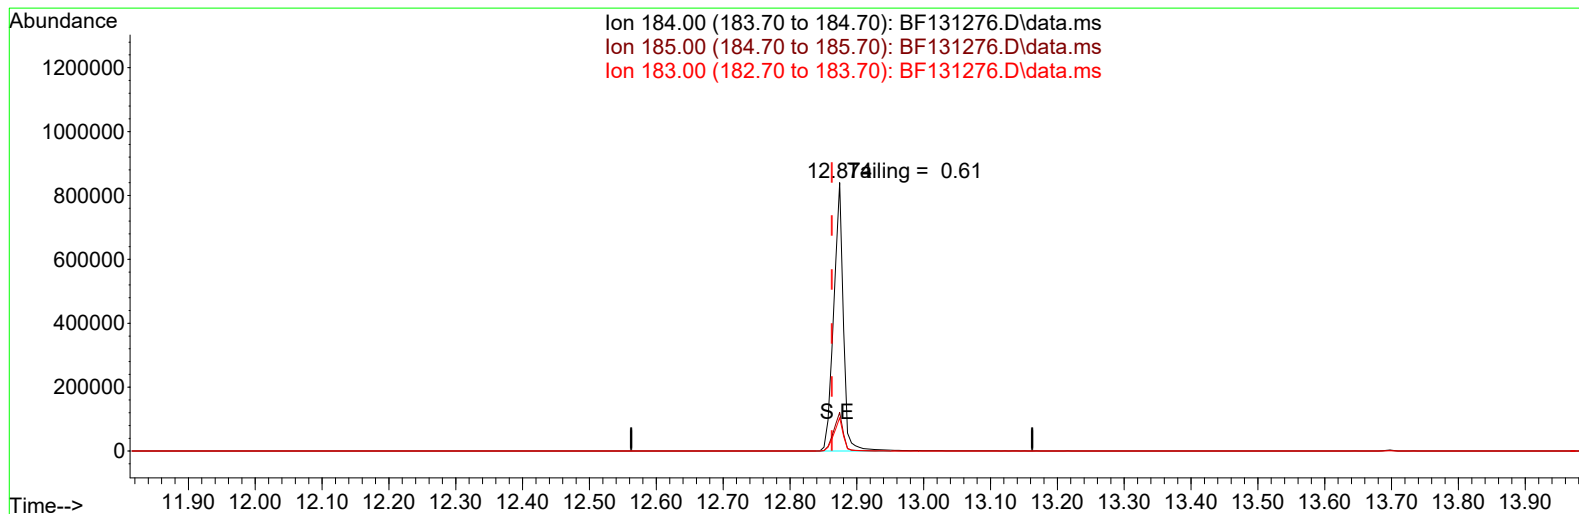

TIC: BF131276.D\data.ms

(77) Benzidine

12.874min (+ 0.012) 0.00 ng

response 844124

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.40	14.41
183.00	11.60	12.40
0.00	0.00	0.00