

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF111815\
 Data File : BF083027.D
 Acq On : 19 Nov 2015 00:22
 Operator : UM/IZ
 Sample : G4426-03 10X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-3

Quant Time: Nov 19 01:53:24 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 18 13:32:32 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.73	152	110374	20.00	ng	-0.01
21) Naphthalene-d8	8.02	136	454406	20.00	ng	0.00
38) Acenaphthene-d10	9.77	164	204692	20.00	ng	-0.01
63) Phenanthrene-d10	11.24	188	313753	20.00	ng	-0.01
75) Chrysene-d12	13.87	240	272672	20.00	ng	-0.02
86) Perylene-d12	15.27	264	223181	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.32	112	112317	15.83	ng	-0.01
7) Phenol-d6	6.37	99	152428	16.16	ng	-0.02
23) Nitrobenzene-d5	7.29	82	92269	8.84	ng	-0.02
41) 2,4,6-Tribromophenol	10.56	330	22420	9.55	ng	-0.01
44) 2-Fluorobiphenyl	9.09	172	156795	10.98	ng	-0.01
78) Terphenyl-d14	12.83	244	105839	9.21	ng	-0.01
Target Compounds						Qvalue
37) 2-Methylnaphthalene	8.73	142	50119	3.09	ng	96
49) Dimethylphthalate	9.49	163	49698	2.96	ng	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF111815\
Data File : BF083027.D
Acq On : 19 Nov 2015 00:22
Operator : UM/IZ
Sample : G4426-03 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-3

Quant Time: Nov 19 01:53:24 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 18 13:32:32 2015
Response via : Initial Calibration

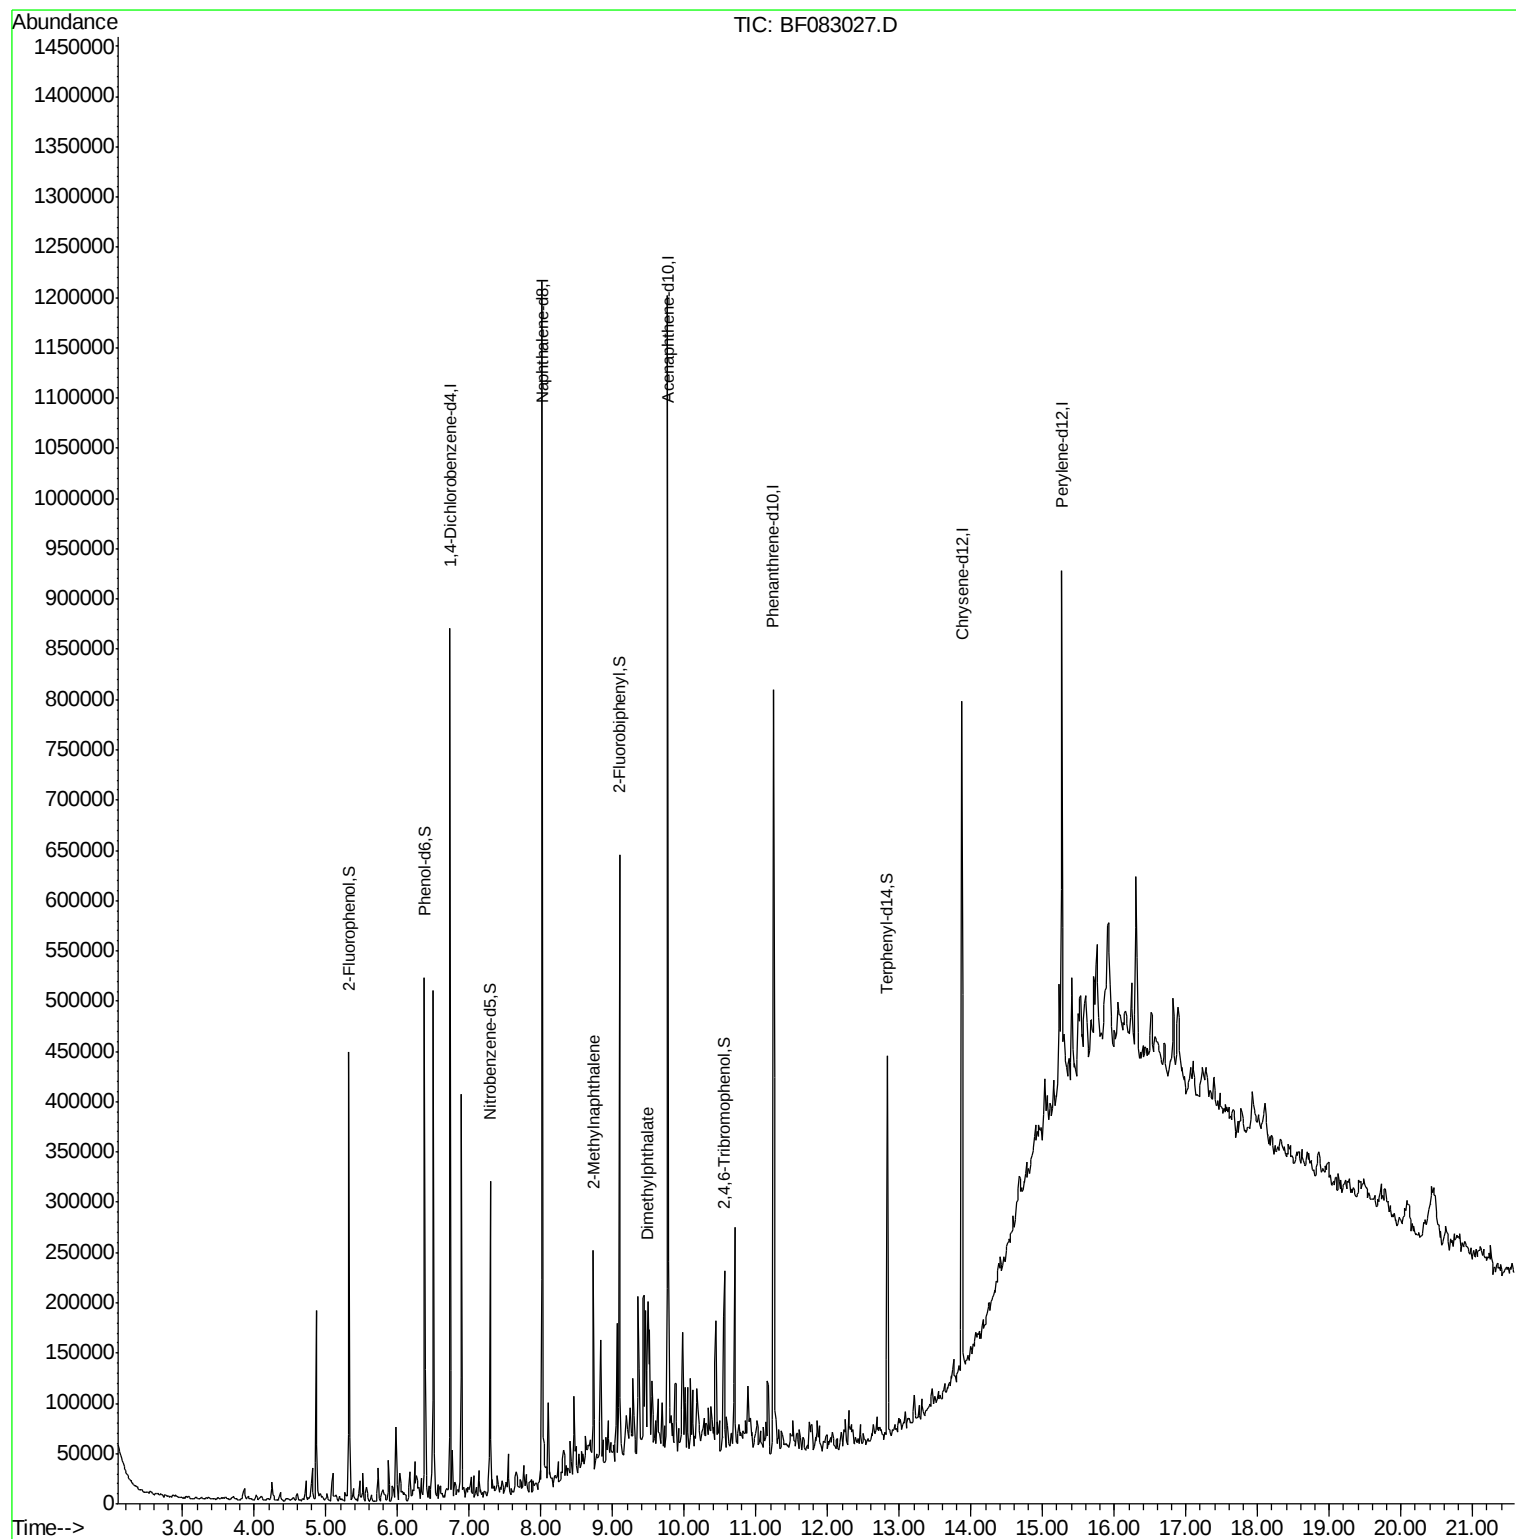

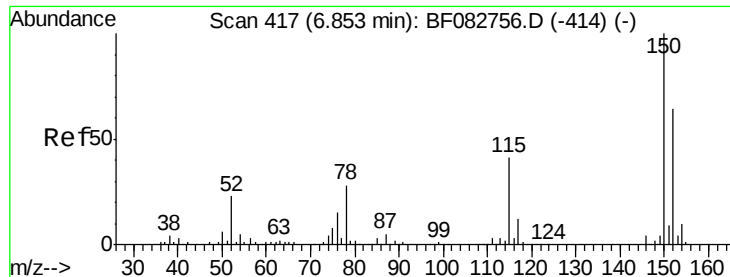

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.73 min Scan# 406

Delta R.T. -0.01 min

Lab File: BF083027.D

Acq: 19 Nov 2015 00:22

Instrument :

BNA_F

ClientSampleId :

SB-3


Tgt Ion:152 Resp: 110374

Ion Ratio Lower Upper

152 100

150 158.4 127.0 190.4




115 68.6 47.0 70.6

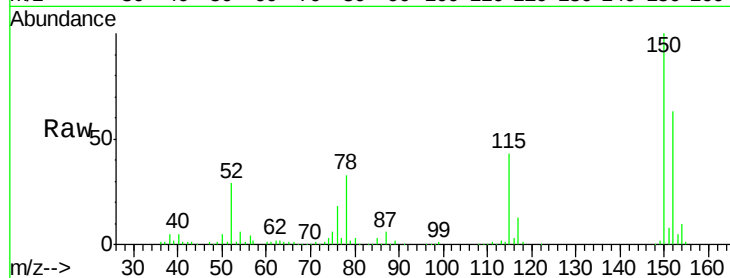

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

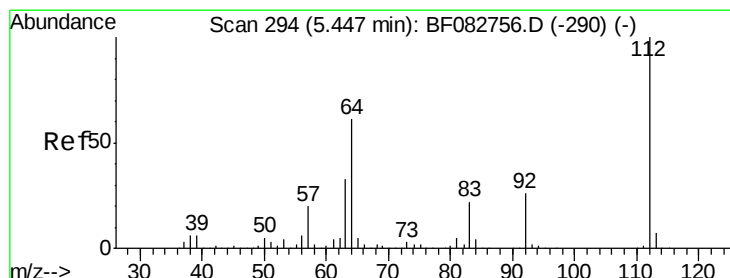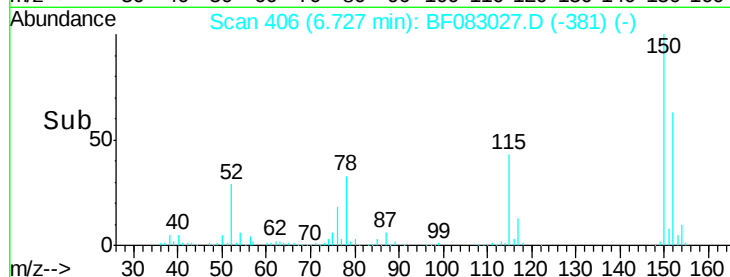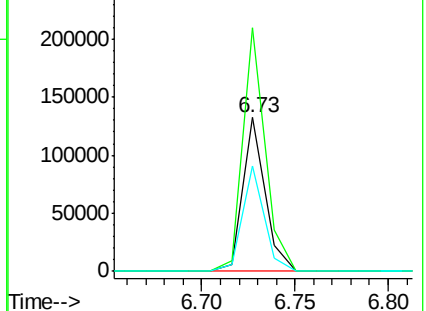

#5

2-Fluorophenol

Concen: 15.83 ng

RT: 5.32 min Scan# 283

Delta R.T. -0.01 min

Lab File: BF083027.D

Acq: 19 Nov 2015 00:22


Tgt Ion:112 Resp: 112317

Ion Ratio Lower Upper

112 100

64 61.8 48.9 73.3



63 32.6 28.1 42.1

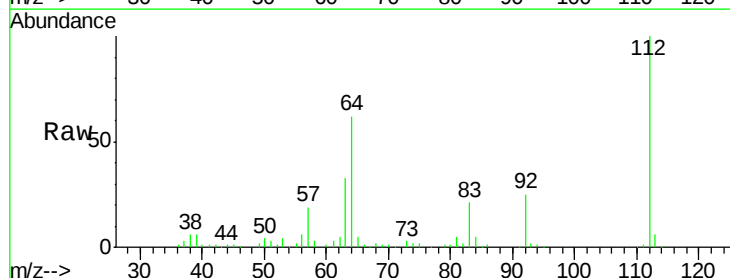


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

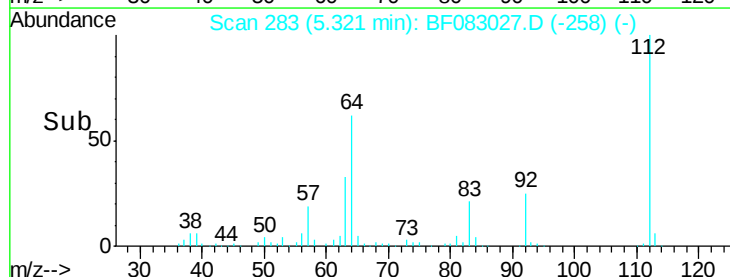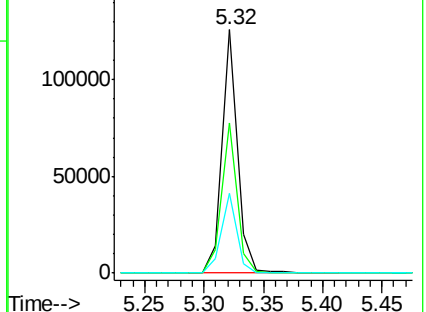

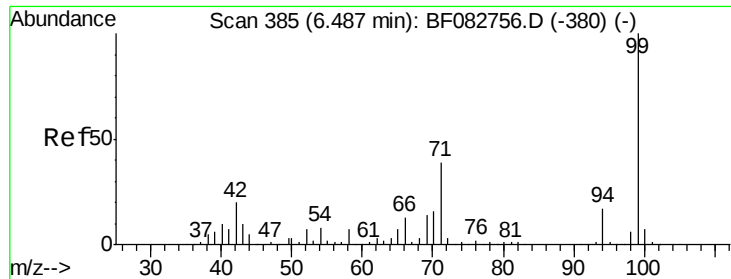

#7

Phenol-d6

Concen: 16.16 ng

RT: 6.37 min Scan# 375

Delta R.T. -0.02 min

Lab File: BF083027.D

Acq: 19 Nov 2015 00:22

Instrument :

BNA_F

ClientSampleId :

SB-3


Tgt Ion: 99 Resp: 152428

Ion Ratio Lower Upper

99 100

42 21.5 19.2 28.8




71 39.1 35.0 52.4

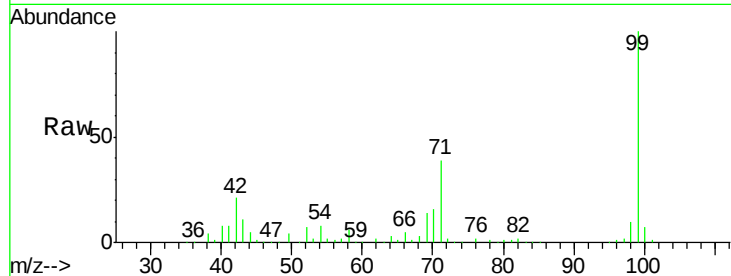

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

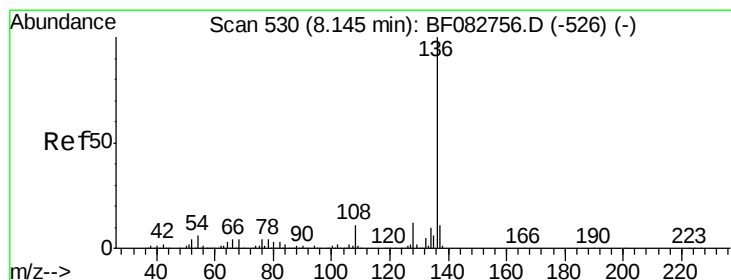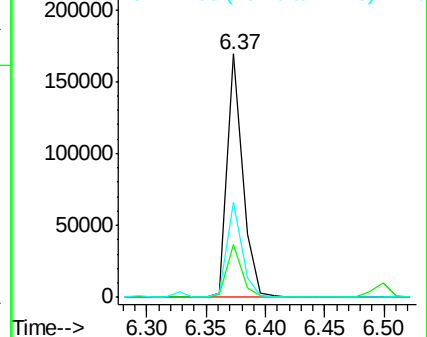

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.02 min Scan# 519

Delta R.T. 0.00 min

Lab File: BF083027.D

Acq: 19 Nov 2015 00:22

Tgt Ion: 136 Resp: 454406


Ion Ratio Lower Upper

136 100

137 10.8 9.1 13.7

54 7.8 9.1 13.7#

68 5.0 4.8 7.2


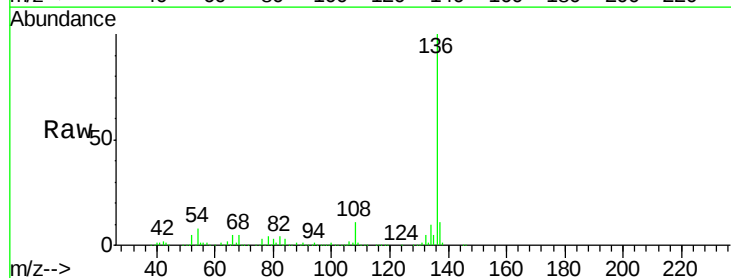



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

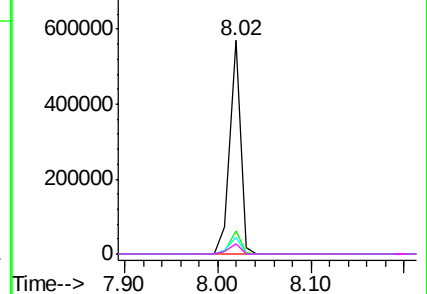


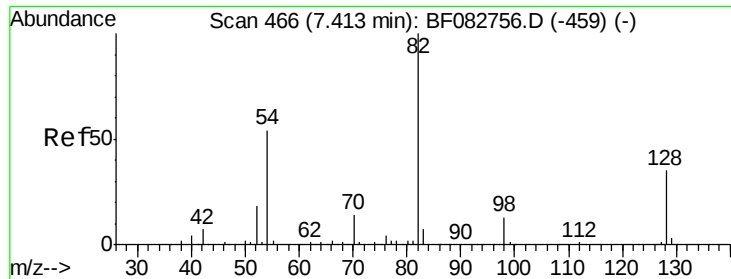




#23
Nitrobenzene-d5
Concen: 8.84 ng
RT: 7.29 min Scan# 455
Delta R.T. -0.02 min
Lab File: BF083027.D
Acq: 19 Nov 2015 00:22

Instrument :
BNA_F
ClientSampleId :
SB-3

Tgt Ion	Ratio	Lower	Upper
82	100		
128	33.1	26.8	40.2
54	52.5	45.7	68.5

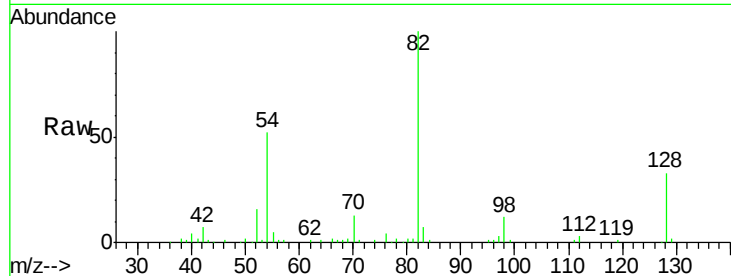


Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 128.00 (127.70 to 128.70): B
Ion 54.00 (53.70 to 54.70): BF0

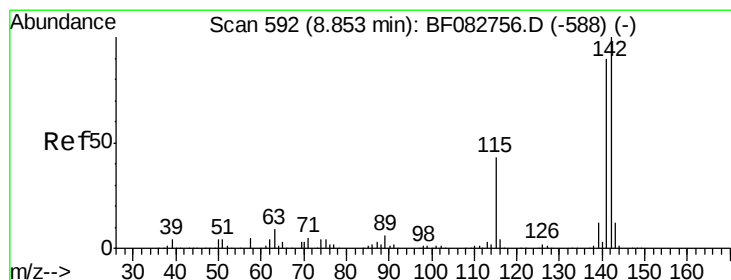
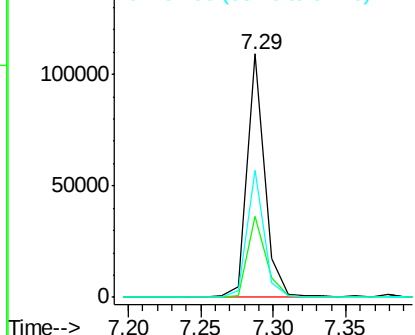



#37
2-Methylnaphthalene
Concen: 3.09 ng
RT: 8.73 min Scan# 581
Delta R.T. -0.01 min
Lab File: BF083027.D
Acq: 19 Nov 2015 00:22

Tgt Ion	Ratio	Lower	Upper
142	100		
141	89.0	72.3	108.5
115	41.6	38.1	57.1

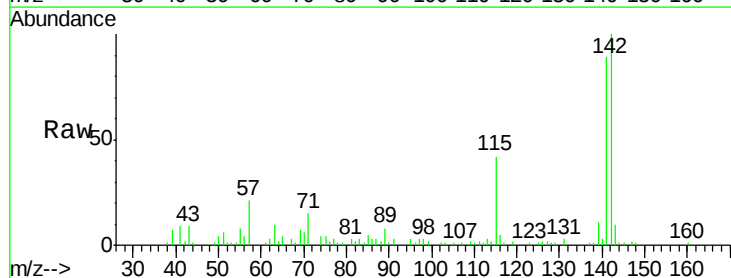

Abundance Ion 142.00 (141.70 to 142.70): B
Ion 141.00 (140.70 to 141.70): B
Ion 115.00 (114.70 to 115.70): B

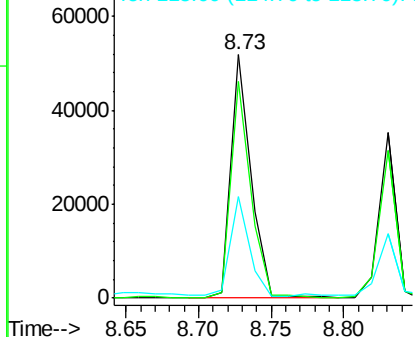


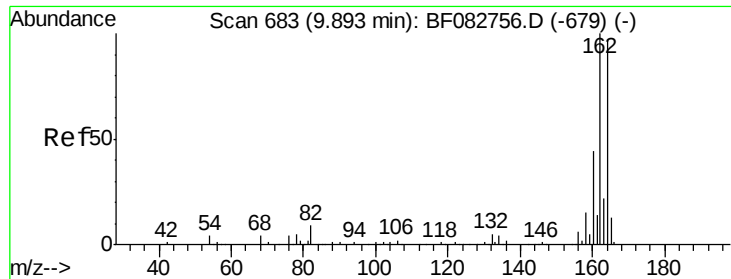




#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.77 min Scan# 672
 Delta R.T. -0.01 min
 Lab File: BF083027.D
 Acq: 19 Nov 2015 00:22

Instrument :
 BNA_F
 ClientSampleId :
 SB-3

Tgt Ion:164 Resp: 204692
 Ion Ratio Lower Upper
 164 100
 162 102.9 84.9 127.3
 160 45.0 37.5 56.3

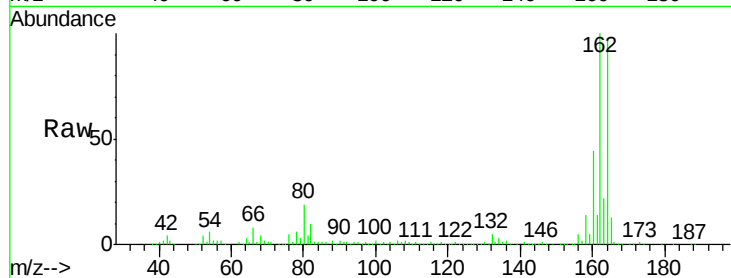


Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

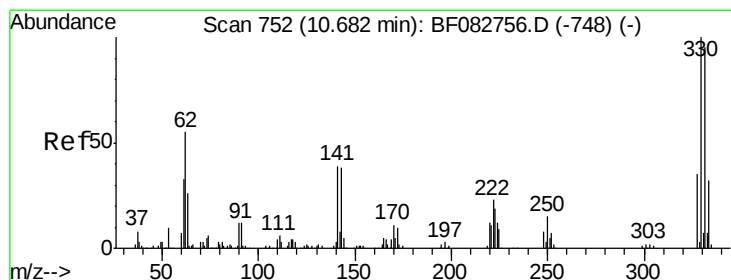
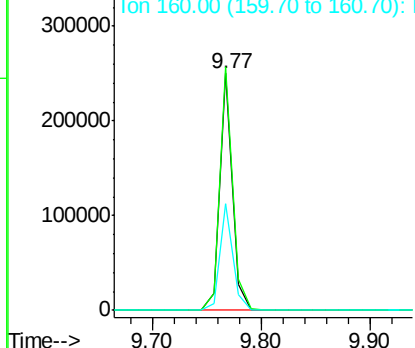



#41
 2,4,6-Tribromophenol
 Concen: 9.55 ng
 RT: 10.56 min Scan# 741
 Delta R.T. -0.01 min
 Lab File: BF083027.D
 Acq: 19 Nov 2015 00:22

Tgt Ion:330 Resp: 22420
 Ion Ratio Lower Upper
 330 100
 332 91.9 76.6 114.8
 141 34.5 41.2 61.8#

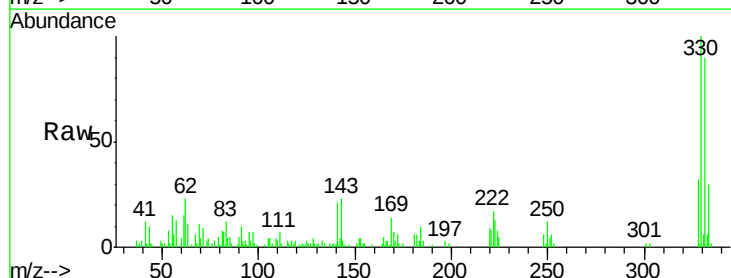

Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

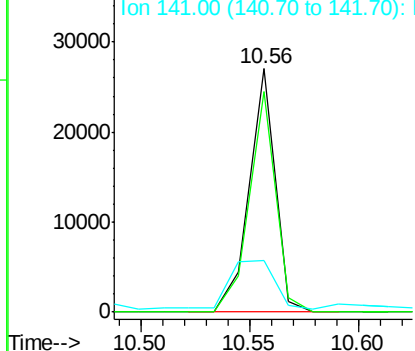

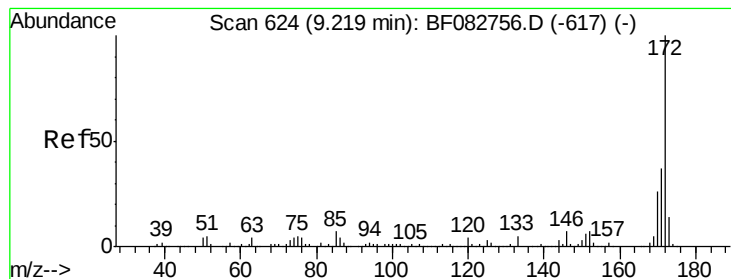

#44

2-Fluorobiphenyl

Concen: 10.98 ng

RT: 9.09 min Scan# 613

Delta R.T. -0.01 min

Lab File: BF083027.D

Acq: 19 Nov 2015 00:22

Instrument :

BNA_F

ClientSampled :

SB-3


Tgt Ion:172 Resp: 156795

Ion Ratio Lower Upper

172 100

171 35.1 30.8 46.2




170 23.0 21.2 31.8

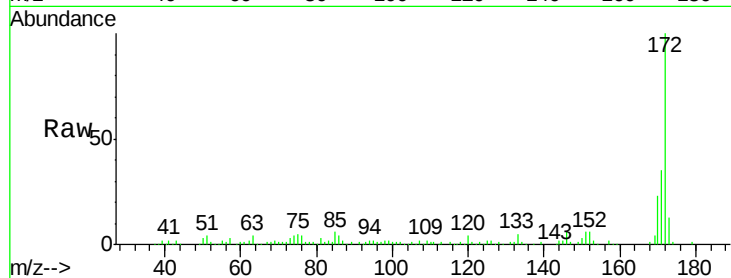

Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

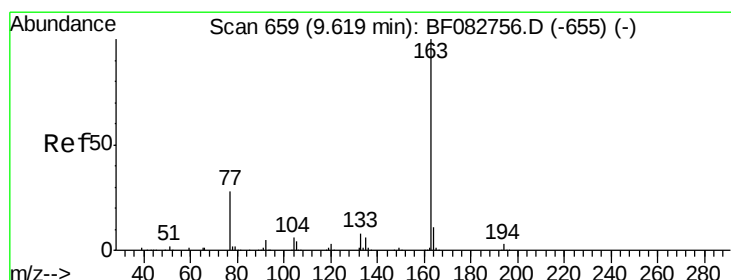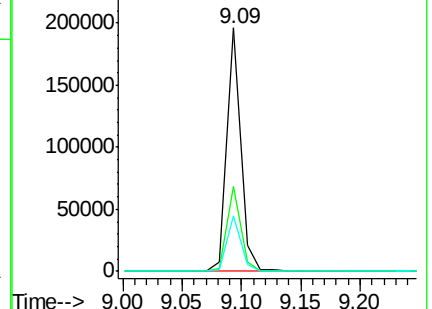

#49

Dimethylphthalate

Concen: 2.96 ng

RT: 9.49 min Scan# 648

Delta R.T. -0.02 min

Lab File: BF083027.D

Acq: 19 Nov 2015 00:22


Tgt Ion:163 Resp: 49698

Ion Ratio Lower Upper

163 100

194 3.8 2.6 4.0



164 9.6 8.7 13.1

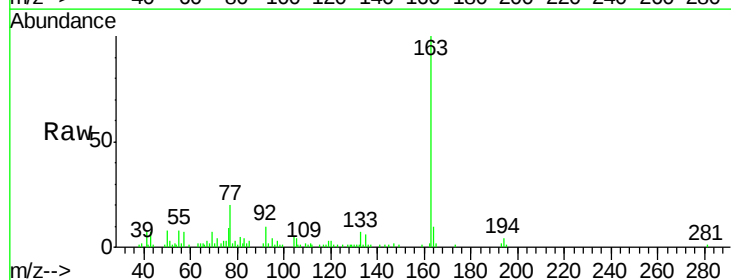


Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E



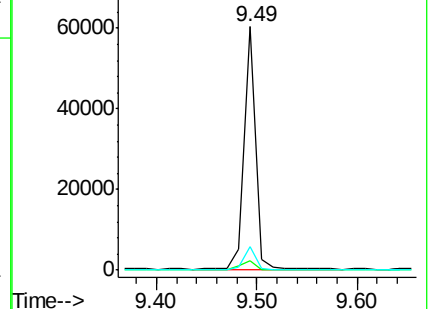





#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.24 min Scan# 801
Delta R.T. -0.01 min
Lab File: BF083027.D
Acq: 19 Nov 2015 00:22




Instrument :
BNA_F
ClientSampleId :
SB-3


Tgt Ion:188 Resp: 313753
Ion Ratio Lower Upper
188 100
94 10.6 6.1 9.1#
80 13.1 7.0 10.6#

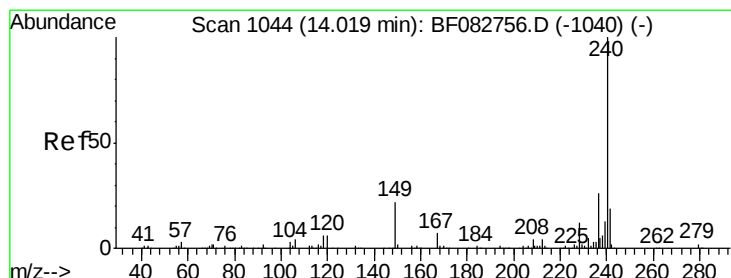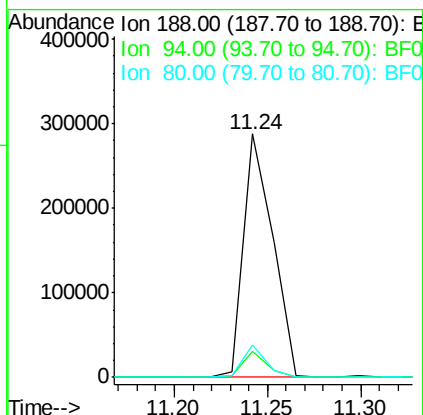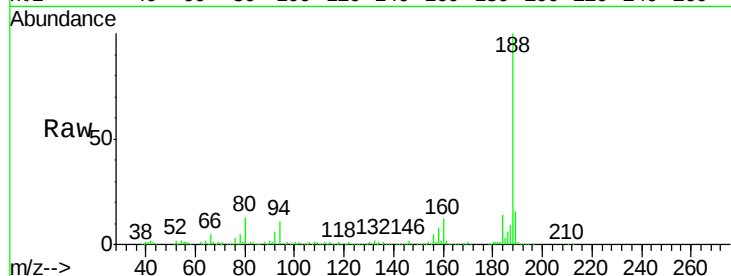

#75
Chrysene-d12
Concen: 20.00 ng
RT: 13.87 min Scan# 1031
Delta R.T. -0.02 min
Lab File: BF083027.D
Acq: 19 Nov 2015 00:22

Tgt Ion:240 Resp: 272672
Ion Ratio Lower Upper
240 100
120 11.4 10.9 16.3
236 26.3 21.6 32.4

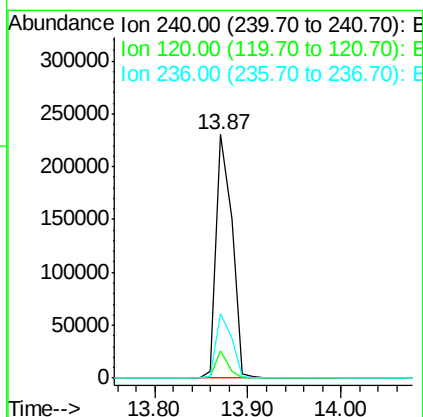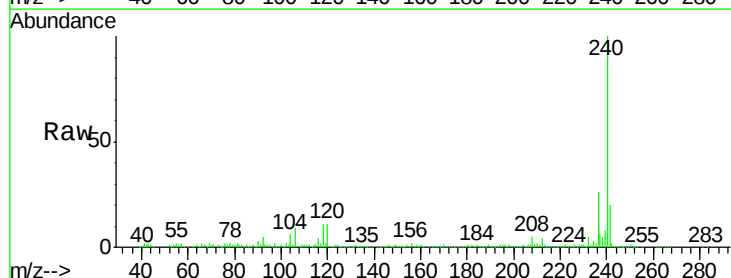

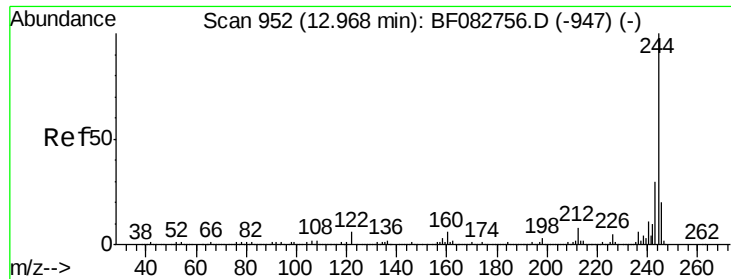

#78

Terphenyl-d14

Concen: 9.21 ng

RT: 12.83 min Scan# 940

Delta R.T. -0.01 min

Lab File: BF083027.D

Acq: 19 Nov 2015 00:22

Instrument :

BNA_F

ClientSampleId :

SB-3


Tgt Ion:244 Resp: 105839

Ion Ratio Lower Upper

244 100

212 7.5 7.6 11.4#




122 8.3 11.3 16.9#

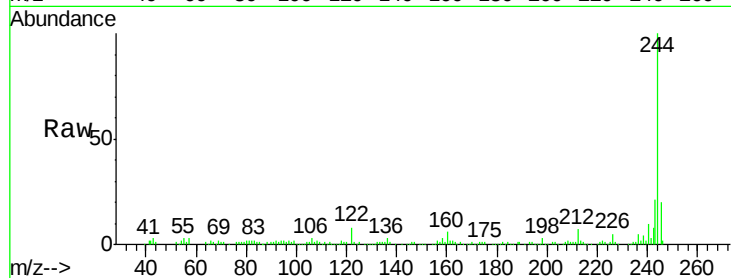

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

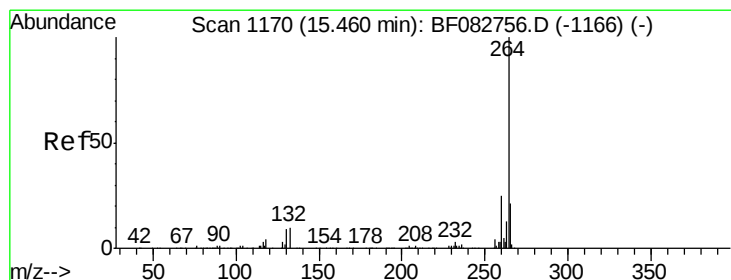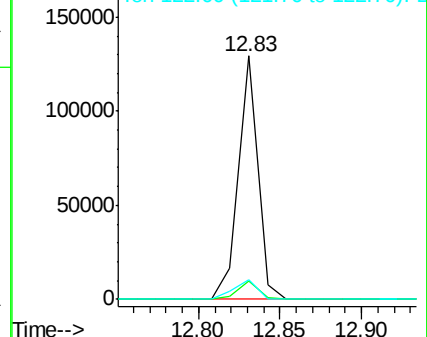

#86

Perylene-d12

Concen: 20.00 ng

RT: 15.27 min Scan# 1153

Delta R.T. -0.01 min

Lab File: BF083027.D

Acq: 19 Nov 2015 00:22


Tgt Ion:264 Resp: 223181

Ion Ratio Lower Upper

264 100

260 23.9 19.8 29.6

265 21.0 17.4 26.0

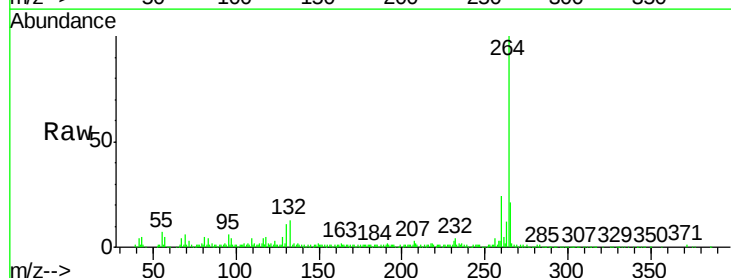

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

