


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF111815\
 Data File : BF083016.D
 Acq On : 18 Nov 2015 18:02
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110715.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 18 13:32:32 2015

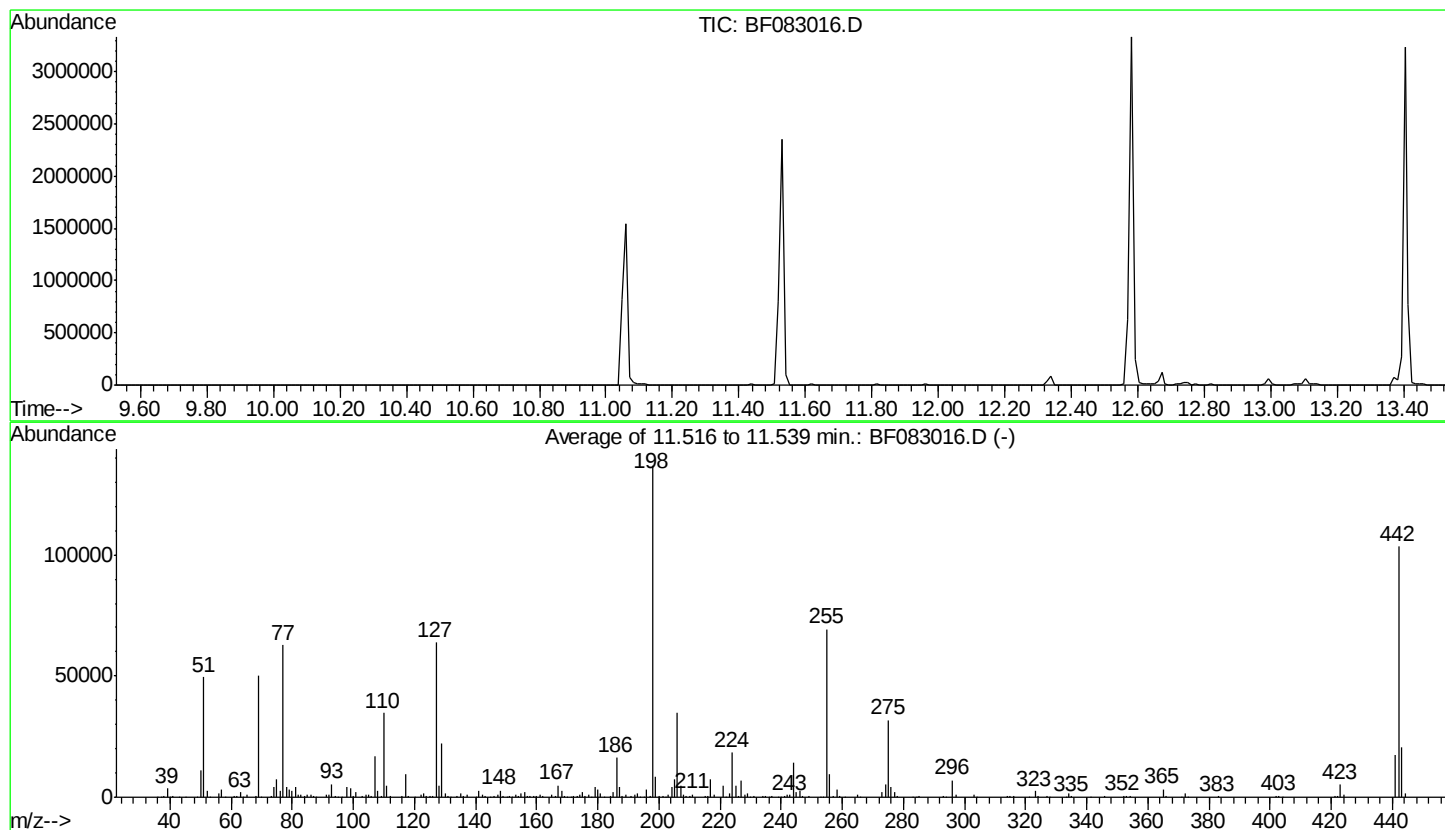

AutoFind: Scans 825, 826, 827; Background Corrected with Scan 821

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.1	49436	PASS
68	69	0.00	2	1.5	742	PASS
69	198	0.00	100	36.7	50194	PASS
70	69	0.00	2	0.3	141	PASS
127	198	10	80	46.6	63689	PASS
197	198	0.00	2	0.4	541	PASS
198	198	100	100	100.0	136814	PASS
199	198	5	9	6.2	8520	PASS
275	198	10	60	23.2	31727	PASS
365	198	1	100	2.3	3189	PASS
441	442	0.01	24	16.8	17398	PASS
442	198	50	100	75.5	103271	PASS
443	442	15	24	20.1	20799	PASS