
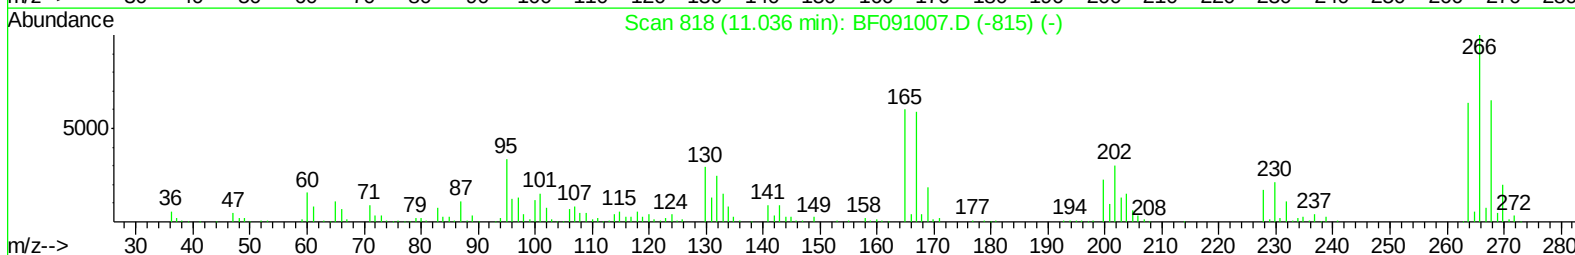
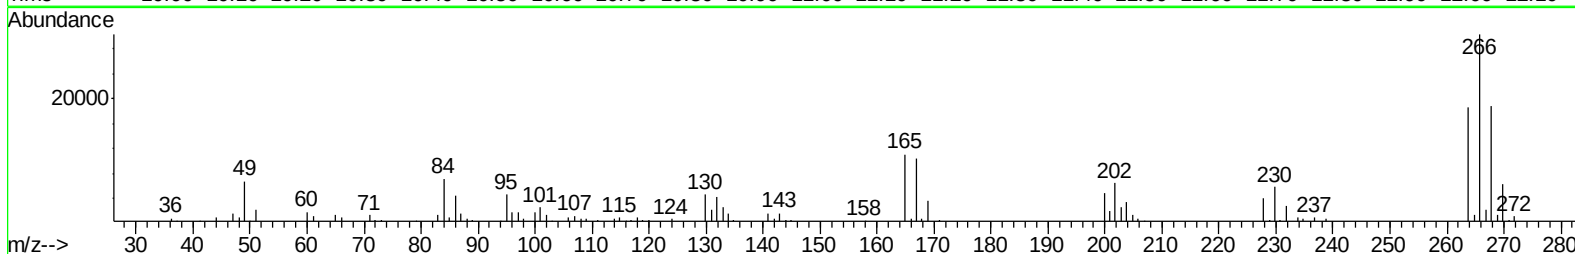


Data Path : Z:\HPCHEM1\BNA_F\Data\BF111816\
Data File : BF091231.D
Acq On : 18 Nov 2016 12:11
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 21 00:11:35 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 08 12:59:29 2016
Response via : Initial Calibration

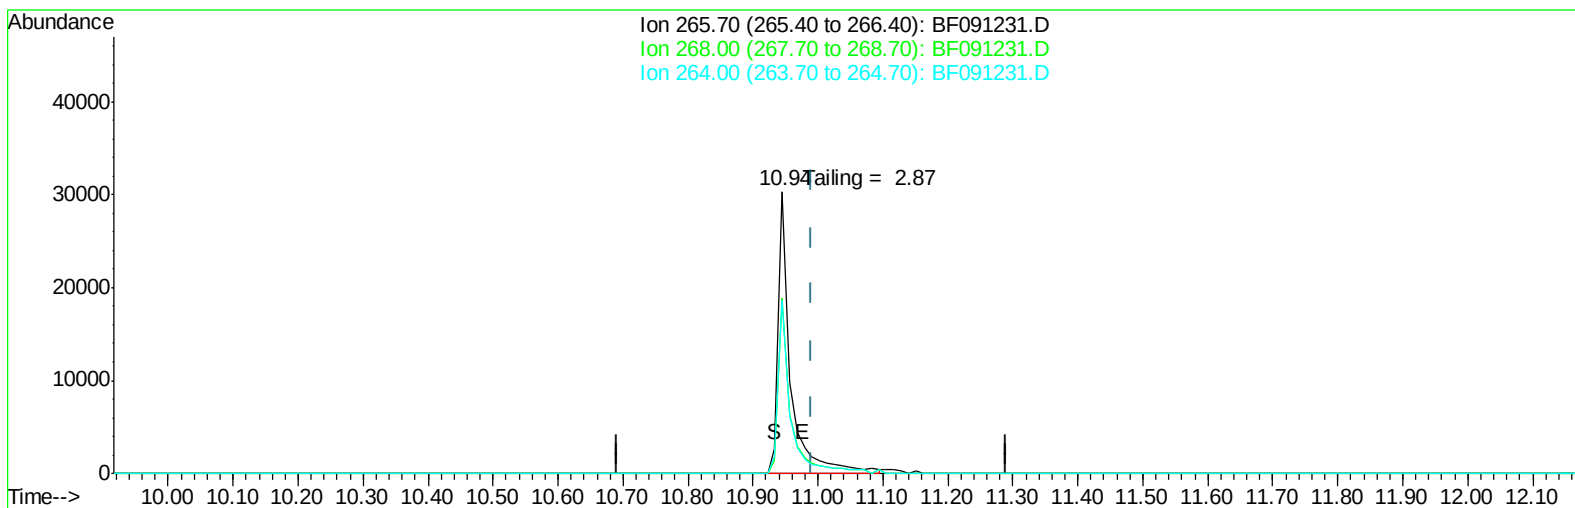

TIC: BF091231.D

(69) Pentachlorophenol (C)




10.945min (-0.046) 0.00ng

response 41191

Ion	Exp%	Act%
265.70	100	100
268.00	65.10	62.10
264.00	63.90	61.18
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF111816\
Data File : BF091231.D
Acq On : 18 Nov 2016 12:11
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 21 00:11:35 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 08 12:59:29 2016
Response via : Initial Calibration

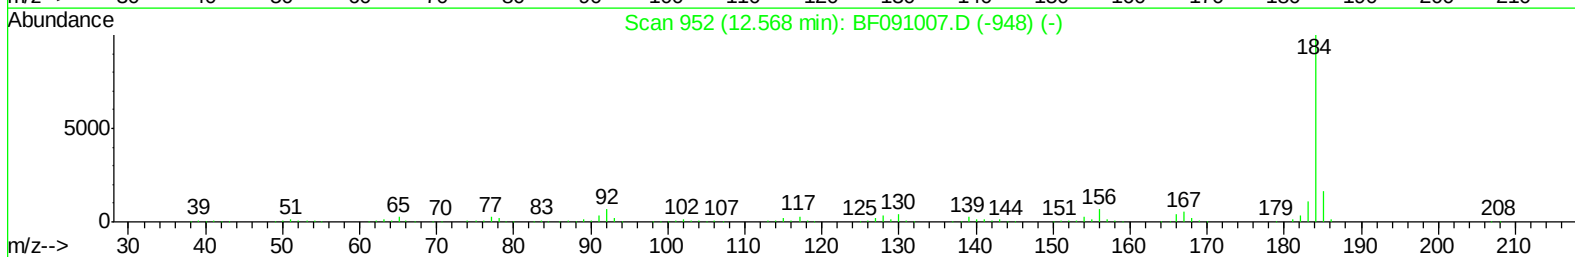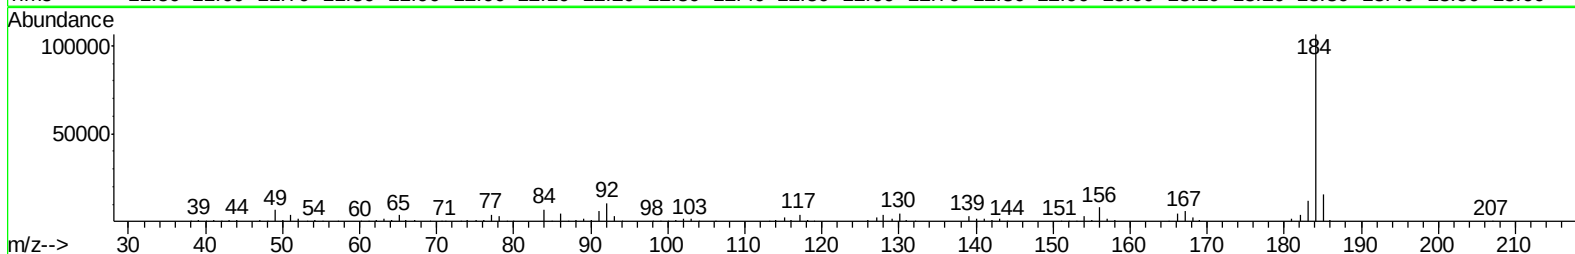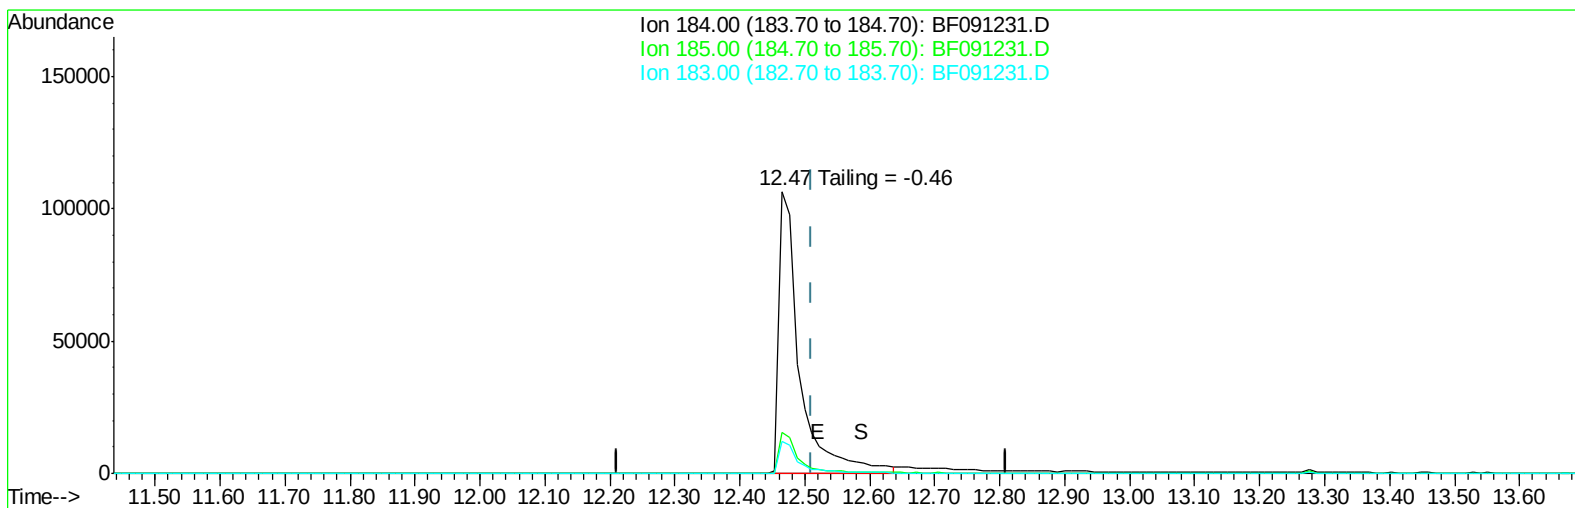

TIC: BF091231.D

(76) Benzidine

12.465min (-0.046) 4833.86ng m

response 234017

Ion	Exp%	Act%
184.00	100	100
185.00	16.20	14.40
183.00	10.90	11.34
0.00	0.00	0.00