

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF111816\
 Data File : BF091239.D
 Acq On : 18 Nov 2016 18:06
 Operator : UM/SJ
 Sample : H5706-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 FK-BPM-02-002-ABCD

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110316.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.738	265	267	287	rBV	738096	1278612	28.14%	3.589%
2	5.196	305	307	325	rBV	3298426	3753814	82.61%	10.536%
3	6.270	398	401	403	rBV	2526766	3223285	70.94%	9.047%
4	6.373	408	410	413	rBV	2783332	3061720	67.38%	8.593%
5	6.613	429	431	440	rBV	532637	883627	19.45%	2.480%
6	6.762	442	444	460	rVB	2731188	2628186	57.84%	7.376%
7	7.184	479	481	483	rBV	1587721	1925694	42.38%	5.405%
8	7.893	541	543	557	rBV	1125142	1277510	28.11%	3.586%
9	8.979	635	638	640	rBV	4035167	4241705	93.35%	11.905%
10	9.379	671	673	678	rVB	130856	124391	2.74%	0.349%
11	9.642	694	696	699	rBV	1579024	1466147	32.27%	4.115%
12	10.076	732	734	738	rBV	384062	373826	8.23%	1.049%
13	10.430	763	765	768	rBV2	1955487	2388218	52.56%	6.703%
14	10.568	775	777	781	rVB	52574	83646	1.84%	0.235%
15	11.128	824	826	828	rBV	1275245	1437511	31.64%	4.035%
16	12.716	962	965	967	rBV	3333418	4543884	100.00%	12.753%
17	13.619	1041	1044	1049	rBV	77757	127653	2.81%	0.358%
18	13.757	1054	1056	1068	rVV	1415945	1509030	33.21%	4.235%
19	15.117	1173	1175	1192	rVB	878156	1301205	28.64%	3.652%


Sum of corrected areas: 35629664

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF111816\
Data File : BF091239.D
Acq On : 18 Nov 2016 18:06
Operator : UM/SJ
Sample : H5706-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FK-BPM-02-002-ABCD

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

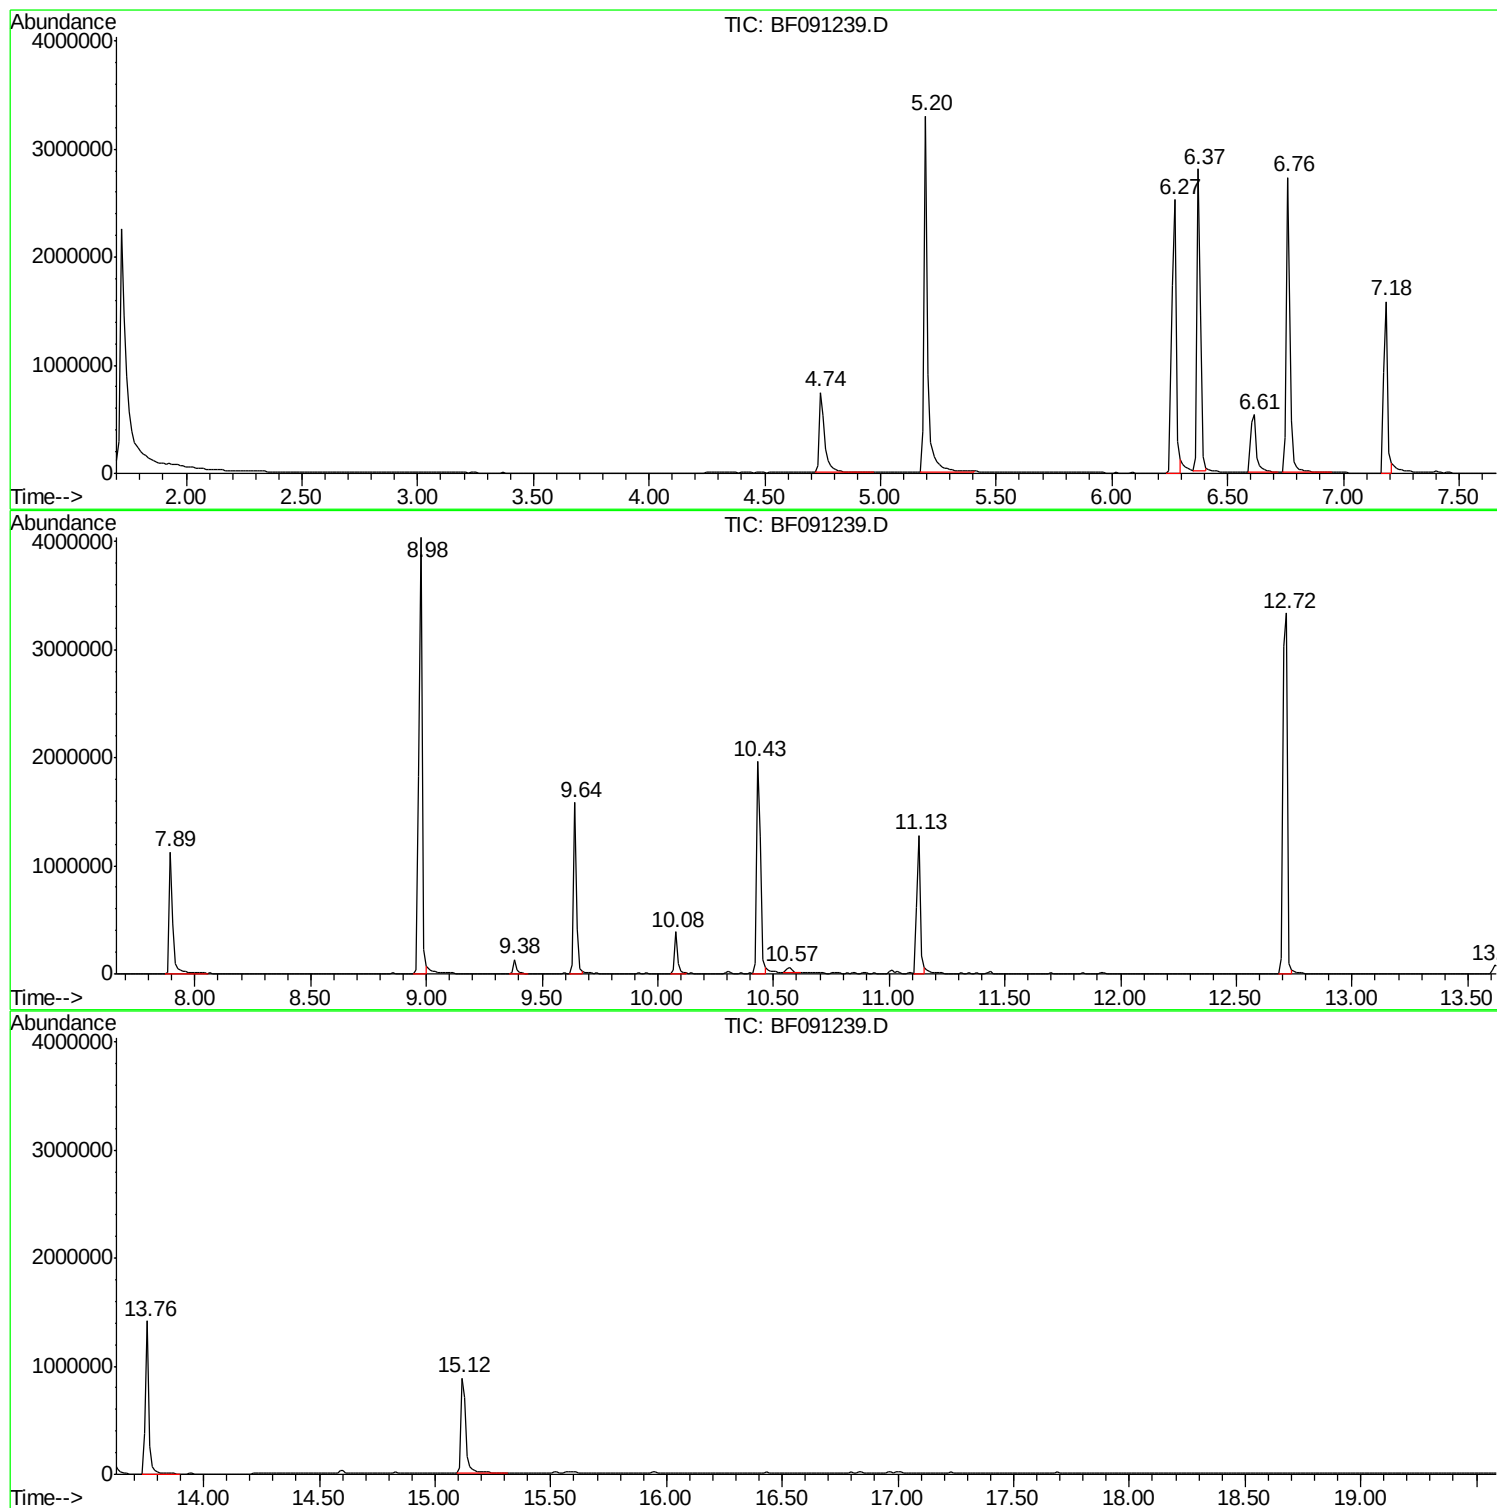

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF111816\
Data File : BF091239.D
Acq On : 18 Nov 2016 18:06
Operator : UM/SJ
Sample : H5706-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FK-BPM-02-002-ABCD










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.74	28.94 ng	1278610	1,4-Dichlorobenzene-d4	6.61

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	64
2			Propane, 2-methyl-2-(1-methyleth...	116	C7H16O	017348-59-3	36
3			3-Hexanol, 4-methyl-	116	C7H16O	000615-29-2	28
4			Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	23
5			2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	9

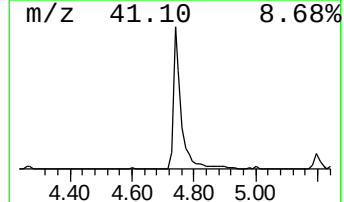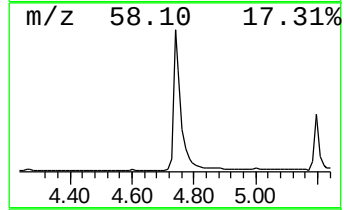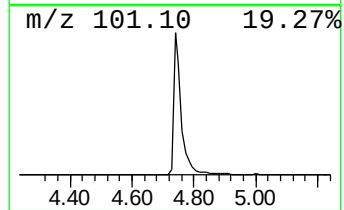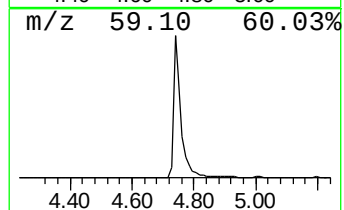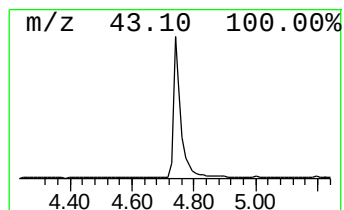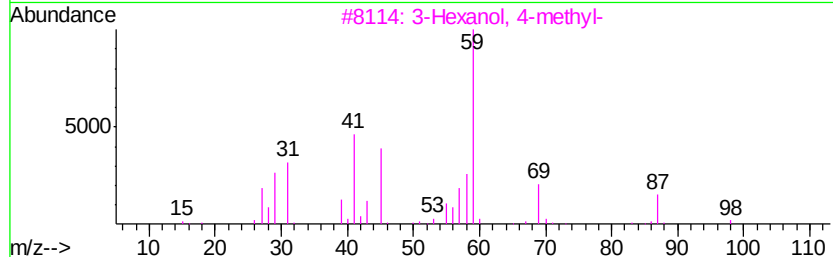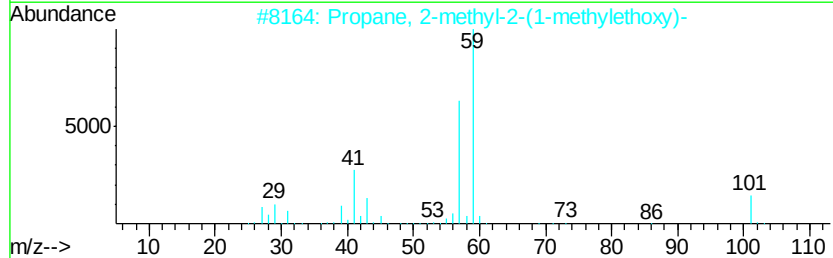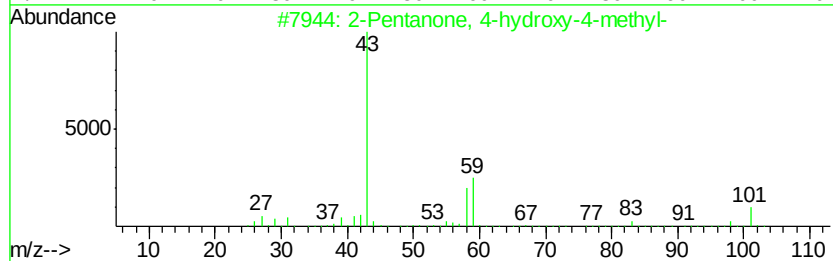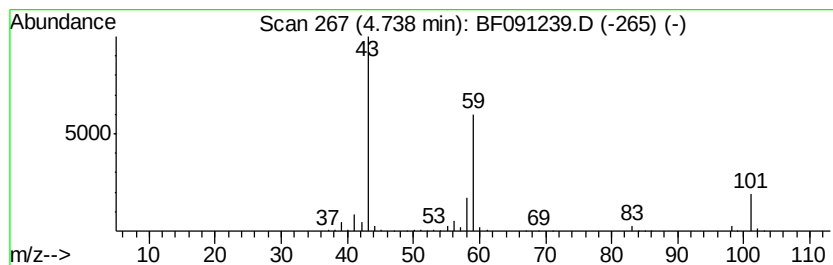

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF111816\
Data File : BF091239.D
Acq On : 18 Nov 2016 18:06
Operator : UM/SJ
Sample : H5706-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FK-BPM-02-002-ABCD










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.37 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.37	69.30 ng	3061720	1,4-Dichlorobenzene-d4	6.61

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	16
2		5-Aminoindole	132	C8H8N2	005192-03-0	12
3		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	9
4		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9
5		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	9

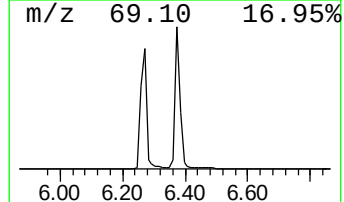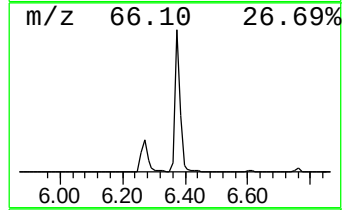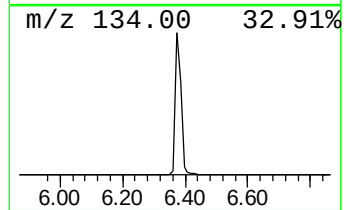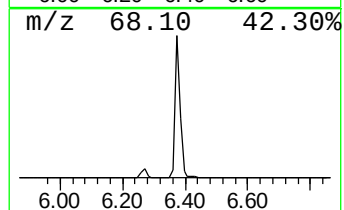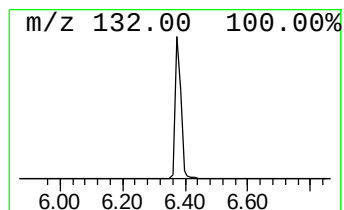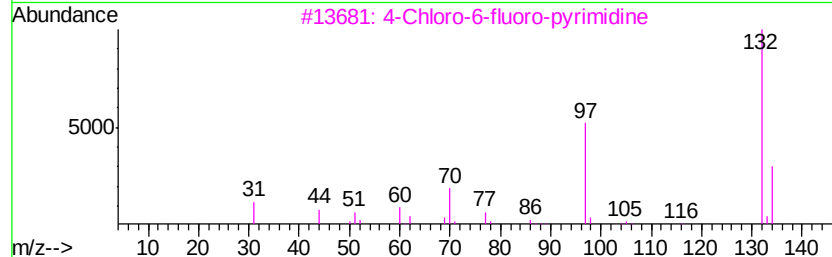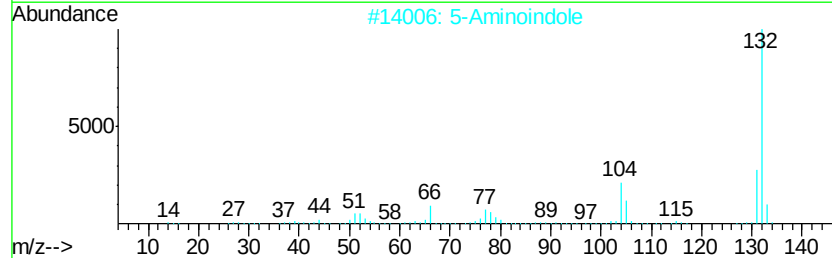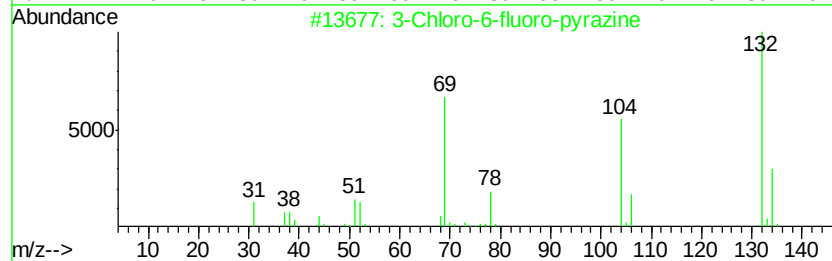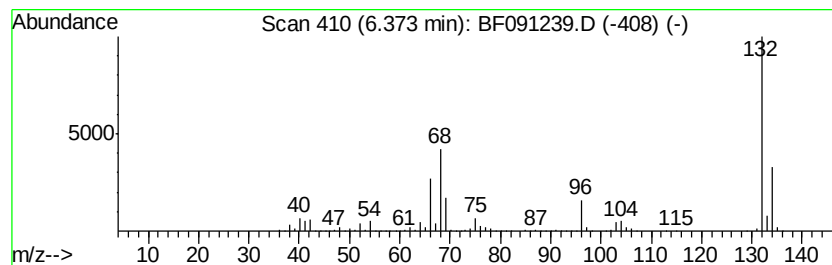

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF111816\
Data File : BF091239.D
Acq On : 18 Nov 2016 18:06
Operator : UM/SJ
Sample : H5706-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FK-BPM-02-002-ABCD

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	4.74	28.9	ng	1278610	1	6.61	883627	20.0
unknown6.37	6.37	69.3	ng	3061720	1	6.61	883627	20.0