


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF111816\
Data File : BF091231.D
Acq On : 18 Nov 2016 12:11
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110316.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Nov 08 12:59:29 2016

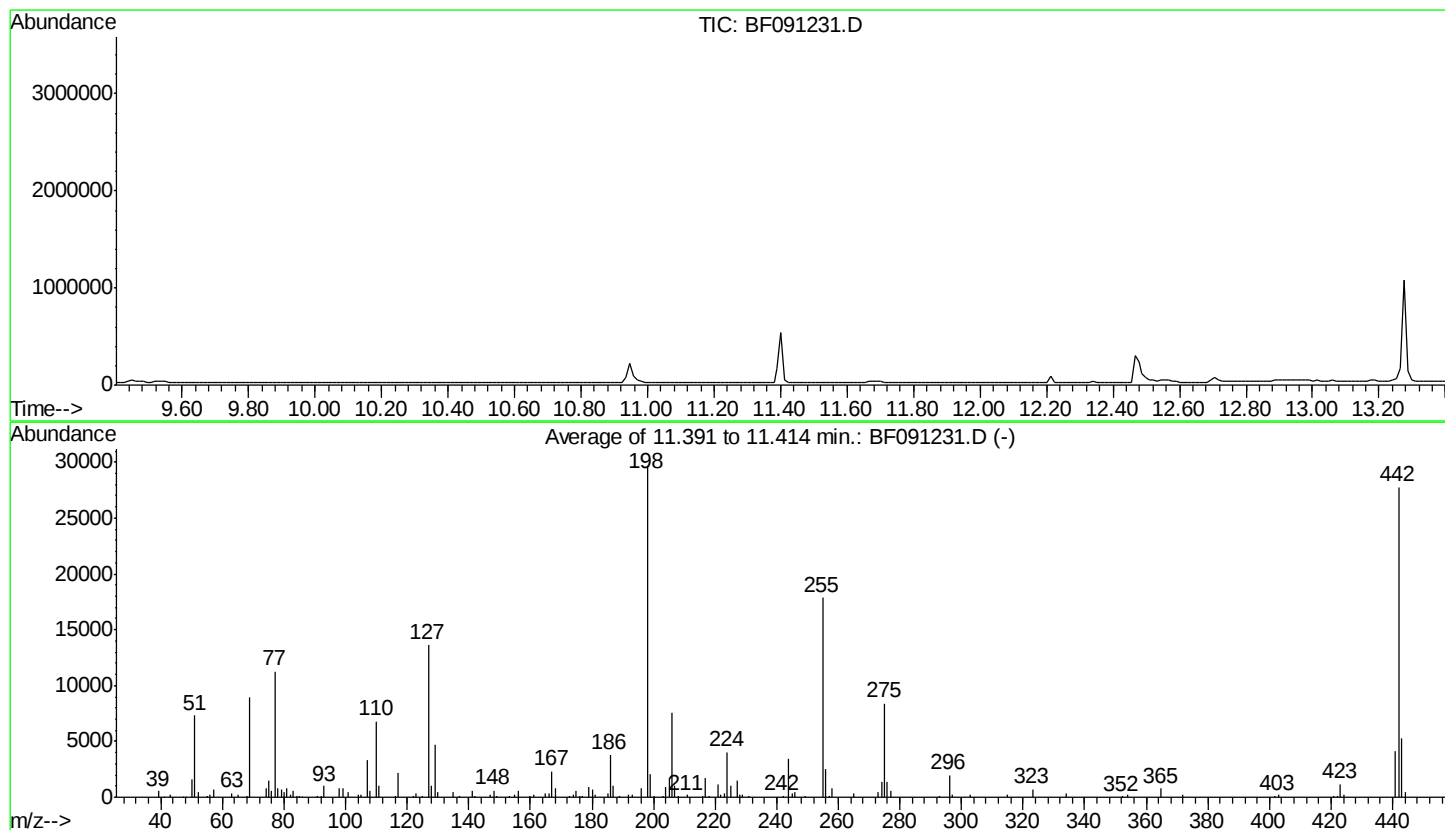

AutoFind: Scans 849, 850, 851; Background Corrected with Scan 845

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.6	7294	PASS
68	69	0.00	2	1.3	113	PASS
69	198	0.00	100	30.1	8933	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.0	13658	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	29693	PASS
199	198	5	9	6.8	2023	PASS
275	198	10	60	28.2	8375	PASS
365	198	1	100	2.5	752	PASS
441	442	0.01	24	15.0	4152	PASS
442	198	50	100	93.5	27757	PASS
443	442	15	24	19.2	5331	PASS