


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF111816\
 Data File : BF091235.D
 Acq On : 18 Nov 2016 16:13
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110316.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 08 12:59:29 2016

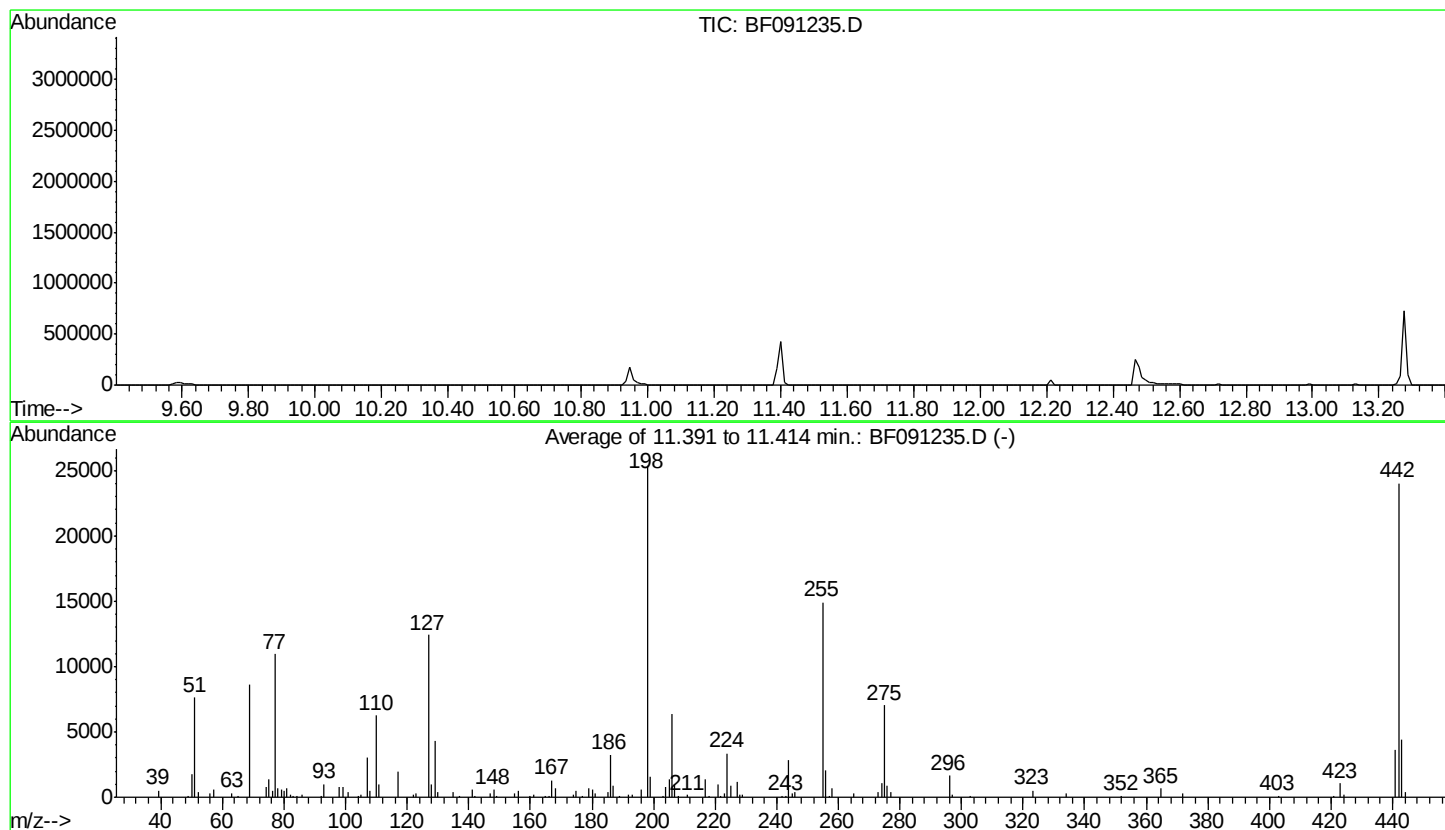

AutoFind: Scans 849, 850, 851; Background Corrected with Scan 845

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.9	7600	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	33.9	8602	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.0	12437	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	25381	PASS
199	198	5	9	6.3	1592	PASS
275	198	10	60	27.7	7036	PASS
365	198	1	100	2.5	647	PASS
441	442	0.01	24	15.0	3606	PASS
442	198	50	100	94.6	24011	PASS
443	442	15	24	18.5	4440	PASS