
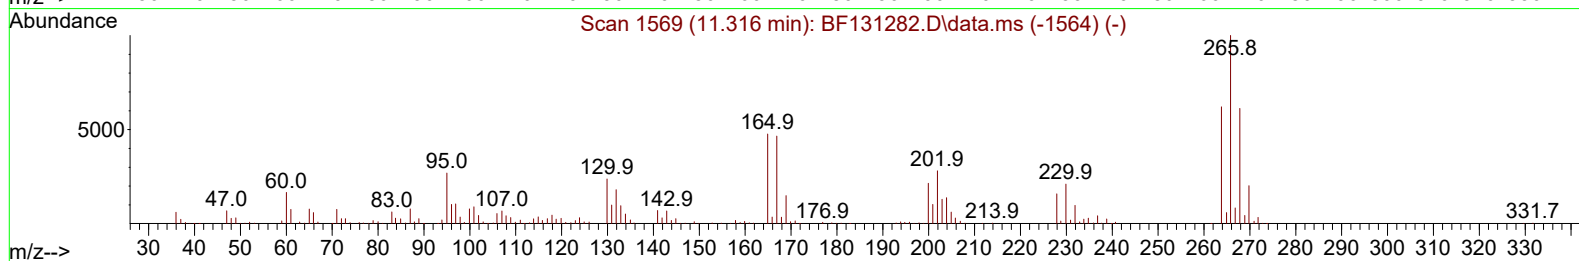
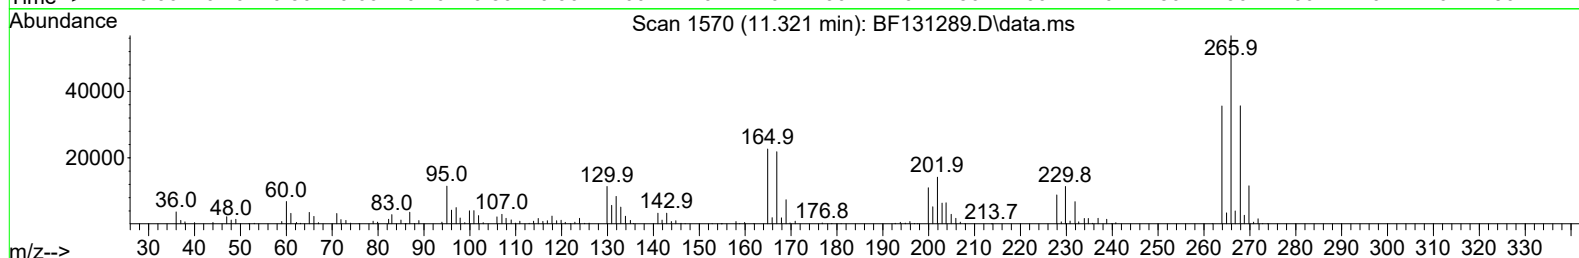


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111822\
 Data File : BF131289.D
 Acq On : 18 Nov 2022 08:35
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 19 05:02:07 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 18 01:41:28 2022
 Response via : Initial Calibration

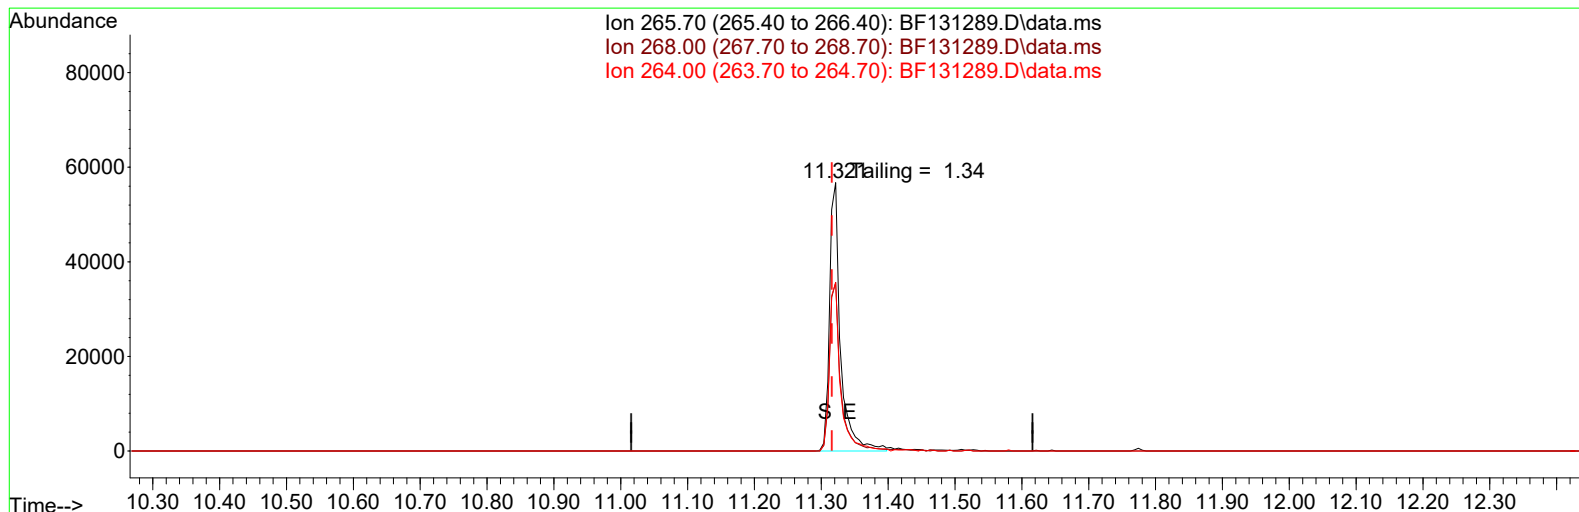

TIC: BF131289.D\data.ms

(70) Pentachlorophenol (C)




11.321min (+ 0.005) 28571.82 ng

response 66175

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	62.84
264.00	62.10	62.71
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111822\
Data File : BF131289.D
Acq On : 18 Nov 2022 08:35
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 19 05:02:07 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 18 01:41:28 2022
Response via : Initial Calibration

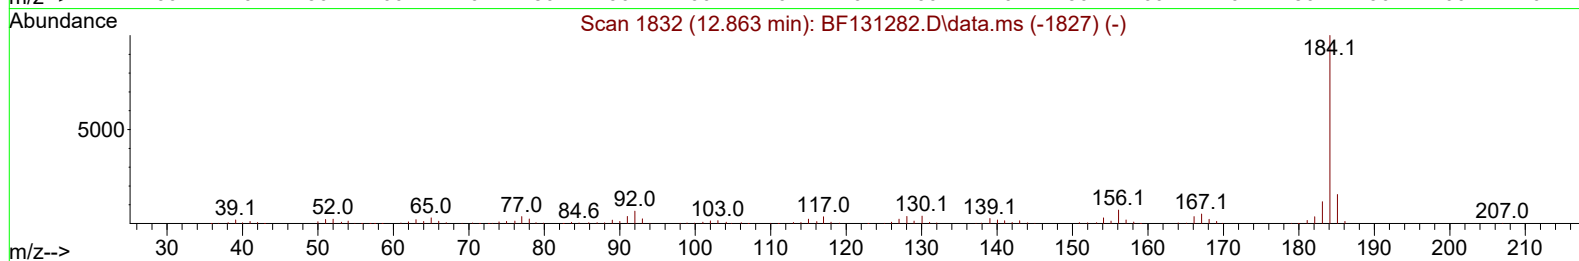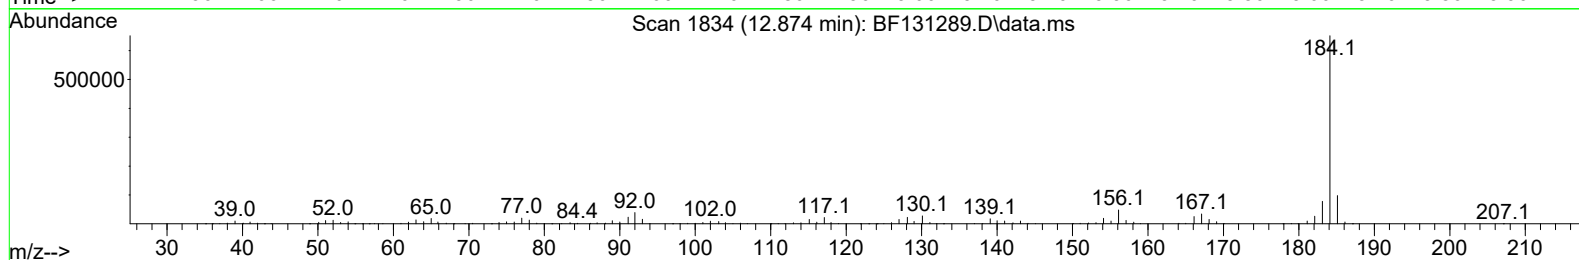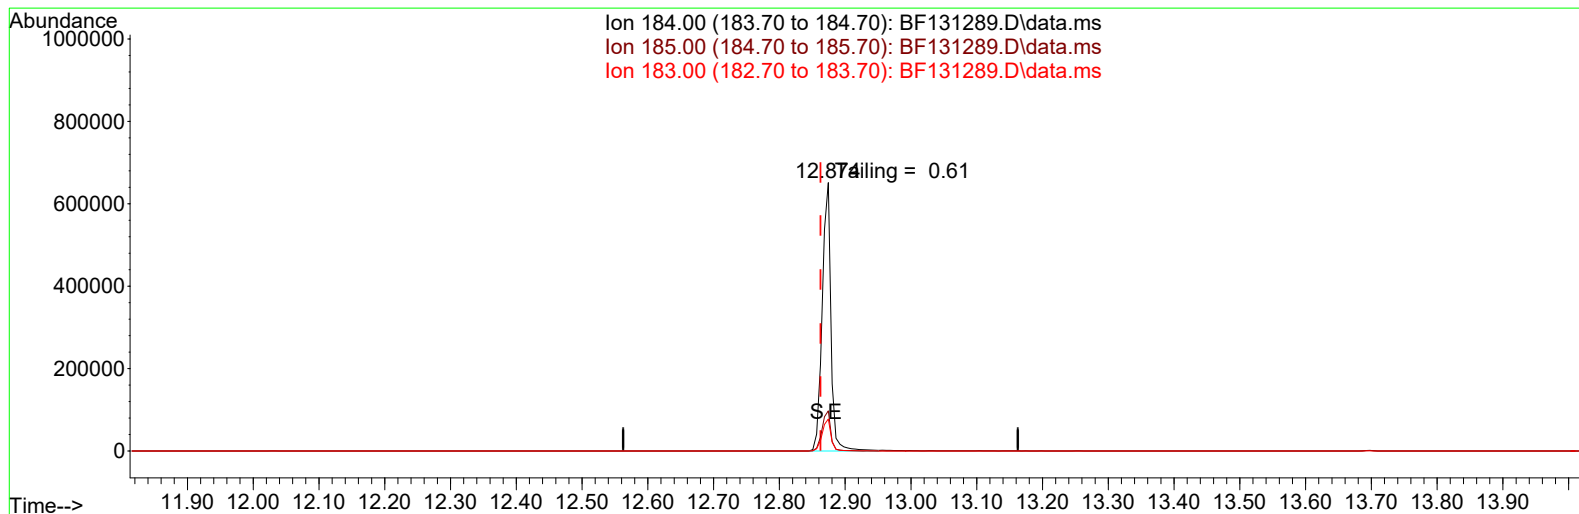

TIC: BF131289.D\data.ms

(77) Benzidine

12.874min (+ 0.012) 0.00 ng

response 604547

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.40	14.98
183.00	11.60	11.95
0.00	0.00	0.00