
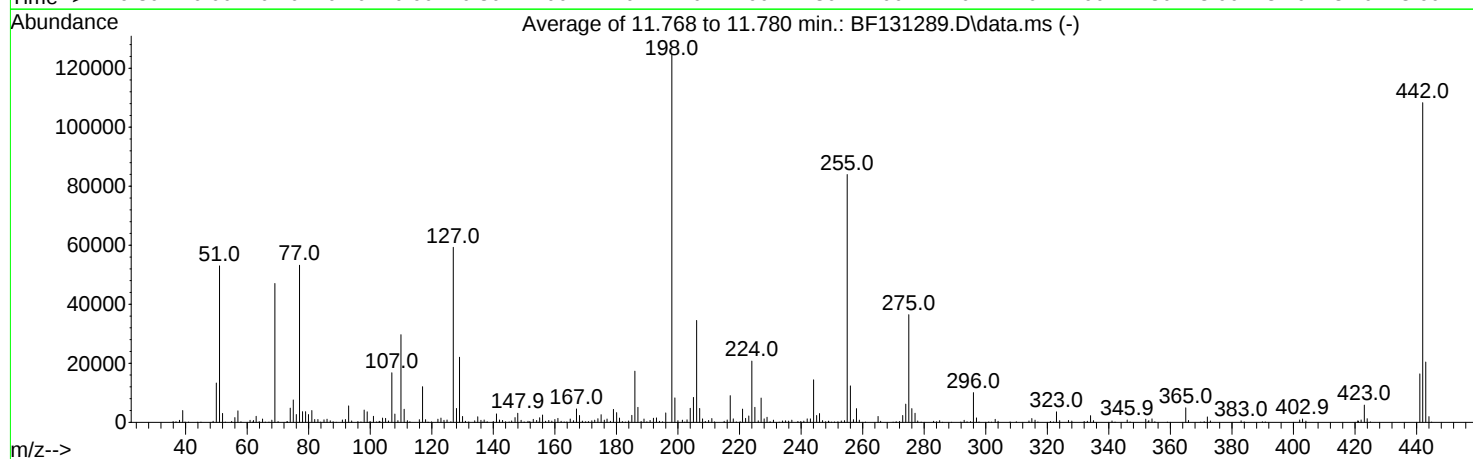


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111822\
 Data File : BF131289.D
 Acq On : 18 Nov 2022 08:35
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Nov 18 01:41:28 2022

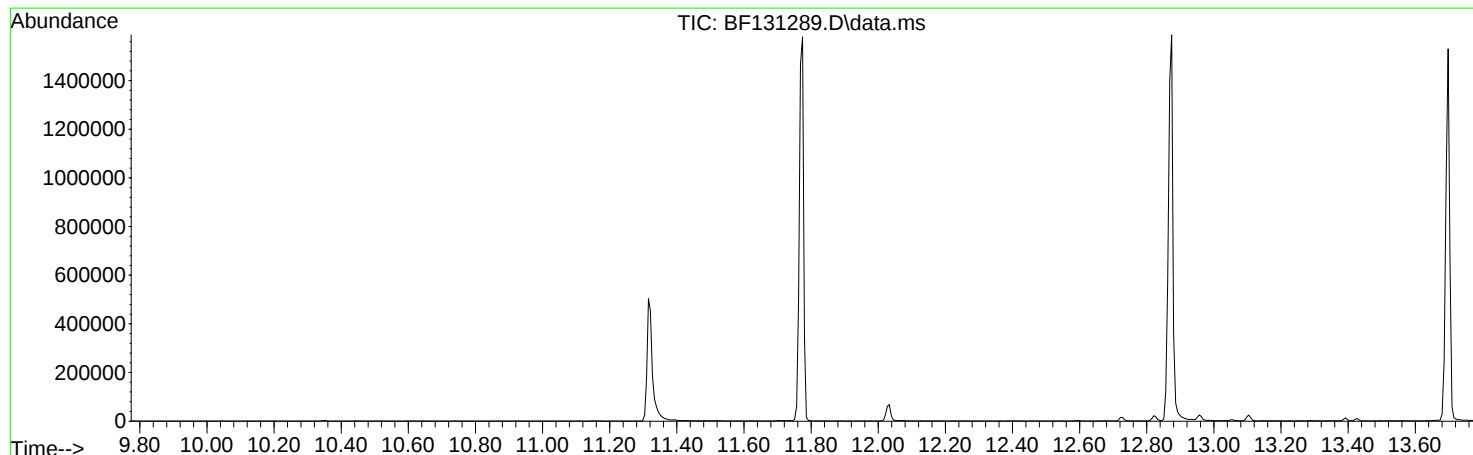




AutoFind: Scans 1646, 1647, 1648; Background Corrected with Scan 1640

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.5	53002	PASS
68	69	0.00	2	1.6	761	PASS
69	198	0.00	100	37.7	47018	PASS
70	69	0.00	2	0.5	238	PASS
127	198	10	80	47.6	59288	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	124667	PASS
199	198	5	9	6.6	8259	PASS
275	198	10	60	29.3	36488	PASS
365	198	1	100	3.9	4890	PASS
441	198	0.01	100	13.2	16408	PASS
442	442	50	100	100.0	108293	PASS
443	442	15	24	18.9	20437	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111822\
 Data File : BF131289.D
 Acq On : 18 Nov 2022 08:35
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Nov 19 05:02:07 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 18 01:41:28 2022
 Response via : Initial Calibration

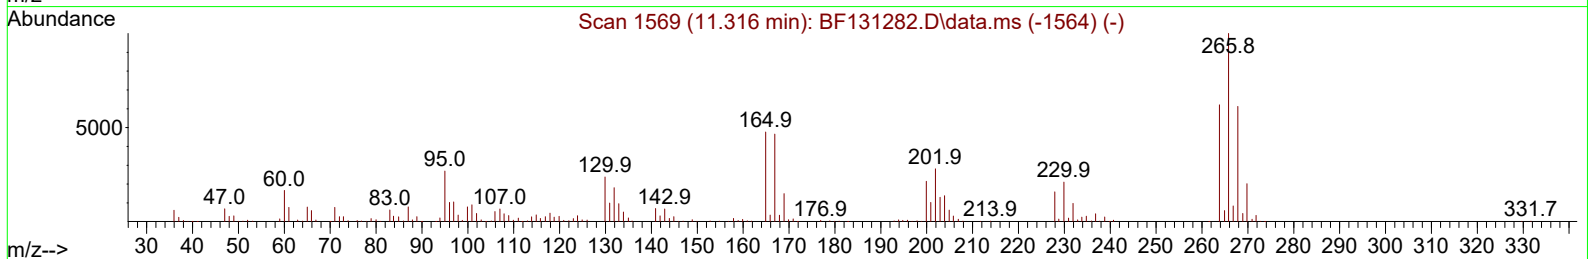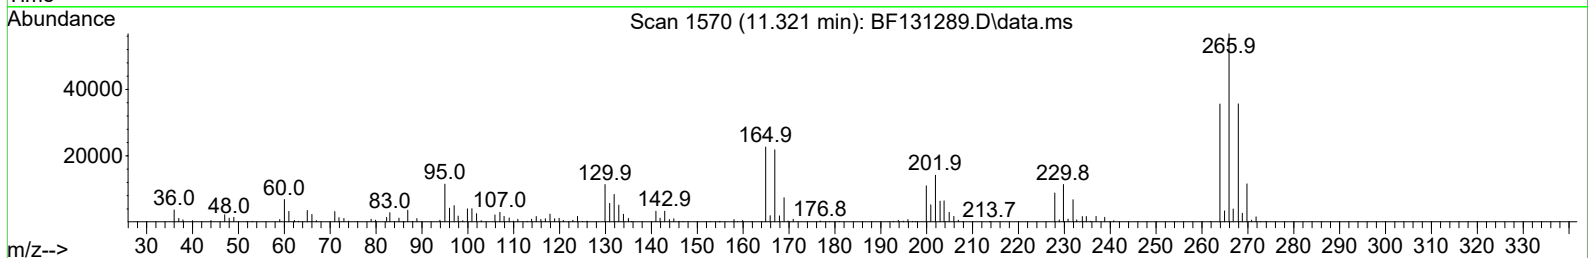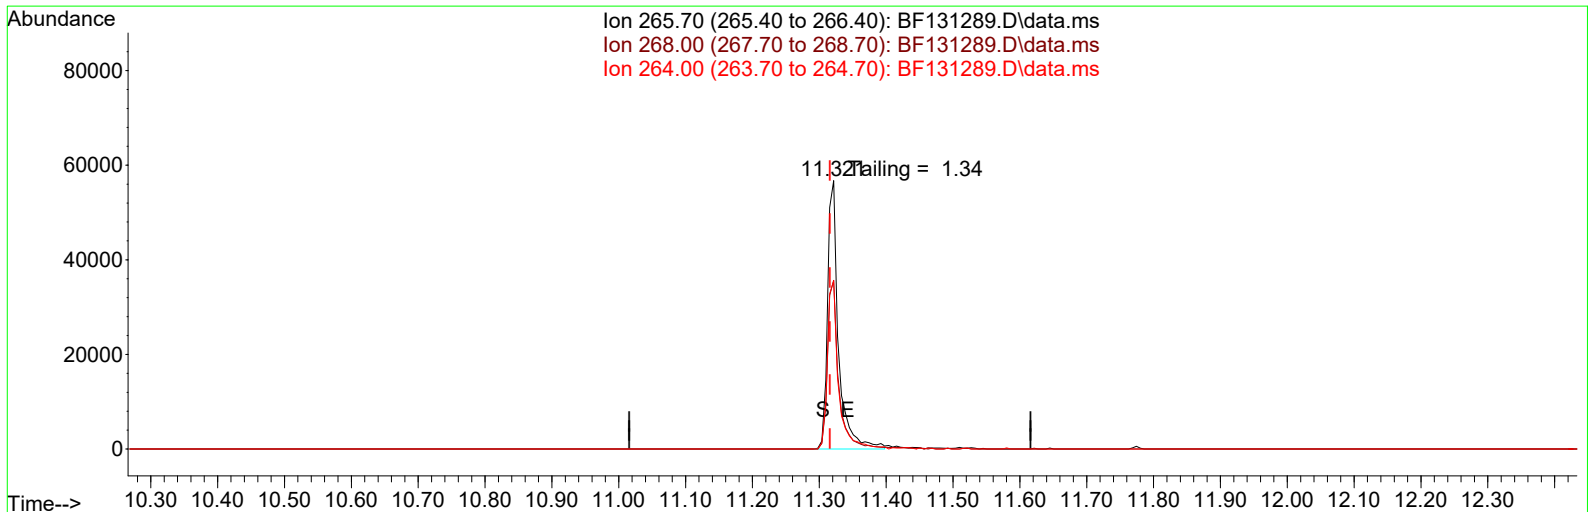

TIC: BF131289.D\data.ms

(70) Pentachlorophenol (C)

11.321min (+ 0.005) 28571.82 ng




response 66175

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	62.84
264.00	62.10	62.71
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111822\
Data File : BF131289.D
Acq On : 18 Nov 2022 08:35
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 19 05:02:07 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 18 01:41:28 2022
Response via : Initial Calibration

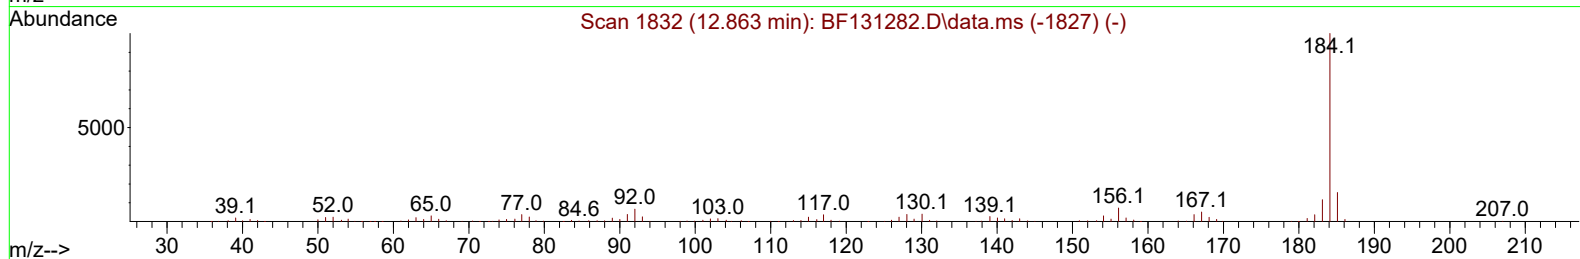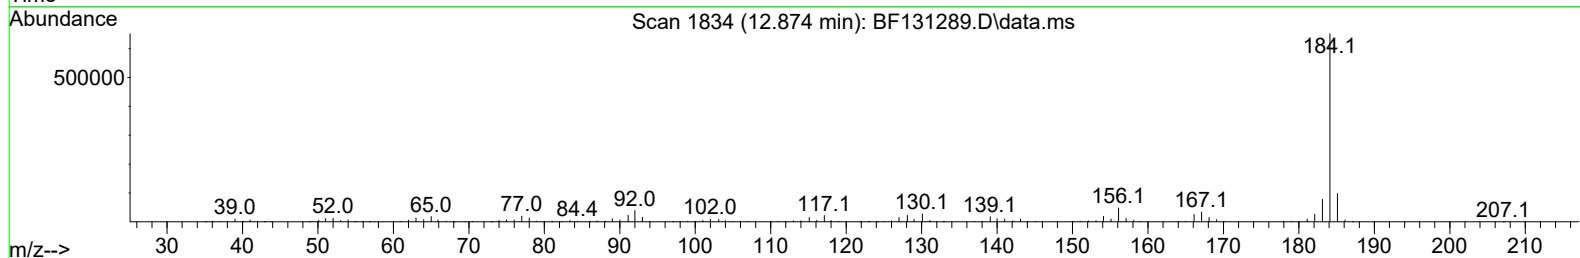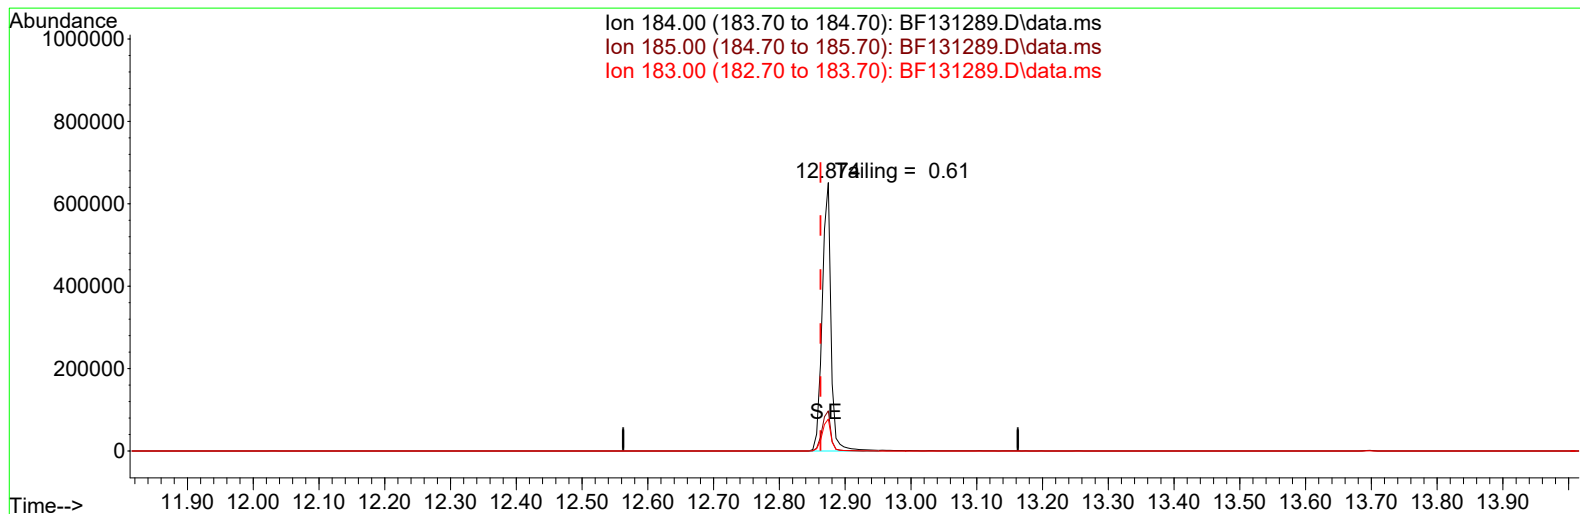

TIC: BF131289.D\data.ms

(77) Benzidine

12.874min (+ 0.012) 0.00 ng

response 604547

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.40	14.98
183.00	11.60	11.95
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/18/2022	BNA_F	<u>BF131289.D</u>
Compound Name	Response	Retention Time
DDT	193372	13.698
DDD	4049	13.392
DDE	836	13.051
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4885	198257	2.46

Instrument :
BNA_F
ClientSampleId :
DFTPP