
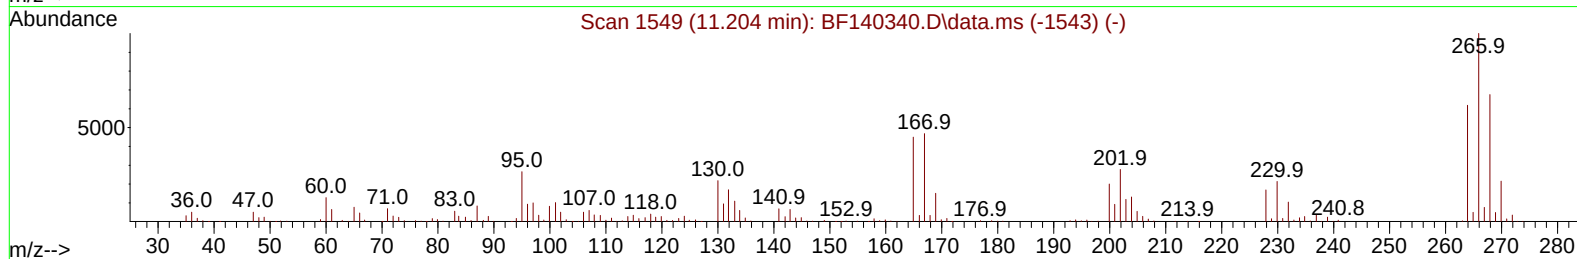
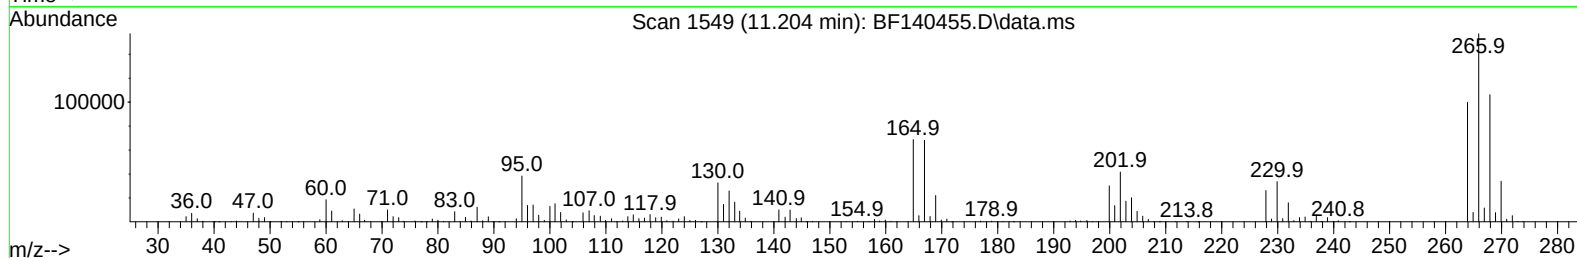


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111824\
Data File : BF140455.D
Acq On : 18 Nov 2024 15:48
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 18 16:27:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 14:40:06 2024
Response via : Initial Calibration

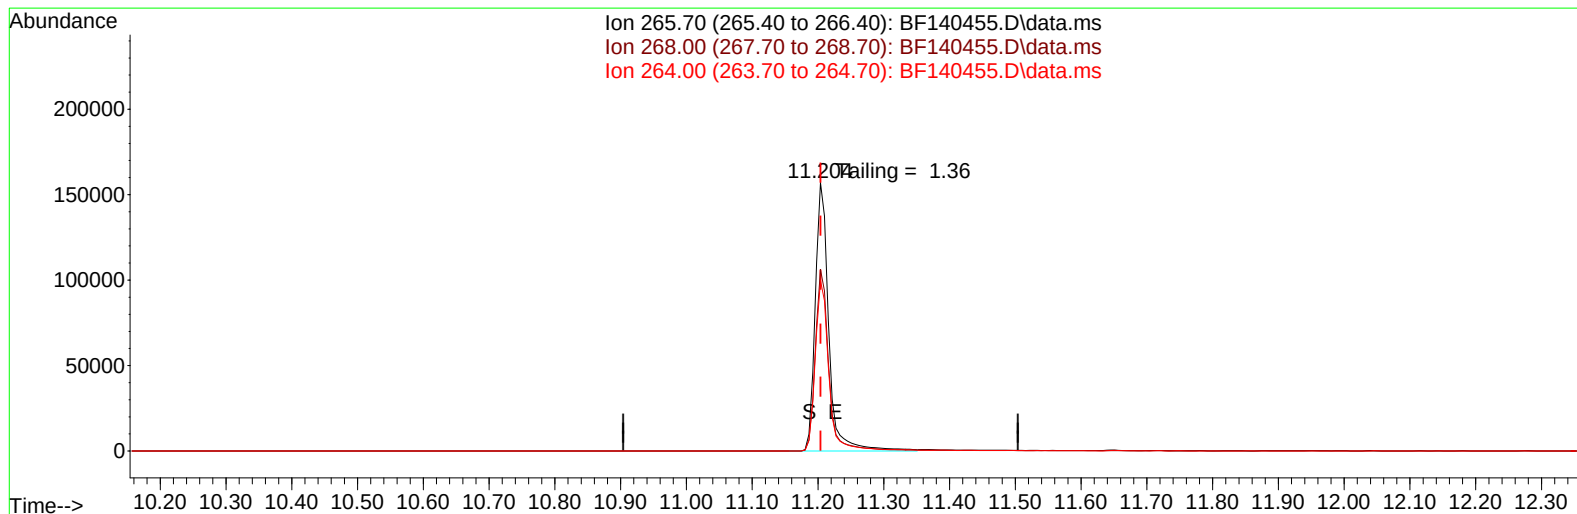

TIC: BF140455.D\data.ms

(70) Pentachlorophenol (C)




11.204min (-0.000) 43255.76 ng

response 225635

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.10	67.63
264.00	62.90	63.51
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111824\
Data File : BF140455.D
Acq On : 18 Nov 2024 15:48
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 18 16:27:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 14:40:06 2024
Response via : Initial Calibration

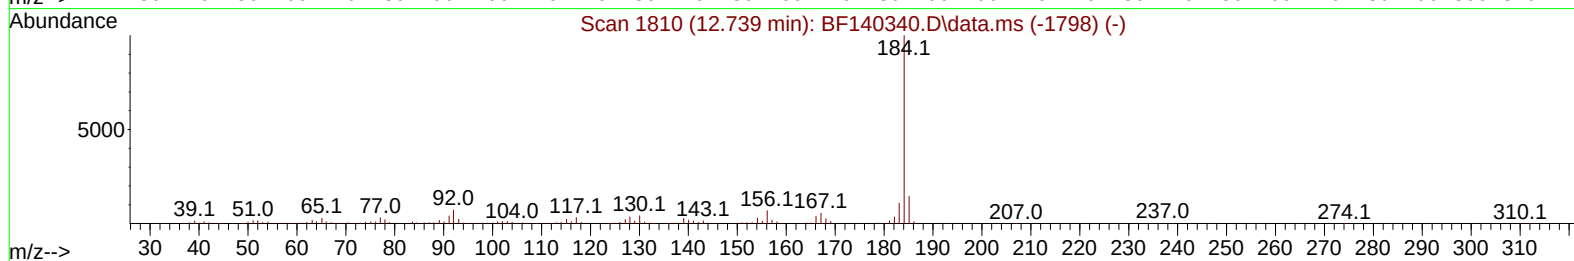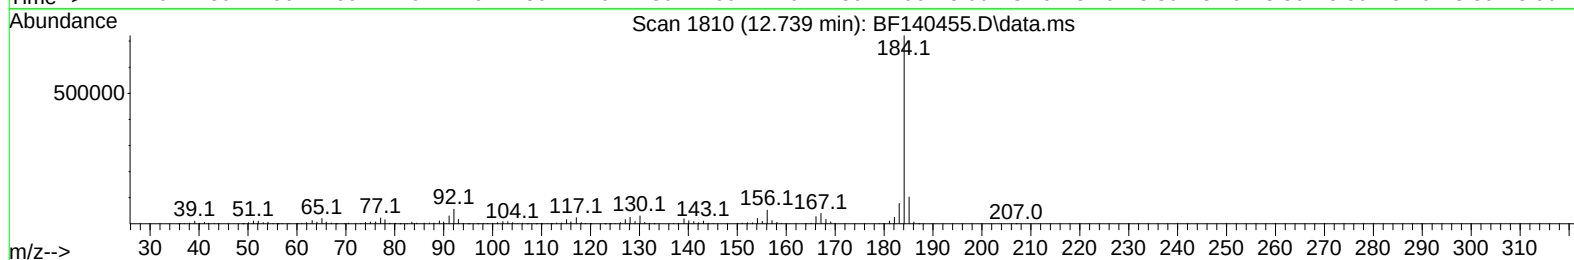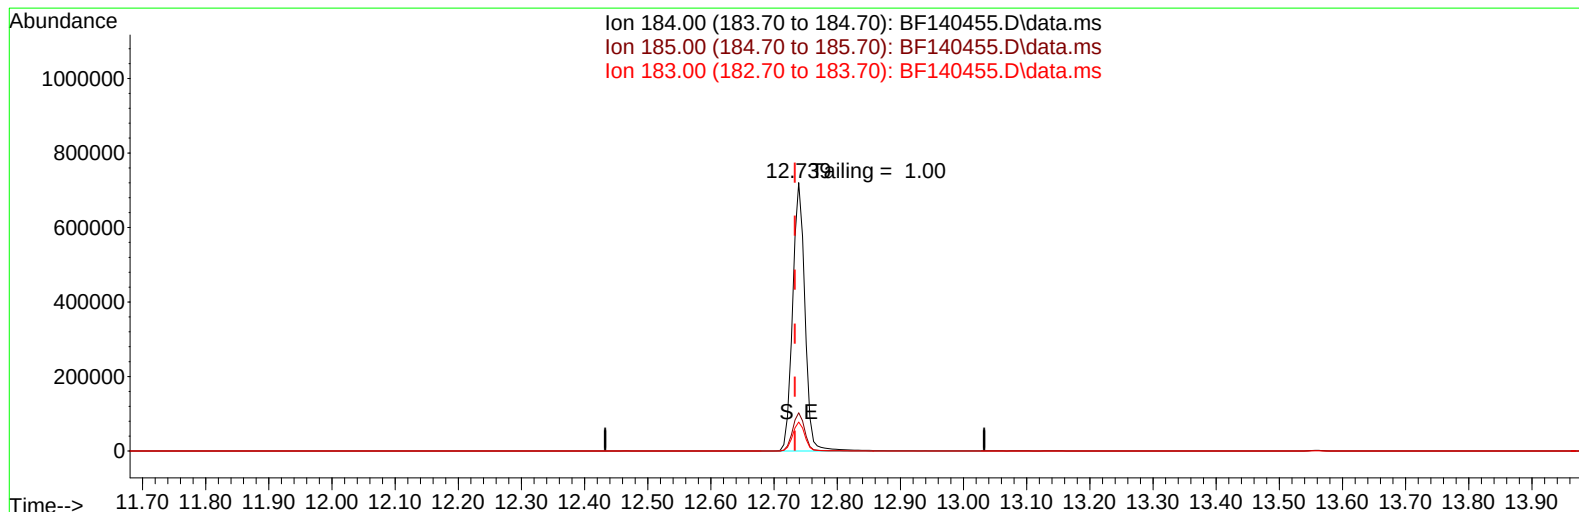

TIC: BF140455.D\data.ms

(77) Benzidine

12.739min (+ 0.006) 31853.14 ng

response **979257**

Ion	Exp%	Act%
-----	------	------

184.00	100.00	100.00
--------	--------	--------

185.00	14.90	14.27
--------	-------	-------

183.00	10.80	10.82
--------	-------	-------

0.00 0.00 0.00