


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111824\
Data File : BF140442.D
Acq On : 18 Nov 2024 09:18
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111324.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Nov 13 14:40:06 2024

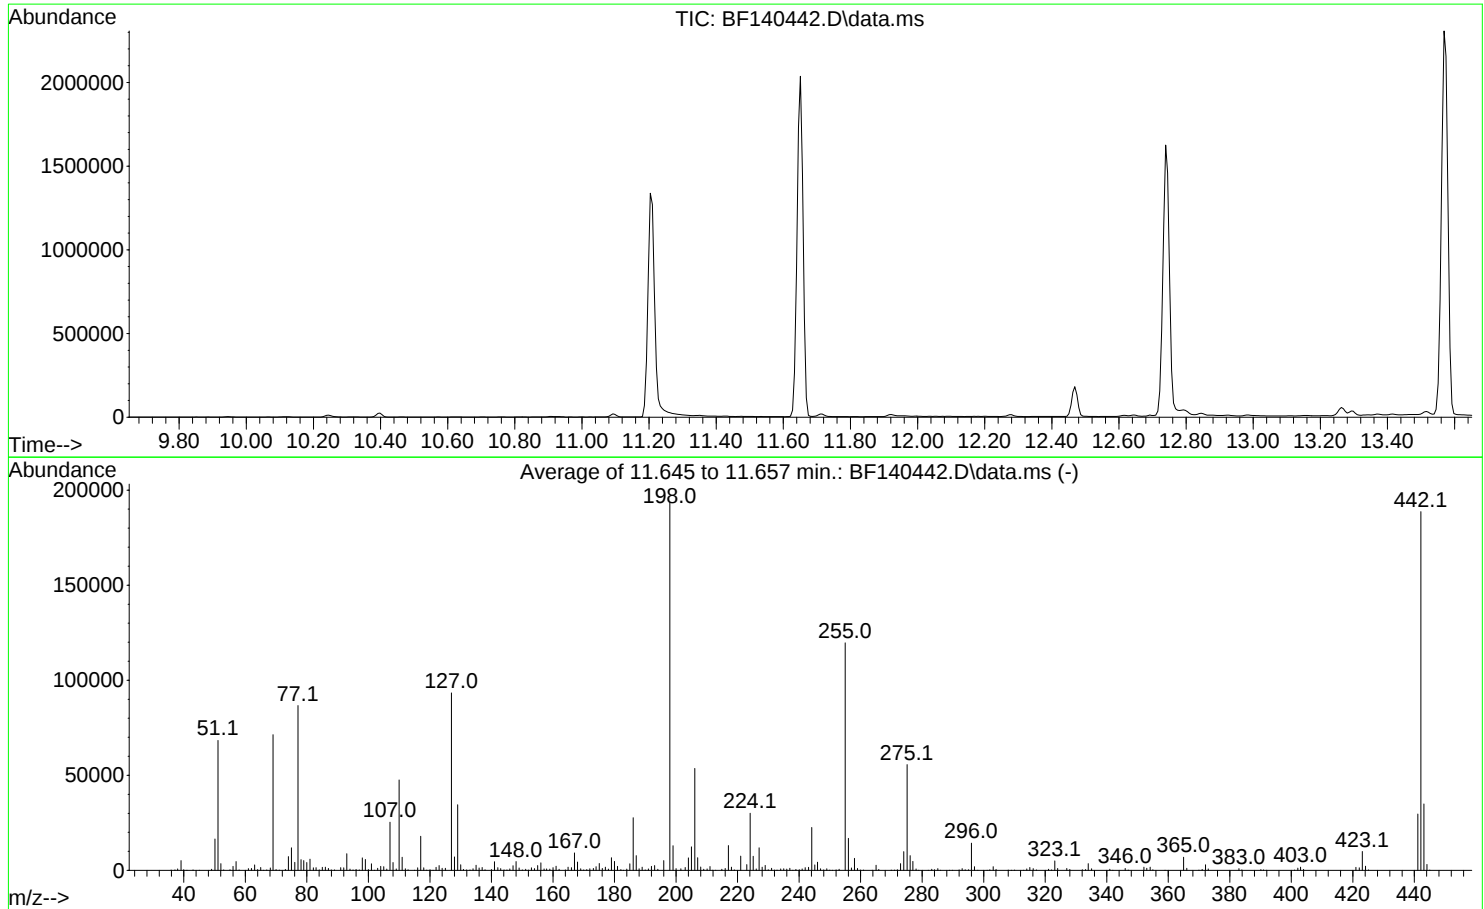

AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.3	68384	PASS
68	69	0.00	2	1.8	1271	PASS
69	198	0.00	100	36.9	71384	PASS
70	69	0.00	2	0.7	466	PASS
127	198	10	80	48.2	93325	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	193493	PASS
199	198	5	9	6.7	12961	PASS
275	198	10	60	28.7	55613	PASS
365	198	1	100	3.6	6893	PASS
441	198	0.01	100	15.3	29637	PASS
442	442	50	100	100.0	188736	PASS
443	442	15	24	18.5	34960	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
11/18/2024	BNA_F	<u>BF140442.D</u>
Compound Name	Response	Retention Time
DDT	601041	13.568
DDD	19319	13.263
DDE	1174	12.927
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
20493	621534	3.30

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111824\
Data File : BF140442.D
Acq On : 18 Nov 2024 09:18
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 18 11:35:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 14:40:06 2024
Response via : Initial Calibration

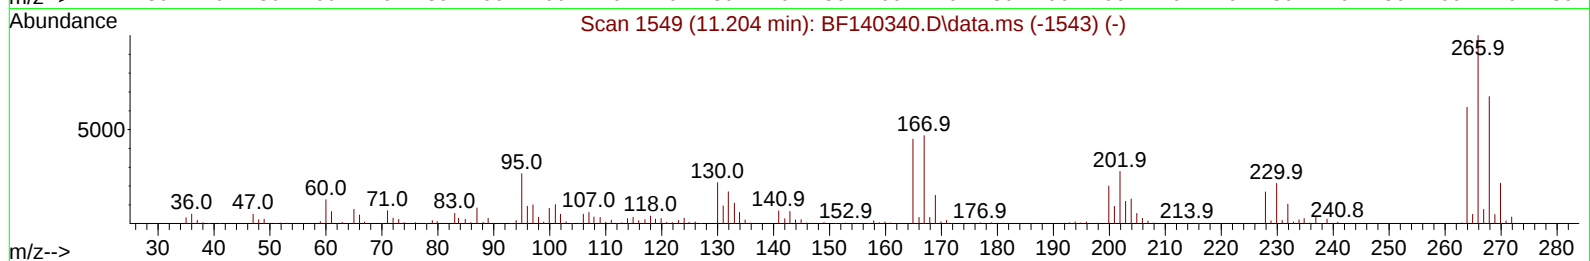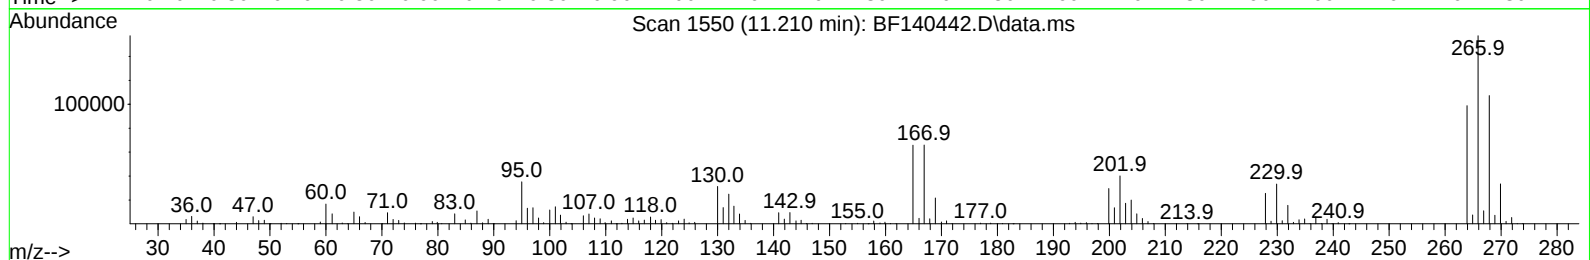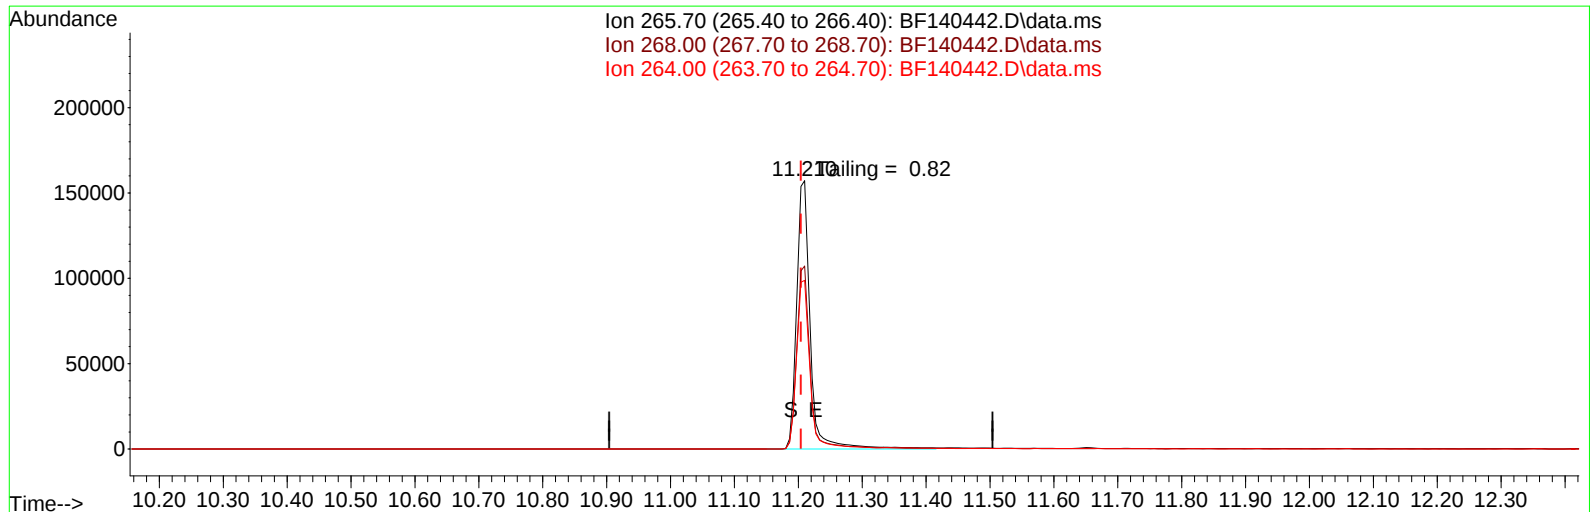

TIC: BF140442.D\data.ms

(70) Pentachlorophenol (C)

11.210min (+ 0.006) 54990.18 ng




response 234207

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.10	68.23
264.00	62.90	62.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111824\
Data File : BF140442.D
Acq On : 18 Nov 2024 09:18
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 18 11:35:59 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 14:40:06 2024
Response via : Initial Calibration

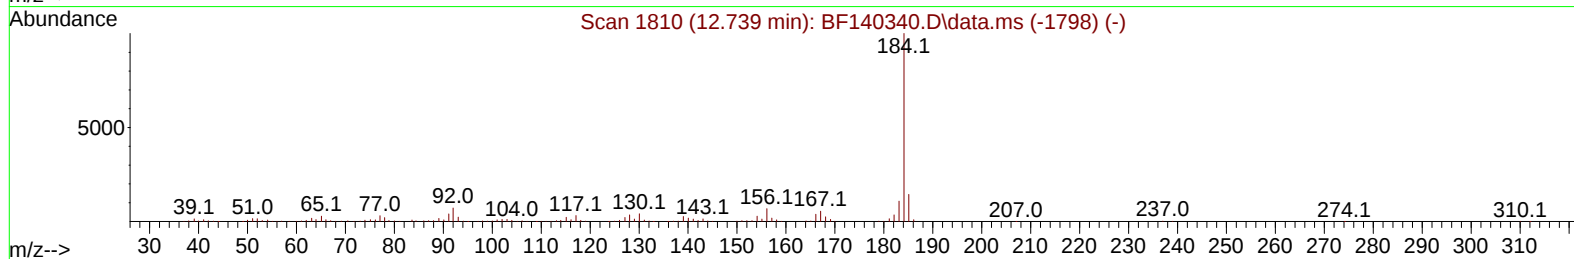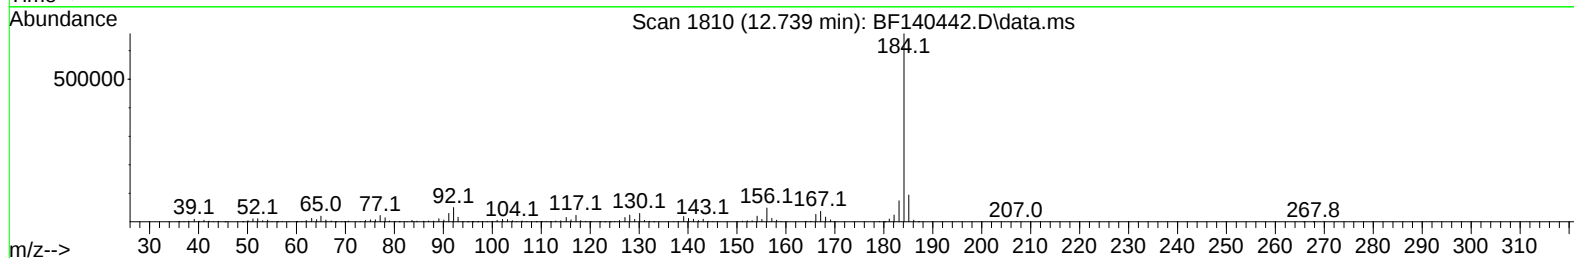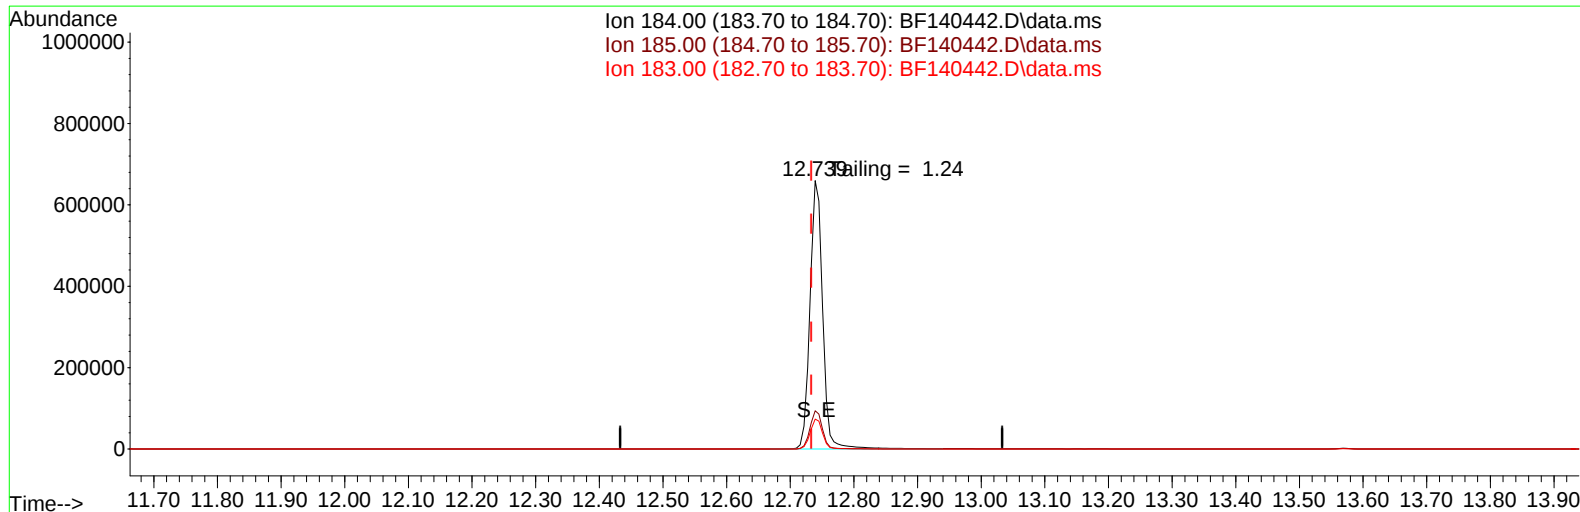

TIC: BF140442.D\data.ms

(77) Benzidine

12.739min (+ 0.006) 29617.83 ng

response 919631

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.26
183.00	10.80	11.18
0.00	0.00	0.00