
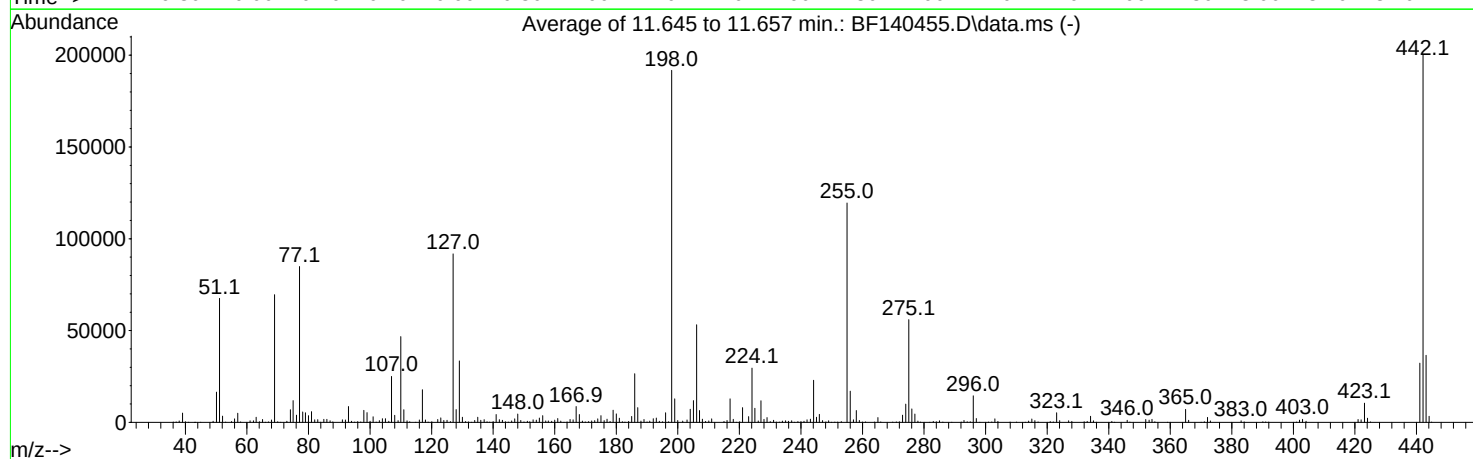


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111824\
Data File : BF140455.D
Acq On : 18 Nov 2024 15:48
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111324.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Nov 13 14:40:06 2024

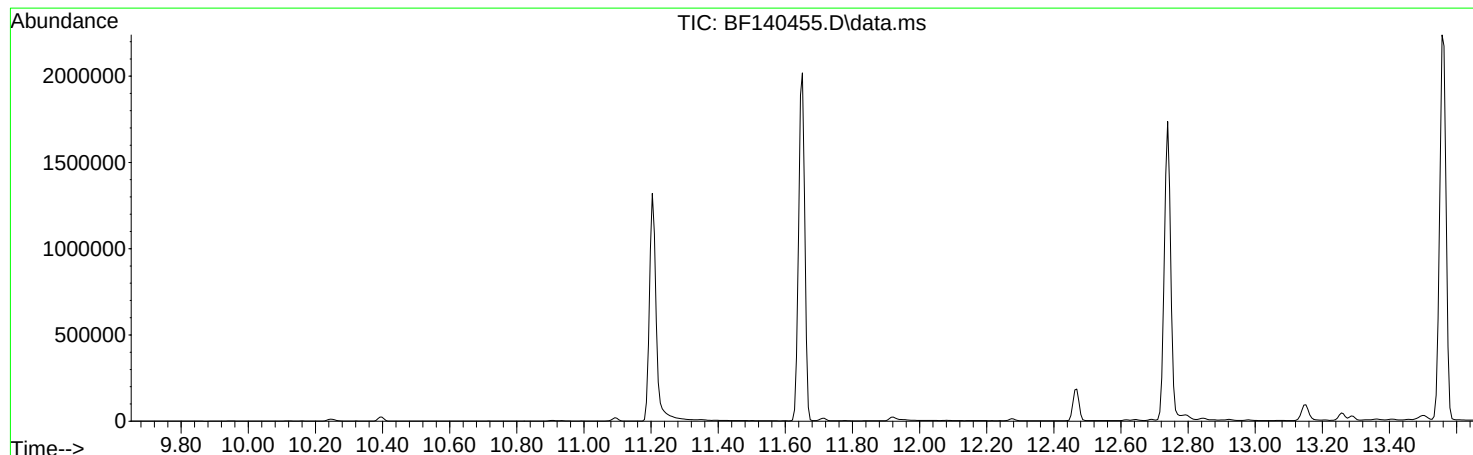

AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.2	67520	PASS
68	69	0.00	2	1.9	1342	PASS
69	198	0.00	100	36.3	69579	PASS
70	69	0.00	2	0.5	373	PASS
127	198	10	80	47.9	91781	PASS
197	198	0.00	2	0.2	361	PASS
198	198	100	100	100.0	191744	PASS
199	198	5	9	6.7	12859	PASS
275	198	10	60	29.2	55968	PASS
365	198	1	100	3.7	7095	PASS
441	198	0.01	100	16.8	32264	PASS
442	442	50	100	100.0	200384	PASS
443	442	15	24	18.2	36493	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
11/18/2024	BNA_F	<u>BF140455.D</u>
Compound Name	Response	Retention Time
DDT	588546	13.563
DDD	13317	13.257
DDE	1536	12.921
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14853	603399	2.46

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111824\
Data File : BF140455.D
Acq On : 18 Nov 2024 15:48
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 18 16:27:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 14:40:06 2024
Response via : Initial Calibration

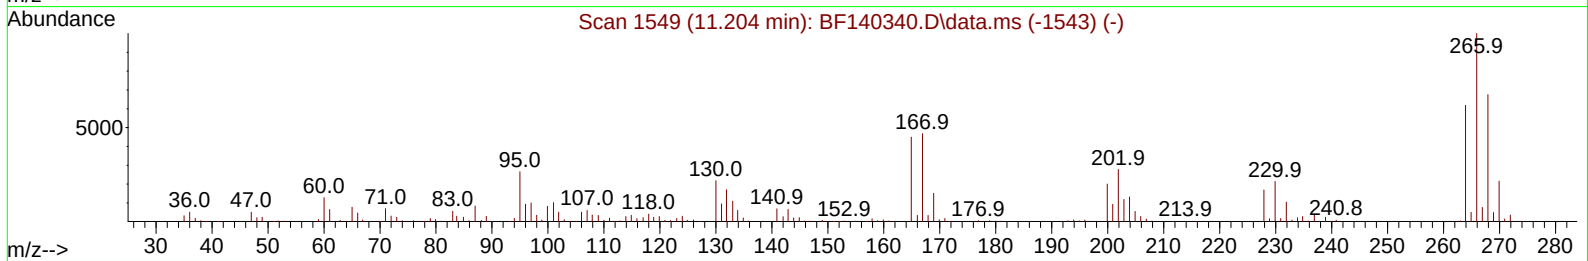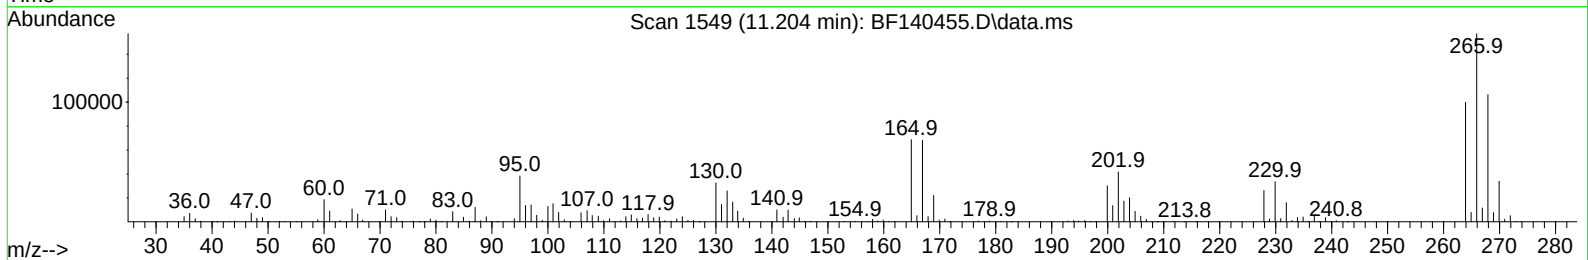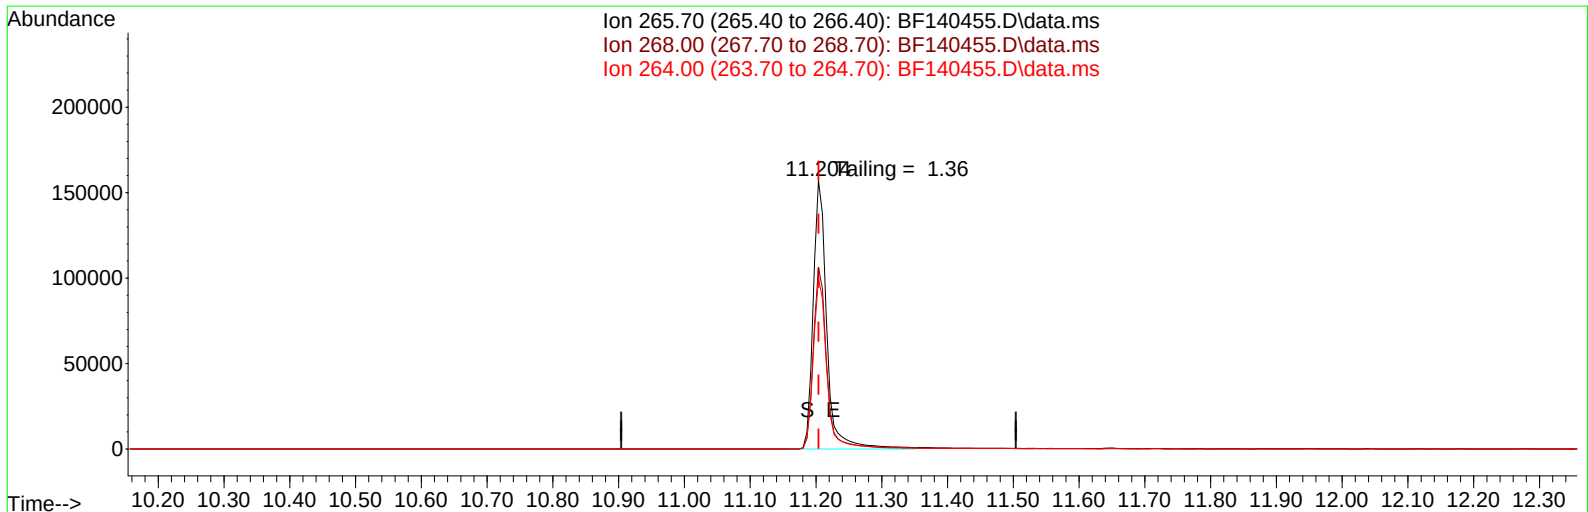

TIC: BF140455.D\data.ms

(70) Pentachlorophenol (C)

11.204min (-0.000) 43255.76 ng




response 225635

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.10	67.63
264.00	62.90	63.51
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111824\
Data File : BF140455.D
Acq On : 18 Nov 2024 15:48
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 18 16:27:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 14:40:06 2024
Response via : Initial Calibration

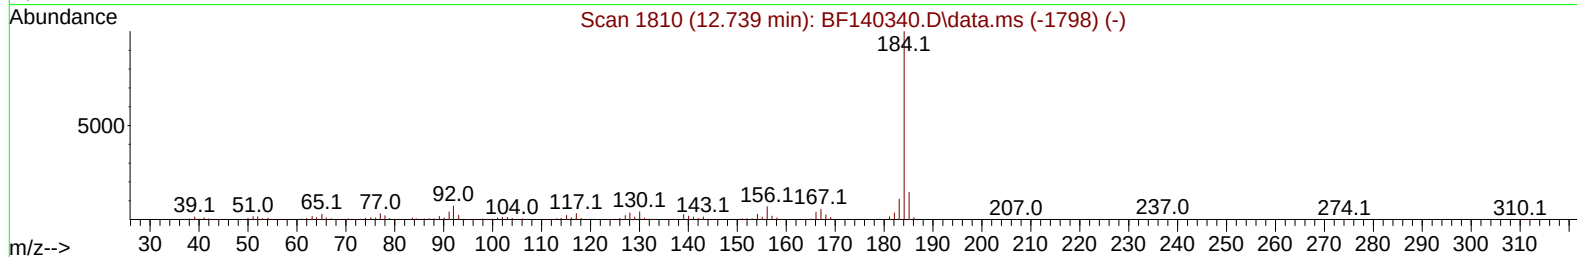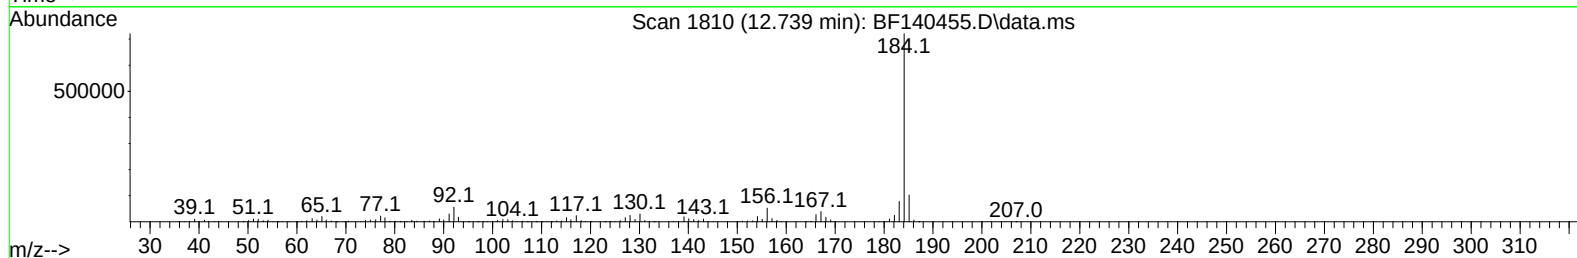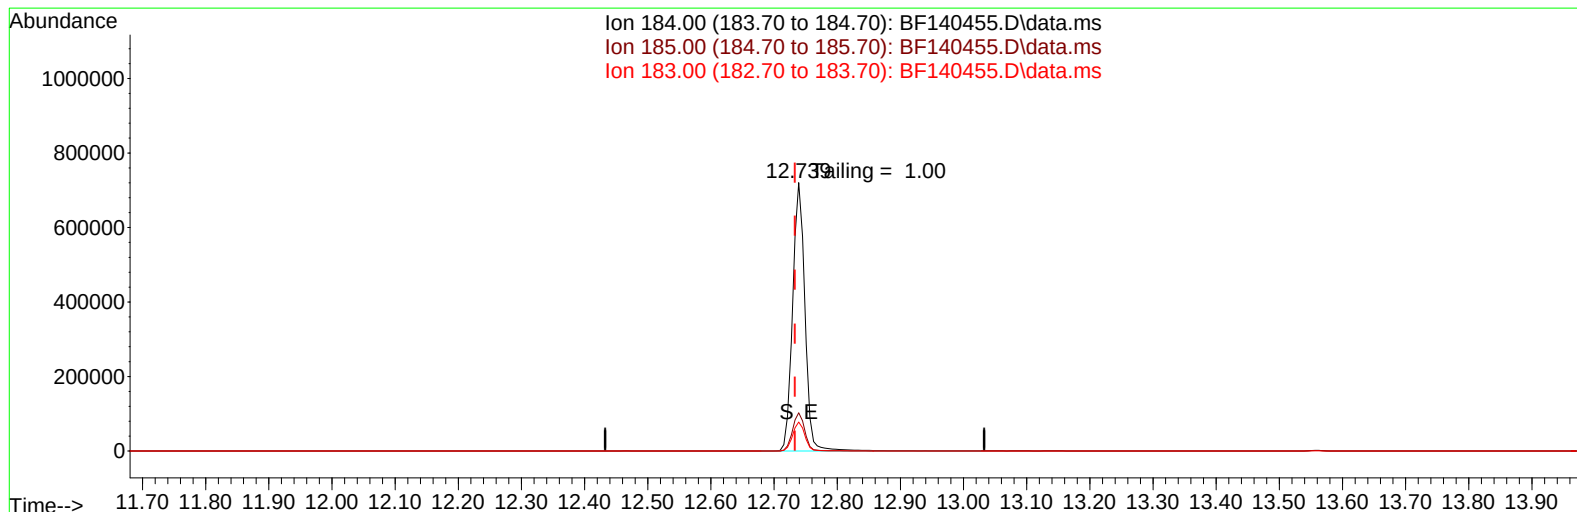

TIC: BF140455.D\data.ms

(77) Benzidine

12.739min (+ 0.006) 31853.14 ng

response 979257

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.27
183.00	10.80	10.82
0.00	0.00	0.00