

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF111915\
 Data File : BF083050.D
 Acq On : 19 Nov 2015 22:36
 Operator : UM/IZ
 Sample : PB86753TB
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB86753TB

Quant Time: Nov 20 06:56:18 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF111915.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 20 01:33:39 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.70	152	134580	20.00	ng	0.00
21) Naphthalene-d8	7.98	136	521145	20.00	ng	-0.01
38) Acenaphthene-d10	9.74	164	280768	20.00	ng	0.00
63) Phenanthrene-d10	11.22	188	558198	20.00	ng	0.00
75) Chrysene-d12	13.85	240	507260	20.00	ng	-0.01
86) Perylene-d12	15.23	264	441098	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.31	112	1327975	153.26	ng	0.02
7) Phenol-d6	6.36	99	1855631	162.60	ng	0.01
23) Nitrobenzene-d5	7.26	82	998389	87.70	ng	-0.01
41) 2,4,6-Tribromophenol	10.53	330	420687	141.12	ng	0.00
44) 2-Fluorobiphenyl	9.07	172	1656495	79.46	ng	-0.01
78) Terphenyl-d14	12.82	244	2079657	96.79	ng	0.01


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF111915\
Data File : BF083050.D
Acq On : 19 Nov 2015 22:36
Operator : UM/IZ
Sample : PB86753TB
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB86753TB

Quant Time: Nov 20 06:56:18 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF111915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 20 01:33:39 2015
Response via : Initial Calibration

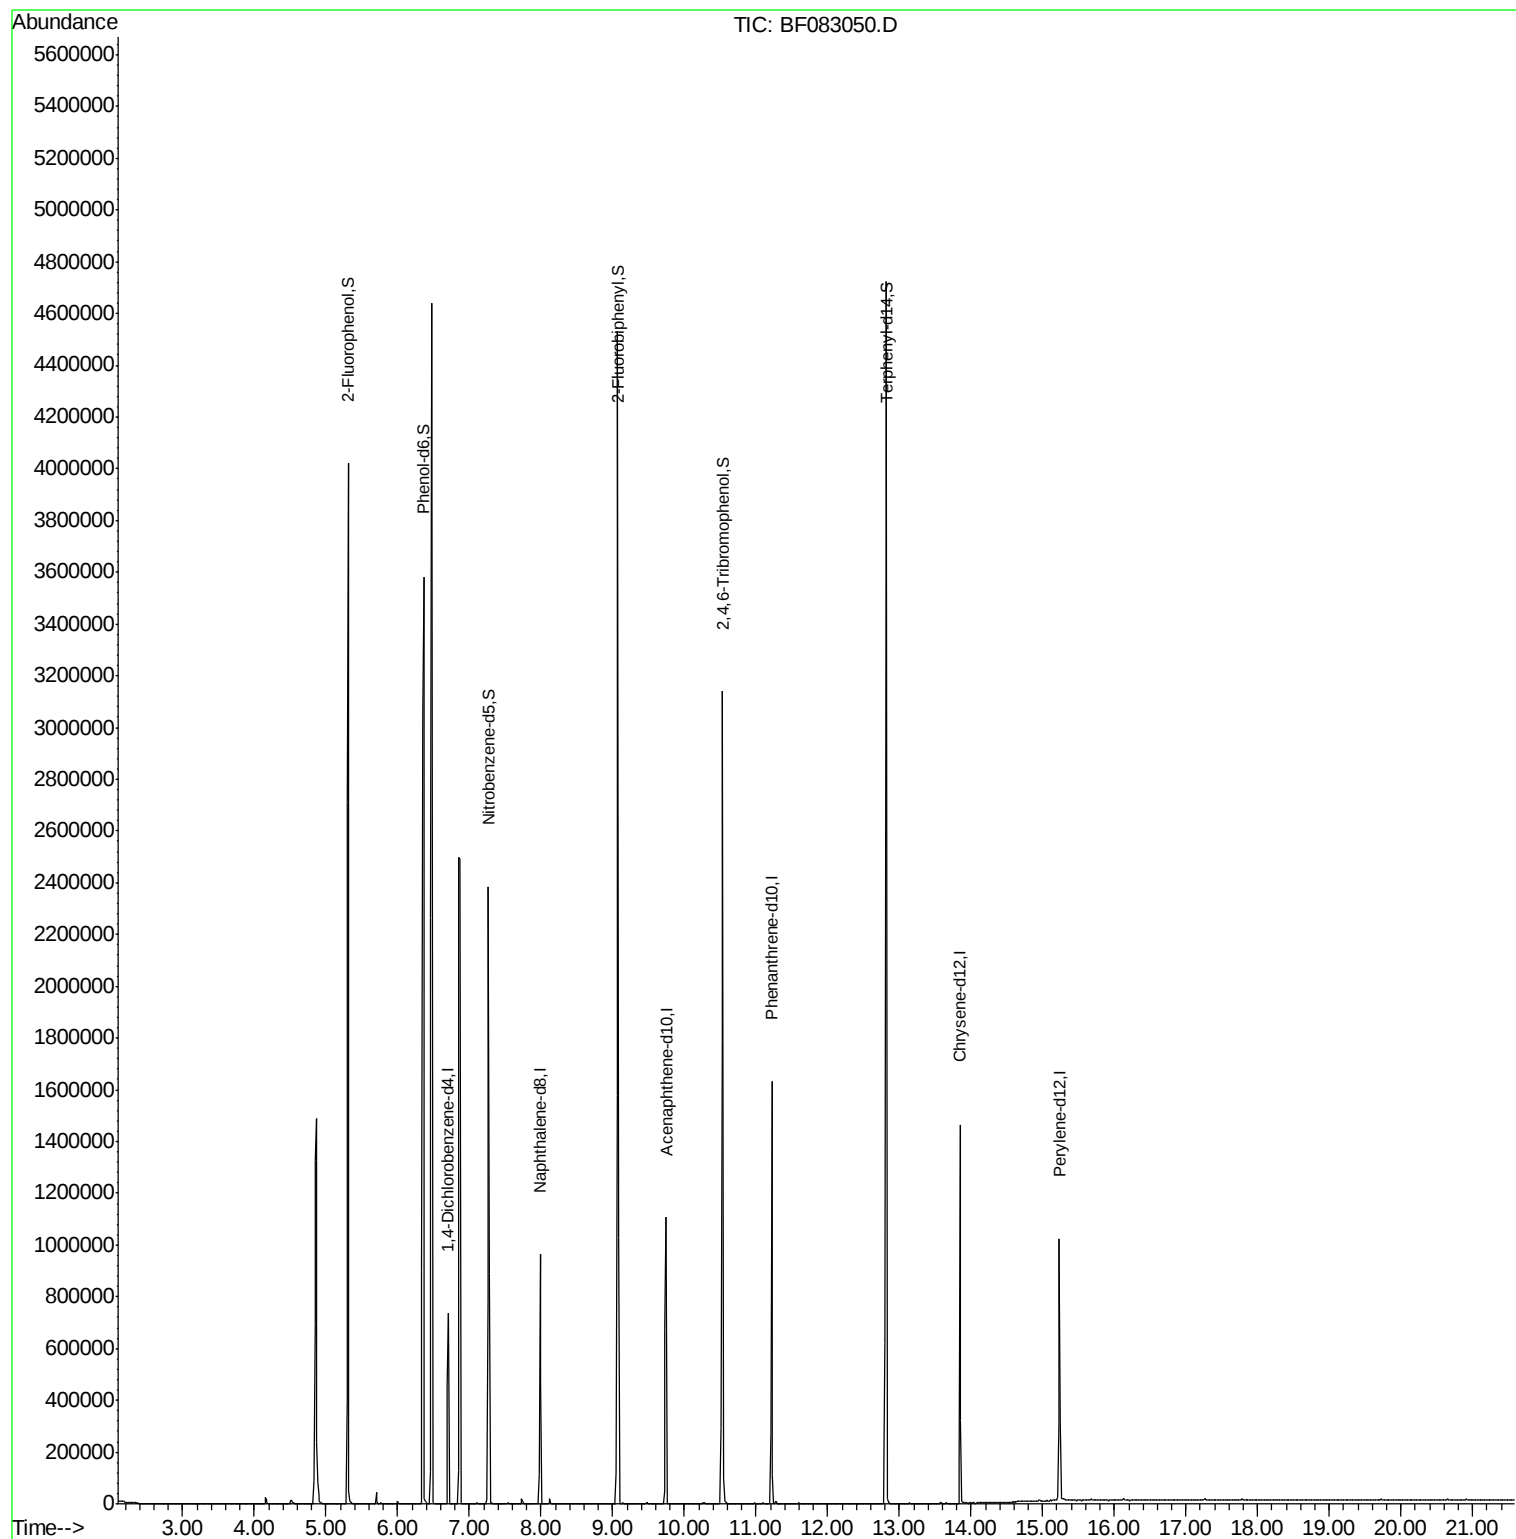

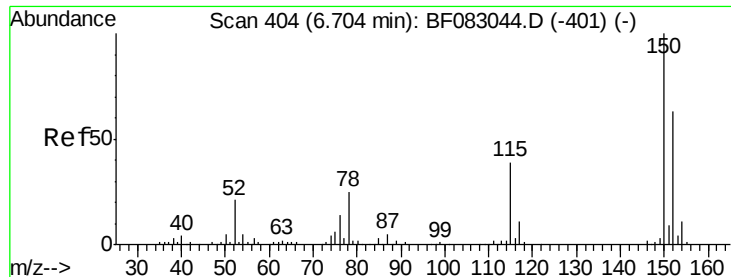

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.70 min Scan# 404

Delta R.T. 0.00 min

Lab File: BF083050.D

Acq: 19 Nov 2015 22:36

Instrument :

BNA_F

ClientSampled :

PB86753TB


Tgt Ion:152 Resp: 134580

Ion Ratio Lower Upper

152 100

150 159.0 126.4 189.6




115 57.8 49.0 73.6

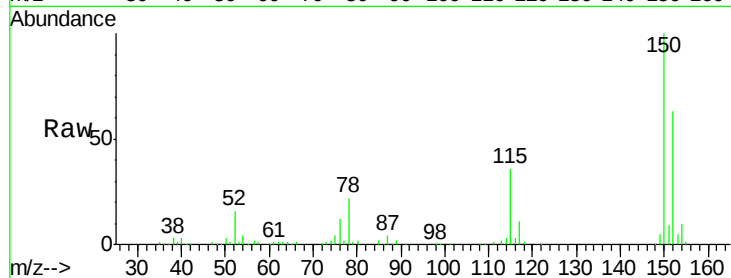

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

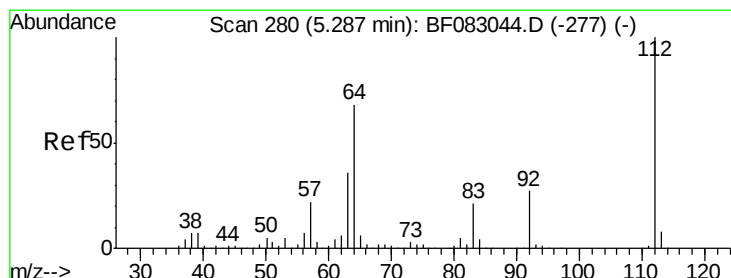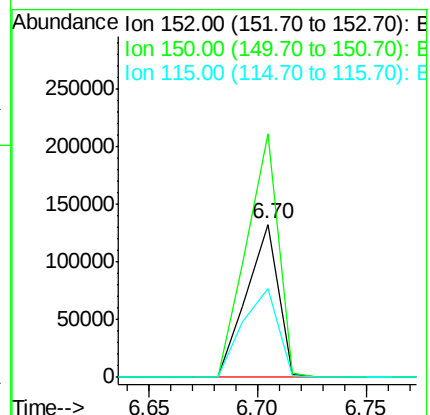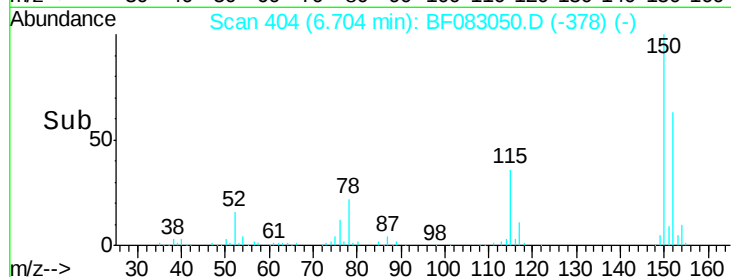

#5

2-Fluorophenol

Concen: 153.26 ng

RT: 5.31 min Scan# 282

Delta R.T. 0.02 min

Lab File: BF083050.D

Acq: 19 Nov 2015 22:36


Tgt Ion:112 Resp: 1327975

Ion Ratio Lower Upper

112 100

64 61.9 54.8 82.2



63 32.3 29.0 43.4

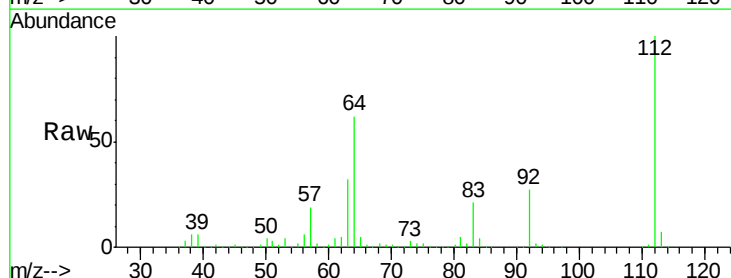


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

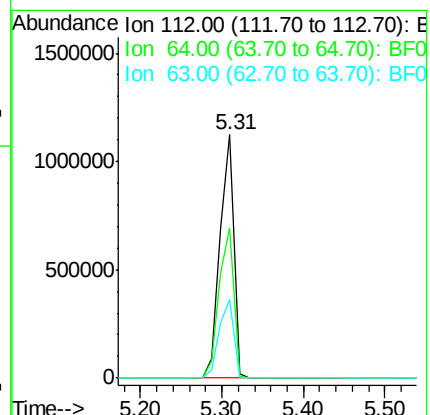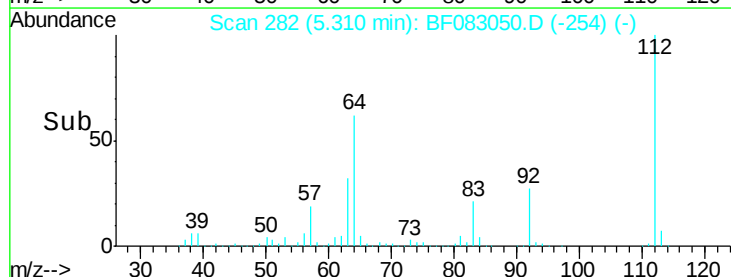

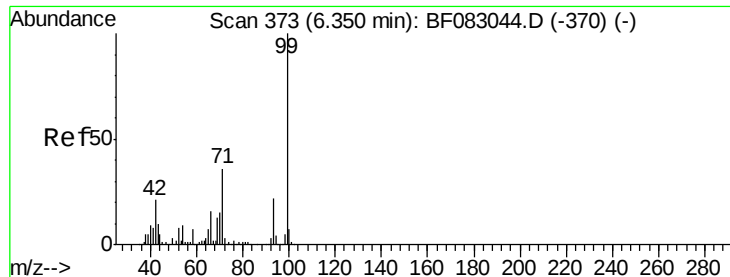

#7

Phenol-d6

Concen: 162.60 ng

RT: 6.36 min Scan# 374

Delta R.T. 0.01 min

Lab File: BF083050.D

Acq: 19 Nov 2015 22:36

Instrument :

BNA_F

ClientSampleId :

PB86753TB


Tgt Ion: 99 Resp: 1855631

Ion Ratio Lower Upper

99 100

42 15.6 16.6 25.0#




71 33.8 29.2 43.8

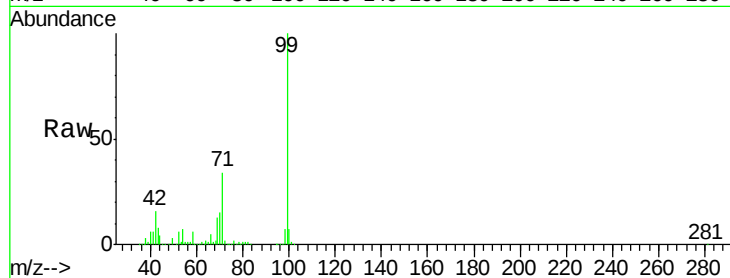

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

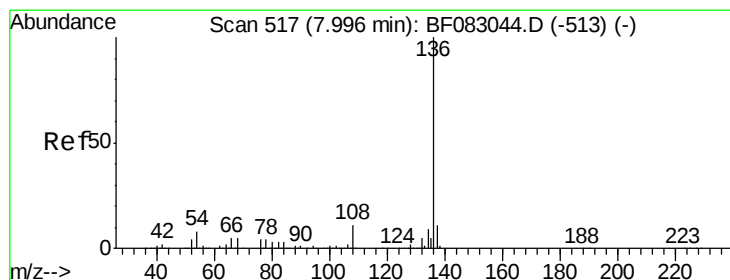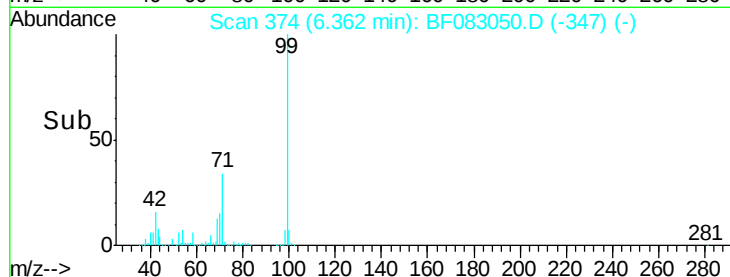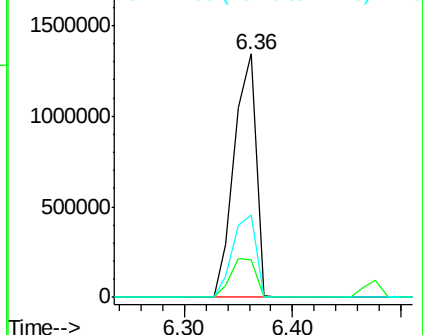

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.98 min Scan# 516

Delta R.T. -0.01 min

Lab File: BF083050.D

Acq: 19 Nov 2015 22:36

Tgt Ion: 136 Resp: 521145


Ion Ratio Lower Upper

136 100

137 10.8 8.6 12.8

54 10.4 6.2 9.2#

68 6.6 4.2 6.2#


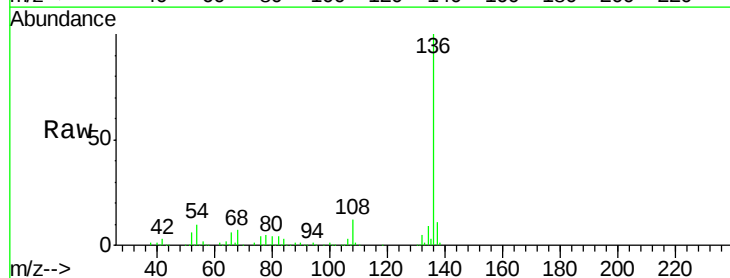



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

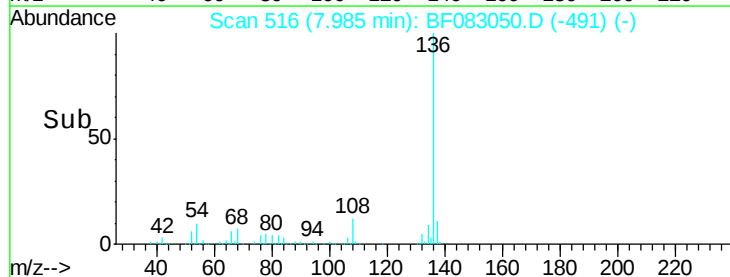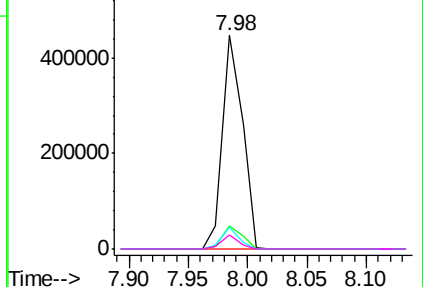


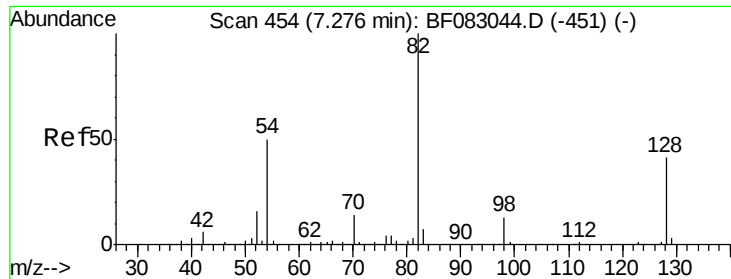




#23
 Nitrobenzene-d5
 Concen: 87.70 ng
 RT: 7.26 min Scan# 453
 Delta R.T. -0.01 min
 Lab File: BF083050.D
 Acq: 19 Nov 2015 22:36

Instrument :
 BNA_F
 ClientSampleId :
 PB86753TB

Tgt Ion	Ratio	Lower	Upper
82	100		
128	36.7	33.1	49.7
54	52.9	39.8	59.6

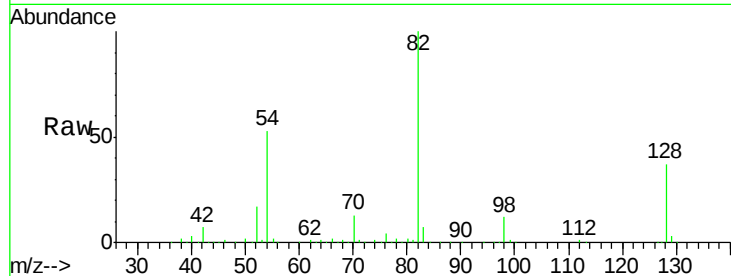


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): B
 Ion 54.00 (53.70 to 54.70): BF0

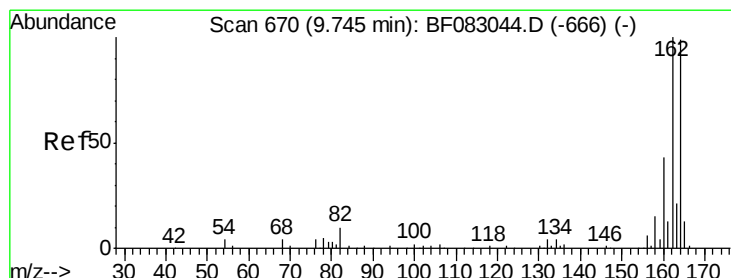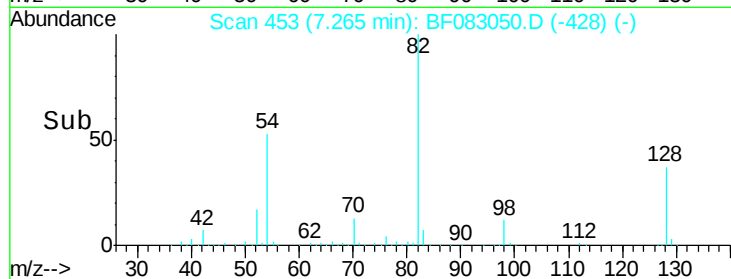
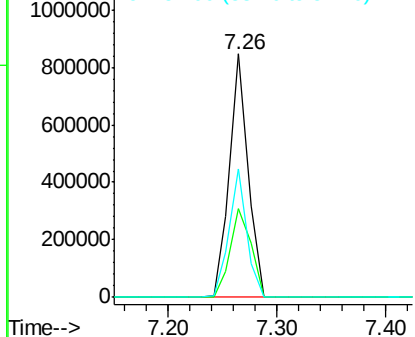



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.74 min Scan# 670
 Delta R.T. 0.00 min
 Lab File: BF083050.D
 Acq: 19 Nov 2015 22:36

Tgt Ion	Ratio	Lower	Upper
164	100		
162	101.8	80.5	120.7
160	44.6	35.0	52.4

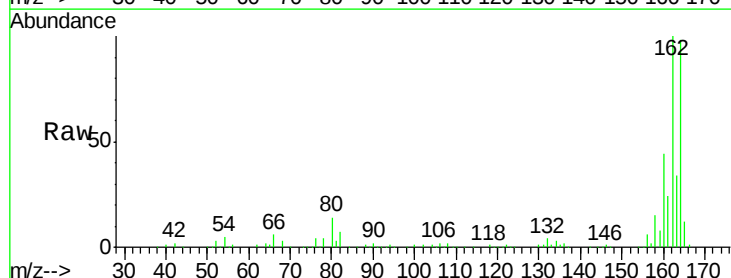

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

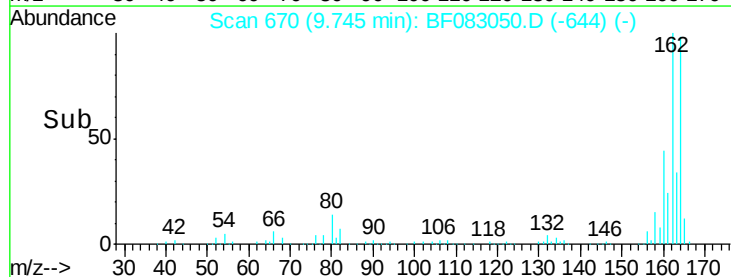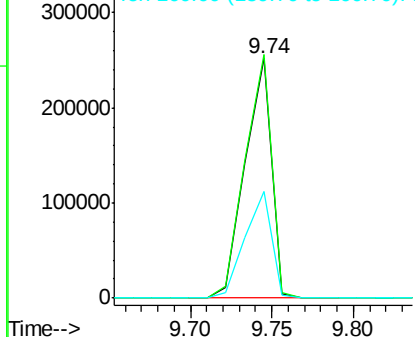


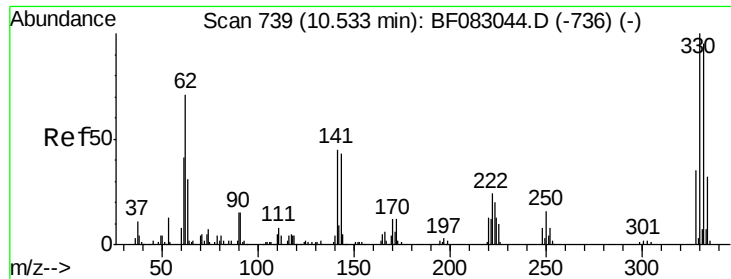




#41
 2,4,6-Tribromophenol
 Concen: 141.12 ng
 RT: 10.53 min Scan# 739
 Delta R.T. 0.00 min
 Lab File: BF083050.D
 Acq: 19 Nov 2015 22:36

Instrument :
 BNA_F
 ClientSampled :
 PB86753TB

Tgt Ion:330 Resp: 420687
 Ion Ratio Lower Upper
 330 100
 332 95.5 77.6 116.4
 141 40.5 34.6 52.0

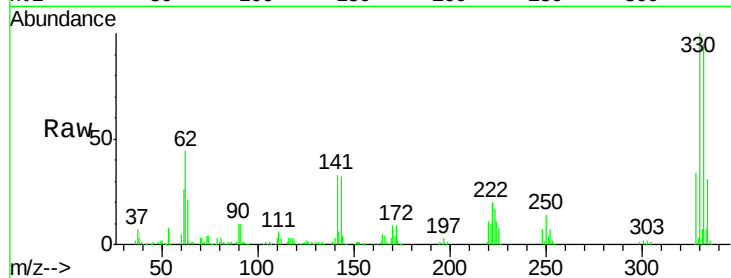


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

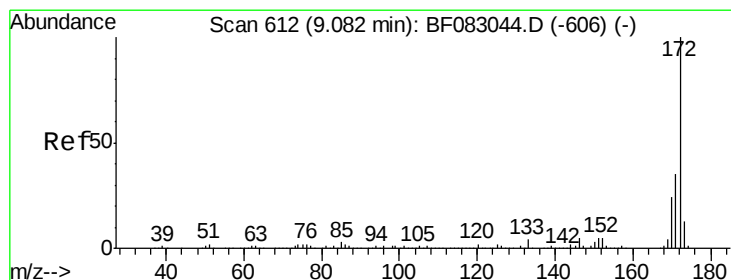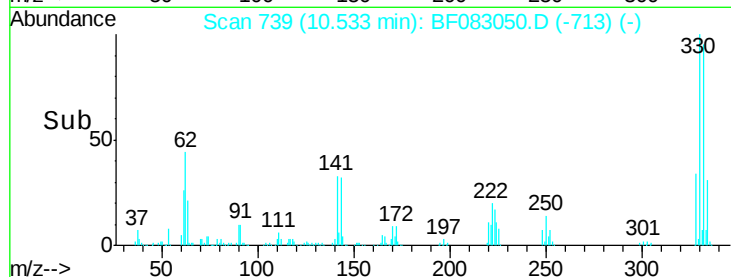
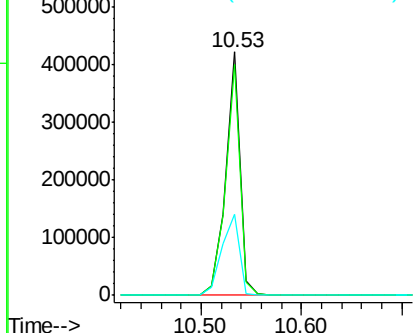



#44
 2-Fluorobiphenyl
 Concen: 79.46 ng
 RT: 9.07 min Scan# 611
 Delta R.T. -0.01 min
 Lab File: BF083050.D
 Acq: 19 Nov 2015 22:36

Tgt Ion:172 Resp: 1656495
 Ion Ratio Lower Upper
 172 100
 171 36.8 28.2 42.4
 170 25.3 19.4 29.0

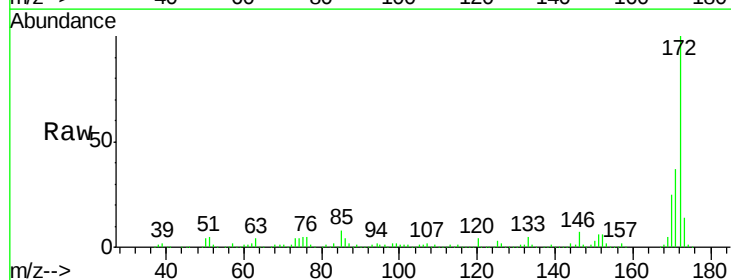

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

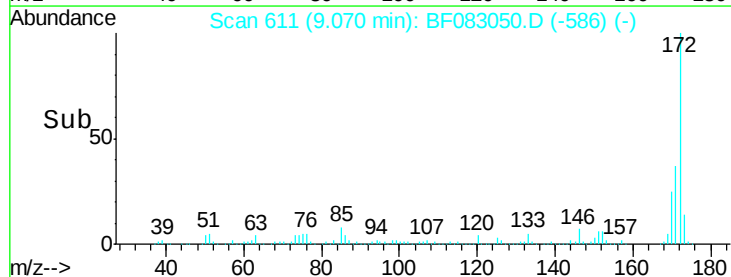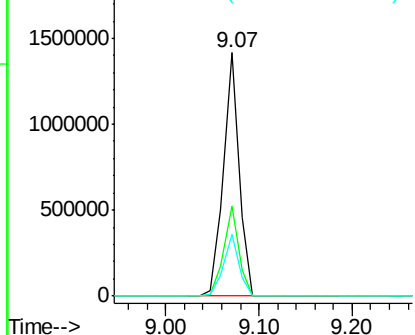


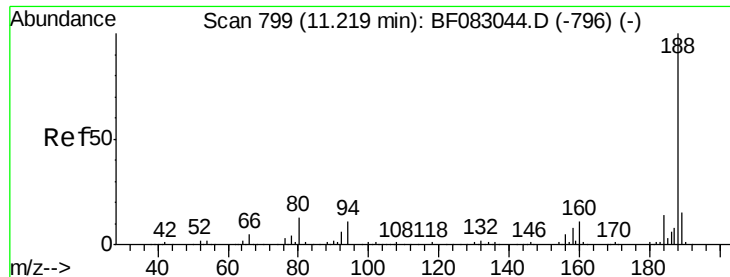




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.22 min Scan# 799
Delta R.T. 0.00 min
Lab File: BF083050.D
Acq: 19 Nov 2015 22:36

Instrument :
BNA_F
ClientSampleId :
PB86753TB

Tgt Ion:188 Resp: 558198
Ion Ratio Lower Upper
188 100
94 8.9 9.0 13.4#
80 10.4 10.2 15.4

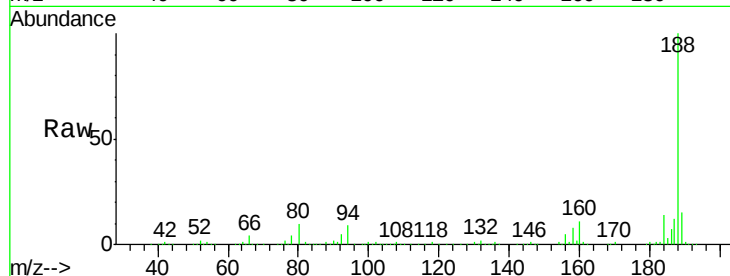


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

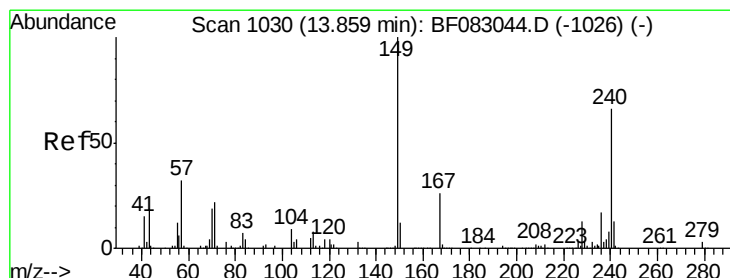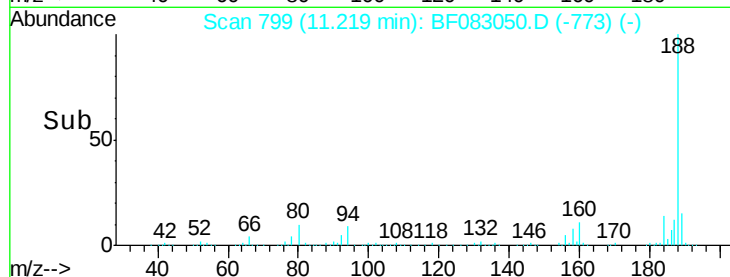
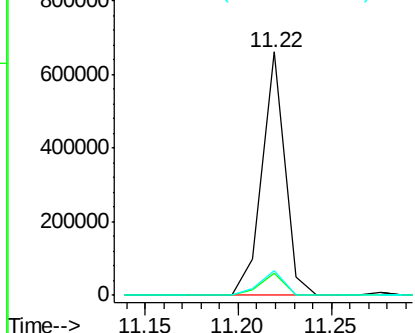



#75
Chrysene-d12
Concen: 20.00 ng
RT: 13.85 min Scan# 1029
Delta R.T. -0.01 min
Lab File: BF083050.D
Acq: 19 Nov 2015 22:36

Tgt Ion:240 Resp: 507260
Ion Ratio Lower Upper
240 100
120 10.7 5.3 7.9#
236 25.9 20.4 30.6

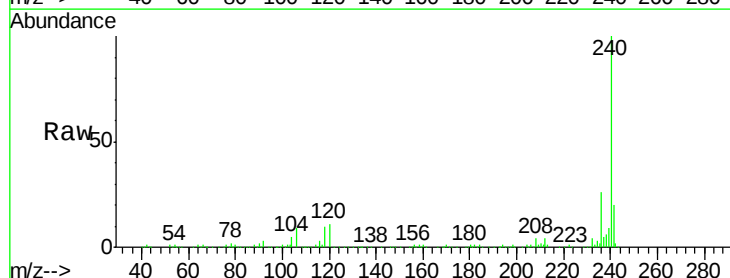

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E



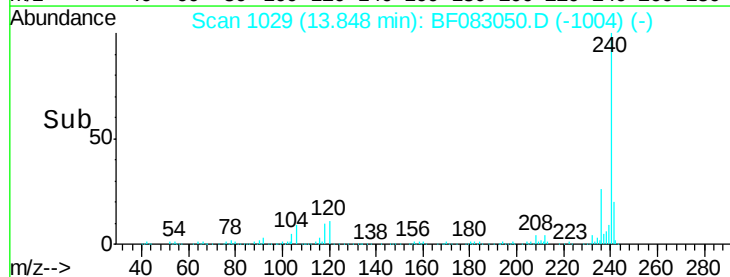
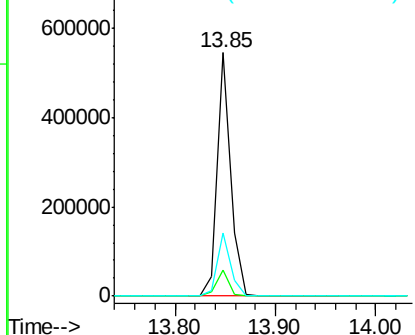


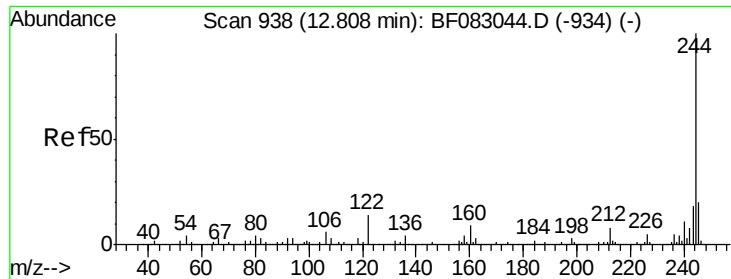

#78
 Terphenyl-d14
 Concen: 96.79 ng
 RT: 12.82 min Scan# 939
 Delta R.T. 0.01 min
 Lab File: BF083050.D
 Acq: 19 Nov 2015 22:36

Instrument :
 BNA_F
 ClientSampleId :
 PB86753TB

Tgt Ion:244 Resp: 2079657
 Ion Ratio Lower Upper
 244 100
 212 7.7 6.4 9.6
 122 7.0 10.9 16.3#

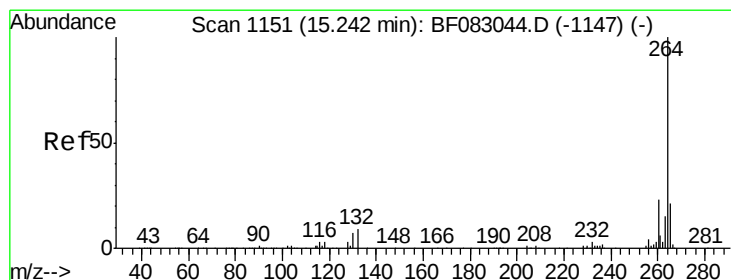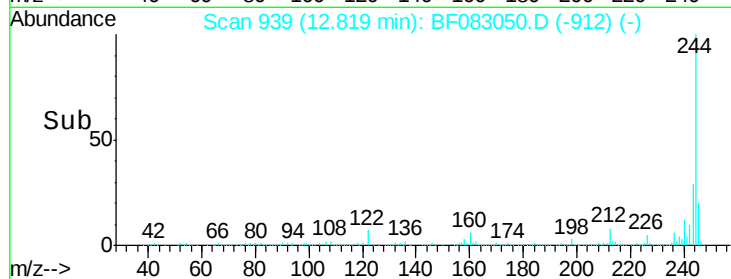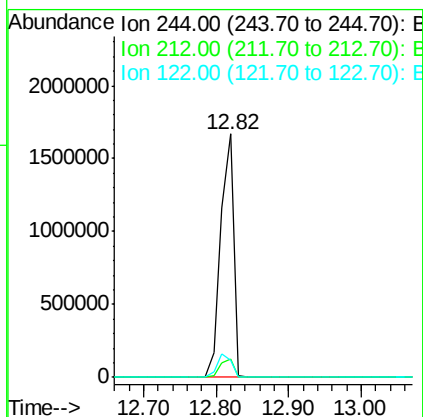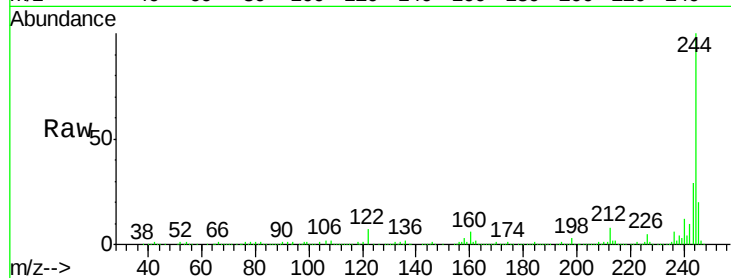

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 15.23 min Scan# 1150
 Delta R.T. -0.01 min
 Lab File: BF083050.D
 Acq: 19 Nov 2015 22:36

Tgt Ion:264 Resp: 441098
 Ion Ratio Lower Upper
 264 100
 260 24.2 18.6 27.8
 265 21.9 17.0 25.6

