


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF111915\
 Data File : BF083040.D
 Acq On : 19 Nov 2015 15:50
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF111915.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Nov 20 01:33:39 2015

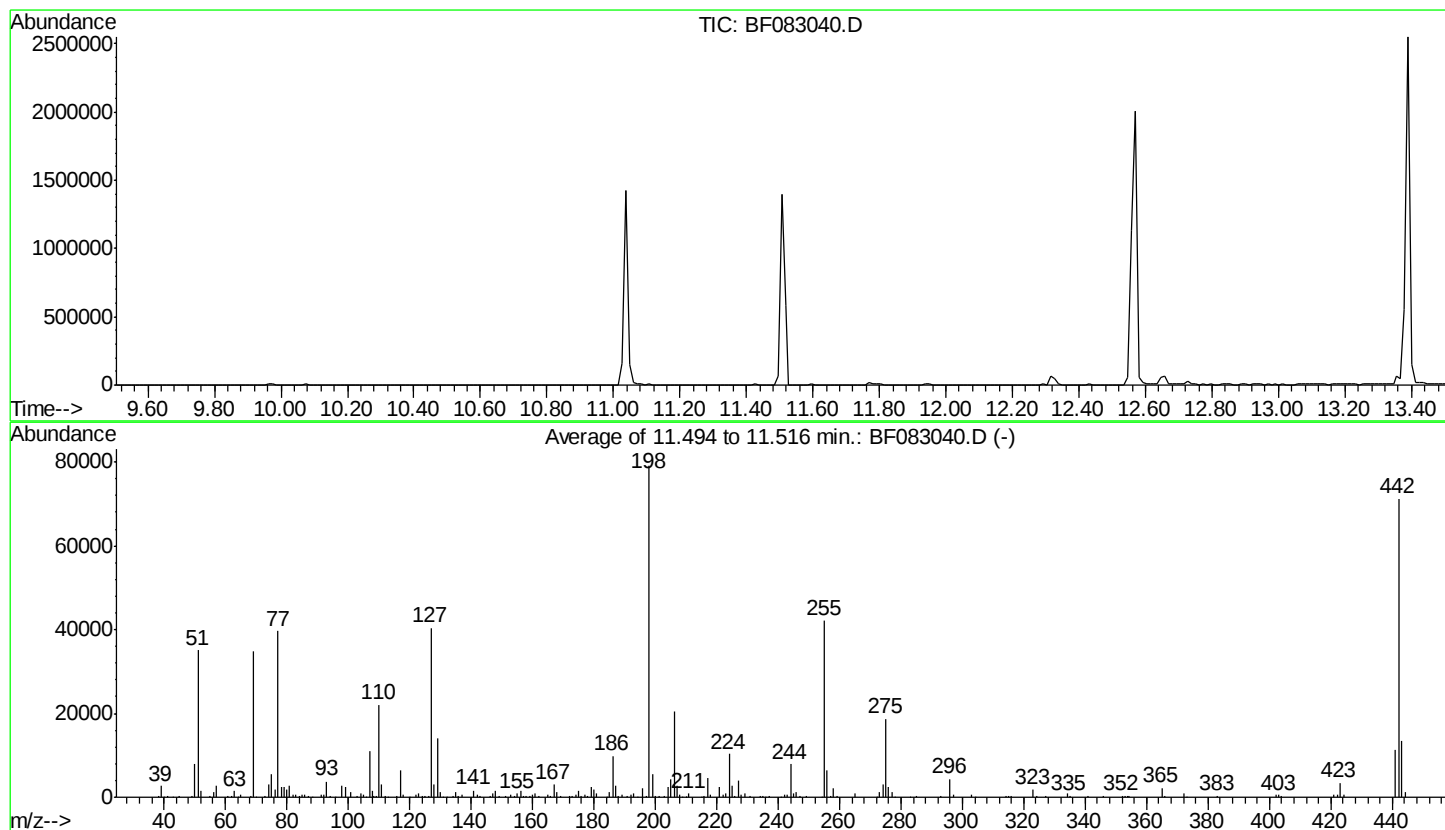

AutoFind: Scans 823, 824, 825; Background Corrected with Scan 820

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.3	35085	PASS
68	69	0.00	2	1.3	441	PASS
69	198	0.00	100	44.0	34814	PASS
70	69	0.00	2	0.4	141	PASS
127	198	10	80	51.1	40427	PASS
197	198	0.00	2	0.5	357	PASS
198	198	100	100	100.0	79137	PASS
199	198	5	9	6.8	5376	PASS
275	198	10	60	23.7	18786	PASS
365	198	1	100	2.7	2152	PASS
441	442	0.01	24	16.1	11450	PASS
442	198	50	100	90.0	71258	PASS
443	442	15	24	18.7	13350	PASS