


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF111915\
 Data File : BF083057.D
 Acq On : 20 Nov 2015 2:27
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF111915.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Nov 20 01:33:39 2015

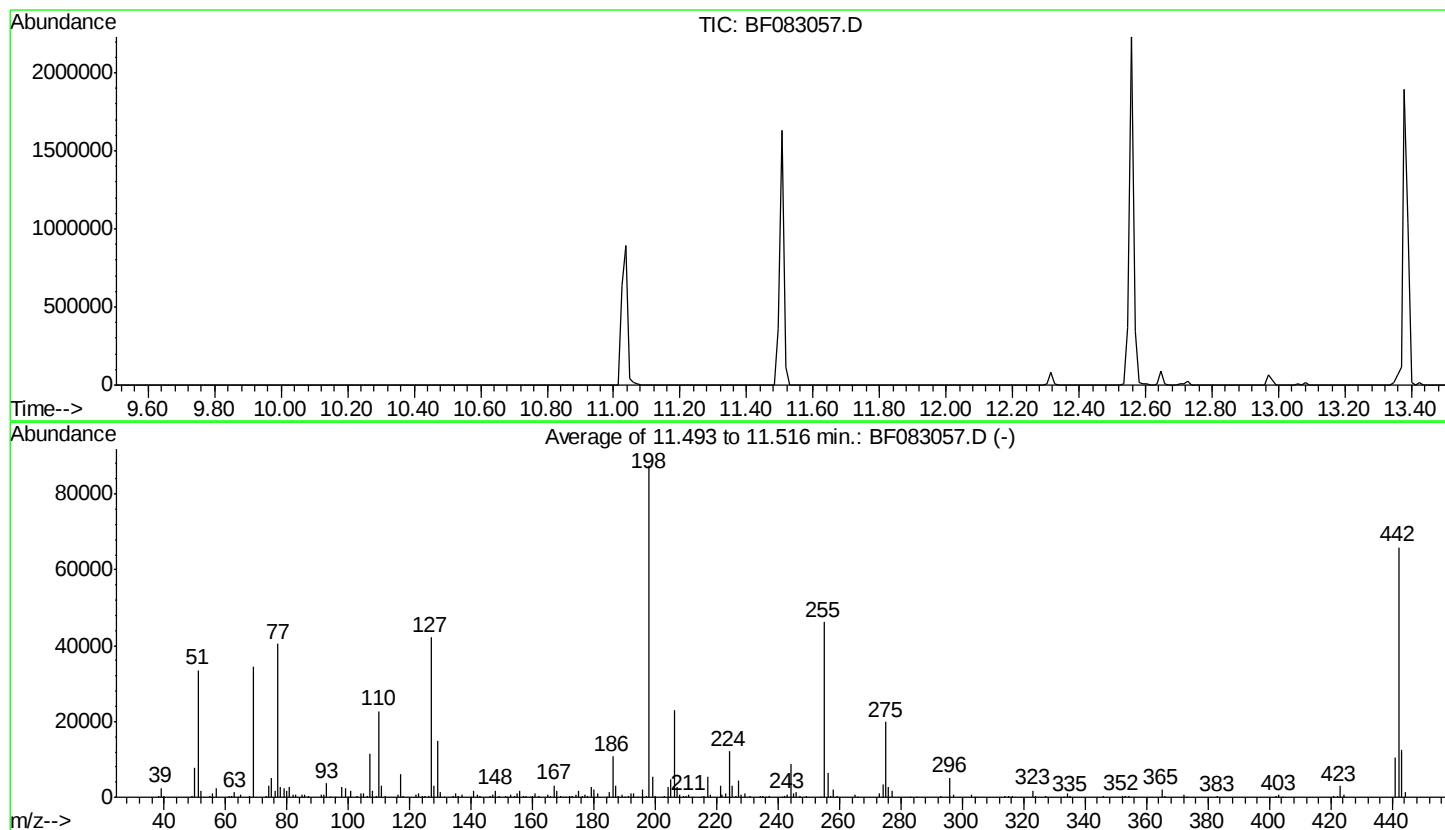

AutoFind: Scans 823, 824, 825; Background Corrected with Scan 820

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.3	33514	PASS
68	69	0.00	2	1.5	515	PASS
69	198	0.00	100	39.3	34356	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.2	42189	PASS
197	198	0.00	2	0.4	353	PASS
198	198	100	100	100.0	87496	PASS
199	198	5	9	6.3	5509	PASS
275	198	10	60	22.7	19835	PASS
365	198	1	100	2.3	1992	PASS
441	442	0.01	24	15.9	10495	PASS
442	198	50	100	75.4	65970	PASS
443	442	15	24	19.0	12505	PASS