

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF111918\
 Data File : BF110878.D
 Acq On : 20 Nov 2018 3:29
 Operator : JU/SJ
 Sample : J5985-09
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 111518-JETT-E-D-S

Quant Time: Nov 20 05:58:40 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 13 12:43:10 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.94	152	51807	20.00	ng	0.00
21) Naphthalene-d8	8.23	136	203492	20.00	ng	0.00
39) Acenaphthene-d10	9.99	164	78630	20.00	ng	0.00
64) Phenanthrene-d10	11.48	188	136702	20.00	ng	0.00
76) Chrysene-d12	14.13	240	131571	20.00	ng	0.00
87) Perylene-d12	15.67	264	80441	20.00	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.56	112	109241	34.25	ng	0.00
7) Phenol-d6	6.57	99	78784	19.32	ng	0.00
23) Nitrobenzene-d5	7.50	82	318577	90.16	ng	-0.01
42) 2,4,6-Tribromophenol	10.78	330	56629	71.47	ng	0.00
45) 2-Fluorobiphenyl	9.30	172	580240	105.39	ng	0.00
79) Terphenyl-d14	13.06	244	447949	63.76	ng	-0.01
Target Compounds						
19) n-Nitroso-di-n-propylamine	7.50	70	42448	16.304	ng	# 81
25) Isophorone	7.50	82	318619	55.016	ng	# 67
50) Dimethylphthalate	9.70	163	17535	2.989	ng	# 98
51) 2,6-Dinitrotoluene	9.99	165	9968	7.723	ng	# 21
57) 2,4-Dinitrotoluene	9.99	165	9968	5.940	ng	# 17
67) 4-Bromophenyl-phenylether	10.78	248	3388	2.242	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF111918\
Data File : BF110878.D
Acq On : 20 Nov 2018 3:29
Operator : JU/SJ
Sample : J5985-09
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
111518-JETT-E-D-S

Quant Time: Nov 20 05:58:40 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 13 12:43:10 2018
Response via : Initial Calibration

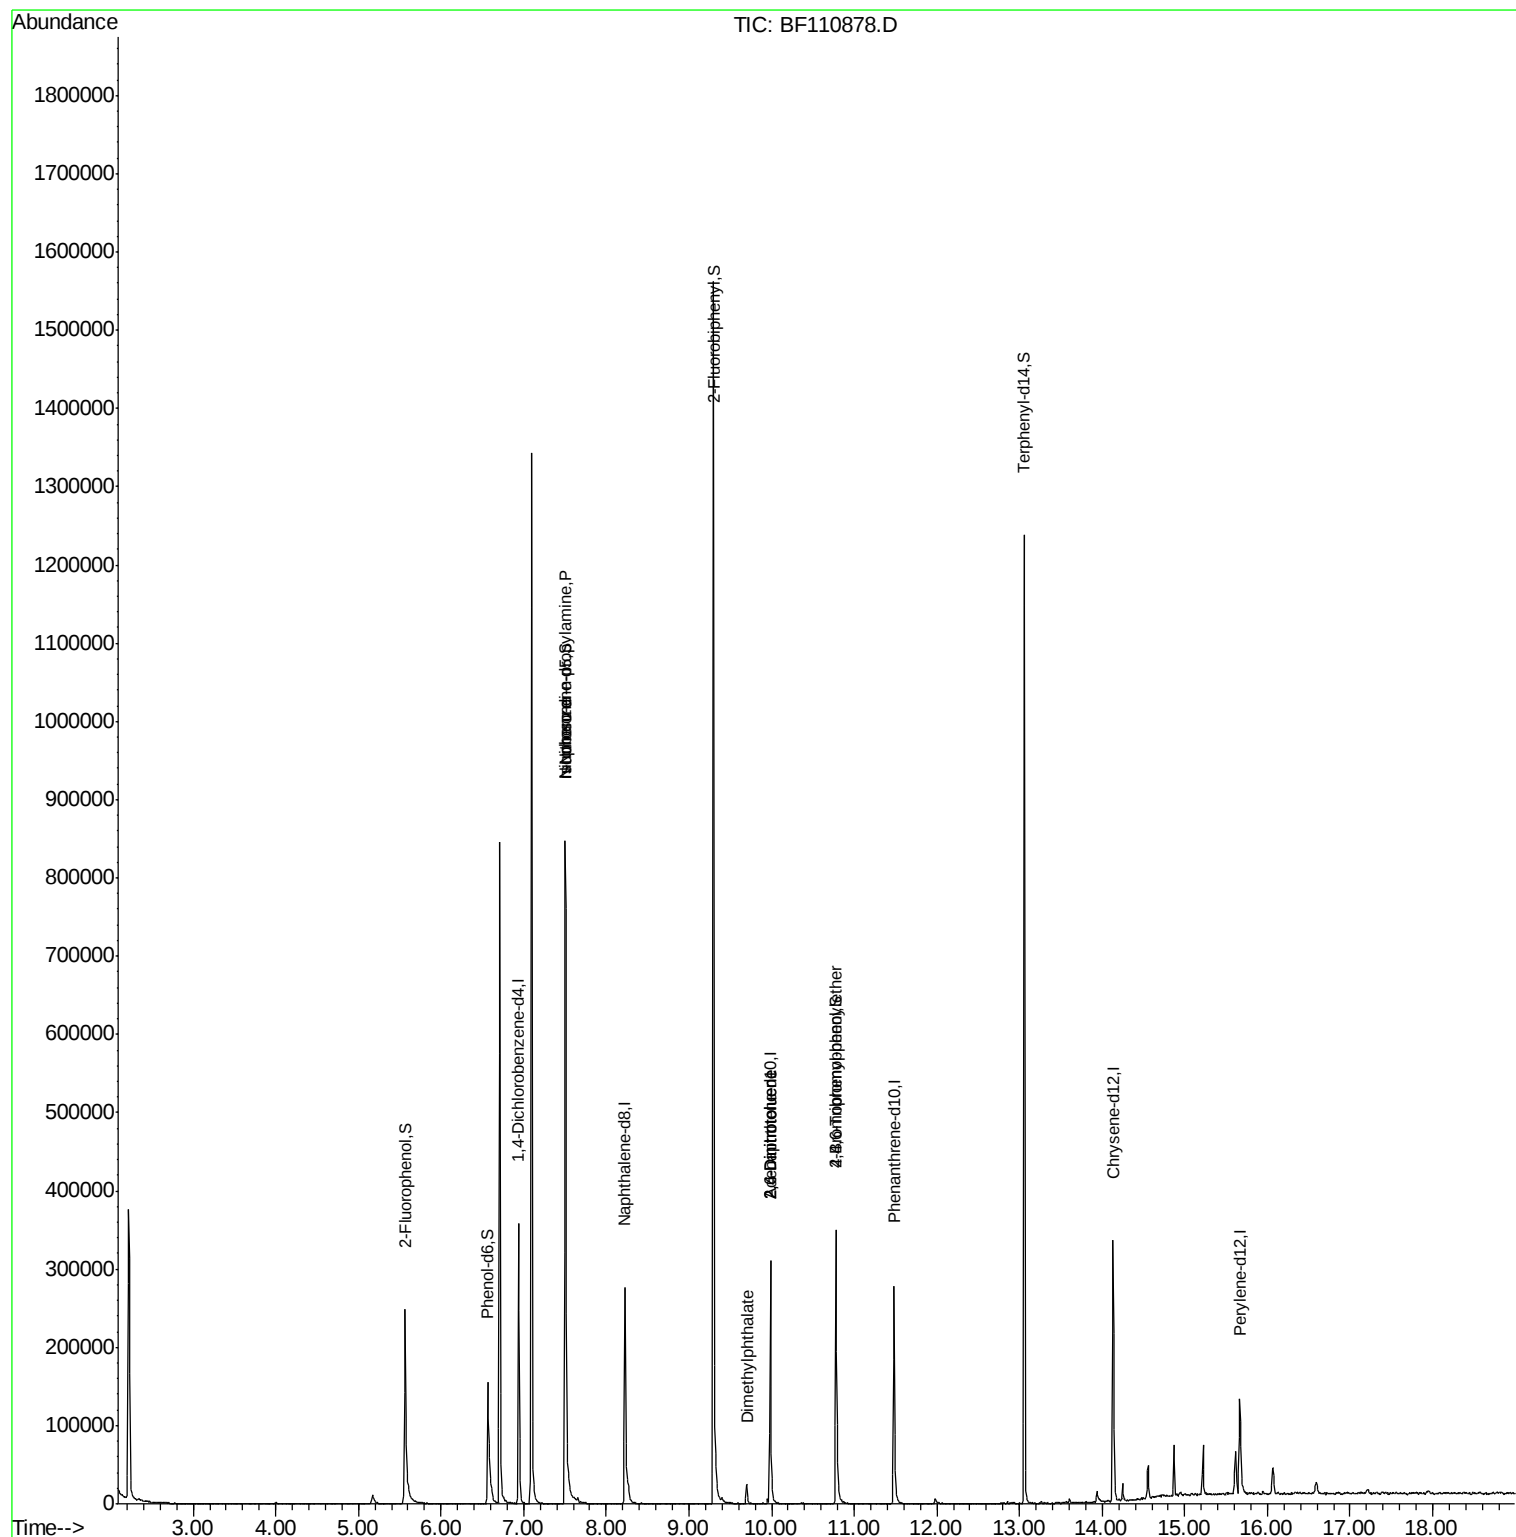


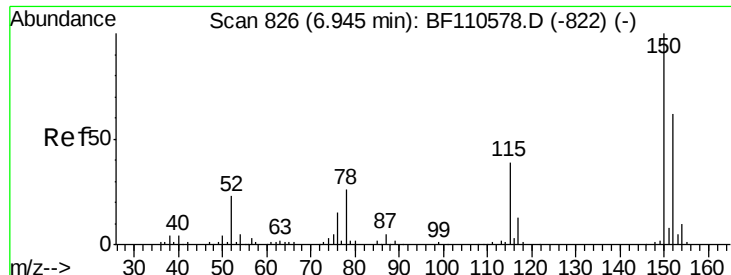



#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.94 min Scan# 825
 Delta R.T. -0.01 min
 Lab File: BF110878.D
 Acq: 20 Nov 2018 3:29

Instrument :
 BNA_F
 ClientSampleId :
 111518-JETT-E-D-S

Tgt Ion:152 Resp: 51807
 Ion Ratio Lower Upper
 152 100
 150 161.2 122.7 184.1
 115 65.4 49.1 73.7

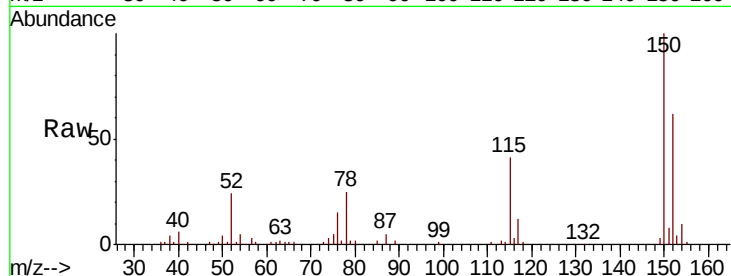


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

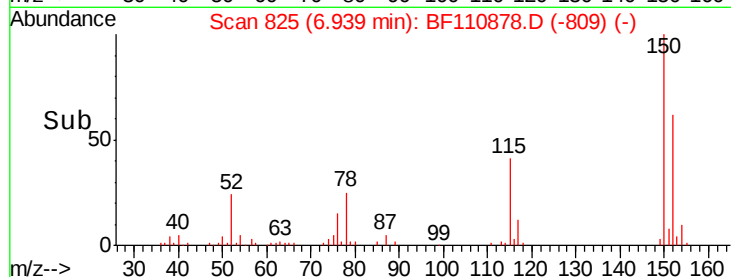
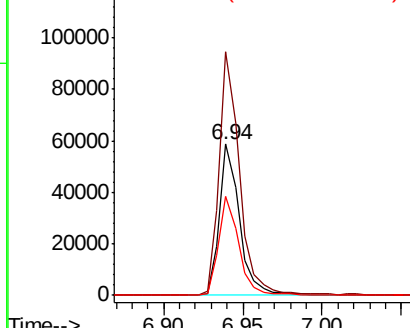


#5
 2-Fluorophenol
 Concen: 34.251 ng
 RT: 5.56 min Scan# 591
 Delta R.T. -0.00 min
 Lab File: BF110878.D
 Acq: 20 Nov 2018 3:29

Tgt Ion:112 Resp: 109241
 Ion Ratio Lower Upper
 112 100
 64 59.4 44.1 66.1
 63 31.4 23.7 35.5

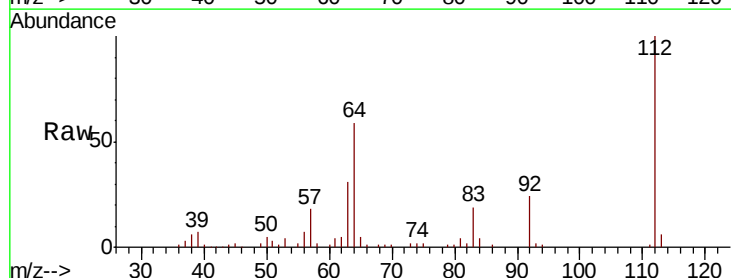

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF1
 Ion 63.00 (62.70 to 63.70): BF1

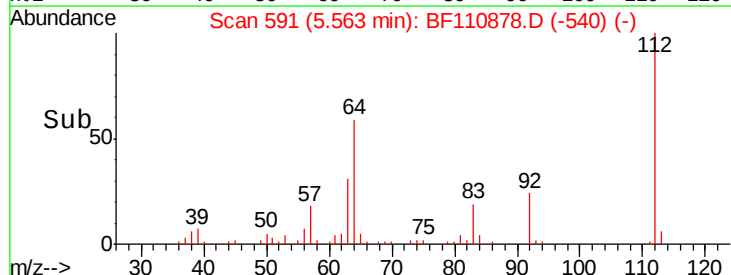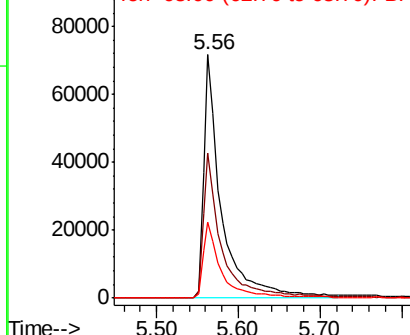



#7

Phenol-d6

Concen: 19.317 ng

RT: 6.57 min Scan# 762

Delta R.T. -0.01 min

Lab File: BF110878.D

Acq: 20 Nov 2018 3:29

Instrument :

BNA_F

ClientSampleId :

111518-JETT-E-D-S


Tgt Ion: 99 Resp: 78784

Ion Ratio Lower Upper




99 100

42 18.1 15.8 23.6

71 35.3 28.0 42.0

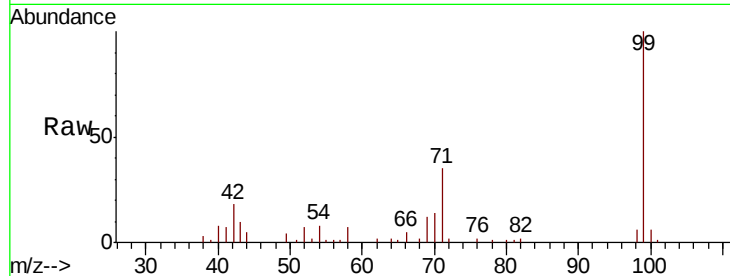

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

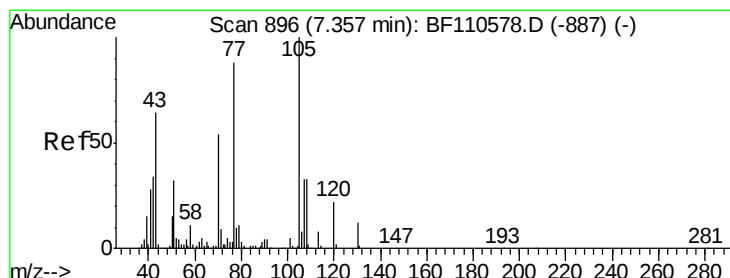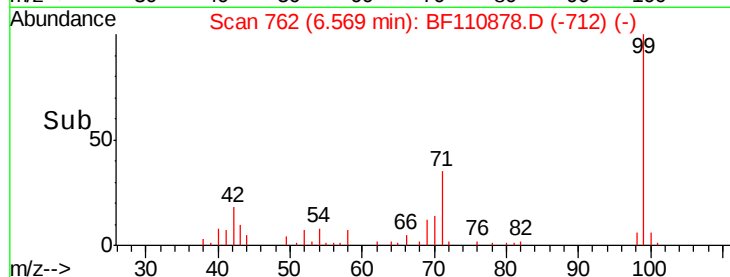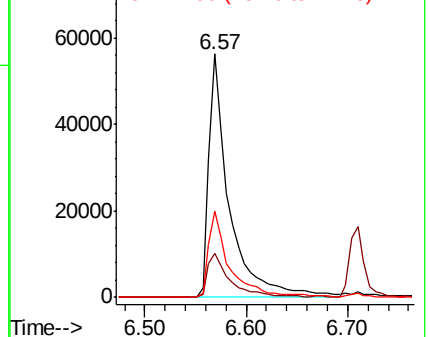

#19

n-Nitroso-di-n-propylamine

Concen: 16.304 ng

RT: 7.50 min Scan# 921

Delta R.T. 0.15 min

Lab File: BF110878.D

Acq: 20 Nov 2018 3:29

Tgt Ion: 70 Resp: 42448


Ion Ratio Lower Upper

70 100



42 50.8 47.4 71.2

101 0.0 7.3 10.9#

130 2.6 16.2 24.2#

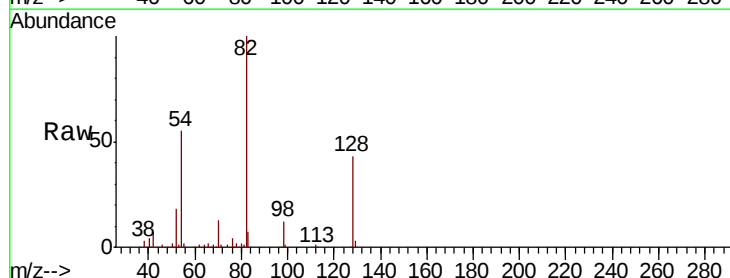

Abundance Ion 70.00 (69.70 to 70.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 101.00 (100.70 to 101.70): E
Ion 130.00 (129.70 to 130.70): E



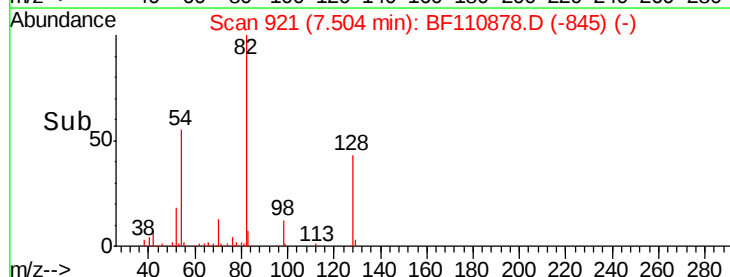
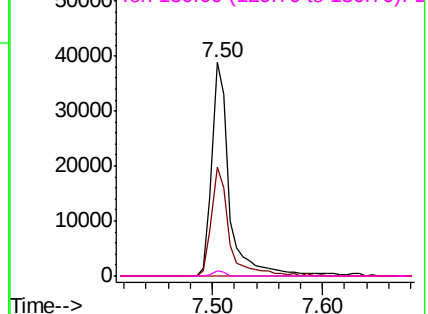




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.23 min Scan# 1044
Delta R.T. 0.00 min
Lab File: BF110878.D
Acq: 20 Nov 2018 3:29




Instrument :
BNA_F
ClientSampleId :
111518-JETT-E-D-S


Tgt Ion:	136	Resp:	203492
Ion	Ratio	Lower	Upper
136	100		
137	10.5	8.8	13.2
54	7.1	5.4	8.2
68	4.9	4.2	6.2

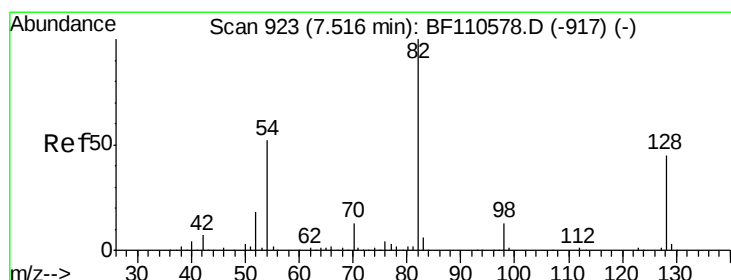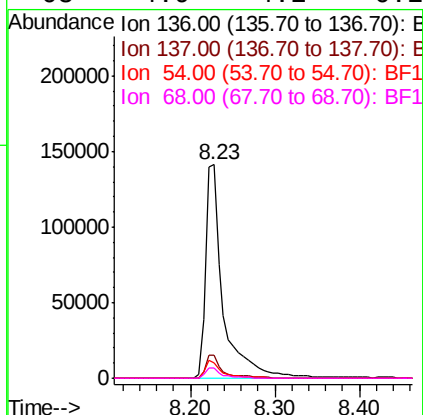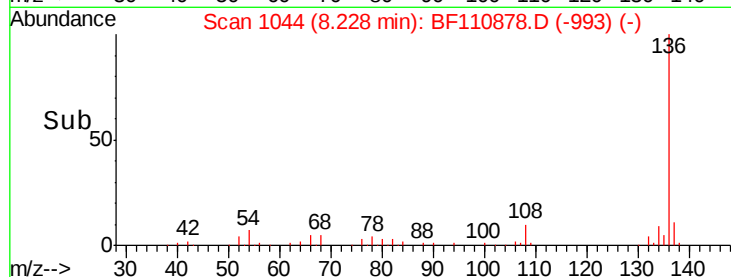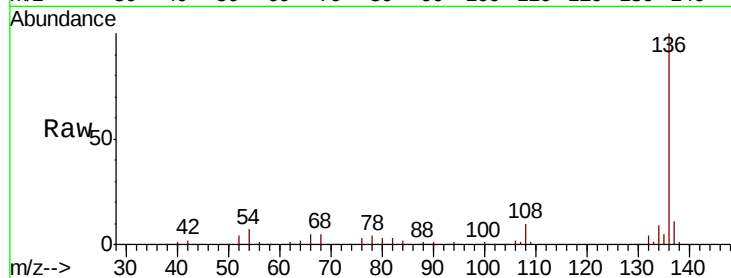

#23
Nitrobenzene-d5
Concen: 90.159 ng
RT: 7.50 min Scan# 921
Delta R.T. -0.01 min
Lab File: BF110878.D
Acq: 20 Nov 2018 3:29

Tgt Ion:	82	Resp:	318577
Ion	Ratio	Lower	Upper
82	100		
128	42.8	34.2	51.2
54	54.6	38.6	58.0

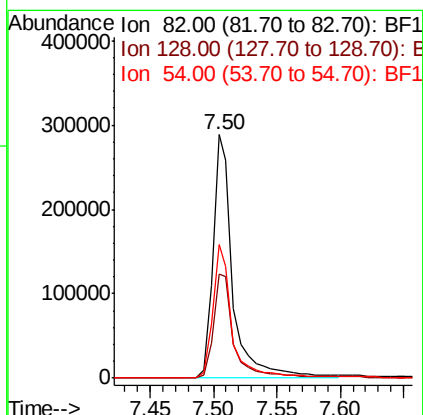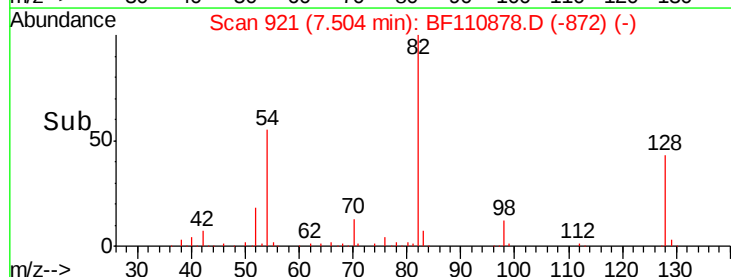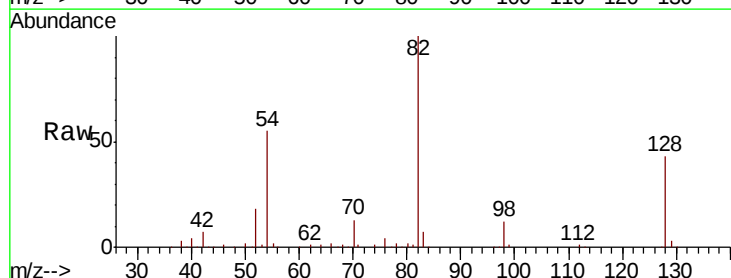

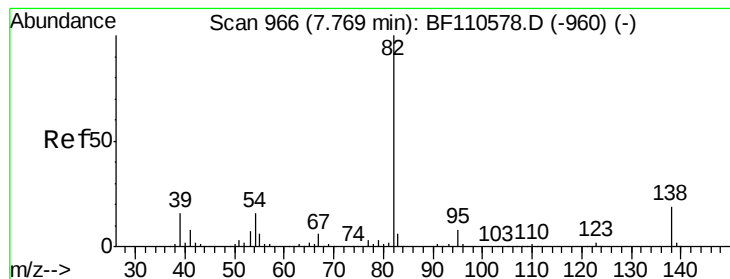

#25

Isophorone

Concen: 55.016 ng

RT: 7.50 min Scan# 921

Delta R.T. -0.26 min

Lab File: BF110878.D

Acq: 20 Nov 2018 3:29

Instrument :

BNA_F

ClientSampleId :

111518-JETT-E-D-S


Tgt Ion: 82 Resp: 318619

Ion Ratio Lower Upper

82 100

95 0.0 5.7 8.5#

138 0.0 13.2 19.8#



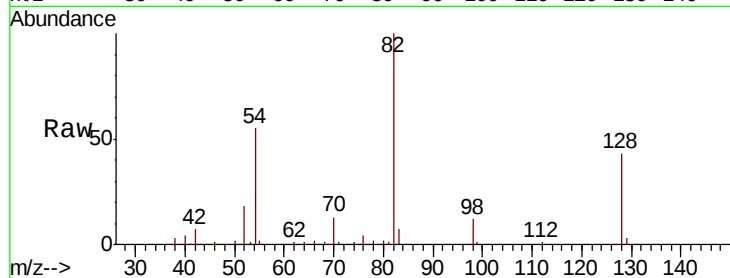


Abundance

Ion 82.00 (81.70 to 82.70): BF1

Ion 95.00 (94.70 to 95.70): BF1

Ion 138.00 (137.70 to 138.70): BF1

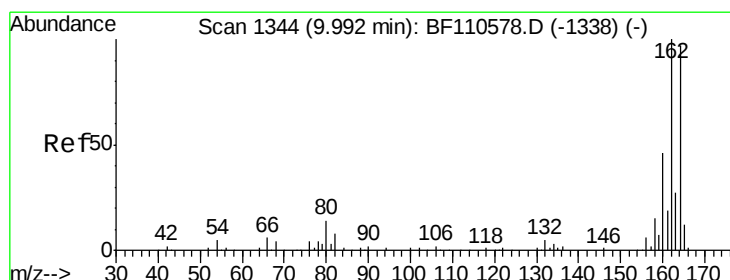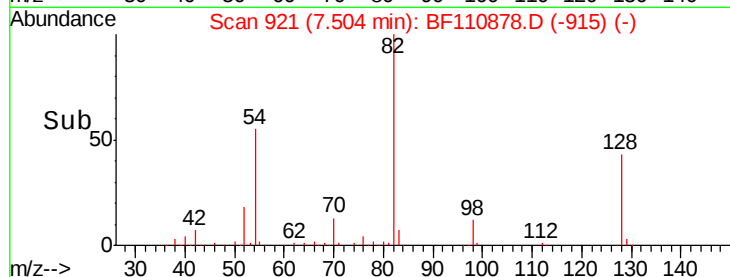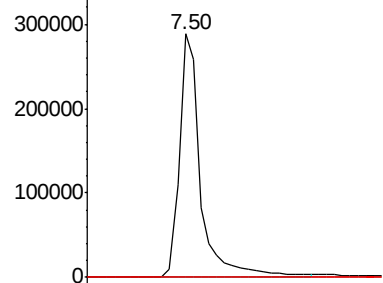

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.99 min Scan# 1343

Delta R.T. -0.01 min

Lab File: BF110878.D

Acq: 20 Nov 2018 3:29


Tgt Ion: 164 Resp: 78630

Ion Ratio Lower Upper

164 100

162 107.7 83.0 124.6

160 48.5 37.0 55.6


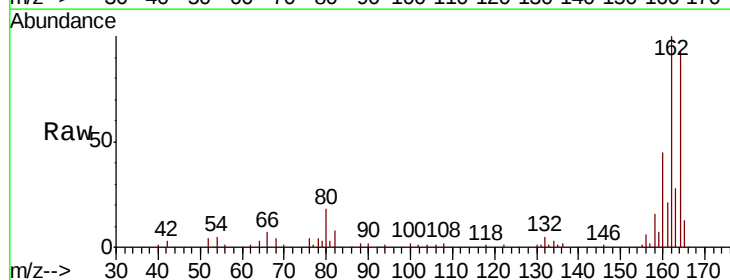



Abundance

Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

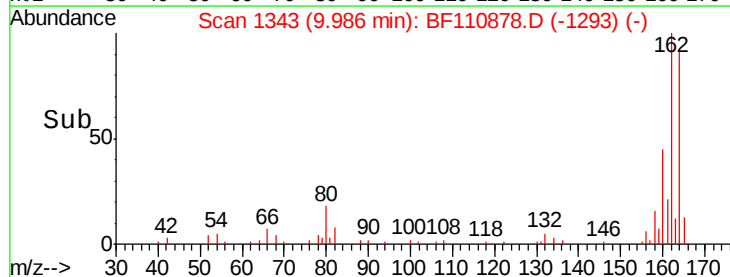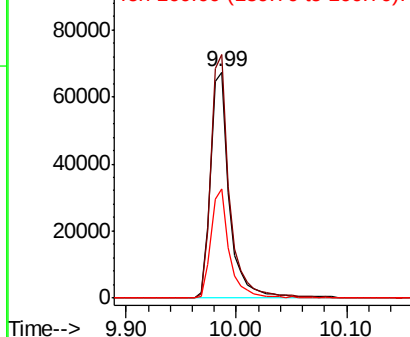


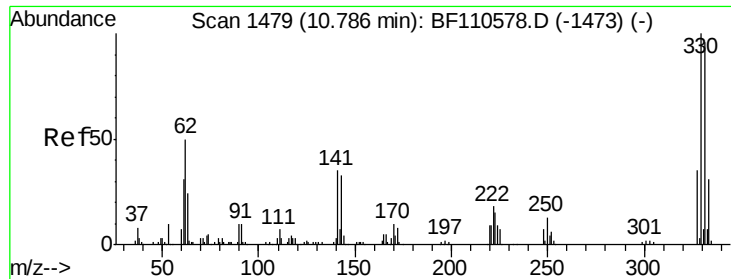

#42
 2,4,6-Tribromophenol
 Concen: 71.475 ng
 RT: 10.78 min Scan# 1478
 Delta R.T. -0.01 min
 Lab File: BF110878.D
 Acq: 20 Nov 2018 3:29

Instrument :
 BNA_F
 ClientSampleId :
 111518-JETT-E-D-S

Tgt Ion	Ratio	Lower	Upper
330	100		
332	93.8	77.1	115.7
141	38.2	27.0	40.4



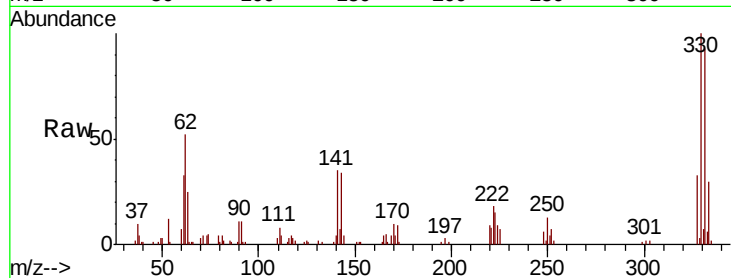


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

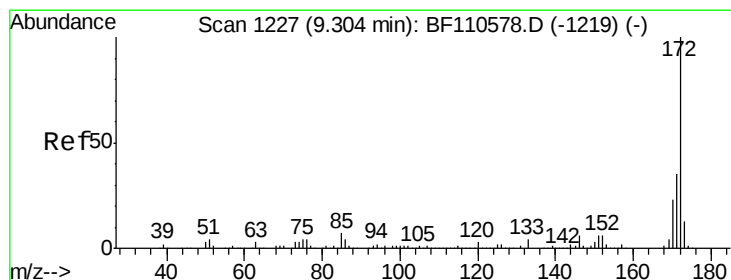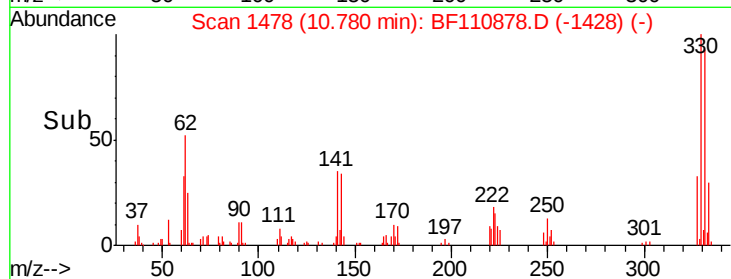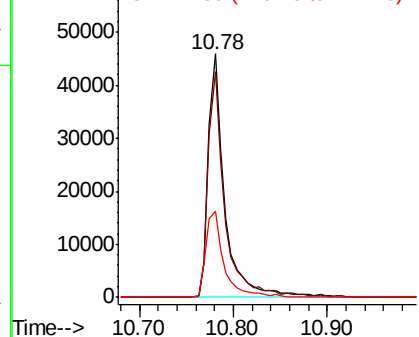

#45
 2-Fluorobiphenyl
 Concen: 105.391 ng
 RT: 9.30 min Scan# 1226
 Delta R.T. -0.01 min
 Lab File: BF110878.D
 Acq: 20 Nov 2018 3:29

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.4	28.6	43.0
170	24.1	19.7	29.5


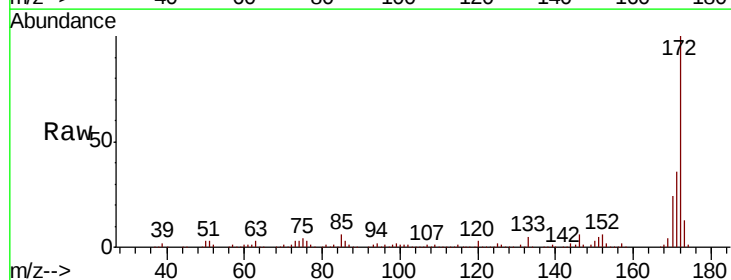



Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

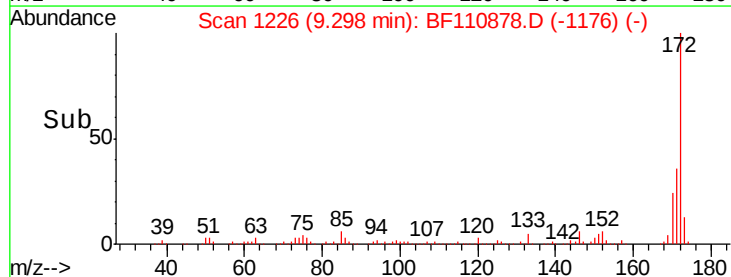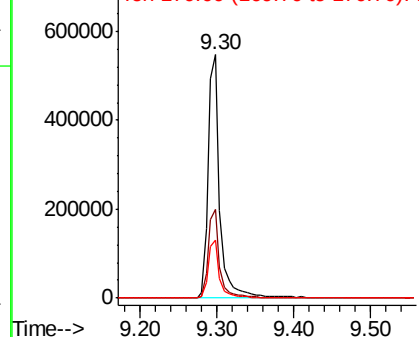


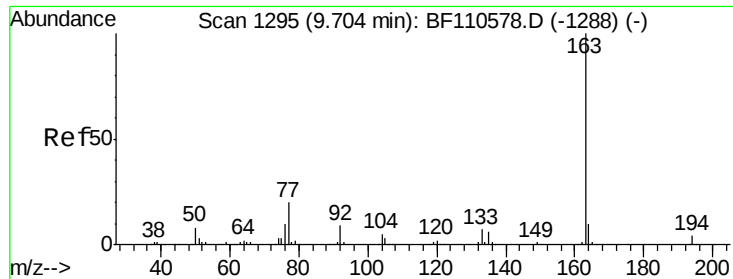




#50
Dimethylphthalate
Concen: 2.989 ng
RT: 9.70 min Scan# 1294
Delta R.T. -0.01 min
Lab File: BF110878.D
Acq: 20 Nov 2018 3:29

Instrument :
BNA_F
ClientSampleId :
111518-JETT-E-D-S

Tgt Ion:163 Resp: 17535
Ion Ratio Lower Upper
163 100
194 3.0 3.2 4.8#
164 10.9 8.1 12.1

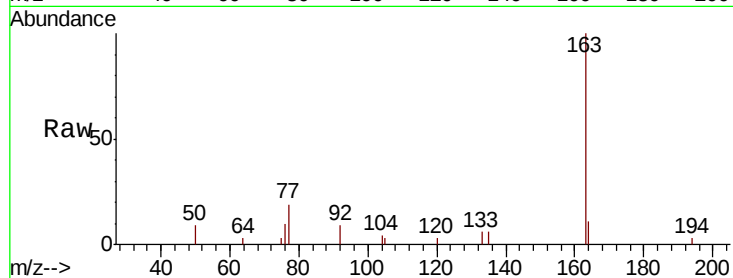


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

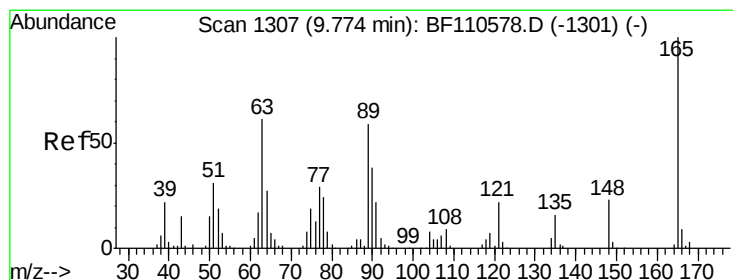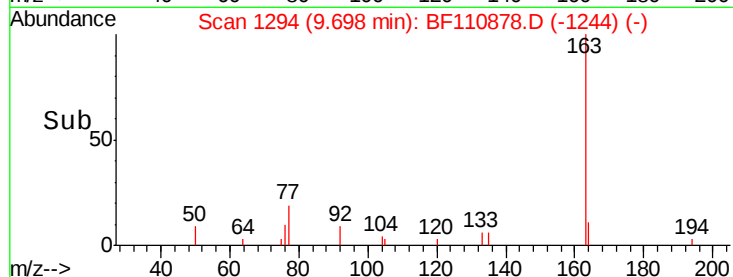
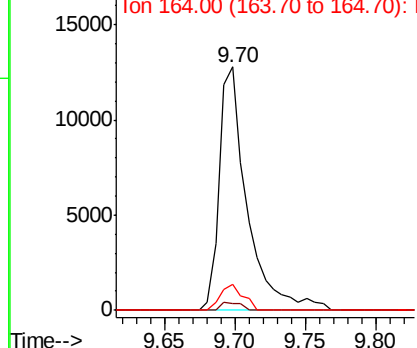


#51
2,6-Dinitrotoluene
Concen: 7.723 ng
RT: 9.99 min Scan# 1343
Delta R.T. 0.21 min
Lab File: BF110878.D
Acq: 20 Nov 2018 3:29

Tgt Ion:165 Resp: 9968
Ion Ratio Lower Upper
165 100
63 0.0 48.9 73.3#
89 0.0 46.6 69.8#

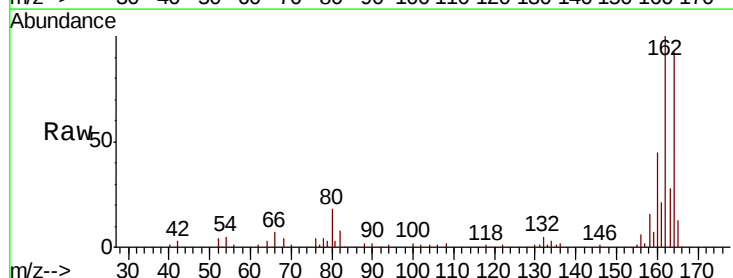

Abundance Ion 165.00 (164.70 to 165.70): E
Ion 63.00 (62.70 to 63.70): BF1
Ion 89.00 (88.70 to 89.70): BF1

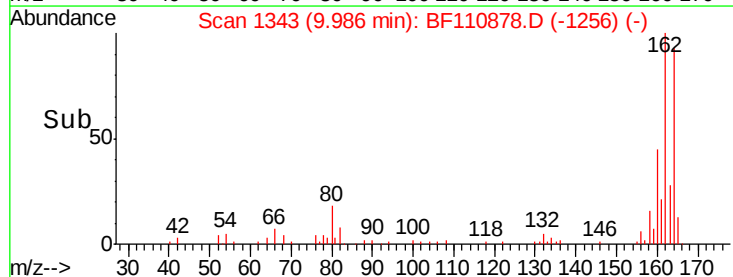
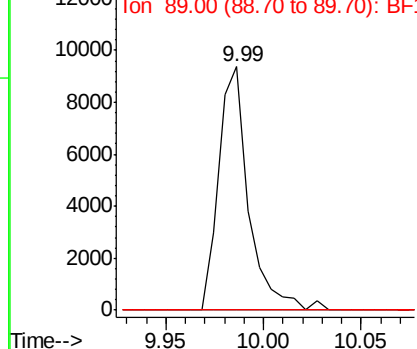




#57
 2,4-Dinitrotoluene
 Concen: 5.940 ng
 RT: 9.99 min Scan# 1343
 Delta R.T. -0.20 min
 Lab File: BF110878.D
 Acq: 20 Nov 2018 3:29

Instrument :
 BNA_F
 ClientSampleId :
 111518-JETT-E-D-S

Tgt Ion:	165	Resp:	9968
Ion	Ratio	Lower	Upper
165	100		
63	0.0	44.8	67.2#
89	0.0	62.2	93.4#
182	0.0	2.1	3.1#

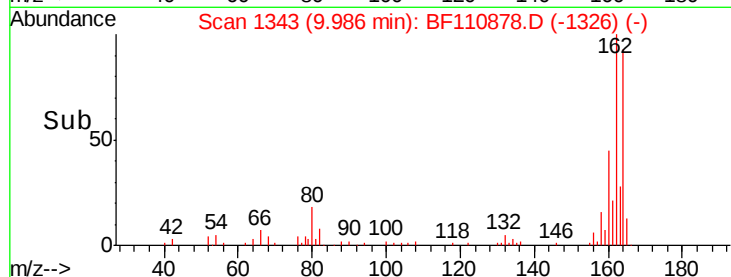
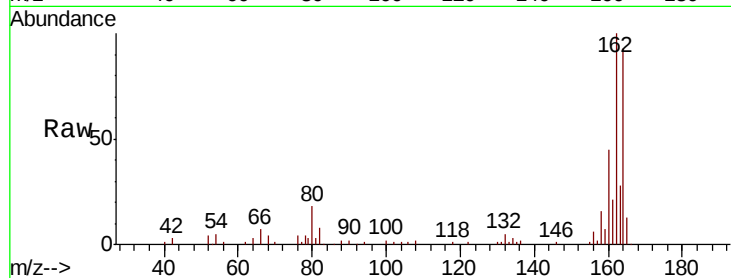


Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF1



Ion 89.00 (88.70 to 89.70): BF1

Ion 182.00 (181.70 to 182.70): E

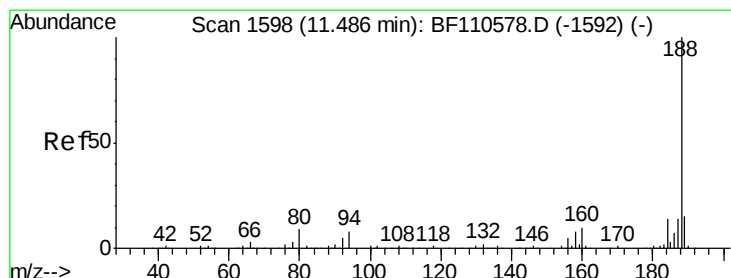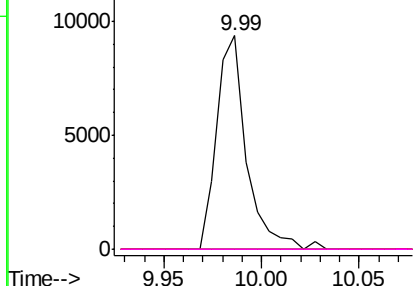

#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 11.48 min Scan# 1597
 Delta R.T. -0.01 min
 Lab File: BF110878.D
 Acq: 20 Nov 2018 3:29


Tgt Ion:	188	Resp:	136702
Ion	Ratio	Lower	Upper
188	100		
94	8.4	7.2	10.8
80	9.8	7.9	11.9

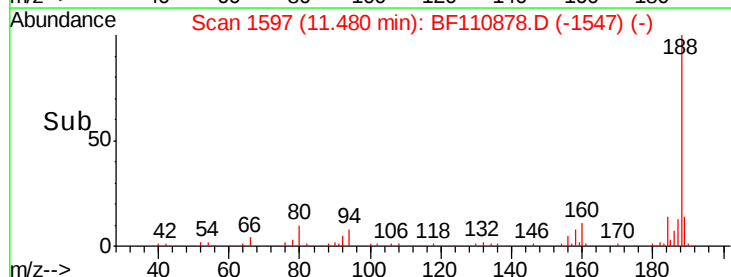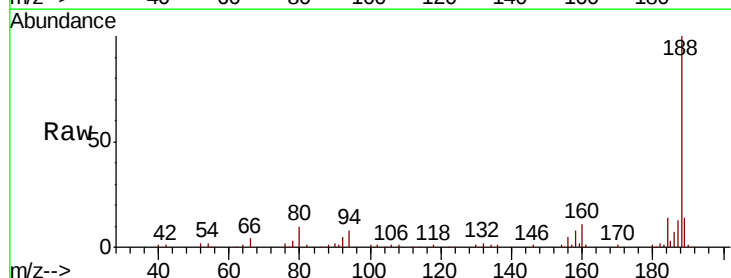


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

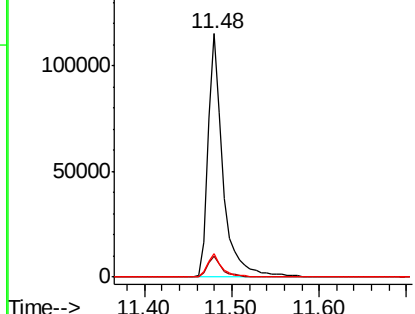


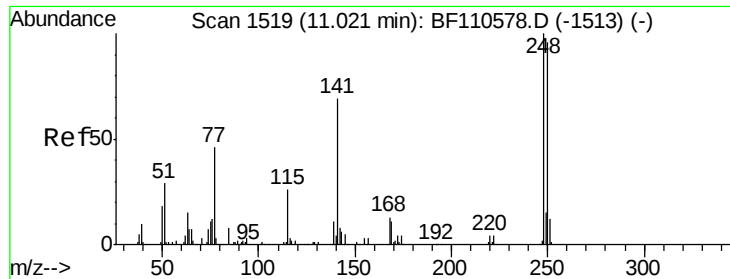




#67
4-Bromophenyl-phenylether
Concen: 2.242 ng
RT: 10.78 min Scan# 1478
Delta R.T. -0.24 min
Lab File: BF110878.D
Acq: 20 Nov 2018 3:29

Instrument :
BNA_F
ClientSampleId :
111518-JETT-E-D-S

Tgt Ion: 248 Resp: 3388
Ion Ratio Lower Upper
248 100
250 207.5 79.4 119.2#
141 567.7 55.9 83.9#

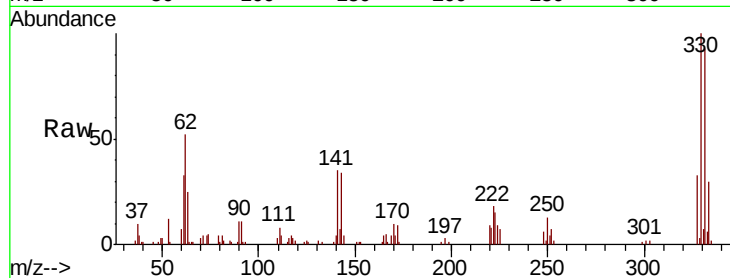


Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E

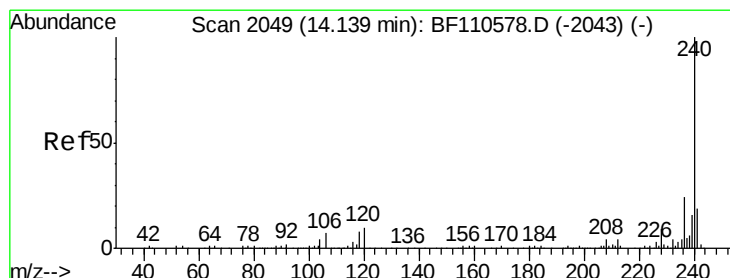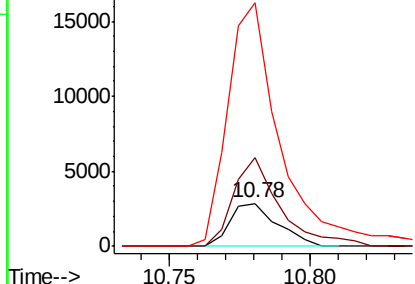
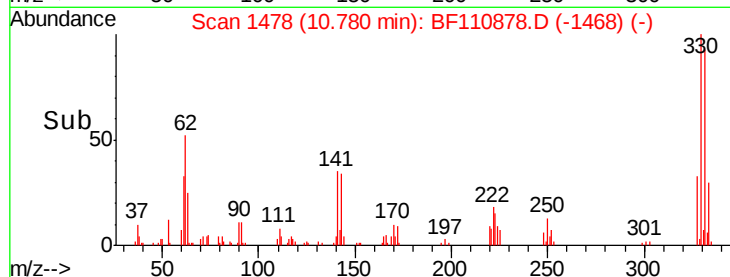



#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.13 min Scan# 2048
Delta R.T. -0.01 min
Lab File: BF110878.D
Acq: 20 Nov 2018 3:29

Tgt Ion: 240 Resp: 131571
Ion Ratio Lower Upper
240 100
120 10.2 8.3 12.5
236 24.4 21.2 31.8

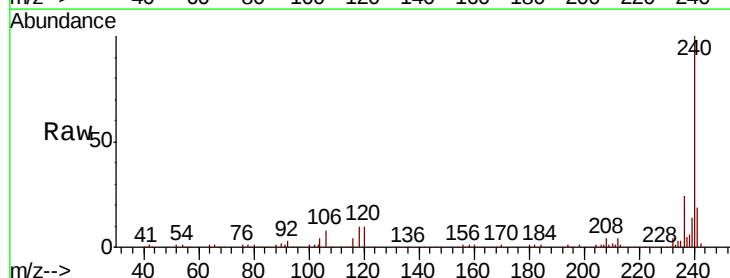

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

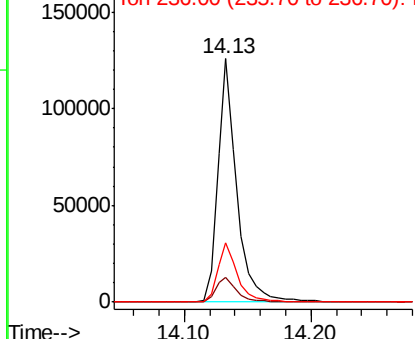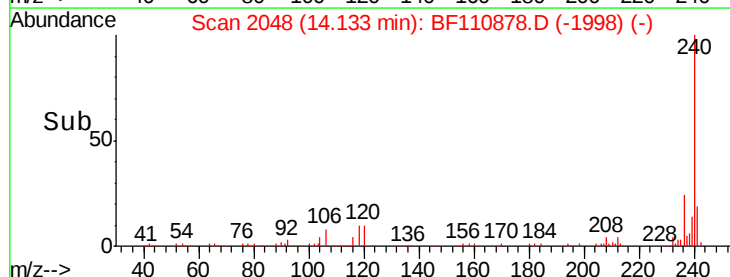

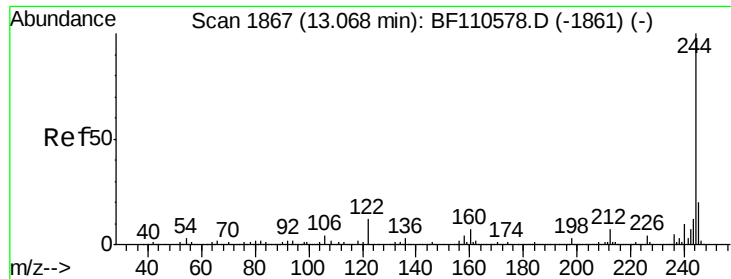

#79

Terphenyl-d14

Concen: 63.760 ng

RT: 13.06 min Scan# 1865

Delta R.T. -0.01 min

Lab File: BF110878.D

Acq: 20 Nov 2018 3:29

Instrument :

BNA_F

ClientSampleId :

111518-JETT-E-D-S


Tgt Ion:244 Resp: 447949

Ion Ratio Lower Upper

244 100

212 6.9 5.8 8.8




122 12.5 8.7 13.1

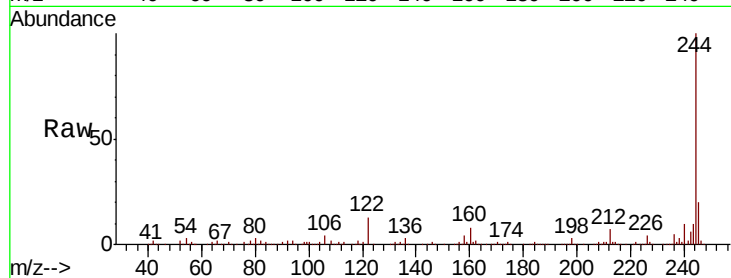

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

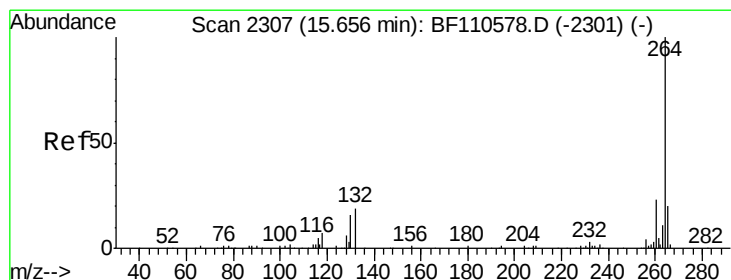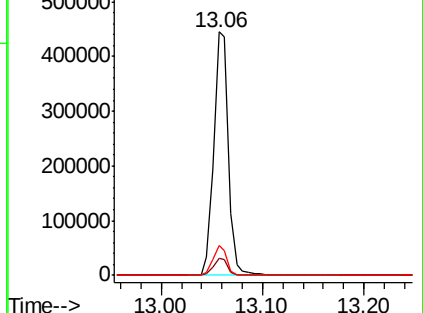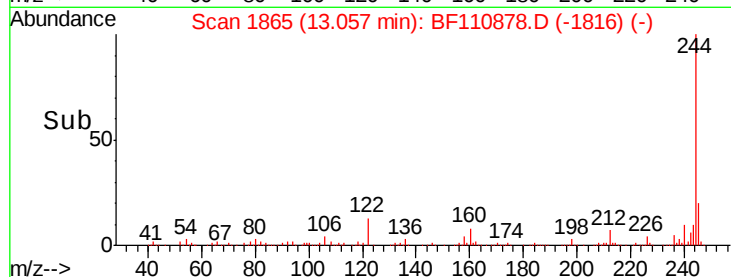

#87

Perylene-d12

Concen: 20.000 ng

RT: 15.67 min Scan# 2309

Delta R.T. 0.01 min

Lab File: BF110878.D

Acq: 20 Nov 2018 3:29


Tgt Ion:264 Resp: 80441

Ion Ratio Lower Upper

264 100

260 23.2 18.7 28.1

265 22.4 16.7 25.1

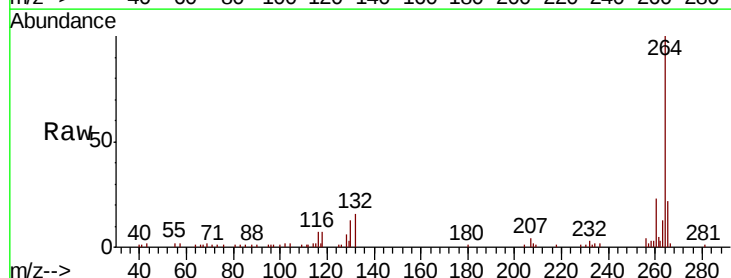

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

