

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF111918\
 Data File : BF110870.D
 Acq On : 19 Nov 2018 23:51
 Operator : JU/SJ
 Sample : J5985-01
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 111518-DBRI-E-D-B

Quant Time: Nov 20 06:10:45 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF110818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 13 12:43:10 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.94	152	54991	20.00	ng	0.00
21) Naphthalene-d8	8.23	136	225653	20.00	ng	0.00
39) Acenaphthene-d10	9.99	164	90558	20.00	ng	0.00
64) Phenanthrene-d10	11.48	188	148385	20.00	ng	0.00
76) Chrysene-d12	14.13	240	125287	20.00	ng	0.00
87) Perylene-d12	15.67	264	78092	20.00	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.56	112	131615	38.88	ng	0.00
7) Phenol-d6	6.57	99	96394	22.27	ng	0.00
23) Nitrobenzene-d5	7.51	82	392727	100.23	ng	0.00
42) 2,4,6-Tribromophenol	10.78	330	69854	76.55	ng	0.00
45) 2-Fluorobiphenyl	9.30	172	725598	114.43	ng	0.00
79) Terphenyl-d14	13.06	244	475913	71.14	ng	0.00
Target Compounds						
10) Phenol	6.59	94	10280	2.048	ng	85
50) Dimethylphthalate	9.69	163	17918	2.652	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF111918\
Data File : BF110870.D
Acq On : 19 Nov 2018 23:51
Operator : JU/SJ
Sample : J5985-01
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
111518-DBRI-E-D-B

Quant Time: Nov 20 06:10:45 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF110818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 13 12:43:10 2018
Response via : Initial Calibration

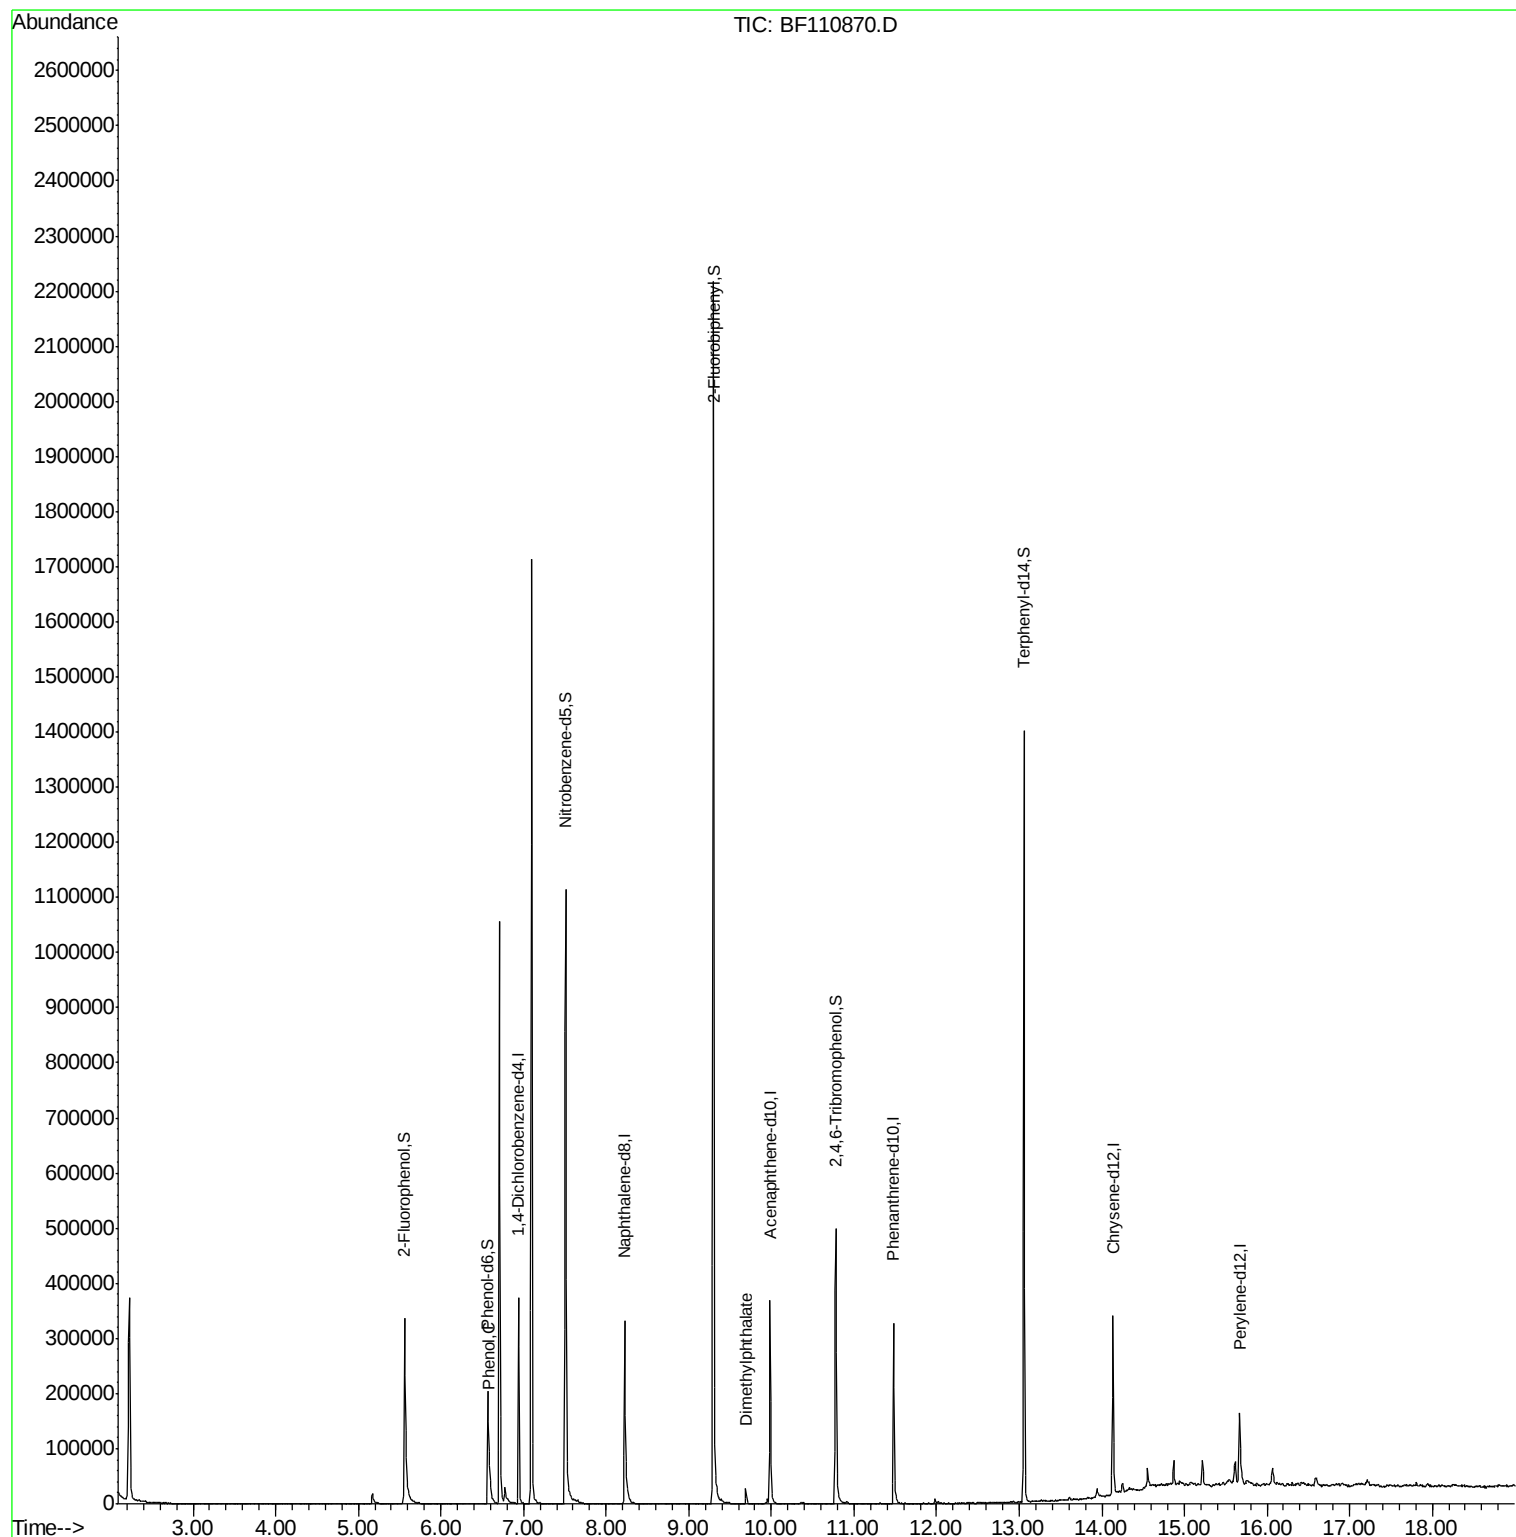

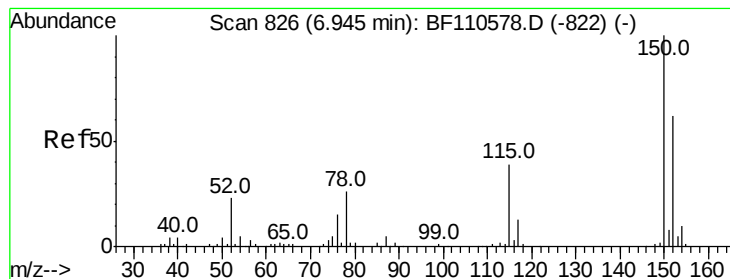


#1




1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.94 min Scan# 825
 Delta R.T. -0.01 min
 Lab File: BF110870.D
 Acq: 19 Nov 2018 23:51

Instrument :
 BNA_F
 ClientSampleId :
 111518-DBRI-E-D-B

Tot Ion:152 Resp: 54991
 Ion Ratio Lower Upper
 152 100
 150 163.7 122.7 184.1
 115 67.0 49.1 73.7

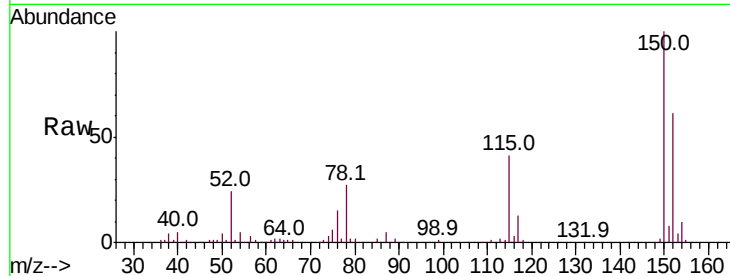


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

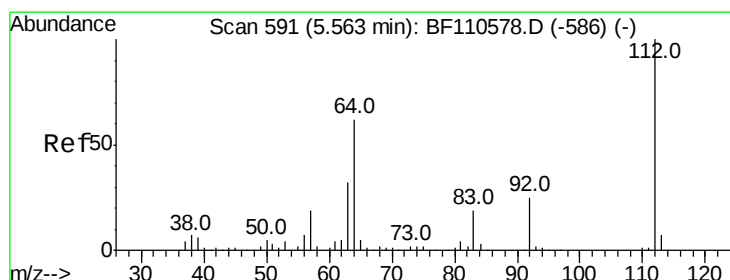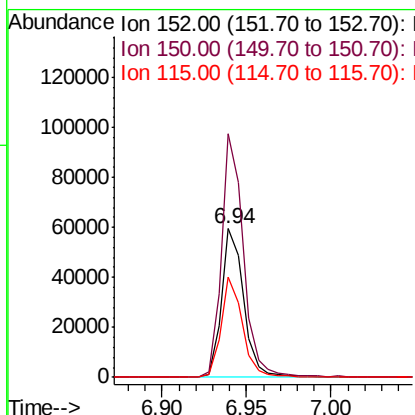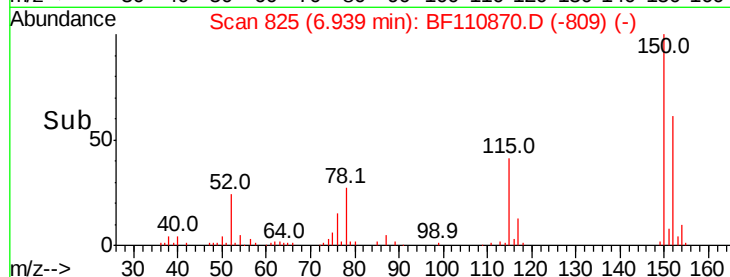



#5

2-Fluorophenol
 Concen: 38.876 ng
 RT: 5.56 min Scan# 591
 Delta R.T. 0.00 min
 Lab File: BF110870.D
 Acq: 19 Nov 2018 23:51

Tgt Ion:112 Resp: 131615
 Ion Ratio Lower Upper
 112 100
 64 62.0 44.1 66.1
 63 33.3 23.7 35.5

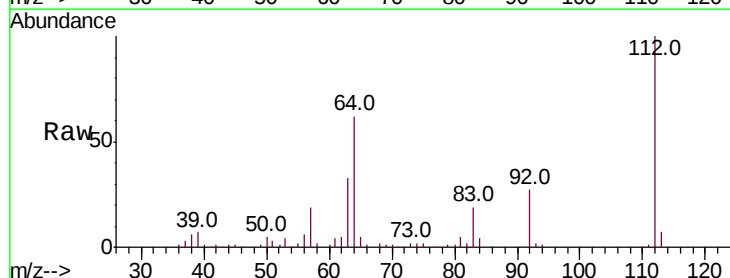

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF1
 Ion 63.00 (62.70 to 63.70): BF1

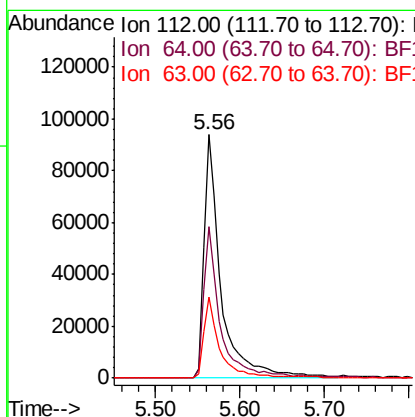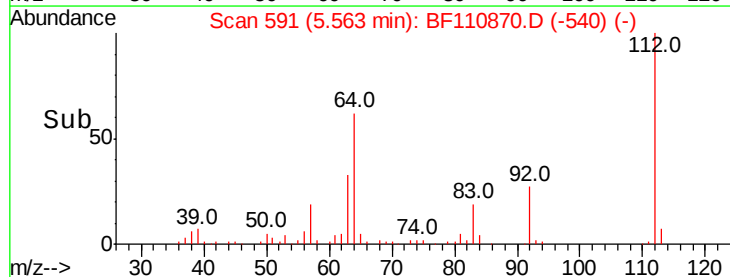



#7

Phenol-d6

Concen: 22.266 ng

RT: 6.57 min Scan# 762

Delta R.T. -0.01 min

Lab File: BF110870.D

Acq: 19 Nov 2018 23:51

Instrument :

BNA_F

ClientSampleId :

111518-DBRI-E-D-B


Tot Ion: 99 Resp: 96394

Ion Ratio Lower Upper




99 100

42 18.9 15.8 23.6

71 36.2 28.0 42.0

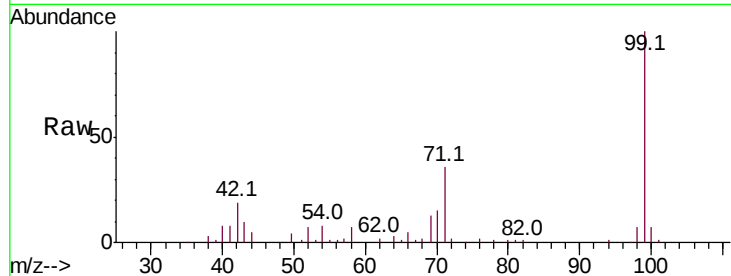

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

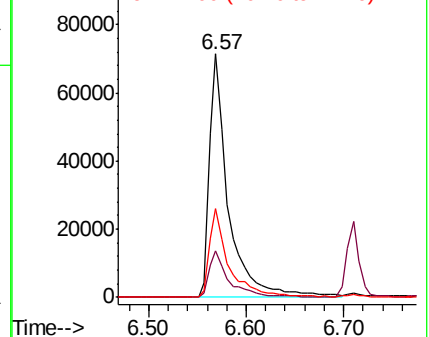

#10

Phenol

Concen: 2.048 ng

RT: 6.59 min Scan# 765

Delta R.T. 0.00 min

Lab File: BF110870.D

Acq: 19 Nov 2018 23:51


Tgt Ion: 94 Resp: 10280

Ion Ratio Lower Upper



94 100


65 37.7 25.3 65.3

66 59.6 54.5 94.5



Abundance Ion 94.00 (93.70 to 94.70): BF1
Ion 65.00 (64.70 to 65.70): BF1
Ion 66.00 (65.70 to 66.70): BF1

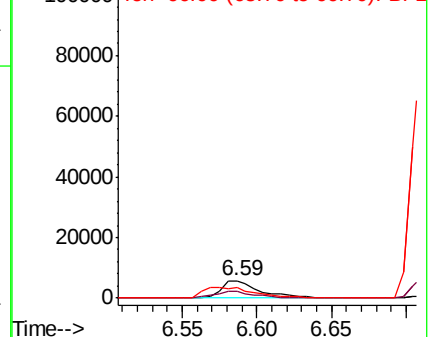

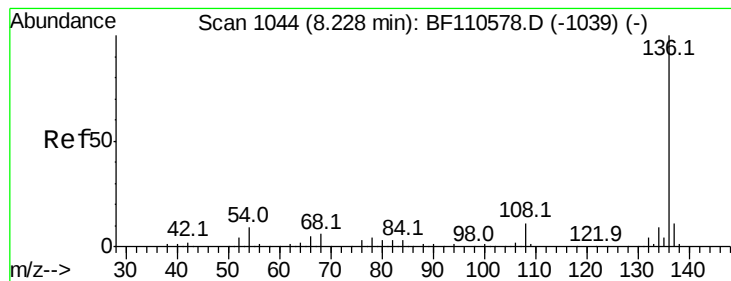

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.23 min Scan# 1044

Delta R.T. 0.00 min

Lab File: BF110870.D

Acq: 19 Nov 2018 23:51

Instrument :

BNA_F

ClientSampleId :

111518-DBRI-E-D-B

Tot Ion:136 Resp: 225653


Ion Ratio Lower Upper

136 100

137 10.6 8.8 13.2

54 7.8 5.4 8.2

68 4.6 4.2 6.2






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1

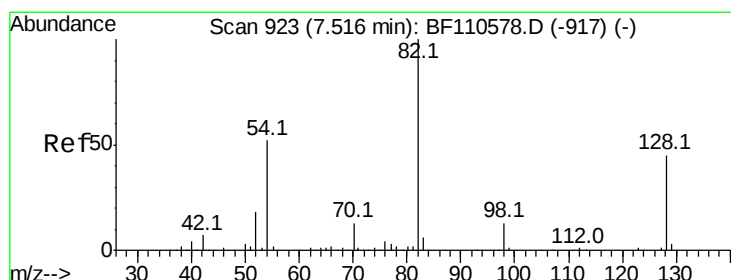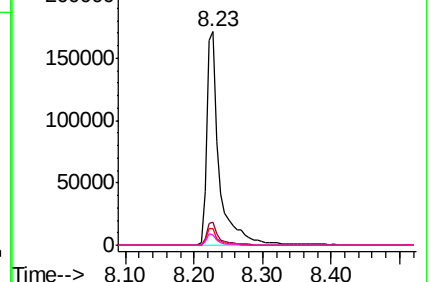

#23

Nitrobenzene-d5

Concen: 100.229 ng

RT: 7.51 min Scan# 922

Delta R.T. -0.01 min

Lab File: BF110870.D

Acq: 19 Nov 2018 23:51


Tgt Ion: 82 Resp: 392727

Ion Ratio Lower Upper

82 100

128 45.6 34.2 51.2



54 52.6 38.6 58.0




Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF1

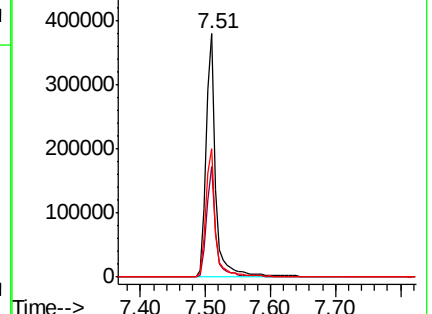




#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.99 min Scan# 1343
Delta R.T. -0.01 min
Lab File: BF110870.D
Acq: 19 Nov 2018 23:51

Instrument :
BNA_F
ClientSampleId :
111518-DBRI-E-D-B

Tot Ion	Ratio	Lower	Upper
164	100		
162	104.2	83.0	124.6
160	46.4	37.0	55.6


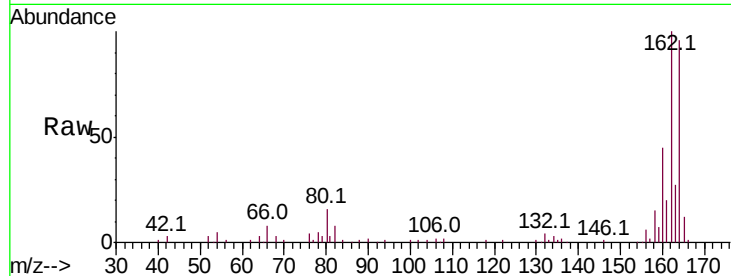


Abundance

Ion 164.00 (163.70 to 164.70): E


Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

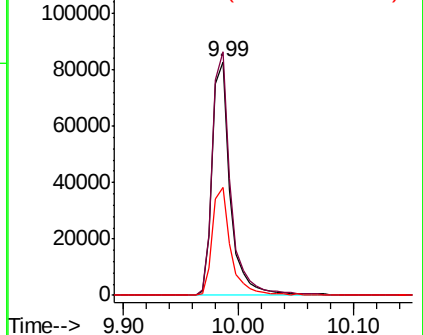

#42
2,4,6-Tribromophenol
Concen: 76.554 ng
RT: 10.78 min Scan# 1478
Delta R.T. -0.01 min
Lab File: BF110870.D
Acq: 19 Nov 2018 23:51

Tgt Ion	Ratio	Lower	Upper
330	100		
332	96.8	77.1	115.7
141	37.8	27.0	40.4


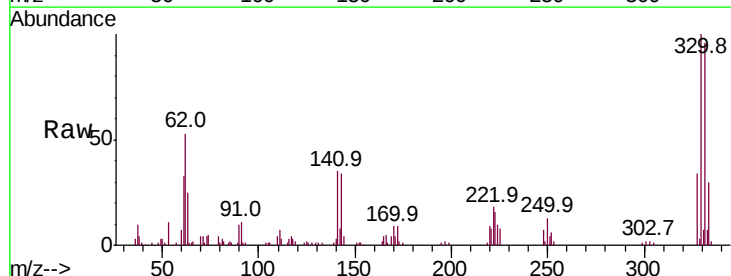



Abundance

Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

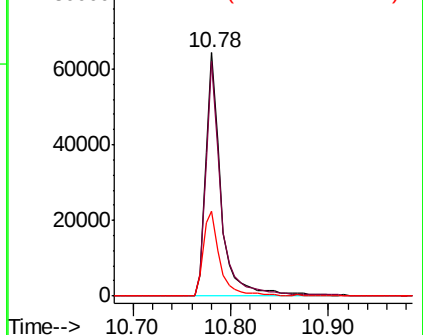







#45
 2-Fluorobiphenyl
 Concen: 114.433 ng
 RT: 9.30 min Scan# 1226
 Delta R.T. -0.01 min
 Lab File: BF110870.D
 Acq: 19 Nov 2018 23:51

Instrument :
 BNA_F
 ClientSampleId :
 111518-DBRI-E-D-B

Tot Ion:172 Resp: 725598
 Ion Ratio Lower Upper
 172 100
 171 35.6 28.6 43.0
 170 23.4 19.7 29.5




Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E


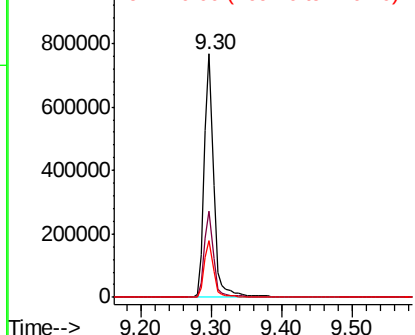



#50
 Dimethylphthalate
 Concen: 2.652 ng
 RT: 9.69 min Scan# 1293
 Delta R.T. -0.01 min
 Lab File: BF110870.D
 Acq: 19 Nov 2018 23:51

Tgt Ion:163 Resp: 17918
 Ion Ratio Lower Upper
 163 100
 194 3.6 3.2 4.8
 164 11.1 8.1 12.1



Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

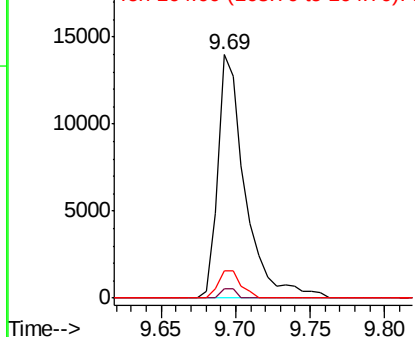

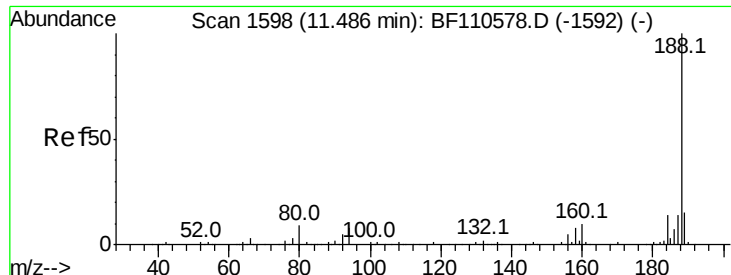

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.48 min Scan# 1597

Delta R.T. -0.01 min

Lab File: BF110870.D

Acq: 19 Nov 2018 23:51

Instrument :

BNA_F

ClientSampleId :

111518-DBRI-E-D-B


Tot Ion:188 Resp: 148385

Ion Ratio Lower Upper

188 100

94 8.4 7.2 10.8




80 8.8 7.9 11.9

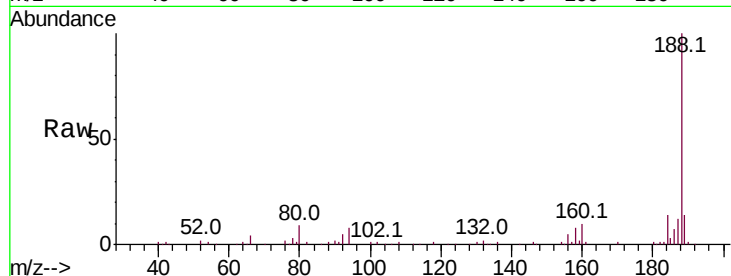

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

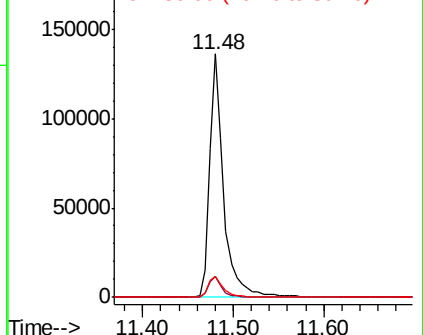

#76

Chrysene-d12

Concen: 20.000 ng

RT: 14.13 min Scan# 2048

Delta R.T. -0.01 min

Lab File: BF110870.D

Acq: 19 Nov 2018 23:51


Tgt Ion:240 Resp: 125287

Ion Ratio Lower Upper

240 100

120 10.5 8.3 12.5



236 25.1 21.2 31.8

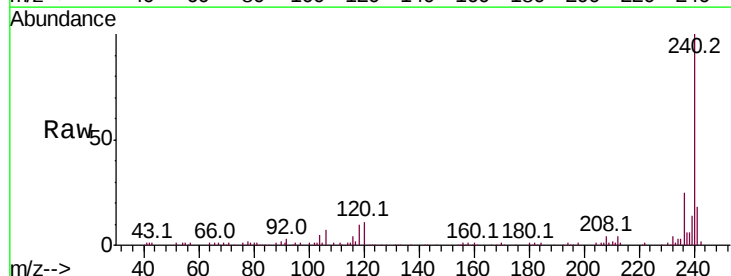


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

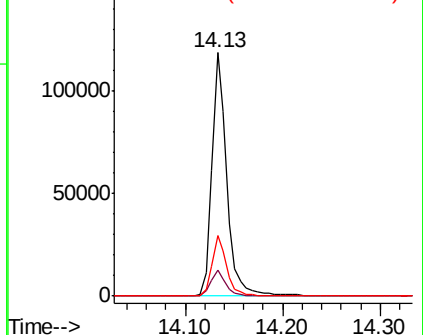

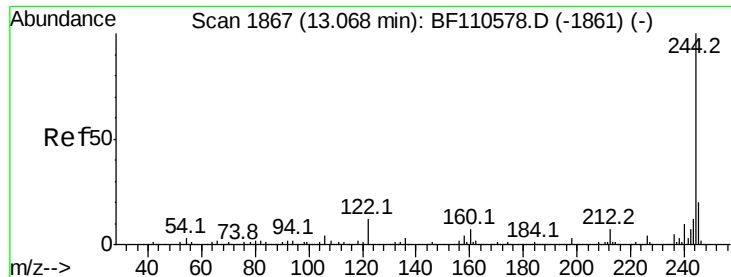

#79

Terphenyl-d14

Concen: 71.139 ng

RT: 13.06 min Scan# 1866

Delta R.T. -0.01 min

Lab File: BF110870.D

Acq: 19 Nov 2018 23:51

Instrument :

BNA_F

ClientSampleId :

111518-DBRI-E-D-B


Tot Ion:244 Resp: 475913

Ion Ratio Lower Upper

244 100

212 7.0 5.8 8.8




122 10.4 8.7 13.1

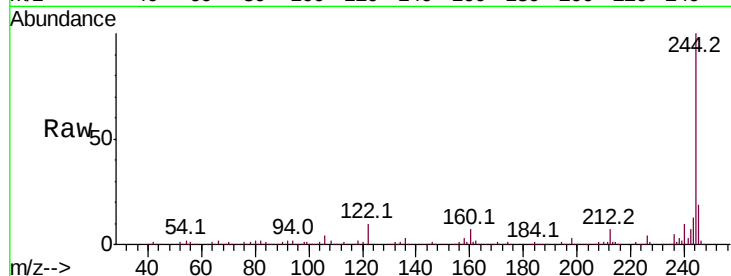

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

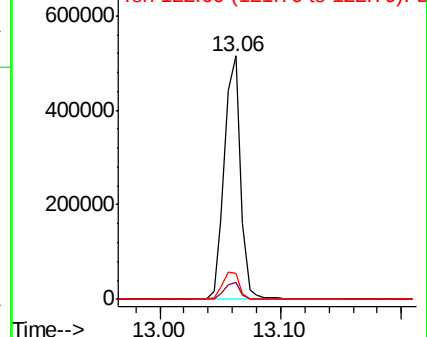

#87

Perylene-d12

Concen: 20.000 ng

RT: 15.67 min Scan# 2309

Delta R.T. 0.01 min

Lab File: BF110870.D

Acq: 19 Nov 2018 23:51


Tgt Ion:264 Resp: 78092

Ion Ratio Lower Upper

264 100

260 22.9 18.7 28.1

265 20.7 16.7 25.1



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

