


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111918\
 Data File : BF110841.D
 Acq On : 19 Nov 2018 9:17
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 13 12:43:10 2018

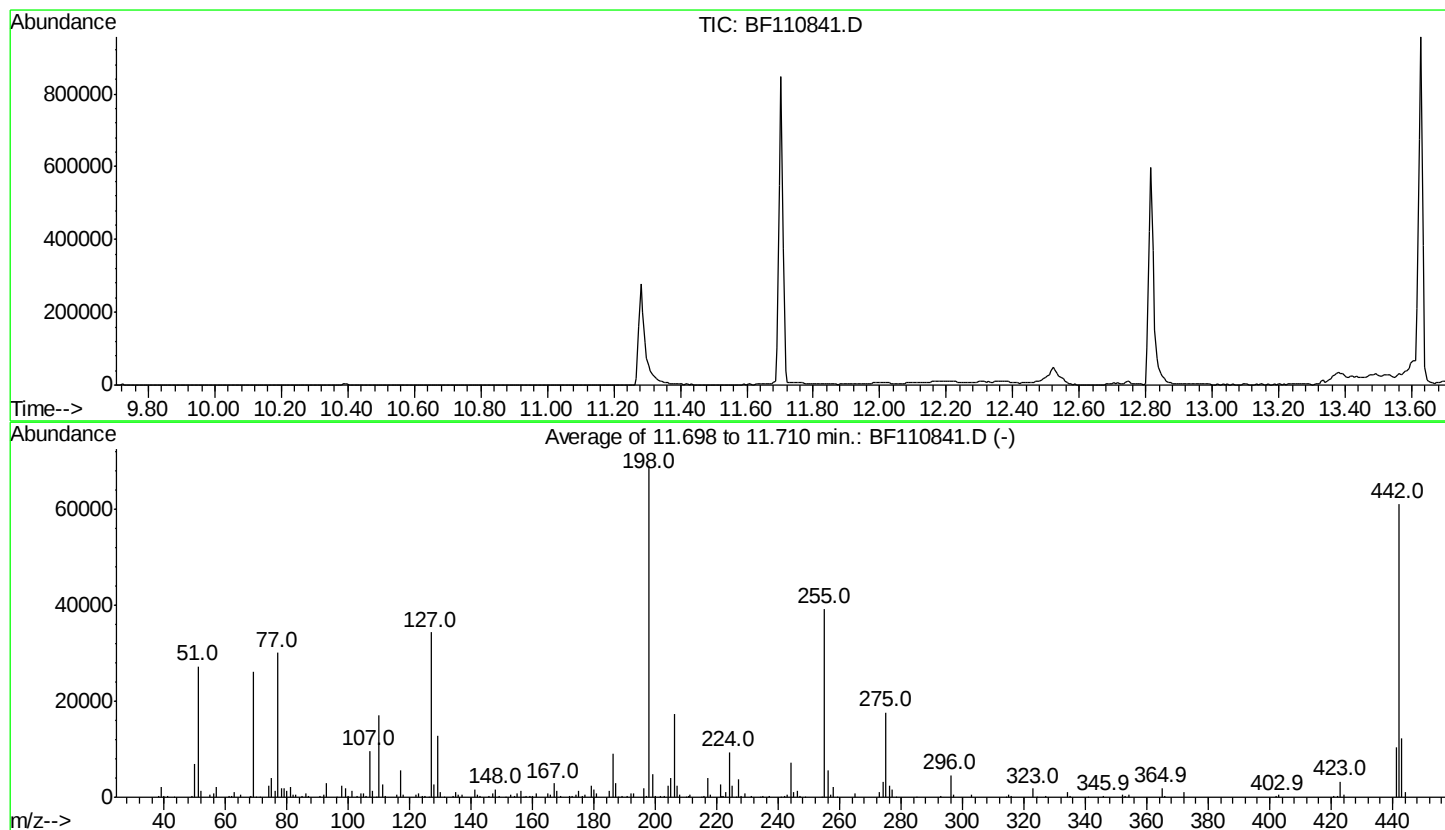

AutoFind: Scans 1634, 1635, 1636; Background Corrected with Scan 1629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.4	27285	PASS
68	69	0.00	2	1.4	378	PASS
69	198	0.00	100	37.7	26077	PASS
70	69	0.00	2	0.4	109	PASS
127	198	10	80	49.8	34445	PASS
197	198	0.00	2	0.2	161	PASS
198	198	100	100	100.0	69194	PASS
199	198	5	9	7.0	4827	PASS
275	198	10	60	25.6	17748	PASS
365	198	1	100	2.8	1961	PASS
441	198	0.01	100	15.0	10361	PASS
442	198	50	100	88.5	61258	PASS
443	442	15	24	19.9	12216	PASS