
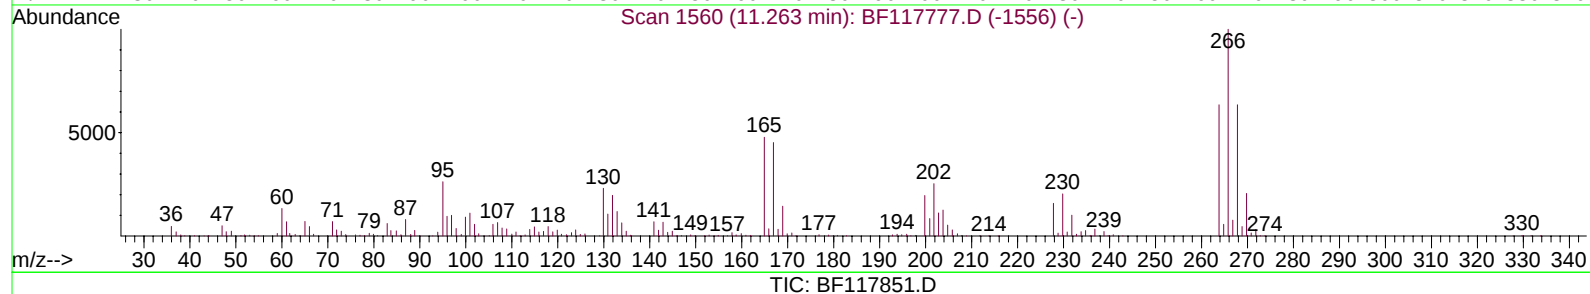
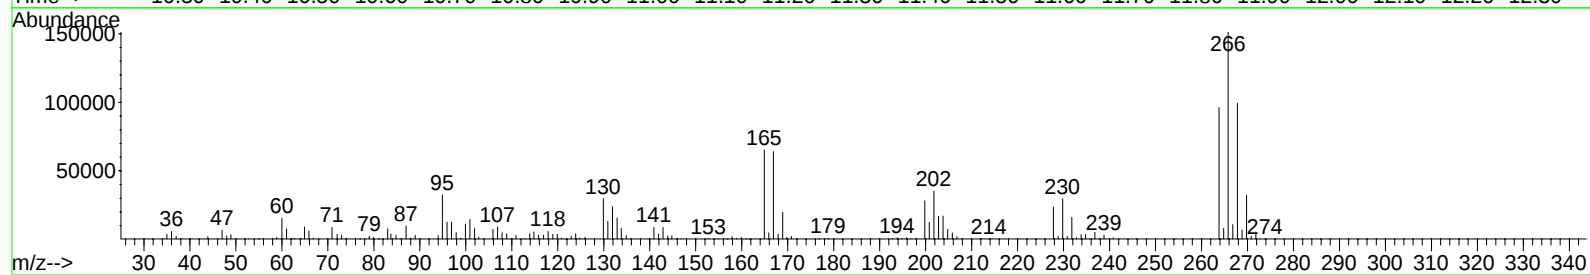


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF111919\
 Data File : BF117851.D
 Acq On : 19 Nov 2019 11:29
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 19 17:41:38 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF111319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 13 18:36:07 2019
 Response via : Initial Calibration

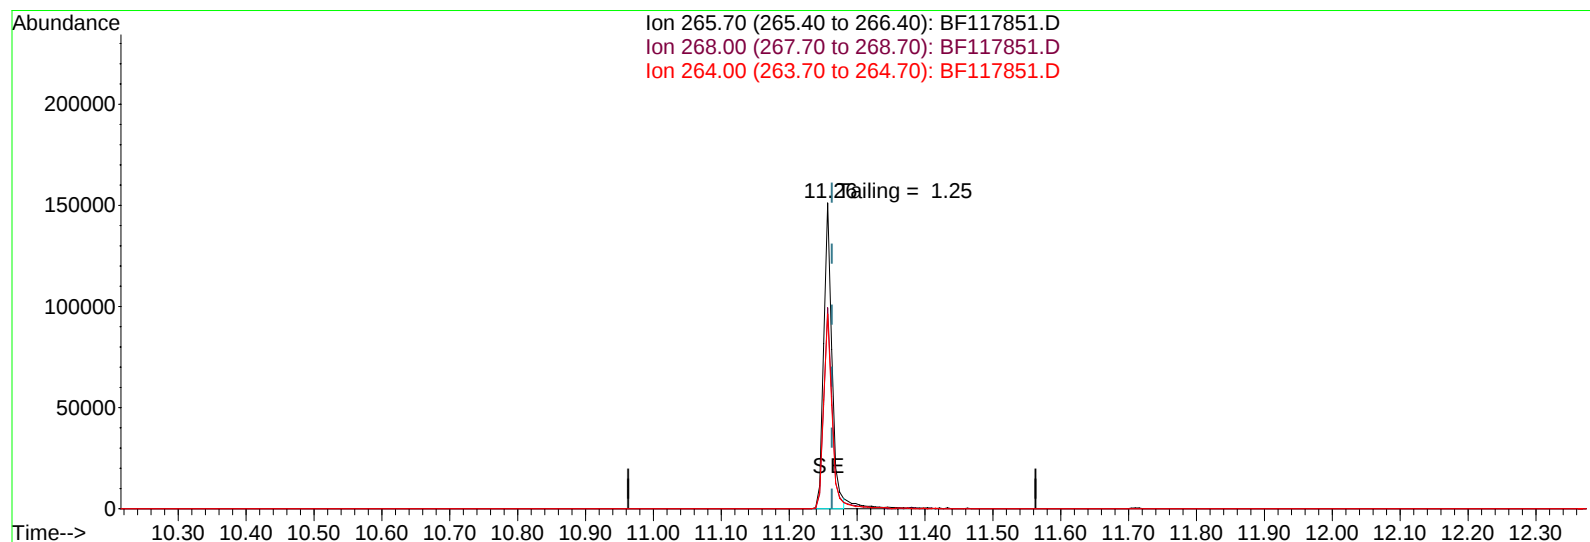

(70) Pentachlorophenol (C)




11.257min (-0.006) 22656.39ng

response 133229

Ion	Exp%	Act%
265.70	100	100
268.00	63.50	65.73
264.00	63.40	63.68
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF111919\
Data File : BF117851.D
Acq On : 19 Nov 2019 11:29
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 19 17:41:38 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF111319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 18:36:07 2019
Response via : Initial Calibration

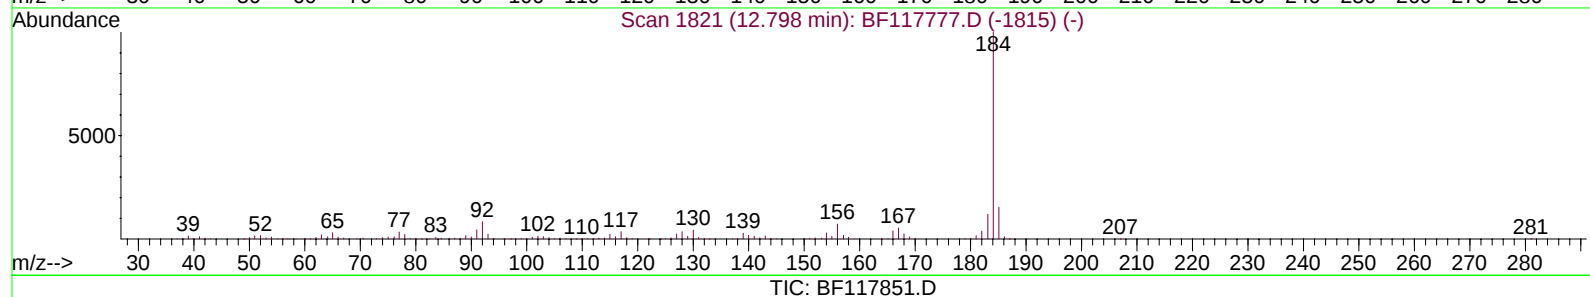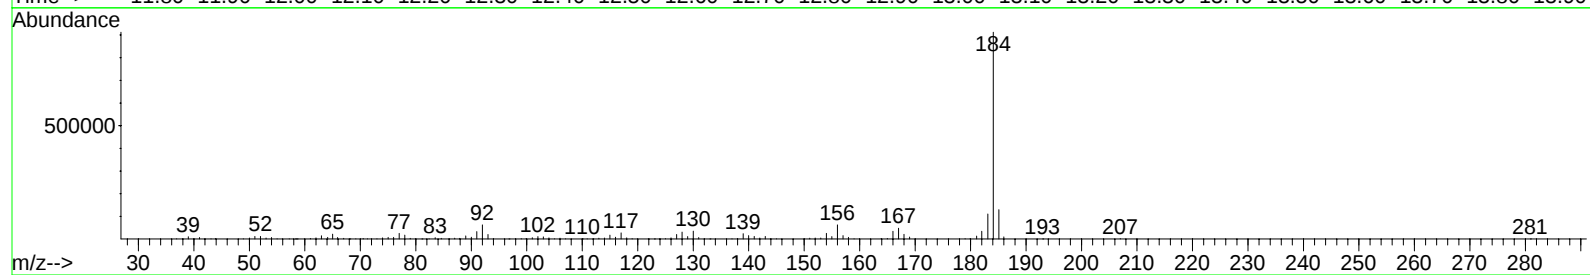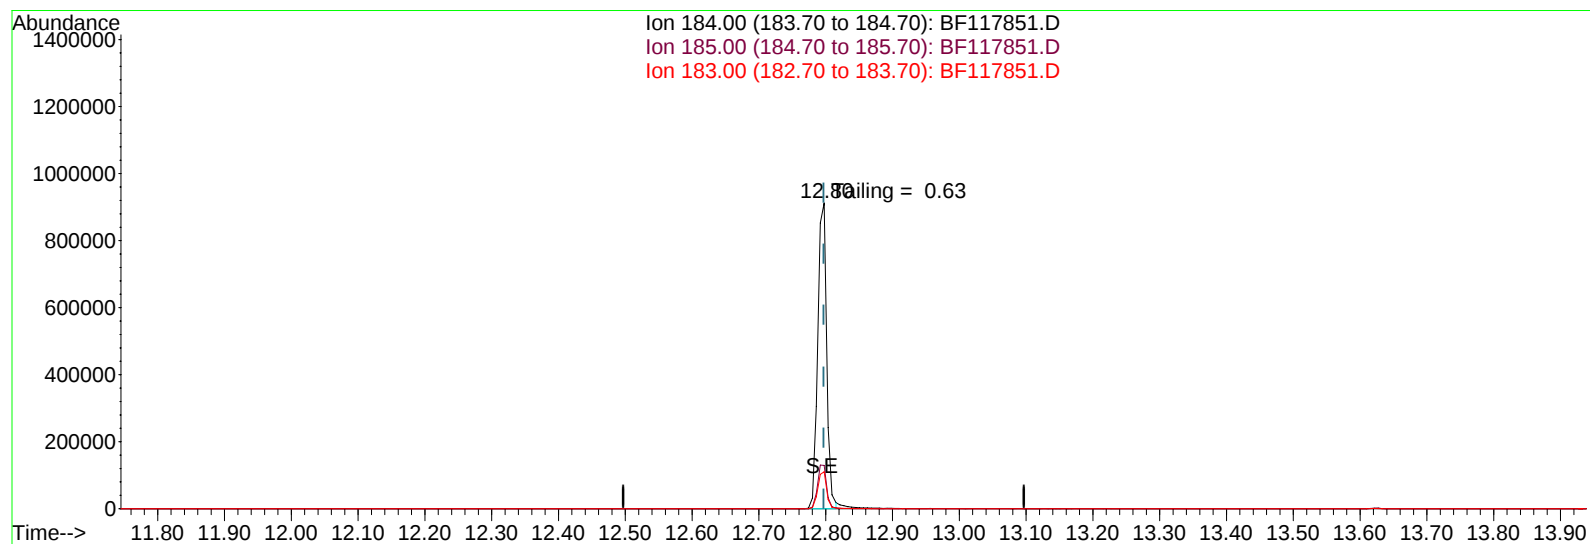

(77) Benzidine

12.798min (+0.001) 0.00ng

response 869689

Ion	Exp%	Act%
184.00	100	100
185.00	15.30	14.20
183.00	11.90	12.09
0.00	0.00	0.00