
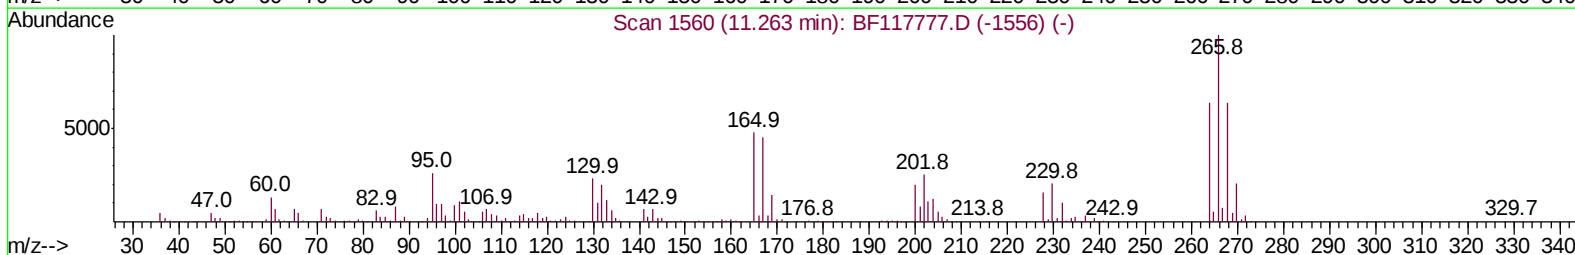
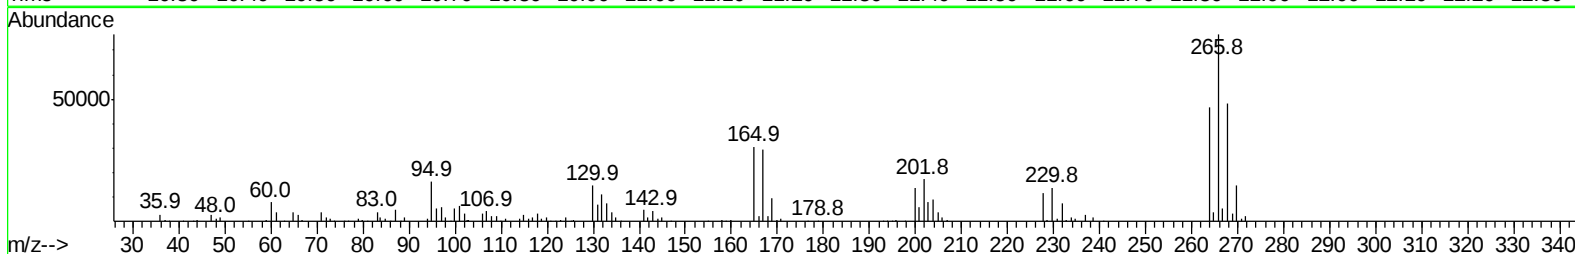


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF111919\
Data File : BF117876.D
Acq On : 20 Nov 2019 1:37
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 20 02:42:26 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF111319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 18:36:07 2019
Response via : Initial Calibration

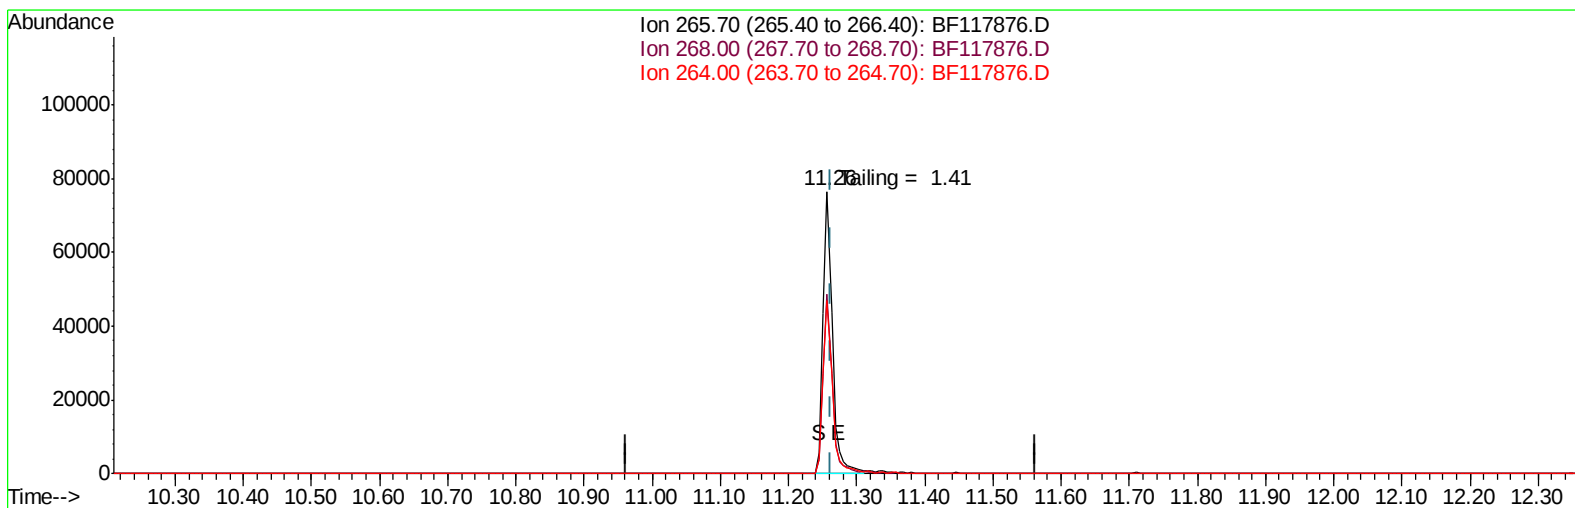

TIC: BF117876.D

(70) Pentachlorophenol (C)




11.257min (-0.006) 28634.83ng

response 71353

Ion	Exp%	Act%
265.70	100	100
268.00	63.50	63.47
264.00	63.40	61.19
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF111919\
Data File : BF117876.D
Acq On : 20 Nov 2019 1:37
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 20 02:42:26 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF111319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 18:36:07 2019
Response via : Initial Calibration

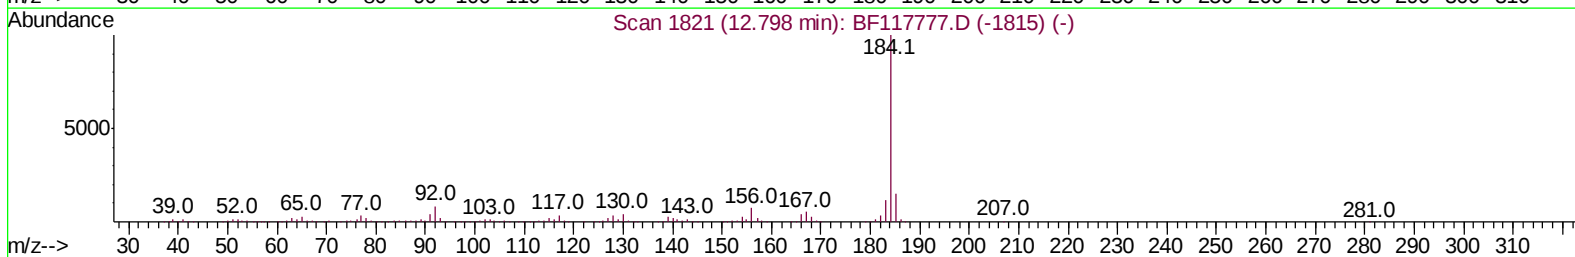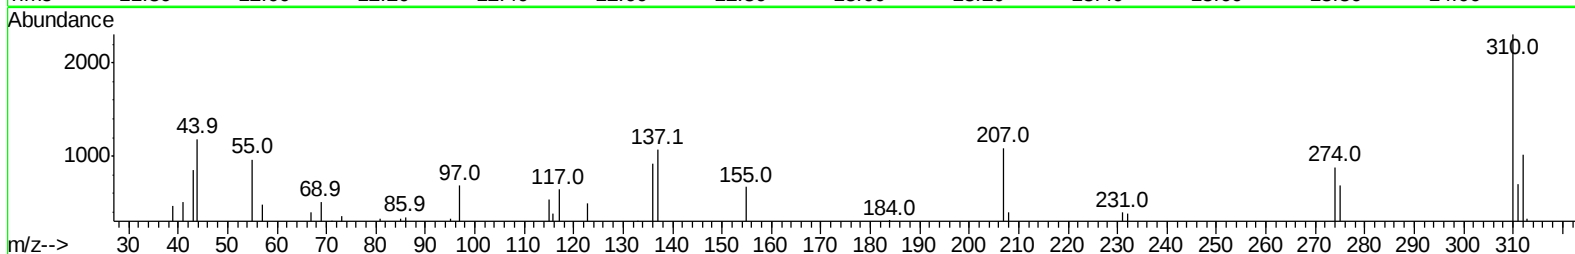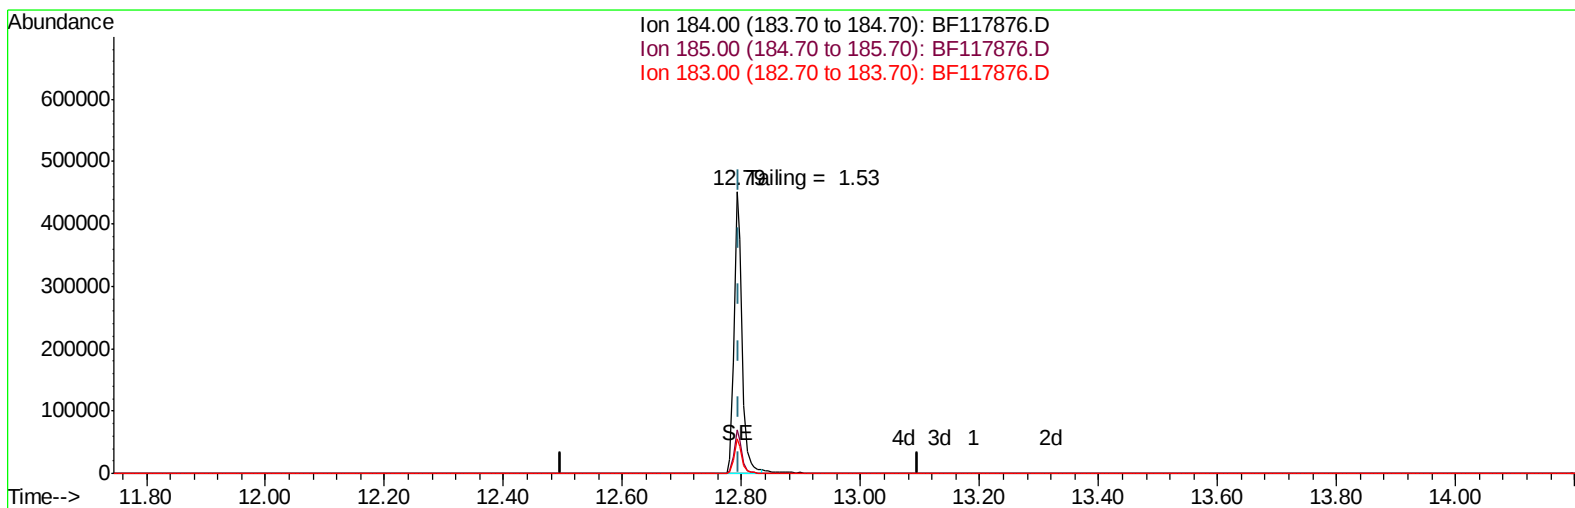

TIC: BF117876.D

(77) Benzidine

13.192min (+0.395) 11.31ng

response 110

Ion	Exp%	Act%
184.00	100	100
185.00	15.30	0.00#
183.00	11.90	0.00#
0.00	0.00	0.00