


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF111919\
 Data File : BF117851.D
 Acq On : 19 Nov 2019 11:29
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF111319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 13 18:36:07 2019

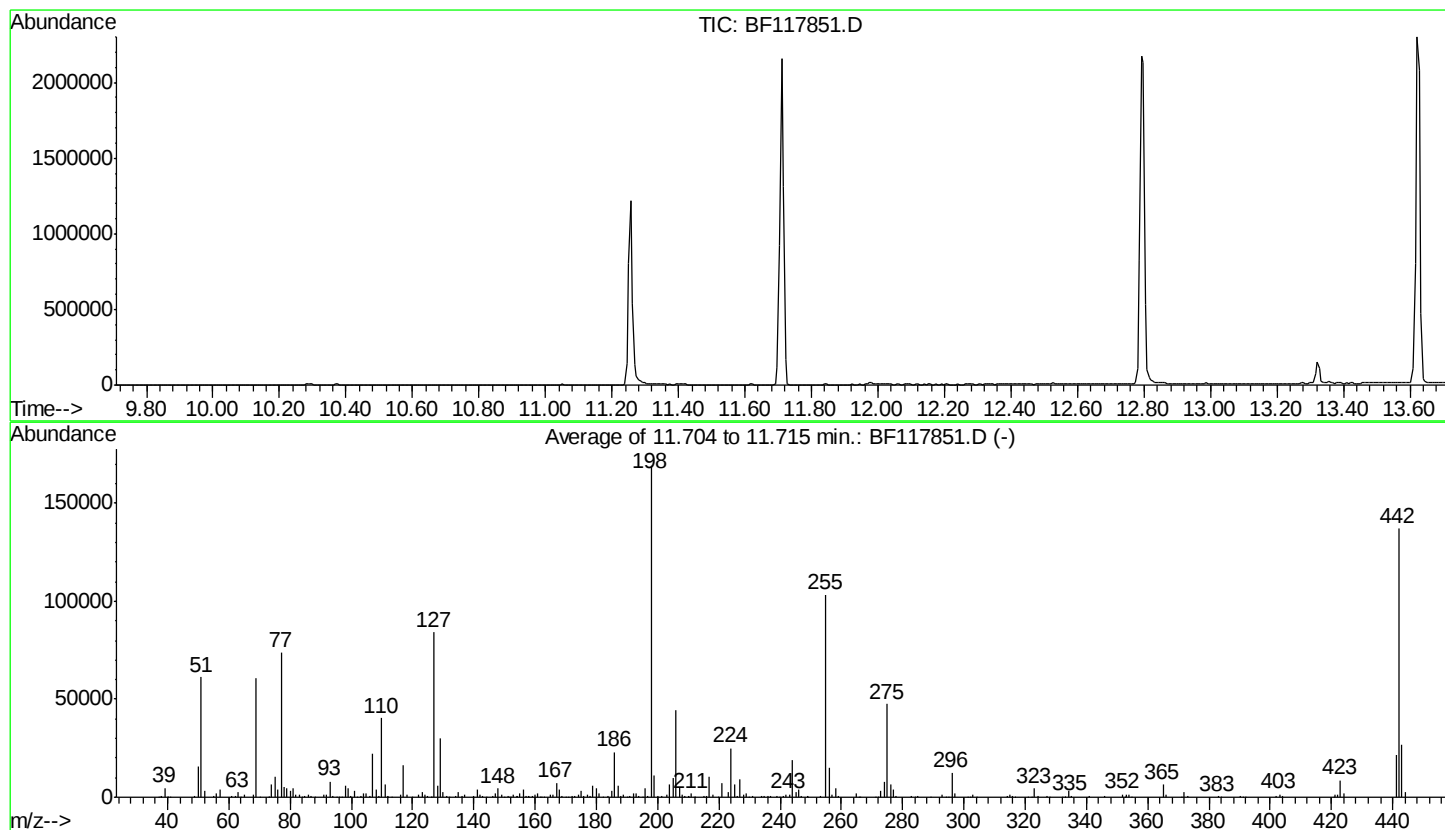

AutoFind: Scans 1635, 1636, 1637; Background Corrected with Scan 1630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.2	61202	PASS
68	69	0.00	2	1.9	1167	PASS
69	198	0.00	100	35.7	60480	PASS
70	69	0.00	2	0.5	322	PASS
127	198	10	80	49.7	84144	PASS
197	198	0.00	2	0.2	421	PASS
198	198	100	100	100.0	169237	PASS
199	198	5	9	6.5	11027	PASS
275	198	10	60	28.1	47472	PASS
365	198	1	100	3.7	6281	PASS
441	198	0.01	100	12.6	21385	PASS
442	198	50	100	80.9	136936	PASS
443	442	15	24	19.4	26532	PASS