


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111924\
Data File : BF140462.D
Acq On : 19 Nov 2024 09:32
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111324.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Nov 13 14:40:06 2024

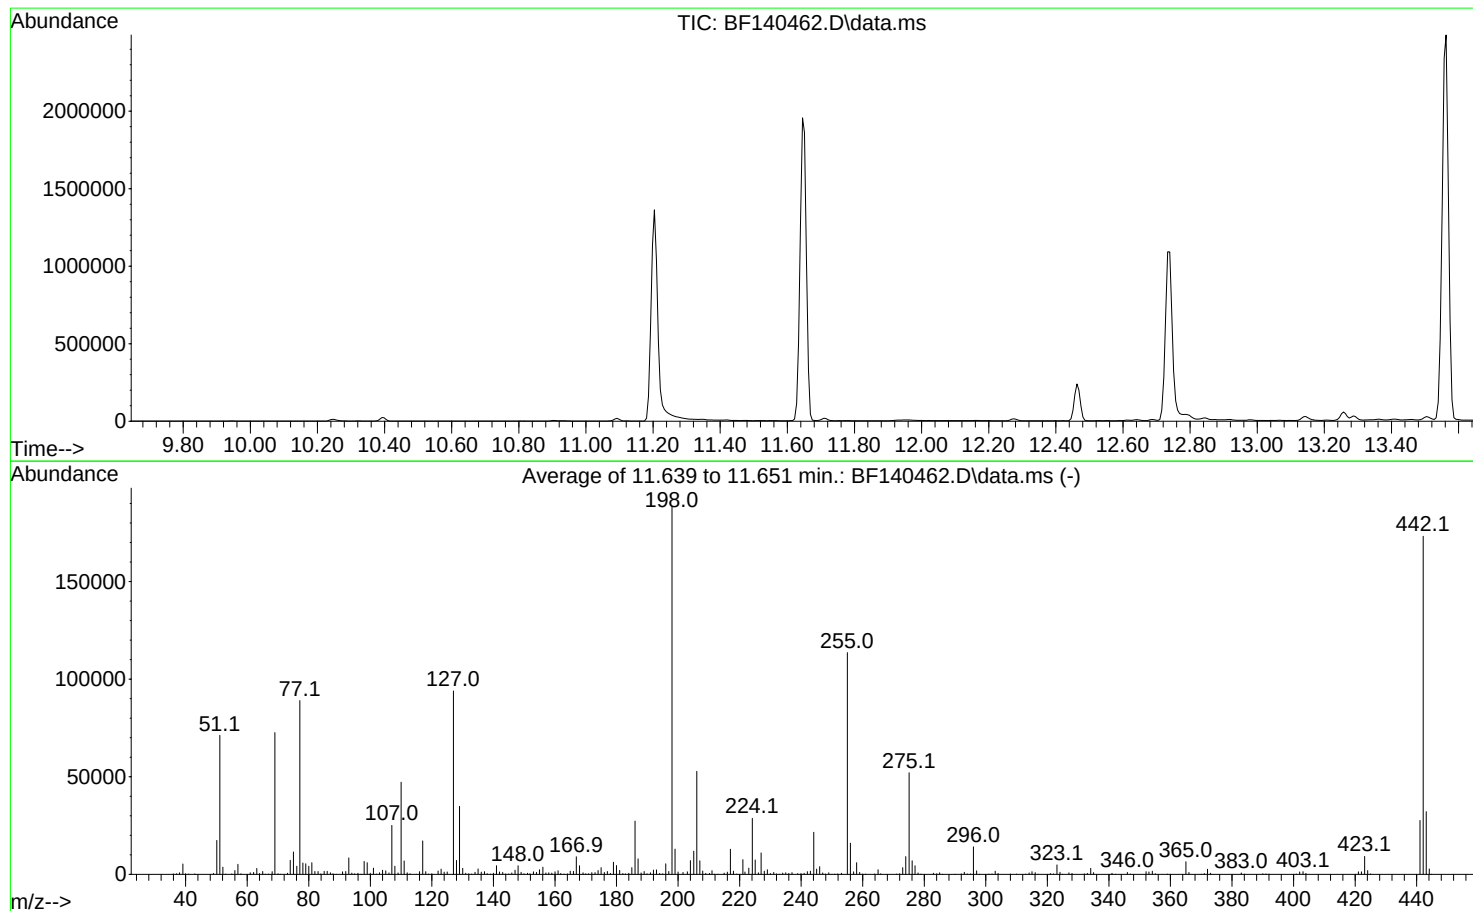

AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.8	71237	PASS
68	69	0.00	2	1.9	1395	PASS
69	198	0.00	100	38.6	72669	PASS
70	69	0.00	2	0.5	372	PASS
127	198	10	80	49.9	93997	PASS
197	198	0.00	2	0.8	1518	PASS
198	198	100	100	100.0	188480	PASS
199	198	5	9	6.9	12968	PASS
275	198	10	60	27.6	52024	PASS
365	198	1	100	3.4	6457	PASS
441	198	0.01	100	14.7	27643	PASS
442	442	50	100	100.0	173237	PASS
443	442	15	24	18.5	32109	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
11/19/2024	BNA_F	<u>BF140462.D</u>
Compound Name	Response	Retention Time
DDT	652325	13.563
DDD	19967	13.257
DDE	1626	12.921
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
21593	673918	3.20

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111924\
Data File : BF140462.D
Acq On : 19 Nov 2024 09:32
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 19 11:21:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 14:40:06 2024
Response via : Initial Calibration

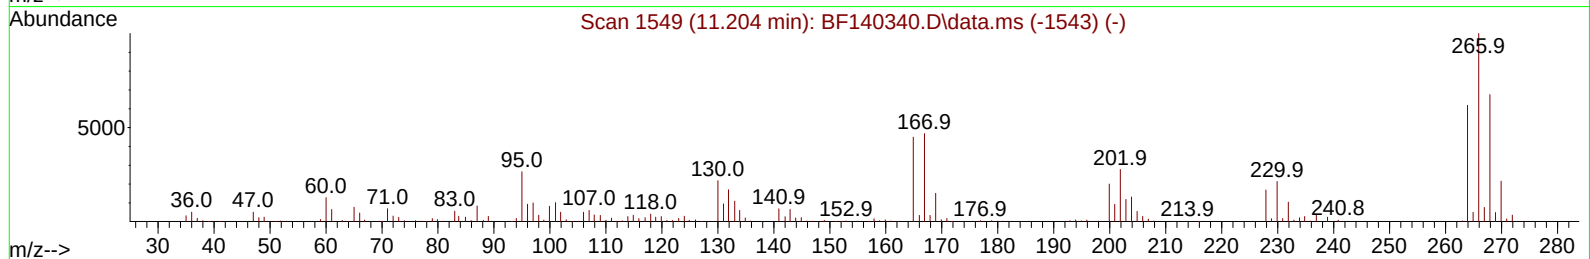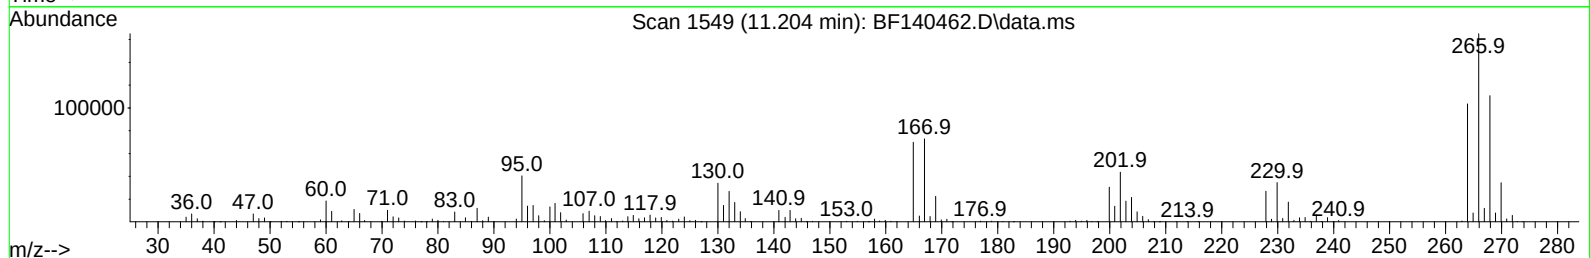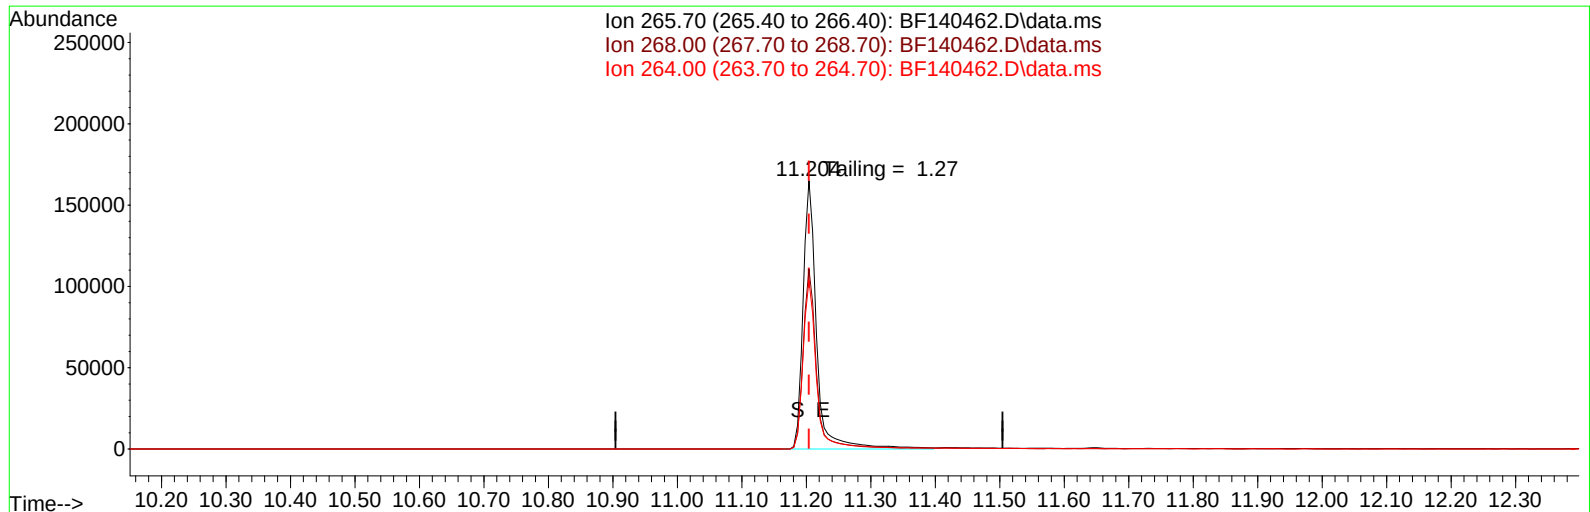

TIC: BF140462.D\data.ms

(70) Pentachlorophenol (C)

11.204min (-0.000) 47510.91 ng

response 242650

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.10	67.06
264.00	62.90	62.78
0.00	0.00	0.00

