

Data Path : Z:\HPCHEM1\BNA F\DATA\BF112014\
 Data File : BF075715.D
 Acq On : 20 Nov 2014 17:59
 Operator : TP / JJ
 Sample : F4836-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Nov 21 01:10:41 2014
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF111914.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 19 18:09:59 2014
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.48	152	62248	20.00	ng	-0.01
21) Naphthalene-d8	9.05	136	264551	20.00	ng	-0.01
38) Acenaphthene-d10	11.23	164	123429	20.00	ng	-0.02
63) Phenanthrene-d10	13.08	188	211357	20.00	ng	-0.01
75) Chrysene-d12	16.37	240	206219	20.00	ng	-0.02
86) Perylene-d12	18.11	264	210595	20.00	ng	-0.06
System Monitoring Compounds						
5) 2-Fluorophenol	5.76	112	252409	63.00	ng	-0.02
7) Phenol-d6	7.03	99	200164	41.08	ng	-0.01
23) Nitrobenzene-d5	8.16	82	341849	79.32	ng	-0.01
41) 2,4,6-Tribromophenol	12.21	330	121064	120.31	ng	-0.02
44) 2-Fluorobiphenyl	10.40	172	651818	82.67	ng	-0.01
78) Terphenyl-d14	15.07	244	484709	58.79	ng	-0.02


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF112014\
Data File : BF075715.D
Acq On : 20 Nov 2014 17:59
Operator : TP / JJ
Sample : F4836-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Nov 21 01:10:41 2014
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF111914.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 19 18:09:59 2014
Response via : Initial Calibration

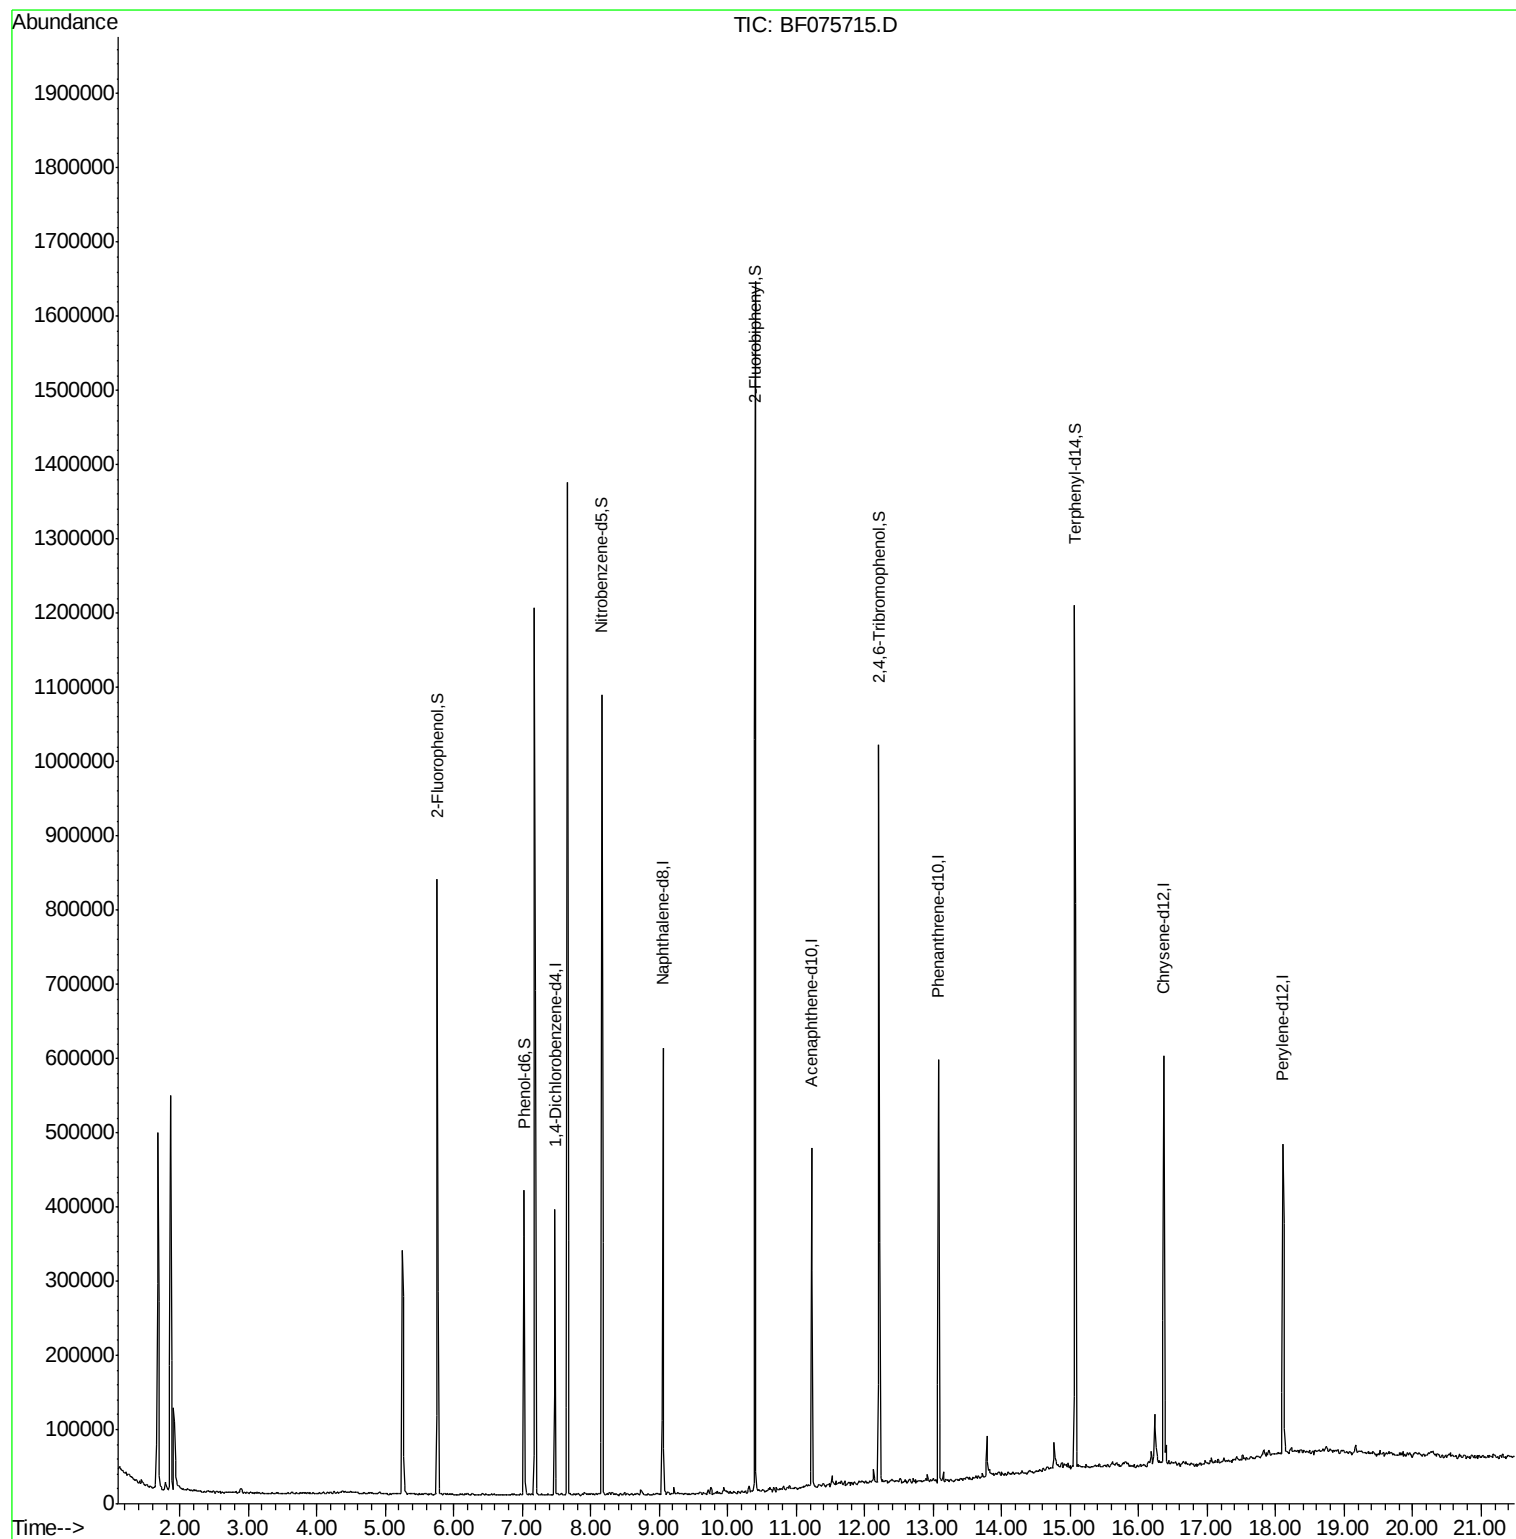


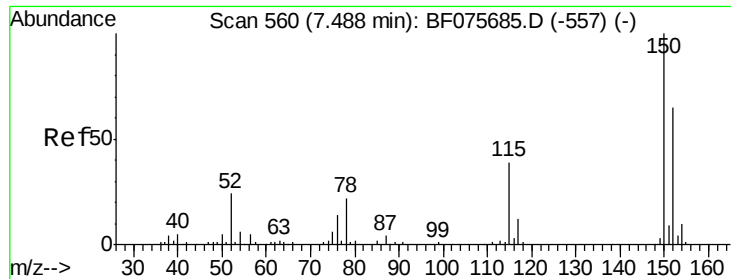




#1
 1,4-Dichlorobenzene-d4
 Concen: 20.00 ng
 RT: 7.48 min Scan# 559
 Delta R.T. -0.01 min
 Lab File: BF075715.D
 Acq: 20 Nov 2014 17:59

Instrument :
 BNA_F
 ClientSampled :

Tot Ion:152 Resp: 62248
 Ion Ratio Lower Upper
 152 100
 150 160.2 127.2 190.8
 115 55.7 57.1 85.7#

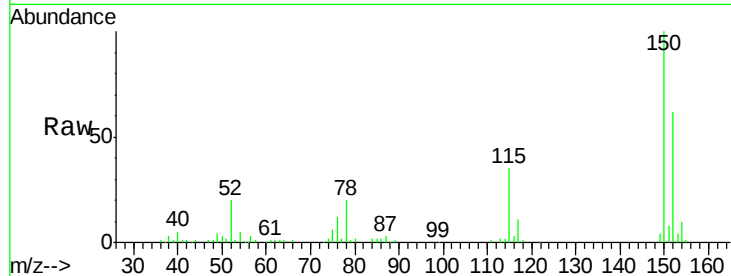


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

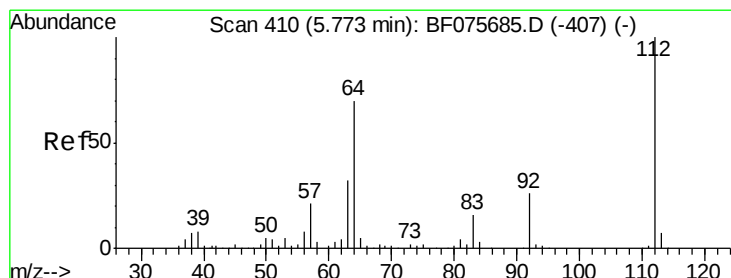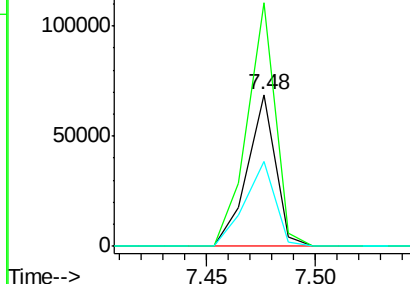
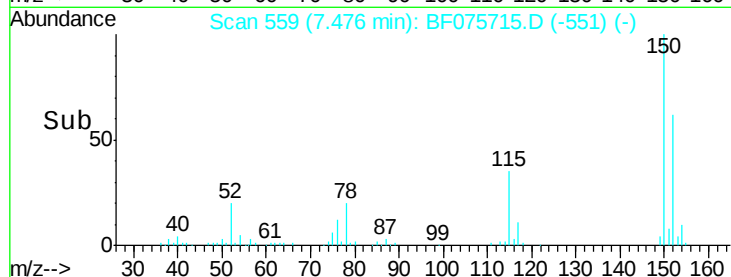



#5
 2-Fluorophenol
 Concen: 63.00 ng
 RT: 5.76 min Scan# 409
 Delta R.T. -0.02 min
 Lab File: BF075715.D
 Acq: 20 Nov 2014 17:59

Tgt Ion:112 Resp: 252409
 Ion Ratio Lower Upper
 112 100
 64 63.1 45.8 68.6
 63 29.5 22.7 34.1

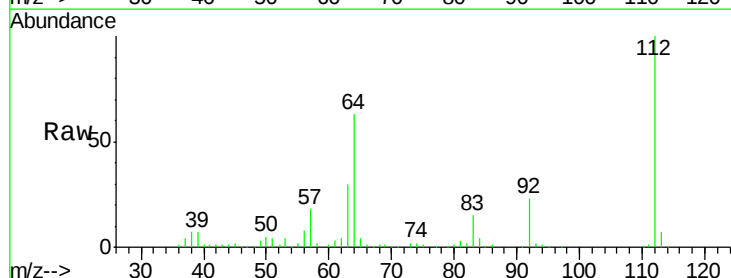

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF0
 Ion 63.00 (62.70 to 63.70): BF0

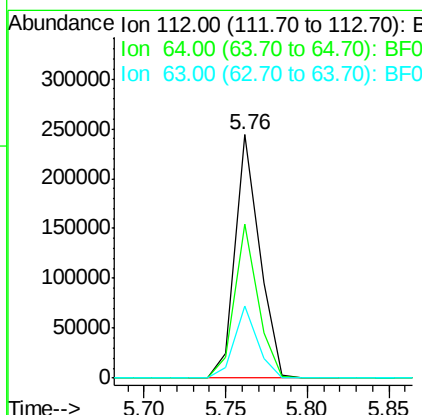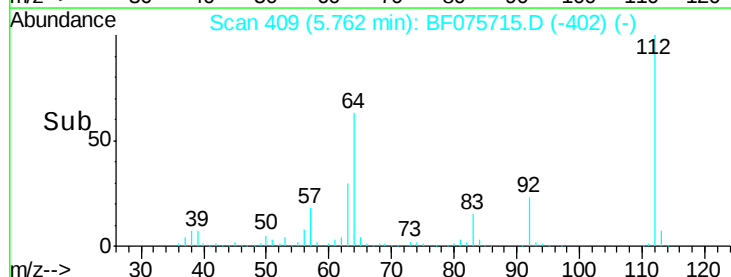

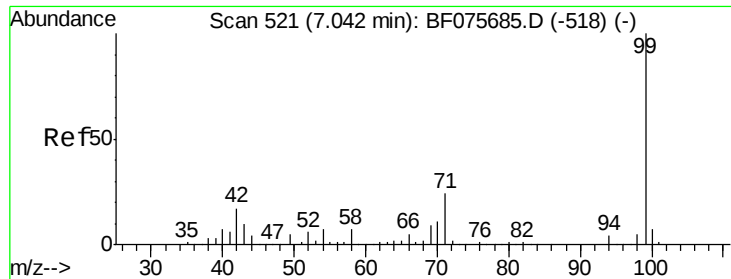

#7

Phenol-d6

Concen: 41.08 ng

RT: 7.03 min Scan# 520

Delta R.T. -0.01 min

Lab File: BF075715.D

Acq: 20 Nov 2014 17:59

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 99 Resp: 200164

Ion Ratio Lower Upper

99 100

42 15.6 19.8 29.6#




71 23.4 25.5 38.3#

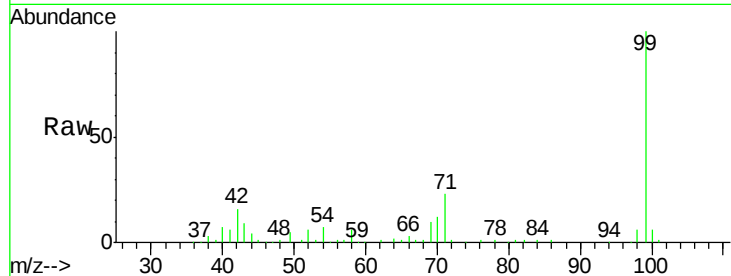

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

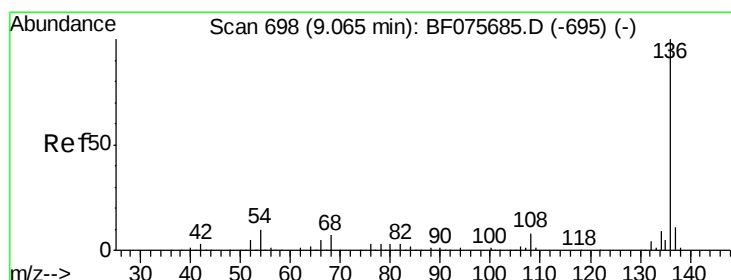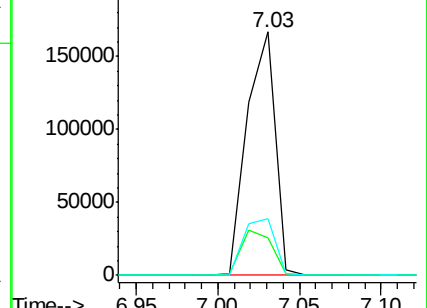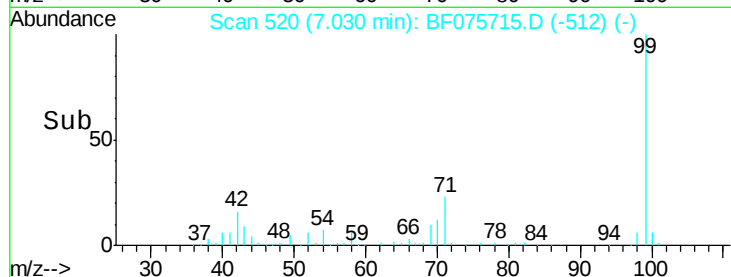

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 9.05 min Scan# 697

Delta R.T. -0.01 min

Lab File: BF075715.D

Acq: 20 Nov 2014 17:59

Tgt Ion: 136 Resp: 264551


Ion Ratio Lower Upper

136 100

137 10.9 8.2 12.4

54 8.8 6.2 9.4

68 6.5 3.4 5.2#


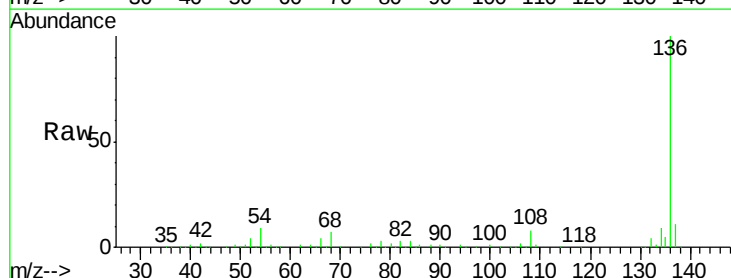



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

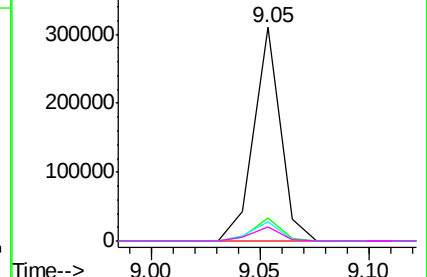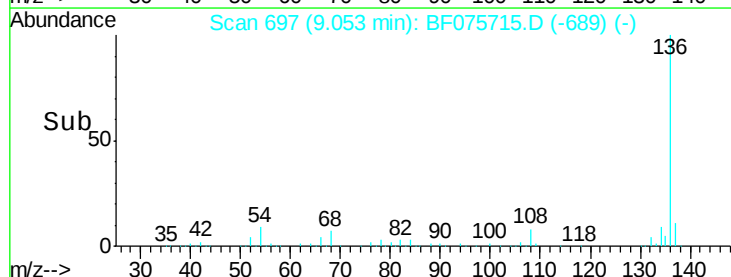


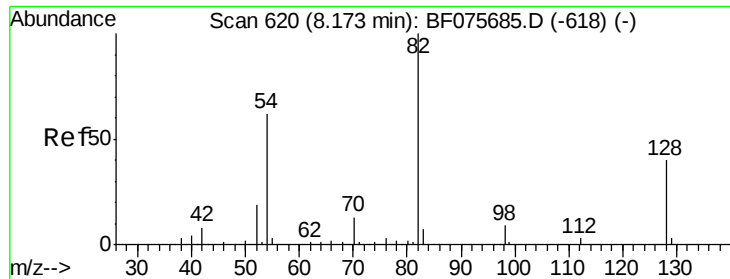




#23
Nitrobenzene-d5
Concen: 79.32 ng
RT: 8.16 min Scan# 619
Delta R.T. -0.01 min
Lab File: BF075715.D
Acq: 20 Nov 2014 17:59

Instrument :
BNA_F
ClientSampled :

Tot Ion: 82 Resp: 341849
Ion Ratio Lower Upper
82 100
128 41.6 37.8 56.6
54 61.5 49.8 74.8

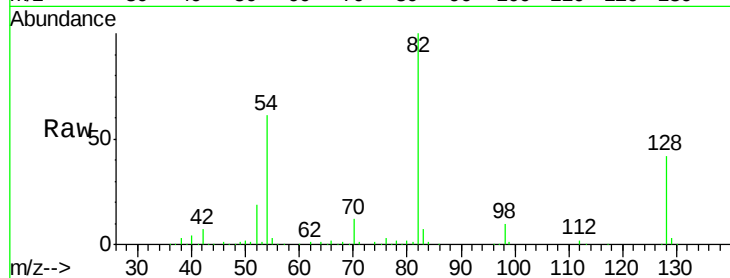


Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF0

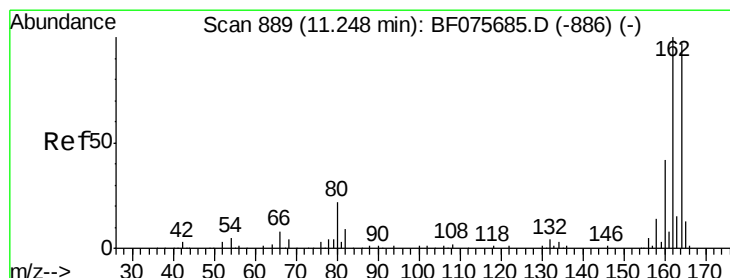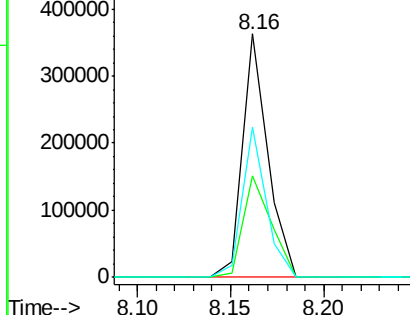
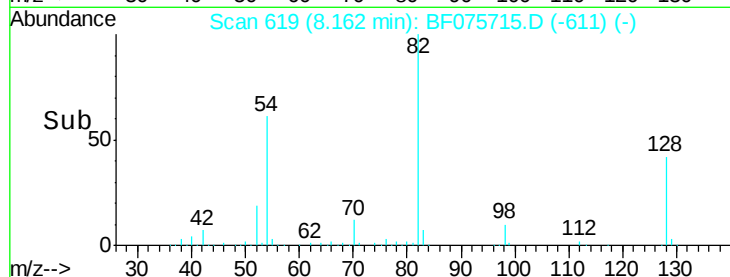



#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 11.23 min Scan# 887
Delta R.T. -0.02 min
Lab File: BF075715.D
Acq: 20 Nov 2014 17:59

Tgt Ion:164 Resp: 123429
Ion Ratio Lower Upper
164 100
162 104.6 79.1 118.7
160 43.9 34.6 51.8

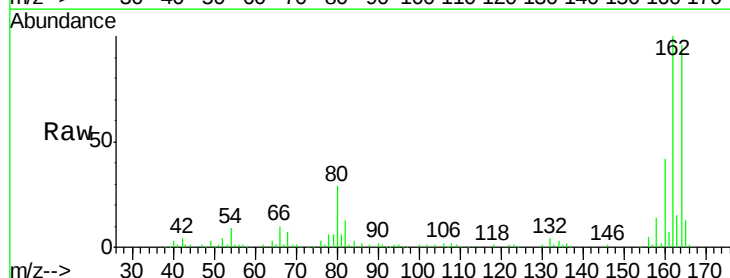

Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

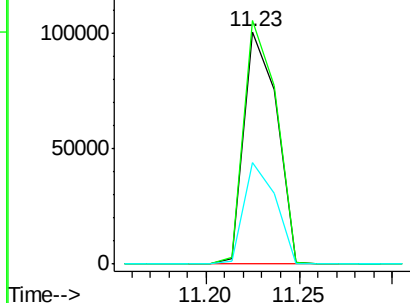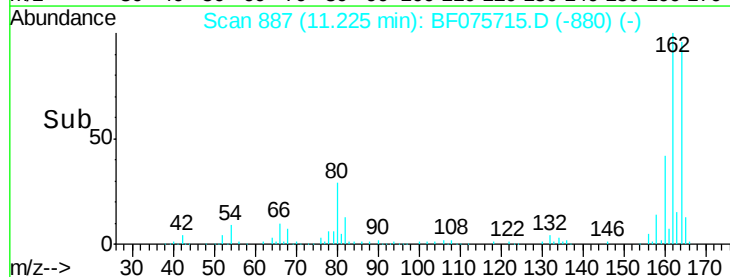


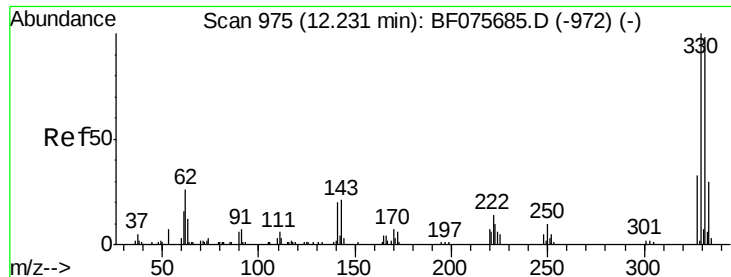




#41
 2,4,6-Tribromophenol
 Concen: 120.31 ng
 RT: 12.21 min Scan# 973
 Delta R.T. -0.02 min
 Lab File: BF075715.D
 Acq: 20 Nov 2014 17:59

Instrument :
 BNA_F
 ClientSampled :

Tot Ion	Ratio	Lower	Upper
330	100		
332	95.6	74.5	111.7
141	35.4	30.7	46.1

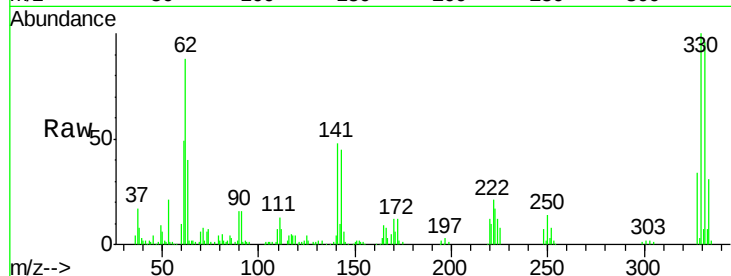


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

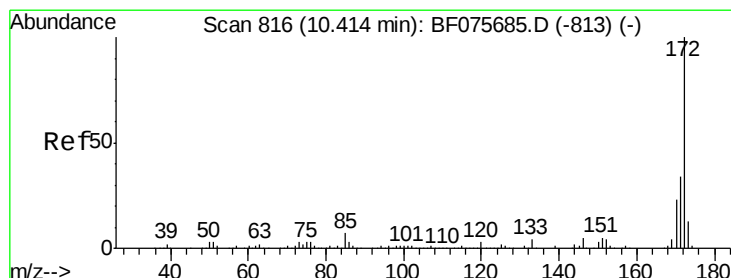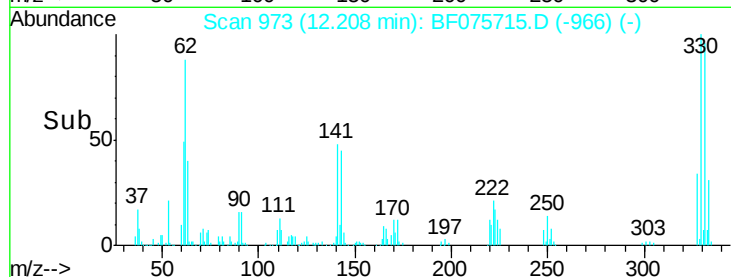
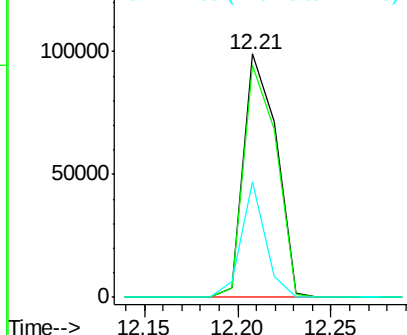



#44
 2-Fluorobiphenyl
 Concen: 82.67 ng
 RT: 10.40 min Scan# 815
 Delta R.T. -0.01 min
 Lab File: BF075715.D
 Acq: 20 Nov 2014 17:59

Tgt Ion	Ratio	Lower	Upper
172	100		
171	33.8	27.3	40.9
170	22.8	18.4	27.6

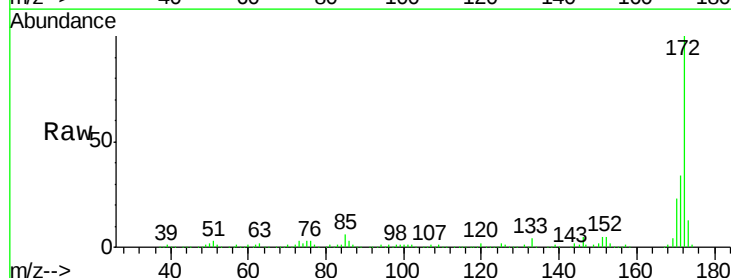

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

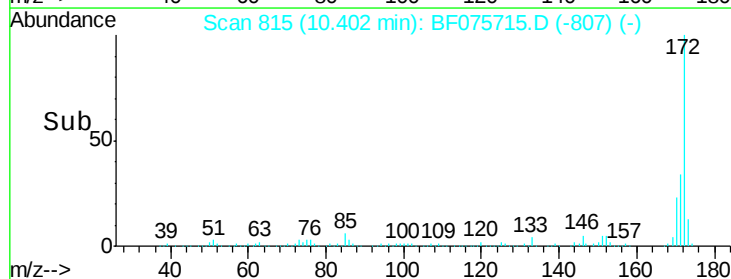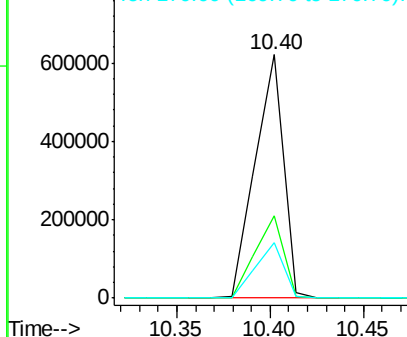


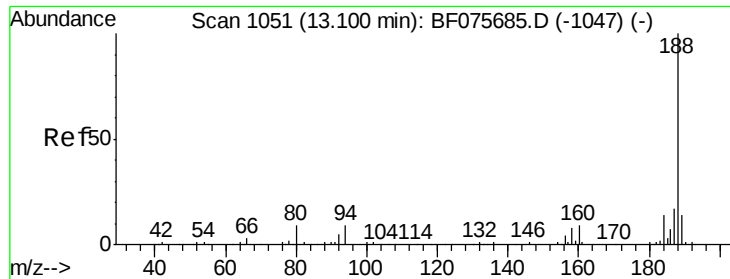




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 13.08 min Scan# 1049
Delta R.T. -0.01 min
Lab File: BF075715.D
Acq: 20 Nov 2014 17:59

Instrument :
BNA_F
ClientSampleId :

Tot Ion:188 Resp: 211357
Ion Ratio Lower Upper
188 100
94 11.5 7.8 11.6
80 12.2 8.0 12.0#

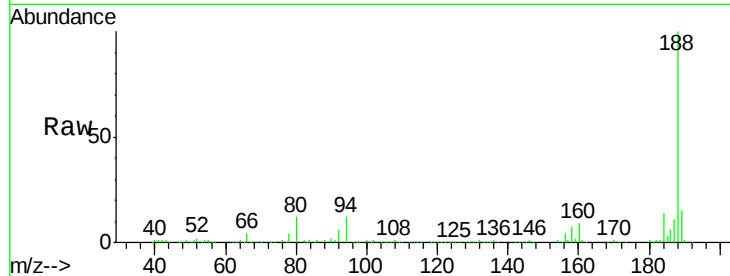


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

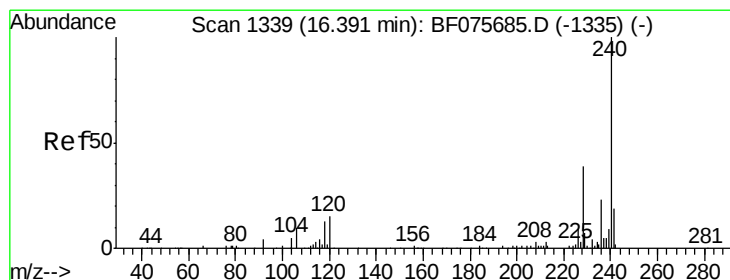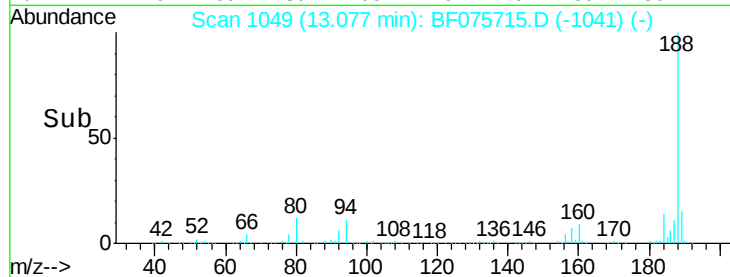
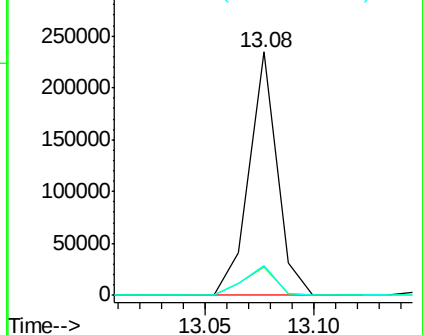



#75
Chrysene-d12
Concen: 20.00 ng
RT: 16.37 min Scan# 1337
Delta R.T. -0.02 min
Lab File: BF075715.D
Acq: 20 Nov 2014 17:59

Tgt Ion:240 Resp: 206219
Ion Ratio Lower Upper
240 100
120 14.6 9.6 14.4#
236 22.4 18.9 28.3

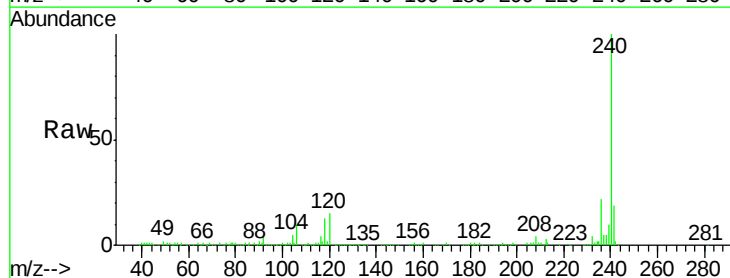

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

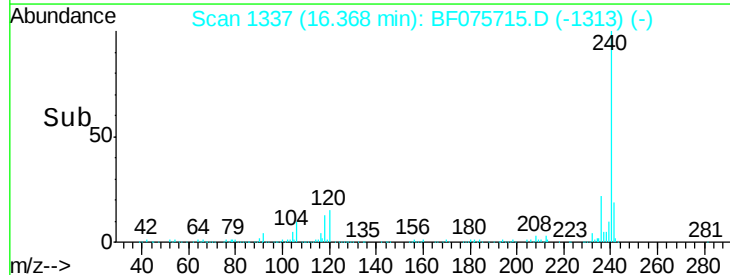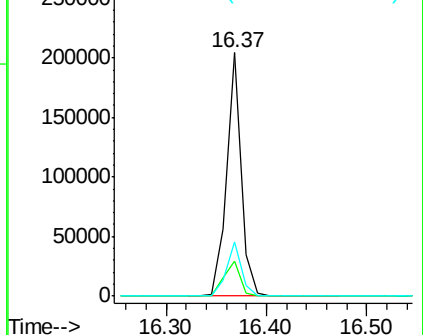


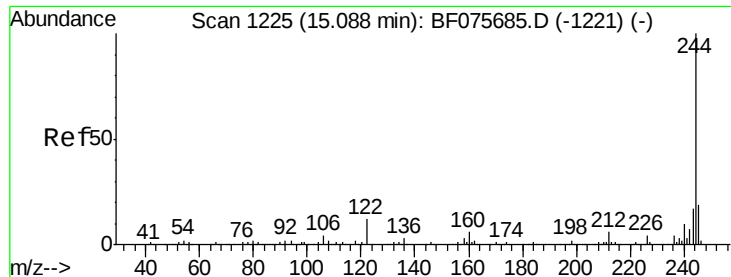




#78
 Terphenyl-d14
 Concen: 58.79 ng
 RT: 15.07 min Scan# 1223
 Delta R.T. -0.02 min
 Lab File: BF075715.D
 Acq: 20 Nov 2014 17:59

Instrument :
 BNA_F
 ClientSampled :

Tot Ion:244 Resp: 484709
 Ion Ratio Lower Upper
 244 100
 212 6.2 5.5 8.3
 122 18.4 9.7 14.5#

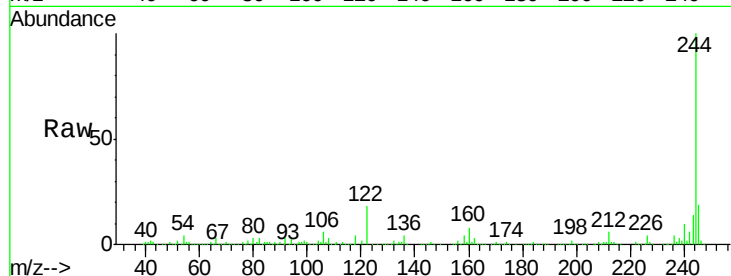


Abundance Ion 244.00 (243.70 to 244.70): E
 Ion 212.00 (211.70 to 212.70): E
 Ion 122.00 (121.70 to 122.70): E

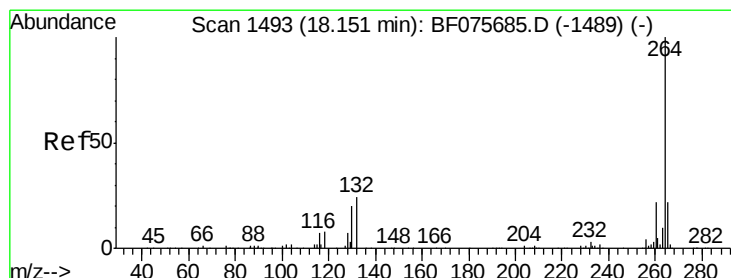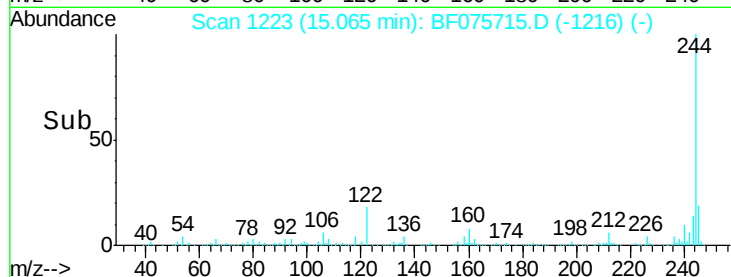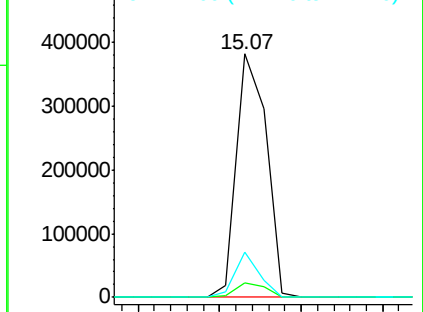

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 18.11 min Scan# 1489
 Delta R.T. -0.06 min
 Lab File: BF075715.D
 Acq: 20 Nov 2014 17:59

Tgt Ion:264 Resp: 210595
 Ion Ratio Lower Upper
 264 100
 260 23.4 17.9 26.9
 265 21.3 16.3 24.5

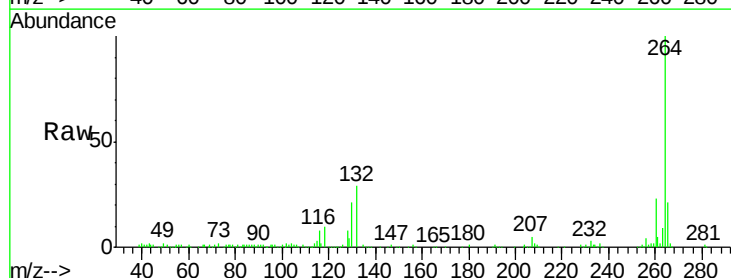

Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

