

Data Path : Z:\HPCHEM1\BNA F\DATA\BF112015\
 Data File : BF083088.D
 Acq On : 20 Nov 2015 18:44
 Operator : UM/IZ
 Sample : G4426-08DL 5X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Nov 20 22:34:53 2015
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF111915.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 20 01:33:39 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.70	152	167561	20.00	ng	0.00
21) Naphthalene-d8	7.98	136	615941	20.00	ng	-0.01
38) Acenaphthene-d10	9.74	164	311795	20.00	ng	0.00
63) Phenanthrene-d10	11.22	188	459510	20.00	ng	0.00
75) Chrysene-d12	13.86	240	400989	20.00	ng	0.00
86) Perylene-d12	15.25	264	347360	20.00	ng	0.01

System Monitoring Compounds						
5) 2-Fluorophenol	5.29	112	283908	26.32	ng	0.00
7) Phenol-d6	6.35	99	375762	26.45	ng	0.00
23) Nitrobenzene-d5	7.26	82	202662	15.06	ng	-0.01
41) 2,4,6-Tribromophenol	10.53	330	41378	12.50	ng	0.00
44) 2-Fluorobiphenyl	9.07	172	351904	15.20	ng	-0.01
78) Terphenyl-d14	12.81	244	206897	12.18	ng	0.00


Target Compounds				Qvalue		
9) Benzaldehyde	6.34	77	759	Below Cal	#	6
19) n-Nitroso-di-n-propylamine	7.26	70	27135	2.61 ng	#	70
25) Isophorone	7.26	82	147698	5.82 ng	#	69
31) Naphthalene	8.01	128	125638	3.91 ng		99
49) Dimethylphthalate	9.47	163	107239	4.18 ng		96
51) Acenaphthene	9.78	154	78359	3.61 ng		96
54) Dibenzofuran	9.95	168	87186	3.00 ng		91
55) 4-Nitrophenol	9.95	139	32162	7.43 ng	#	9
57) Fluorene	10.28	166	99099	4.23 ng		98
70) Phenanthrene	11.24	178	1042892	37.62 ng		99
71) Anthracene	11.30	178	271078	9.71 ng		97
72) Carbazole	11.45	167	116859	4.79 ng		100
74) Fluoranthene	12.43	202	1019249	35.28 ng		99
77) Pyrene	12.66	202	930217	32.95 ng		99
80) Benzo(a)anthracene	13.85	228	589030	23.11 ng		100
82) Chrysene	13.88	228	352228	15.07 ng		96
85) Indeno(1,2,3-cd)pyrene	16.56	276	157281	8.27 ng		95
87) Benzo(b)fluoranthene	14.88	252	617323	25.42 ng		99
88) Benzo(k)fluoranthene	14.88	252	617323	33.36 ng	#	97
89) Benzo(a)pyrene	15.15	252	210543	10.80 ng		94
91) Benzo(g,h,i)perylene	16.95	276	131961	7.98 ng	#	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF112015\
Data File : BF083088.D
Acq On : 20 Nov 2015 18:44
Operator : UM/IZ
Sample : G4426-08DL 5X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Nov 20 22:34:53 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF111915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 20 01:33:39 2015
Response via : Initial Calibration

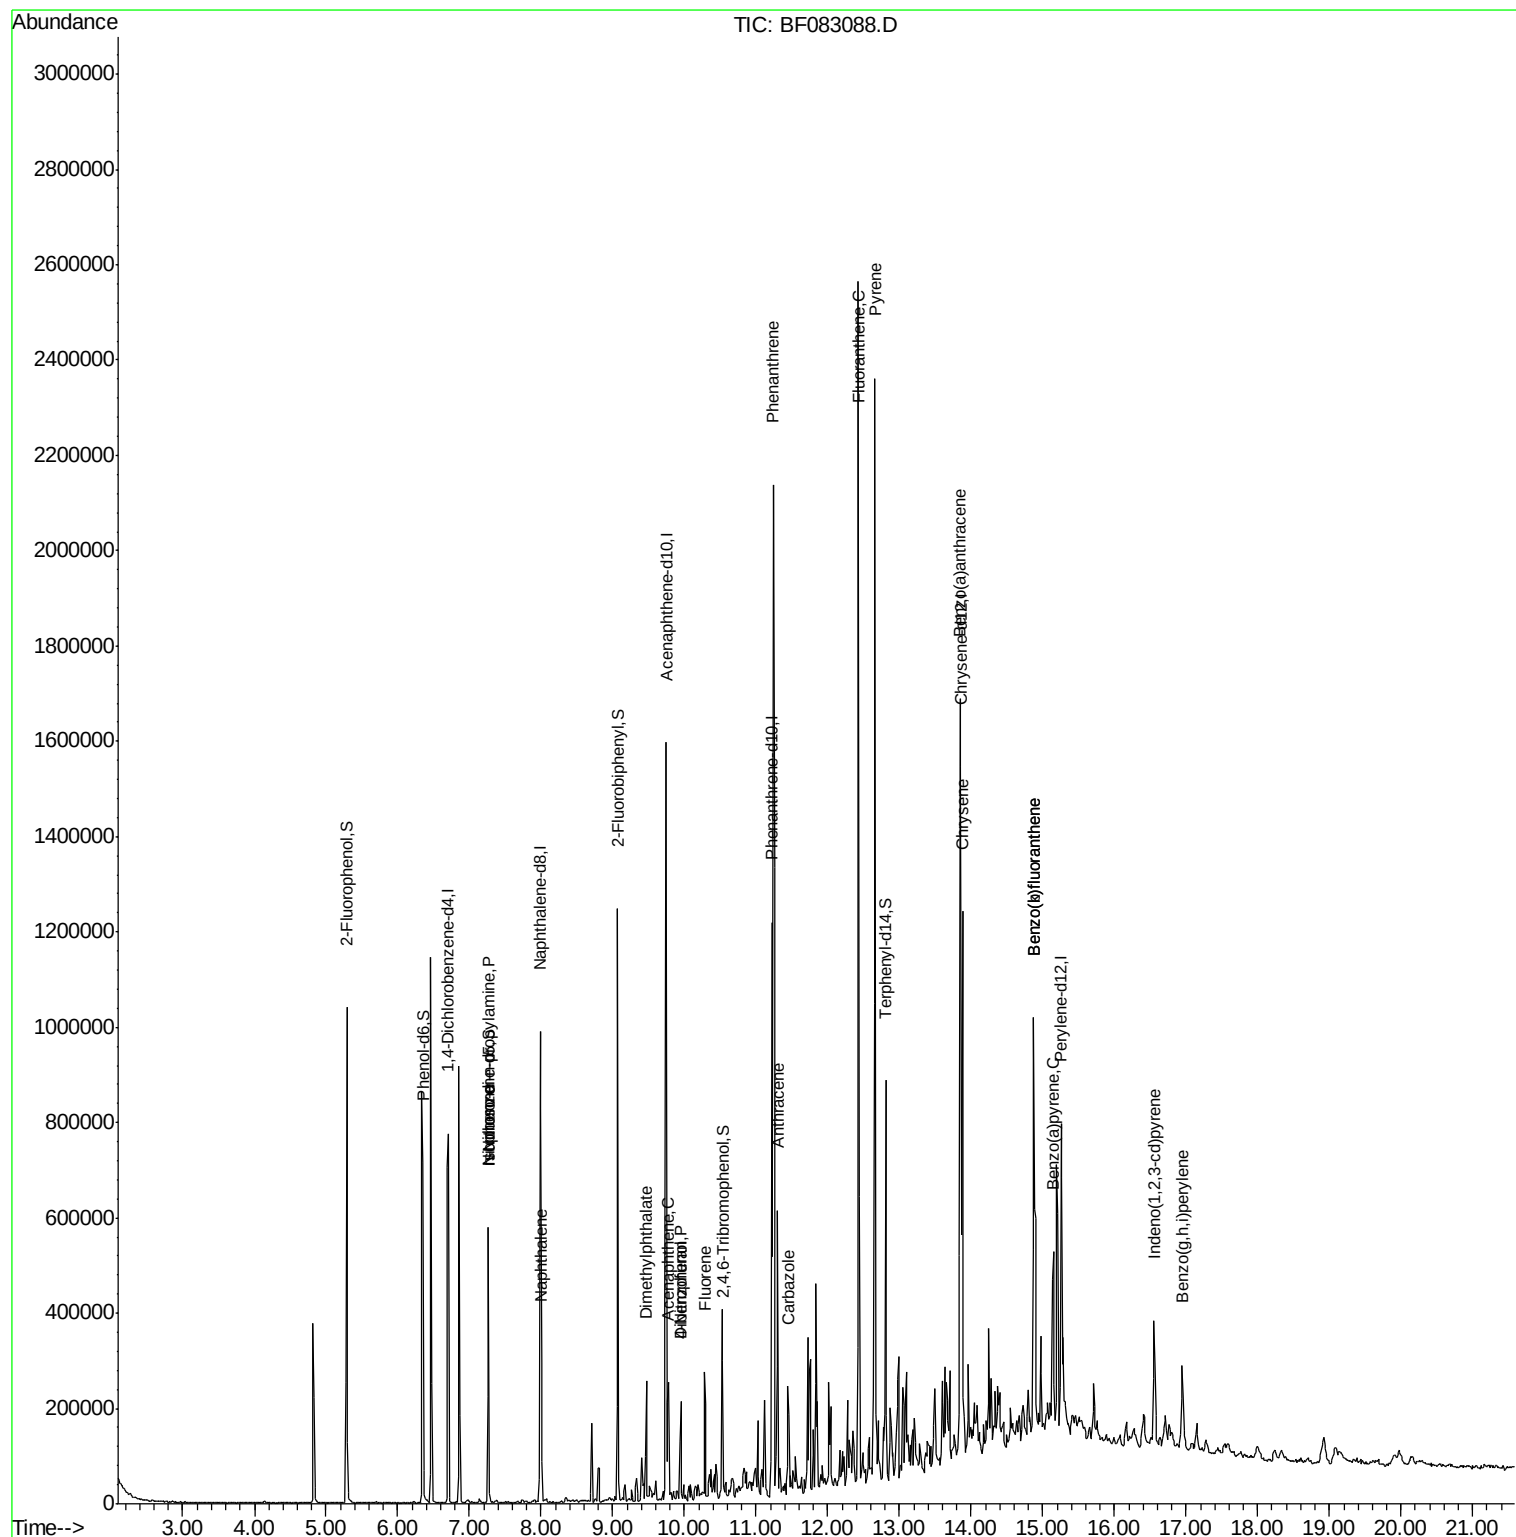

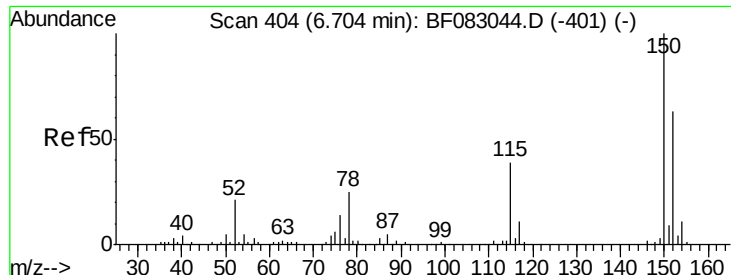


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.70 min Scan# 404
Delta R.T. -0.00 min
Lab File: BF083088.D
Acq: 20 Nov 2015 18:44

Instrument :
BNA_F
ClientSampleId :

Tot Ion:152 Resp: 167561
Ion Ratio Lower Upper
152 100
150 154.0 126.4 189.6
115 55.7 49.0 73.6

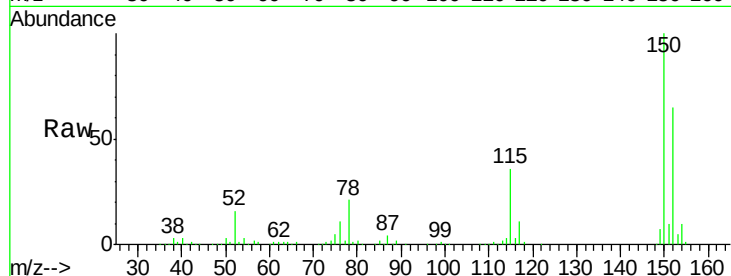


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

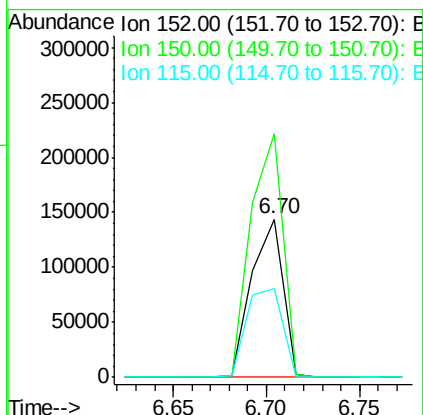



#5


2-Fluorophenol
Concen: 26.32 ng
RT: 5.29 min Scan# 280
Delta R.T. -0.00 min
Lab File: BF083088.D
Acq: 20 Nov 2015 18:44

Tgt Ion:112 Resp: 283908
Ion Ratio Lower Upper
112 100
64 58.6 54.8 82.2
63 29.7 29.0 43.4



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

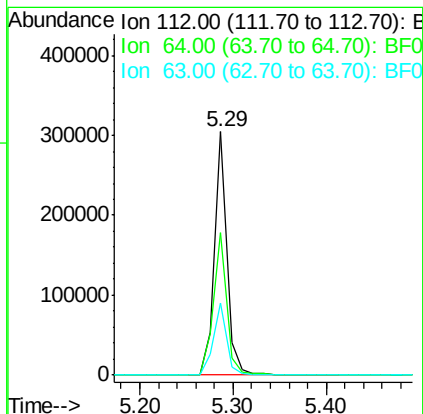



#7

Phenol-d6

Concen: 26.45 ng

RT: 6.35 min Scan# 373

Delta R.T. -0.00 min

Lab File: BF083088.D

Acq: 20 Nov 2015 18:44


Instrument :

BNA_F

ClientSampleId :

Tot Ion: 99 Resp: 375762




Ion	Ratio	Lower	Upper
99	100		
42	14.1	16.6	25.0#
71	31.1	29.2	43.8



Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

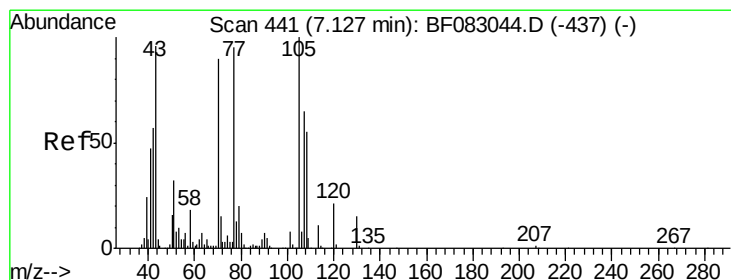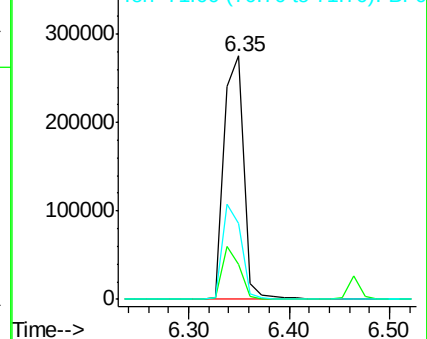

#19

n-Nitroso-di-n-propylamine

Concen: 2.61 ng

RT: 7.26 min Scan# 453


Delta R.T. 0.14 min

Lab File: BF083088.D

Acq: 20 Nov 2015 18:44

Tgt Ion: 70 Resp: 27135

Ion	Ratio	Lower	Upper
70	100		
42	39.5	50.2	75.2#
101	0.0	6.8	10.2#
130	2.1	12.9	19.3#


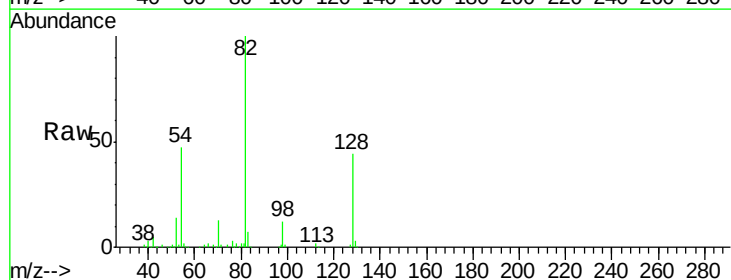



Abundance Ion 70.00 (69.70 to 70.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 101.00 (100.70 to 101.70): BF0

Ion 130.00 (129.70 to 130.70): BF0

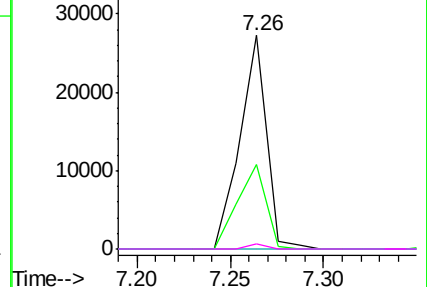



#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.98 min Scan# 516

Delta R.T. -0.01 min

Lab File: BF083088.D

Acq: 20 Nov 2015 18:44

Instrument :

BNA_F

ClientSampleId :

Tot Ion:136 Resp: 615941


Ion Ratio Lower Upper

136 100

137 10.7 8.6 12.8

54 11.3 6.2 9.2#

68 7.7 4.2 6.2#



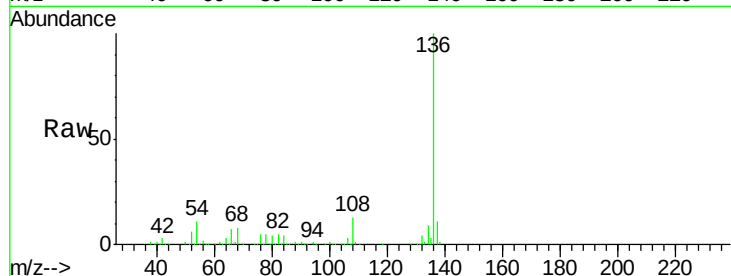


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

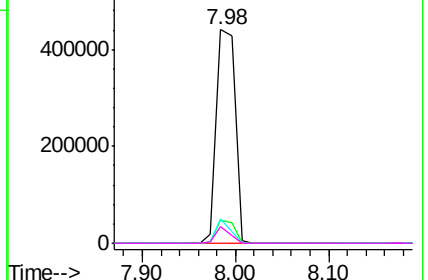

#23

Nitrobenzene-d5

Concen: 15.06 ng

RT: 7.26 min Scan# 453

Delta R.T. -0.01 min

Lab File: BF083088.D

Acq: 20 Nov 2015 18:44


Tgt Ion: 82 Resp: 202662

Ion Ratio Lower Upper

82 100

128 43.8 33.1 49.7



54 47.2 39.8 59.6




Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF0

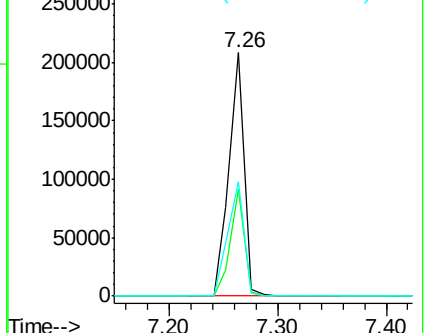



#25

Isophorone

Concen: 5.82 ng

RT: 7.26 min Scan# 453

Delta R.T. -0.27 min

Lab File: BF083088.D

Acq: 20 Nov 2015 18:44

Instrument :

BNA_F

ClientSampleId :





Tot Ion: 82 Resp: 147698

Ion Ratio Lower Upper

82 100

95 0.0 5.7 8.5#

138 0.0 12.2 18.4#

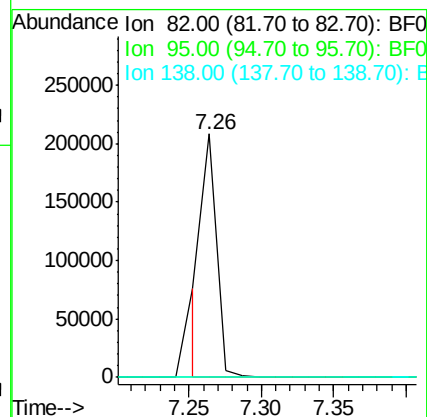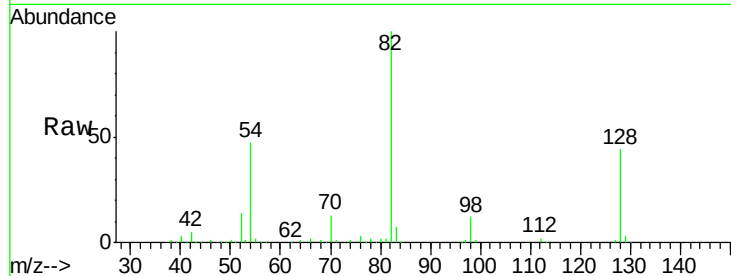

#31

Naphthalene

Concen: 3.91 ng

RT: 8.01 min Scan# 518

Delta R.T. -0.01 min

Lab File: BF083088.D

Acq: 20 Nov 2015 18:44




Tgt Ion: 128 Resp: 125638


Ion Ratio Lower Upper

128 100

129 11.8 9.0 13.4

127 13.4 10.9 16.3

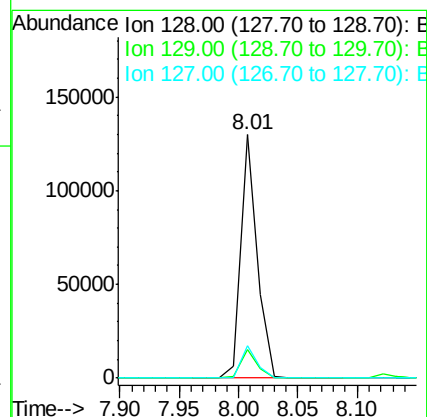



#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.74 min Scan# 670

Delta R.T. -0.00 min

Lab File: BF083088.D

Acq: 20 Nov 2015 18:44

Instrument :

BNA_F

ClientSampleId :


Tot Ion:164 Resp: 311795

Ion Ratio Lower Upper

164 100

162 100.4 80.5 120.7




160 44.3 35.0 52.4



Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

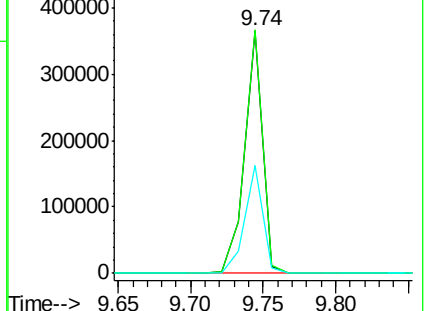

#41

2,4,6-Tribromophenol

Concen: 12.50 ng

RT: 10.53 min Scan# 739

Delta R.T. -0.00 min

Lab File: BF083088.D

Acq: 20 Nov 2015 18:44


Tgt Ion:330 Resp: 41378

Ion Ratio Lower Upper

330 100

332 102.2 77.6 116.4



141 43.7 34.6 52.0




Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

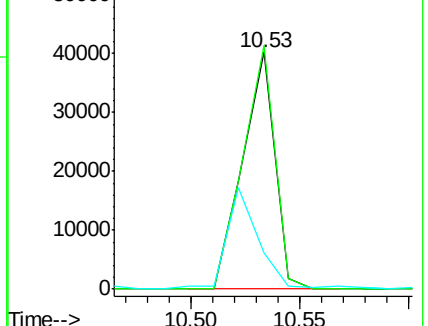


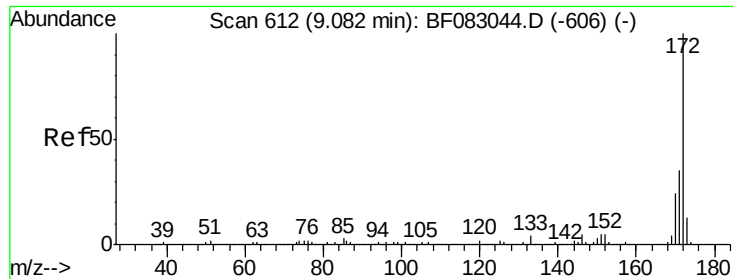




#44
2-Fluorobiphenyl
Concen: 15.20 ng
RT: 9.07 min Scan# 611
Delta R.T. -0.01 min
Lab File: BF083088.D
Acq: 20 Nov 2015 18:44

Instrument :
BNA_F
ClientSampled :

Tot Ion:172 Resp: 351904
Ion Ratio Lower Upper
172 100
171 34.4 28.2 42.4
170 23.7 19.4 29.0

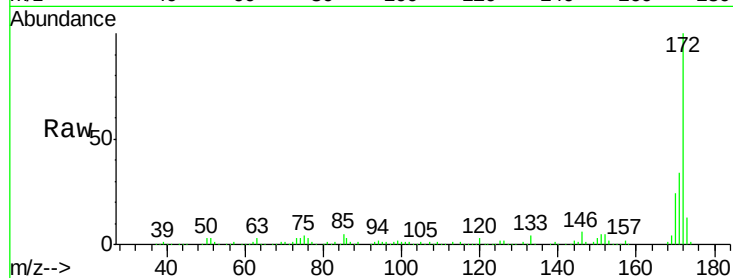


Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

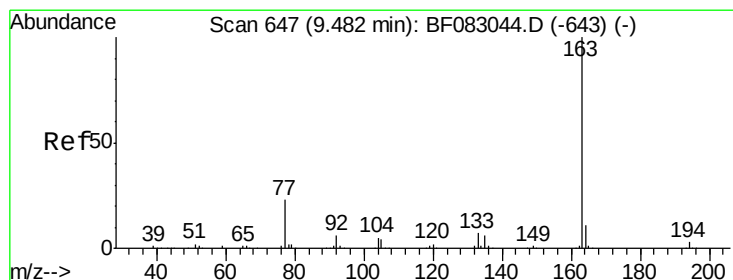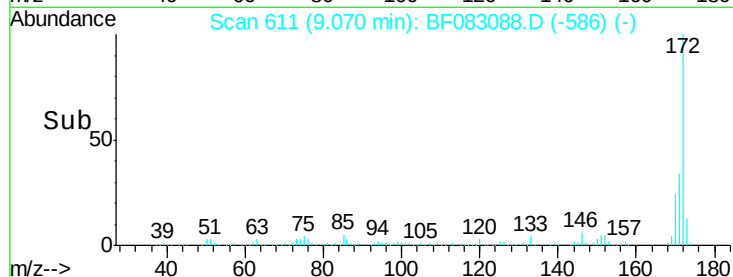
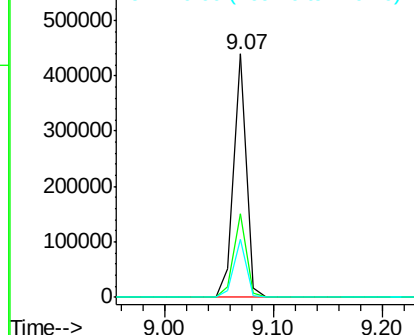



#49
Dimethylphthalate
Concen: 4.18 ng
RT: 9.47 min Scan# 646
Delta R.T. -0.01 min
Lab File: BF083088.D
Acq: 20 Nov 2015 18:44

Tgt Ion:163 Resp: 107239
Ion Ratio Lower Upper
163 100
194 4.0 2.7 4.1
164 9.1 8.5 12.7

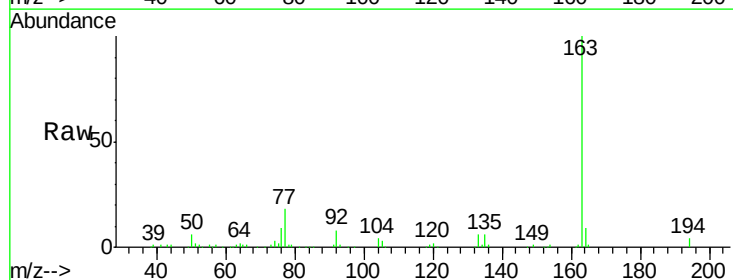

Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

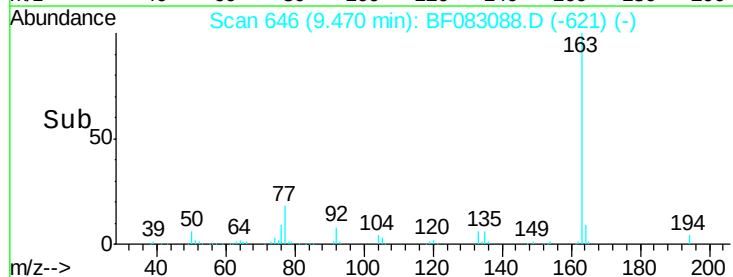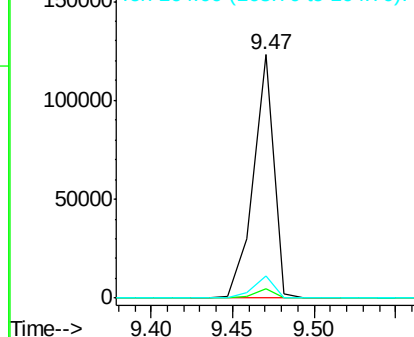



#51

Acenaphthene

Concen: 3.61 ng

RT: 9.78 min Scan# 673

Delta R.T. -0.00 min

Lab File: BF083088.D

Acq: 20 Nov 2015 18:44

Instrument :

BNA_F

ClientSampled :


Tot Ion:154 Resp: 78359

Ion Ratio Lower Upper

154 100

153 108.7 90.1 135.1




152 51.4 43.3 64.9

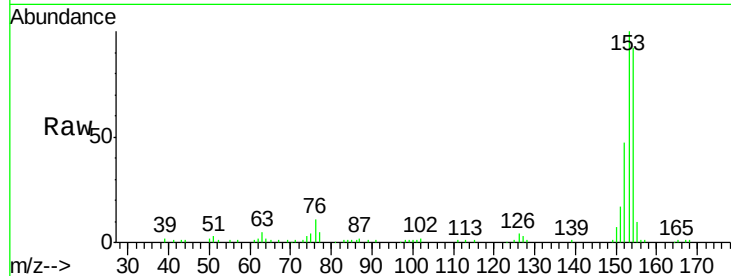

Abundance Ion 154.00 (153.70 to 154.70): E

Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

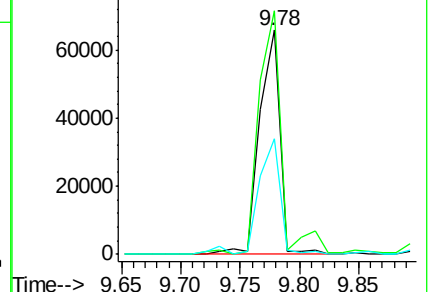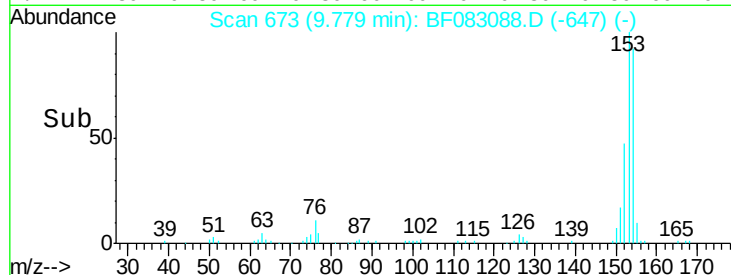

#54

Dibenzofuran

Concen: 3.00 ng

RT: 9.95 min Scan# 688

Delta R.T. -0.00 min

Lab File: BF083088.D

Acq: 20 Nov 2015 18:44


Tgt Ion:168 Resp: 87186

Ion Ratio Lower Upper

168 100

139 34.9 33.5 50.3



169 12.9 11.2 16.8




Abundance Ion 168.00 (167.70 to 168.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 169.00 (168.70 to 169.70): E

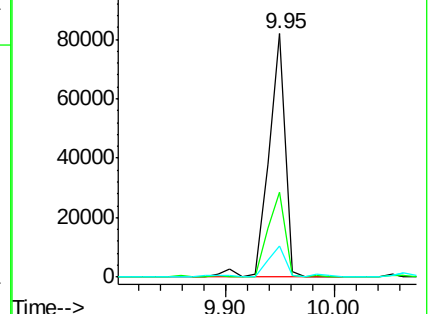







#55
4-Nitrophenol
Concen: 7.43 ng
RT: 9.95 min Scan# 688
Delta R.T. 0.07 min
Lab File: BF083088.D
Acq: 20 Nov 2015 18:44

Instrument :
BNA_F
ClientSampleId :

Tot Ion:139 Resp: 32162
Ion Ratio Lower Upper
139 100
109 1.5 54.6 94.6#
65 2.4 74.4 114.4#

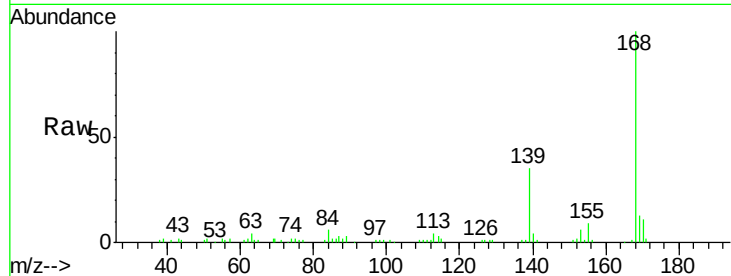


Abundance Ion 139.00 (138.70 to 139.70): E
Ion 109.00 (108.70 to 109.70): E
Ion 65.00 (64.70 to 65.70): BF0


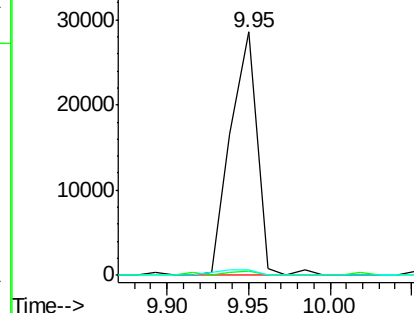



#57
Fluorene
Concen: 4.23 ng
RT: 10.28 min Scan# 717
Delta R.T. -0.01 min
Lab File: BF083088.D
Acq: 20 Nov 2015 18:44

Tgt Ion:166 Resp: 99099
Ion Ratio Lower Upper
166 100
165 98.0 77.1 115.7
167 15.4 11.0 16.4

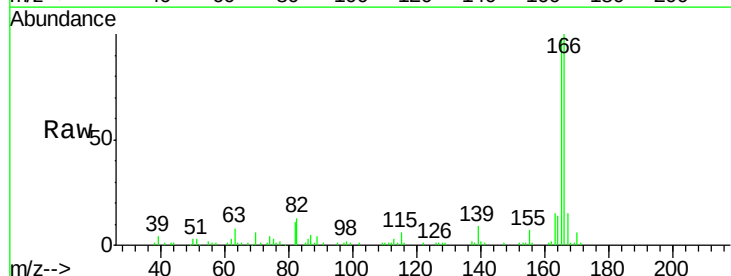

Abundance Ion 166.00 (165.70 to 166.70): E
Ion 165.00 (164.70 to 165.70): E
Ion 167.00 (166.70 to 167.70): E

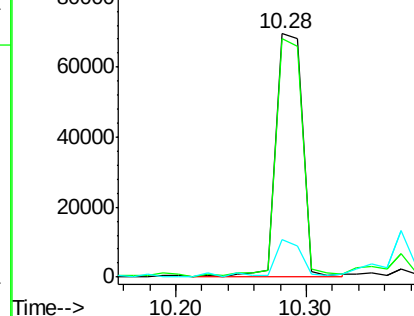







#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.22 min Scan# 799
Delta R.T. -0.00 min
Lab File: BF083088.D
Acq: 20 Nov 2015 18:44

Instrument :
BNA_F
ClientSampleId :

Tot Ion:188 Resp: 459510
Ion Ratio Lower Upper
188 100
94 10.8 9.0 13.4
80 11.9 10.2 15.4




Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0


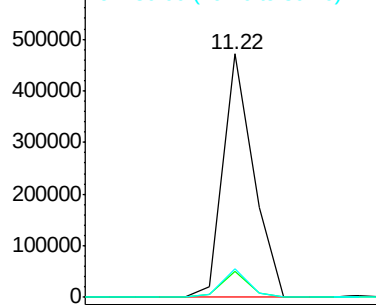



#70
Phenanthrene
Concen: 37.62 ng
RT: 11.24 min Scan# 801
Delta R.T. -0.01 min
Lab File: BF083088.D
Acq: 20 Nov 2015 18:44

Tgt Ion:178 Resp: 1042892
Ion Ratio Lower Upper
178 100
176 20.1 15.6 23.4
179 16.0 12.3 18.5



Abundance Ion 178.00 (177.70 to 178.70): E
Ion 176.00 (175.70 to 176.70): E
Ion 179.00 (178.70 to 179.70): E

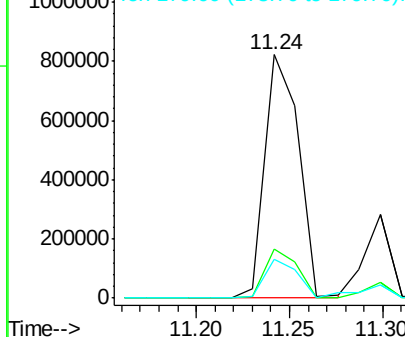



#71

Anthracene

Concen: 9.71 ng

RT: 11.30 min Scan# 806

Delta R.T. -0.00 min

Lab File: BF083088.D

Acq: 20 Nov 2015 18:44

Instrument :

BNA_F

ClientSampleId :


Tot Ion:178 Resp: 271078

Ion Ratio Lower Upper

178 100

176 18.1 15.8 23.6




179 15.1 13.1 19.7



Abundance Ion 178.00 (177.70 to 178.70): E

Ion 176.00 (175.70 to 176.70): E

Ion 179.00 (178.70 to 179.70): E

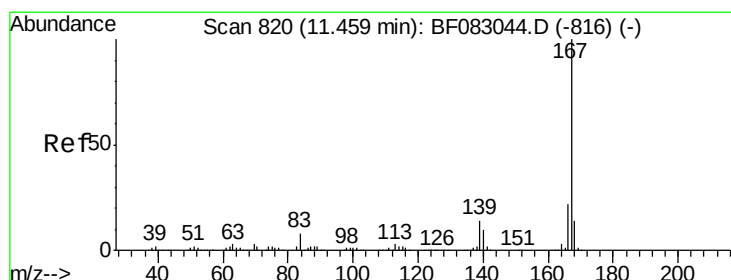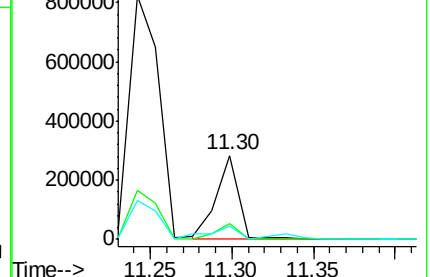

#72

Carbazole

Concen: 4.79 ng

RT: 11.45 min Scan# 819

Delta R.T. -0.01 min

Lab File: BF083088.D

Acq: 20 Nov 2015 18:44


Tgt Ion:167 Resp: 116859

Ion Ratio Lower Upper

167 100

166 21.8 17.8 26.6



139 13.7 11.0 16.4




Abundance Ion 167.00 (166.70 to 167.70): E

Ion 166.00 (165.70 to 166.70): E

Ion 139.00 (138.70 to 139.70): E

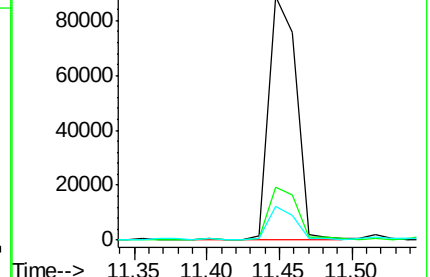



#74

Fluoranthene

Concen: 35.28 ng

RT: 12.43 min Scan# 905

Delta R.T. -0.00 min

Lab File: BF083088.D

Acq: 20 Nov 2015 18:44

Instrument :

BNA_F

ClientSampled :


Tot Ion:202 Resp: 1019249

Ion Ratio Lower Upper

202 100

101 11.4 0.0 31.1




203 18.1 0.0 38.4

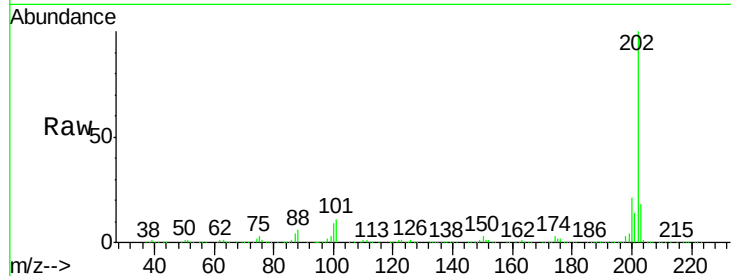

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E

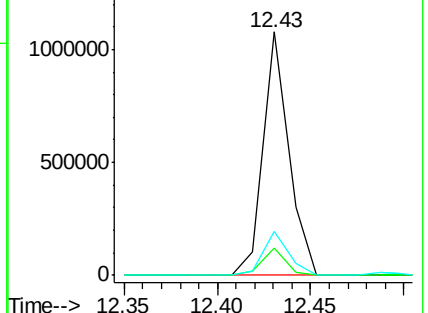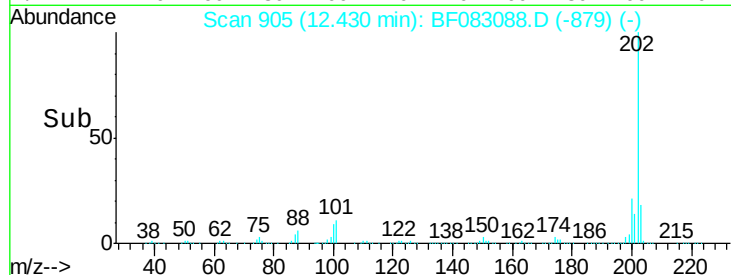

#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.86 min Scan# 1030

Delta R.T. -0.00 min

Lab File: BF083088.D

Acq: 20 Nov 2015 18:44


Tgt Ion:240 Resp: 400989

Ion Ratio Lower Upper

240 100

120 6.9 5.3 7.9



236 26.1 20.4 30.6




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

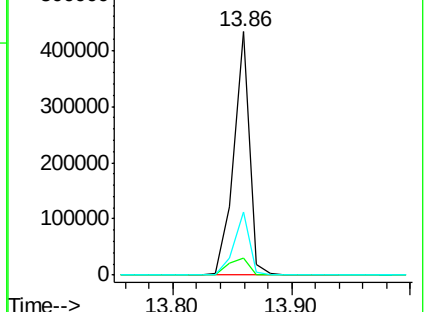

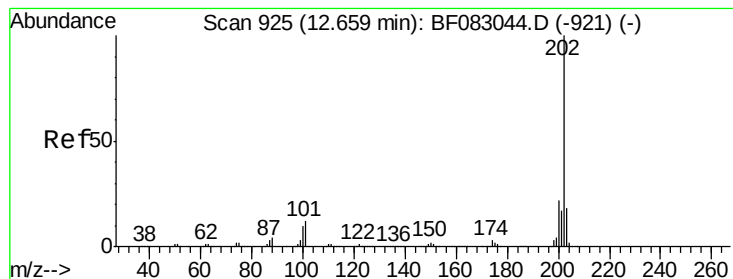

#77

Pvrene

Concen: 32.95 ng

RT: 12.66 min Scan# 925

Delta R.T. -0.00 min

Lab File: BF083088.D

Acq: 20 Nov 2015 18:44

Instrument :

BNA_F

ClientSampleId :


Tot Ion:202 Resp: 930217

Ion Ratio Lower Upper

202 100

200 21.3 17.6 26.4




203 18.3 14.6 22.0

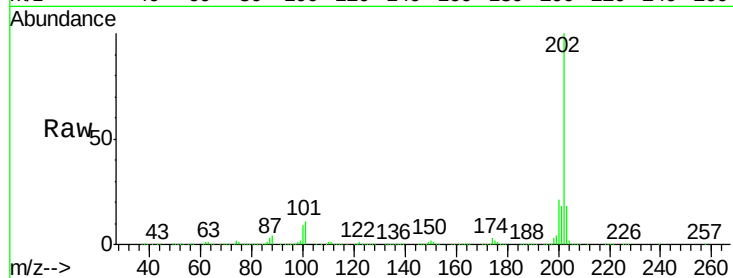

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E

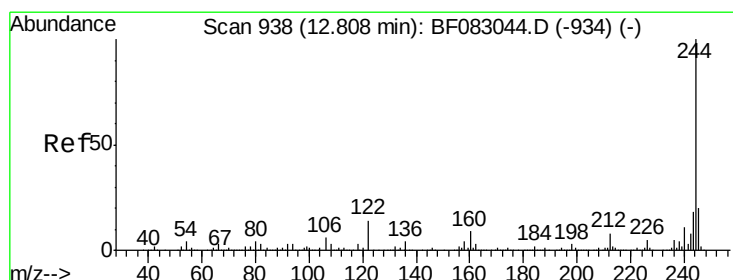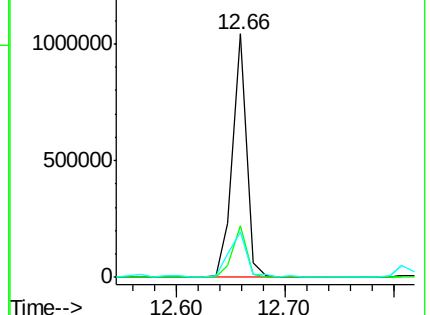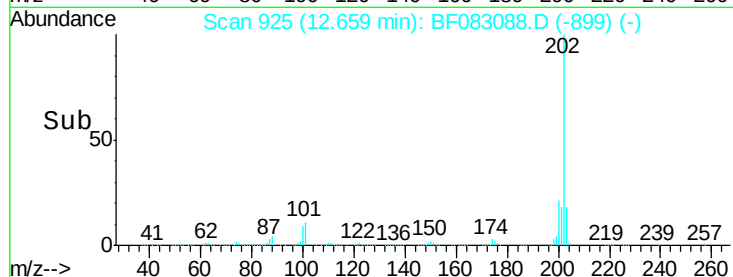

#78

Terphenyl-d14

Concen: 12.18 ng

RT: 12.81 min Scan# 938

Delta R.T. -0.00 min

Lab File: BF083088.D

Acq: 20 Nov 2015 18:44


Tgt Ion:244 Resp: 206897

Ion Ratio Lower Upper

244 100

212 6.8 6.4 9.6



122 9.2 10.9 16.3#

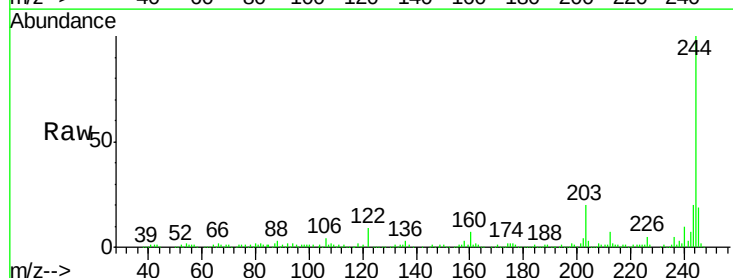


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

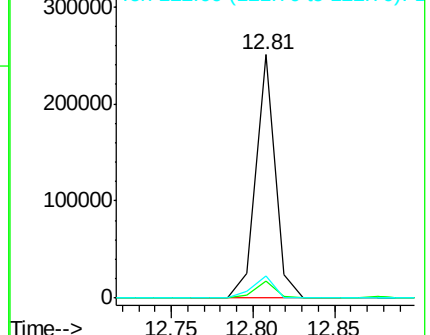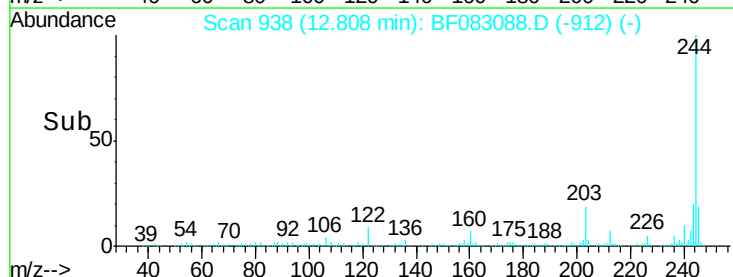


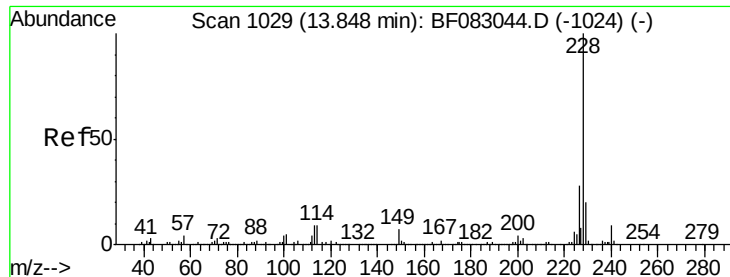




#80
Benzo(a)anthracene
Concen: 23.11 ng
RT: 13.85 min Scan# 1029
Delta R.T. -0.00 min
Lab File: BF083088.D
Acq: 20 Nov 2015 18:44

Instrument :
BNA_F
ClientSampleId :

Tot Ion:228 Resp: 589030
Ion Ratio Lower Upper
228 100
226 28.0 22.6 34.0
229 20.3 16.1 24.1

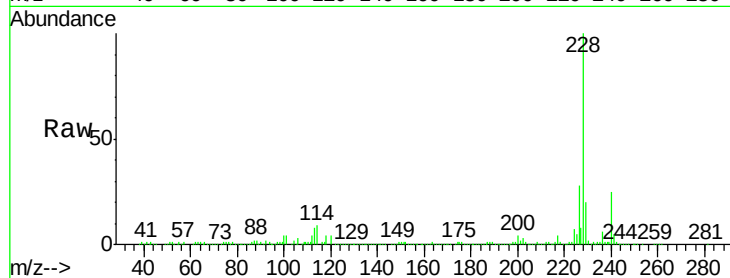


Abundance Ion 228.00 (227.70 to 228.70): E
Ion 226.00 (225.70 to 226.70): E
Ion 229.00 (228.70 to 229.70): E

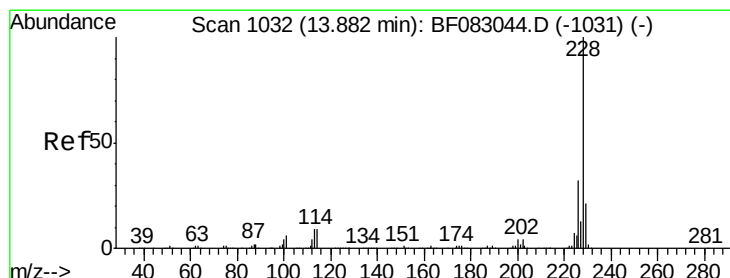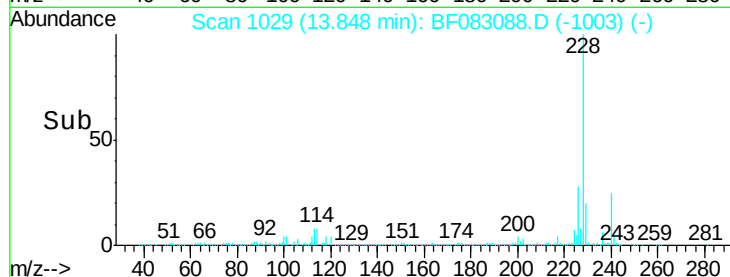
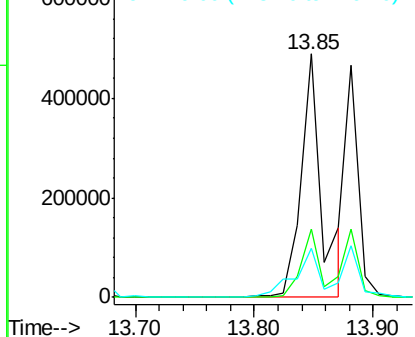



#82
Chrysene
Concen: 15.07 ng
RT: 13.88 min Scan# 1032
Delta R.T. -0.00 min
Lab File: BF083088.D
Acq: 20 Nov 2015 18:44

Tgt Ion:228 Resp: 352228
Ion Ratio Lower Upper
228 100
226 29.4 25.3 37.9
229 22.2 16.4 24.6

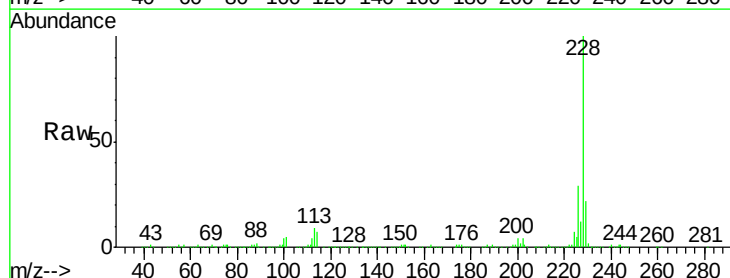

Abundance Ion 228.00 (227.70 to 228.70): E
Ion 226.00 (225.70 to 226.70): E
Ion 229.00 (228.70 to 229.70): E

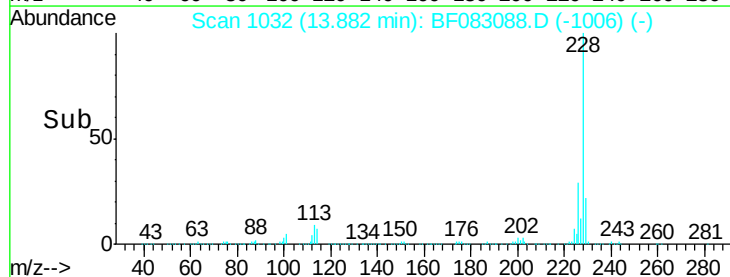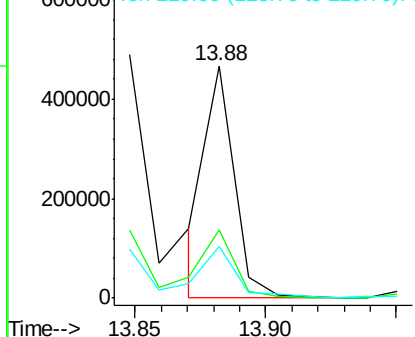



#85

Indeno(1,2,3-cd)pyrene

Concen: 8.27 ng

RT: 16.56 min Scan# 1266

Delta R.T. 0.01 min

Lab File: BF083088.D

Acq: 20 Nov 2015 18:44

Instrument :

BNA_F

ClientSampleId :


Tot Ion:276 Resp: 157281

Ion Ratio Lower Upper

276 100

138 18.5 16.3 24.5




277 28.1 19.8 29.8

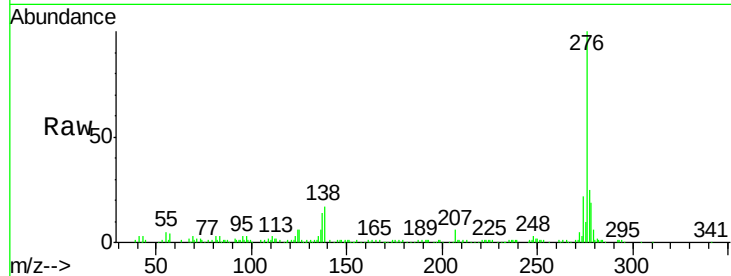

Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

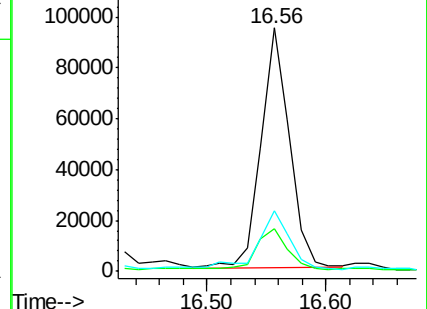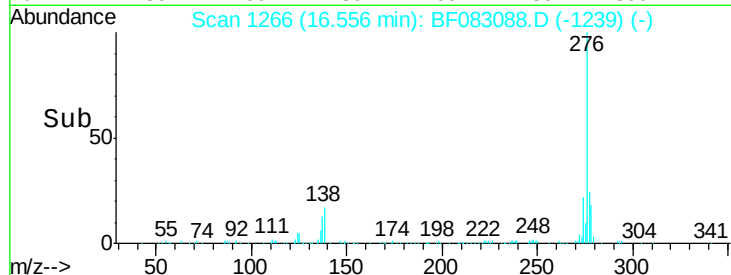

#86

Perylene-d12

Concen: 20.00 ng

RT: 15.25 min Scan# 1152

Delta R.T. 0.01 min

Lab File: BF083088.D

Acq: 20 Nov 2015 18:44


Tgt Ion:264 Resp: 347360

Ion Ratio Lower Upper

264 100

260 23.7 18.6 27.8



265 21.9 17.0 25.6




Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E



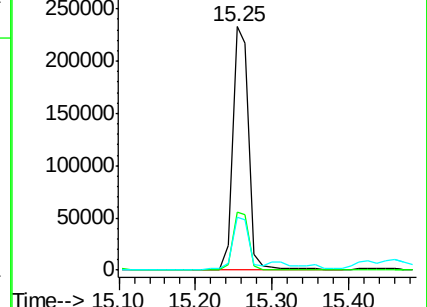





#87
Benzo(b)fluoranthene
Concen: 25.42 ng
RT: 14.88 min Scan# 1119
Delta R.T. 0.02 min
Lab File: BF083088.D
Acq: 20 Nov 2015 18:44




Instrument :
BNA_F
ClientSampleId :


Tot Ion:252 Resp: 617323
Ion Ratio Lower Upper
252 100
253 22.4 17.6 26.4
125 8.8 7.7 11.5

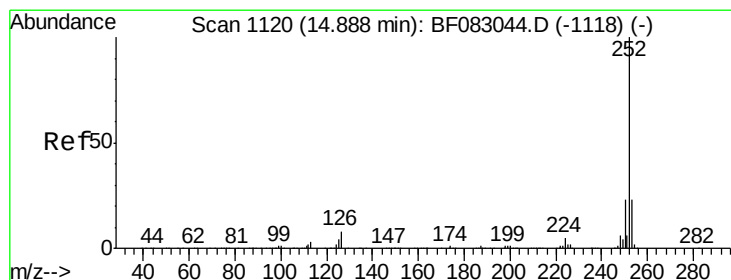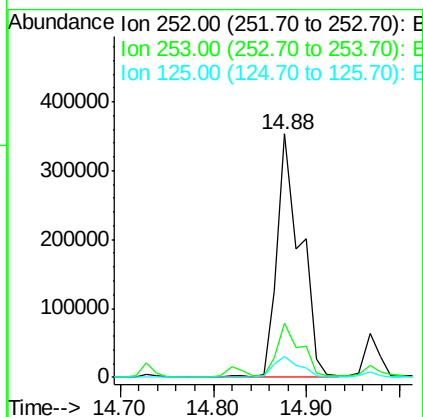

#88
Benzo(k)fluoranthene
Concen: 33.36 ng
RT: 14.88 min Scan# 1119
Delta R.T. -0.01 min
Lab File: BF083088.D
Acq: 20 Nov 2015 18:44

Tgt Ion:252 Resp: 617323
Ion Ratio Lower Upper
252 100
253 22.4 17.8 26.6
125 8.8 3.8 5.6#

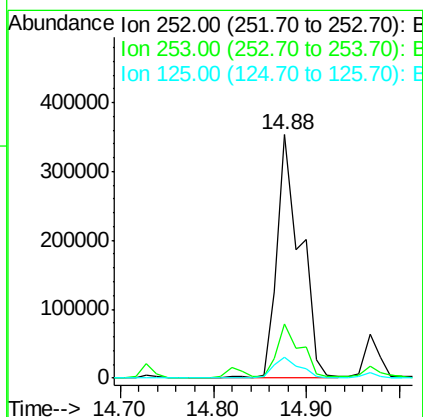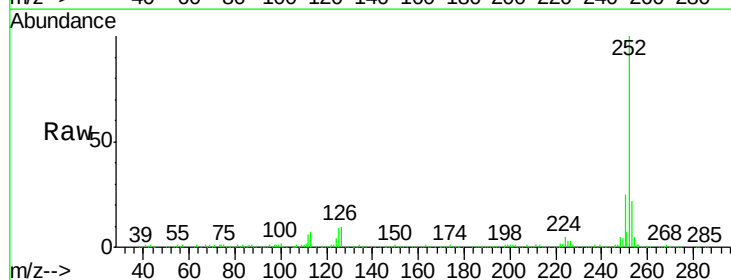



#89

Benzo(a)pyrene

Concen: 10.80 ng

RT: 15.15 min Scan# 1143

Delta R.T. -0.03 min

Lab File: BF083088.D

Acq: 20 Nov 2015 18:44

Instrument :

BNA_F

ClientSampled :


Tot Ion:252 Resp: 210543

Ion Ratio Lower Upper

252 100

253 25.2 17.5 26.3




125 9.4 6.4 9.6



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

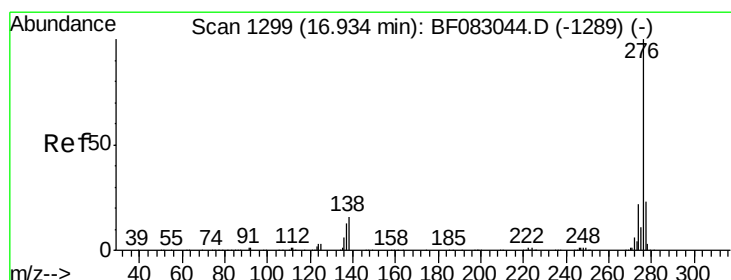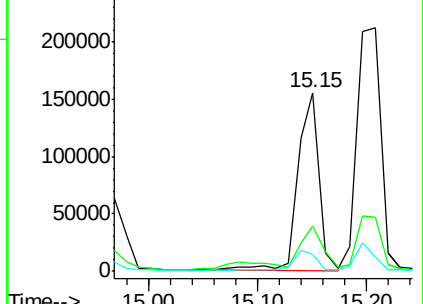

#91

Benzo(g,h,i)perylene

Concen: 7.98 ng

RT: 16.95 min Scan# 1300

Delta R.T. 0.01 min

Lab File: BF083088.D

Acq: 20 Nov 2015 18:44


Tgt Ion:276 Resp: 131961

Ion Ratio Lower Upper

276 100

277 25.0 18.6 27.8

138 20.2 12.5 18.7#



Abundance Ion 276.00 (275.70 to 276.70): E

Ion 277.00 (276.70 to 277.70): E

Ion 138.00 (137.70 to 138.70): E

