
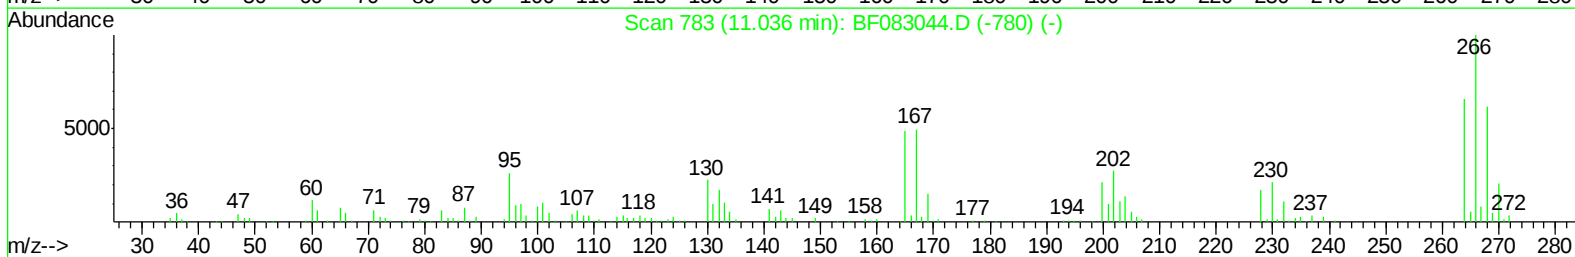
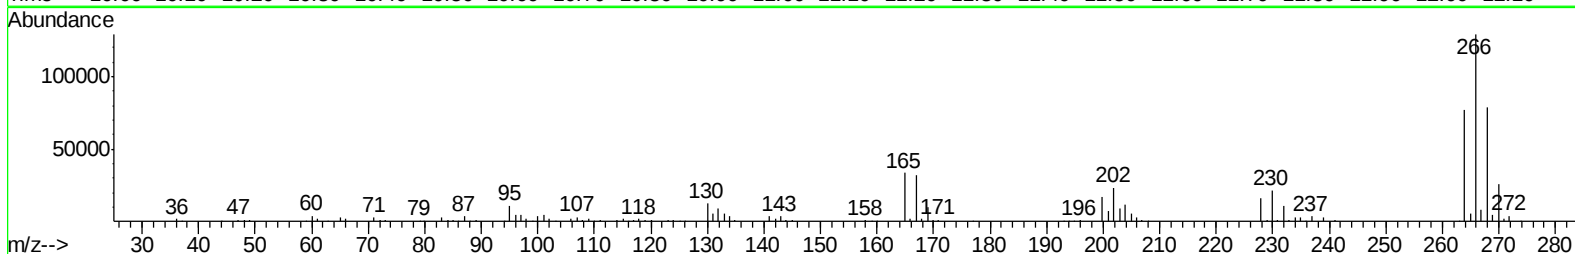


Data Path : Z:\HPCHEM1\BNA_F\Data\BF112015\
Data File : BF083072.D
Acq On : 20 Nov 2015 9:45
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 20 10:09:34 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 18 13:32:32 2015
Response via : Initial Calibration

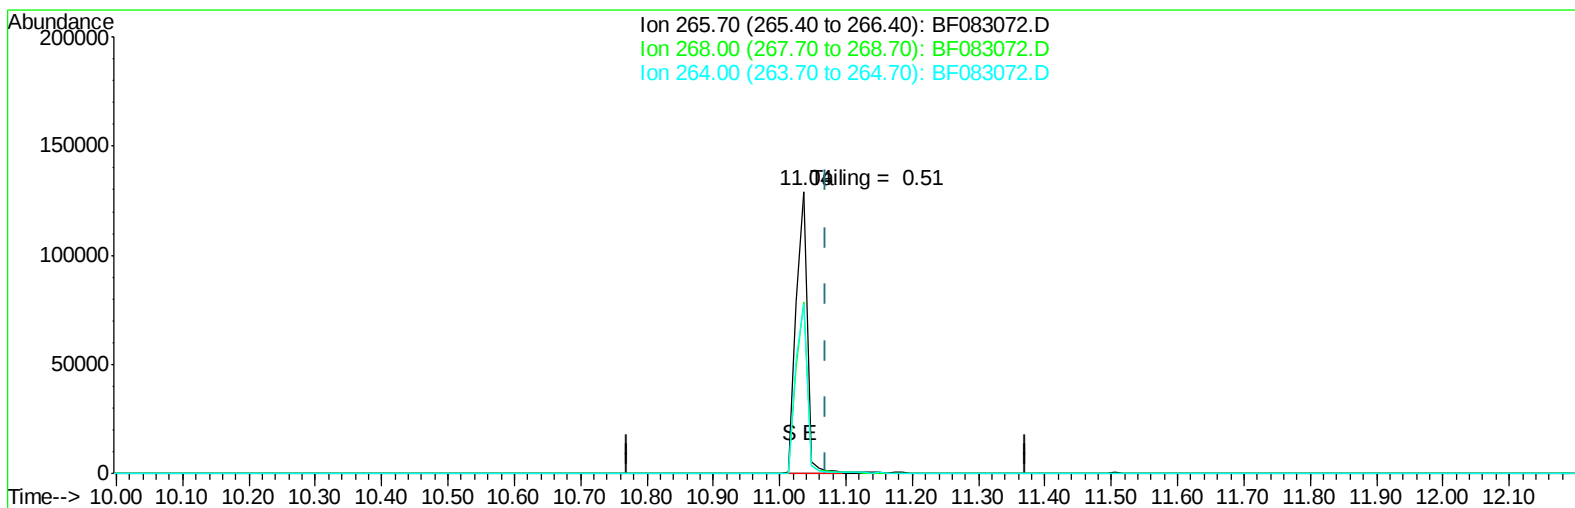

TIC: BF083072.D

(69) Pentachlorophenol (C)




11.036min (-0.034) 0.00ng

response 152633

Ion	Exp%	Act%
265.70	100	100
268.00	63.80	61.04
264.00	63.20	59.92
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF112015\
Data File : BF083072.D
Acq On : 20 Nov 2015 9:45
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 20 10:09:34 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 18 13:32:32 2015
Response via : Initial Calibration

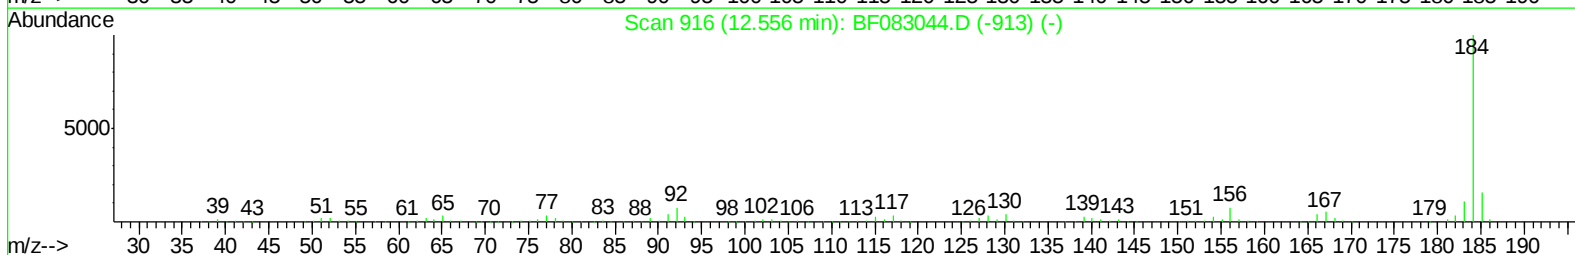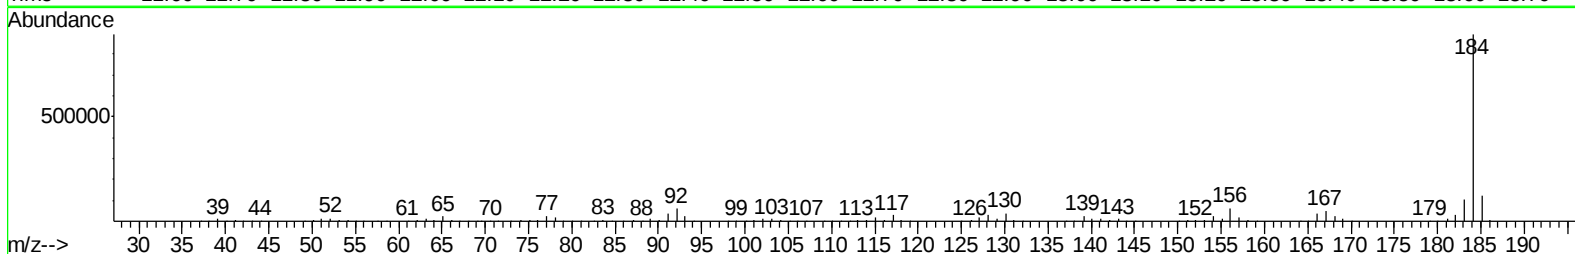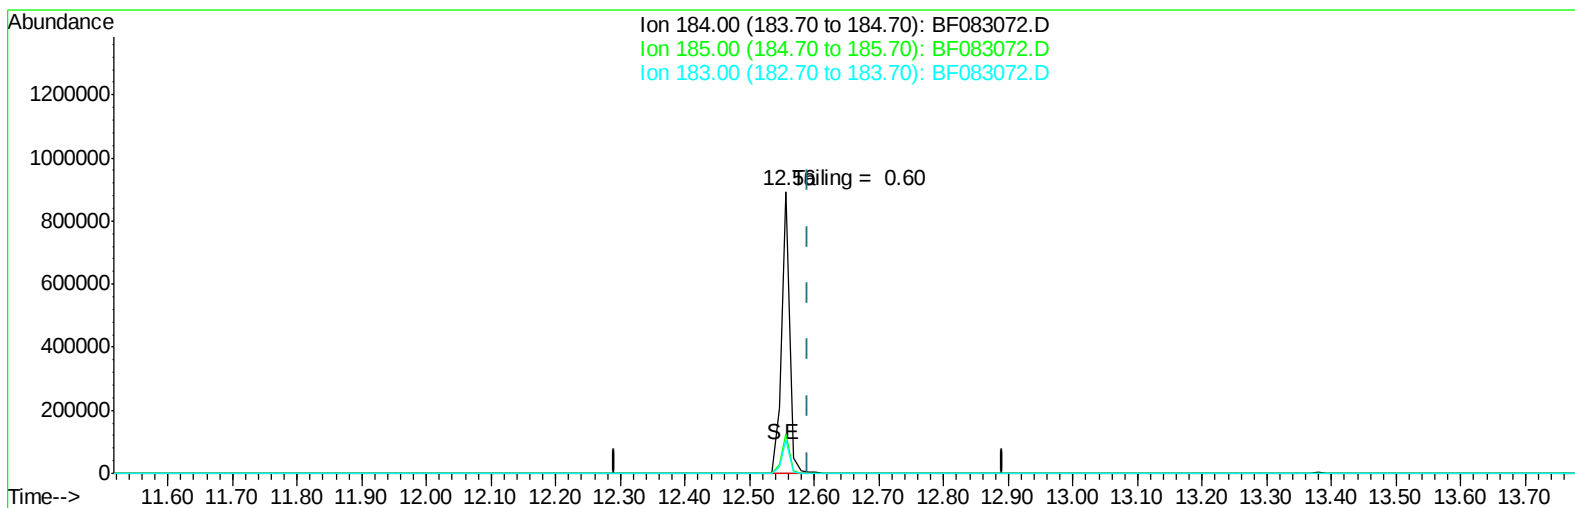

TIC: BF083072.D

(76) Benzidine

12.556min (-0.034) 0.00ng

response 809779

Ion	Exp%	Act%
184.00	100	100
185.00	15.00	13.96
183.00	12.00	11.79
0.00	0.00	0.00