

Data Path : V:\HPCHEM1\BNA F\DATA\BF112015\
 Data File : BF083086.D
 Acq On : 20 Nov 2015 17:21
 Operator : UM/IZ
 Sample : G4452-08
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 RW-20151116-08

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF111915.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.841	238	241	244	rBV	1235886	1950557	44.57%	5.177%
2	5.299	278	281	284	rBV	4047842	3835804	87.66%	10.181%
3	6.350	370	373	376	rBV2	3502402	4178019	95.48%	11.089%
4	6.476	381	384	386	rBV	3390642	4149582	94.83%	11.014%
5	6.705	401	404	406	rBV	642497	851668	19.46%	2.261%
6	6.853	415	417	420	rBV	2742812	3105185	70.96%	8.242%
7	7.265	450	453	455	rBV	2525608	2334251	53.34%	6.196%
8	7.379	461	463	468	rVB	38238	47079	1.08%	0.125%
9	7.985	514	516	519	rBV	1091319	1073986	24.54%	2.851%
10	9.070	608	611	613	rBV	4942184	4376008	100.00%	11.615%
11	9.471	643	646	648	rBV	781427	844316	19.29%	2.241%
12	9.745	667	670	672	rBV	1056543	1165809	26.64%	3.094%
13	10.191	708	709	711	rVB	81143	63657	1.45%	0.169%
14	10.522	736	738	741	rBV2	1517314	1670005	38.16%	4.433%
15	10.659	749	750	754	rVB	55714	95485	2.18%	0.253%
16	11.116	787	790	791	rBV	51682	62237	1.42%	0.165%
17	11.219	796	799	801	rBV	1248658	1104633	25.24%	2.932%
18	11.471	818	821	825	rBV2	54982	108114	2.47%	0.287%
19	11.539	825	827	829	rVB	55072	49116	1.12%	0.130%
20	12.019	867	869	874	rBV2	52706	73490	1.68%	0.195%
21	12.431	903	905	907	rVB	142428	164998	3.77%	0.438%
22	12.648	921	924	927	rBV2	158493	193918	4.43%	0.515%
23	12.808	936	938	940	rVB	3575397	3166278	72.36%	8.404%
24	12.979	950	953	956	rBV2	35890	60590	1.38%	0.161%
25	13.517	994	1000	1003	rBV7	17217	60899	1.39%	0.162%
26	13.734	1017	1019	1024	rBV2	56117	114911	2.63%	0.305%
27	13.848	1026	1029	1035	rVB2	1170730	1327784	30.34%	3.524%
28	13.962	1036	1039	1041	rBV3	39541	79172	1.81%	0.210%
29	14.854	1114	1117	1121	rBV	131779	267365	6.11%	0.710%
30	15.128	1138	1141	1143	rBV	52597	92956	2.12%	0.247%
31	15.174	1143	1145	1148	rVB	85968	106742	2.44%	0.283%
32	15.231	1148	1150	1153	rBV	535123	809981	18.51%	2.150%
33	16.523	1261	1263	1267	rVB2	38365	91412	2.09%	0.243%

Data Path : V:\HPCHEM1\BNA_F\DATA\BF112015\
Data File : BF083086.D
Acq On : 20 Nov 2015 17:21
Operator : UM/IZ
Sample : G4452-08
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RW-20151116-08

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF111915.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION


Sum of corrected areas: 37676007

Data Path : V:\HPCHEM1\BNA F\DATA\BF112015\
Data File : BF083086.D
Acq On : 20 Nov 2015 17:21
Operator : UM/IZ
Sample : G4452-08
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RW-20151116-08

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF111915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

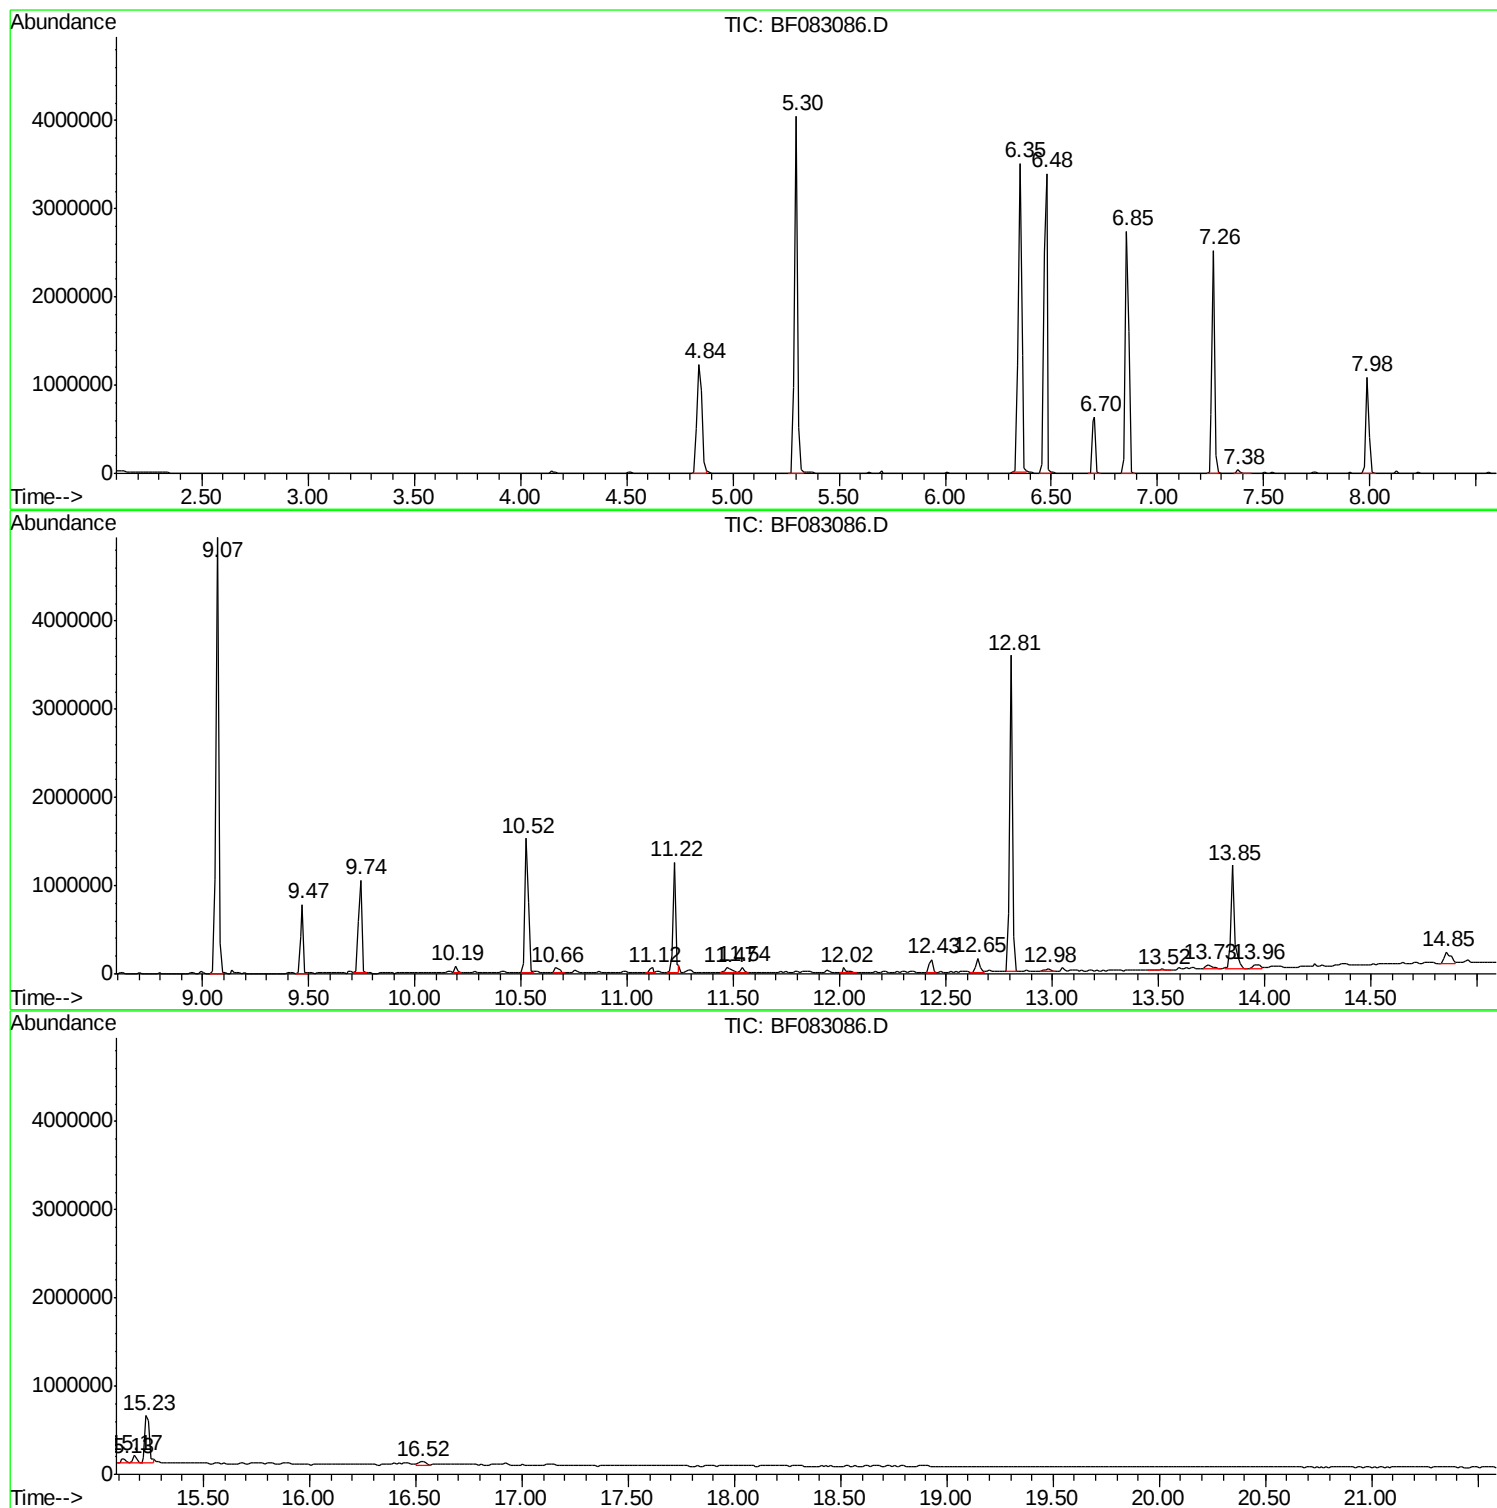

Data Path : V:\HPCHEM1\BNA_F\DATA\BF112015\
Data File : BF083086.D
Acq On : 20 Nov 2015 17:21
Operator : UM/IZ
Sample : G4452-08
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RW-20151116-08










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF111915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.84	45.81 ng	1950560	1,4-Dichlorobenzene-d4	6.70

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	64
2			Propane, 2-methyl-2-(1-methyleth...	116	C7H16O	017348-59-3	36
3			3-Hexanol, 4-methyl-	116	C7H16O	000615-29-2	33
4			Acetic acid, cyano-, 1,1-dimethyl...	141	C7H11NO2	001116-98-9	32
5			2-Hexanol, 2-methyl-	116	C7H16O	000625-23-0	28

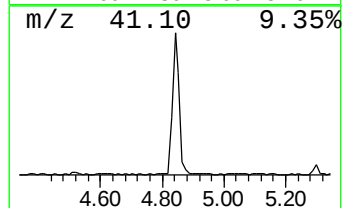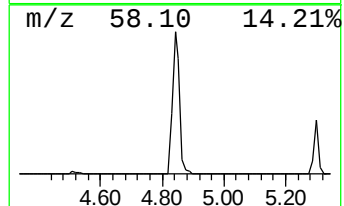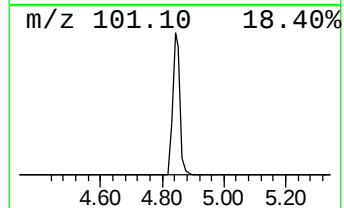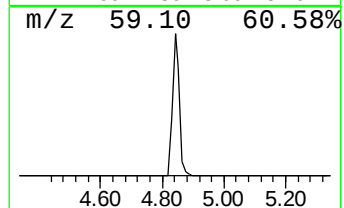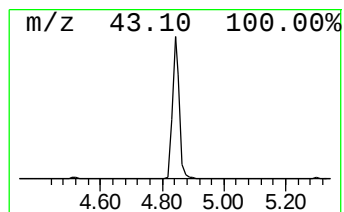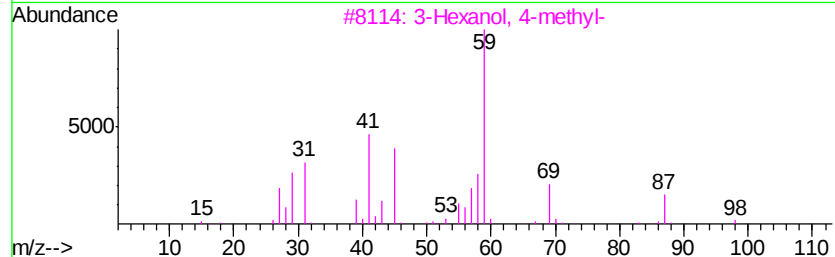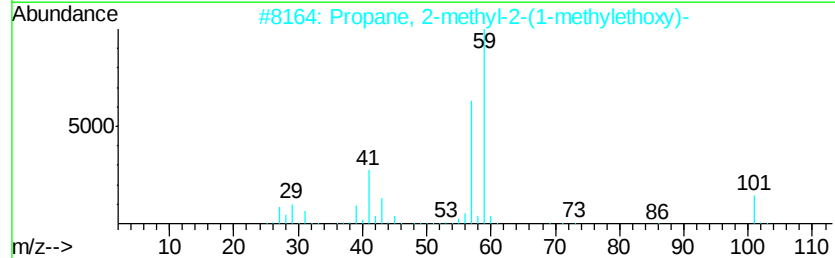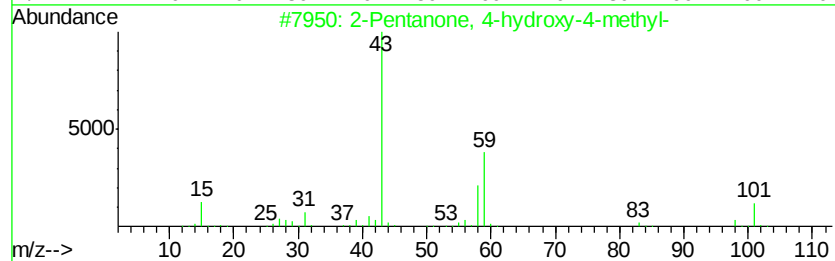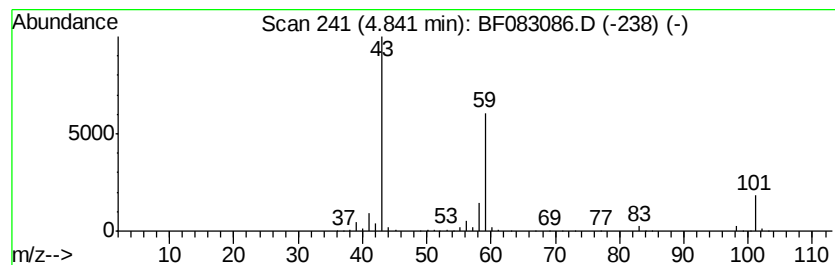

Data Path : V:\HPCHEM1\BNA_F\DATA\BF112015\
Data File : BF083086.D
Acq On : 20 Nov 2015 17:21
Operator : UM/IZ
Sample : G4452-08
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RW-20151116-08

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF111915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	4.84	45.8	ng	1950560	1	6.70	851668	20.0