


Data Path : V:\HPCHEM1\BNA_F\DATA\BF112015\
 Data File : BF083072.D
 Acq On : 20 Nov 2015 9:45
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF111915.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Nov 20 01:33:39 2015

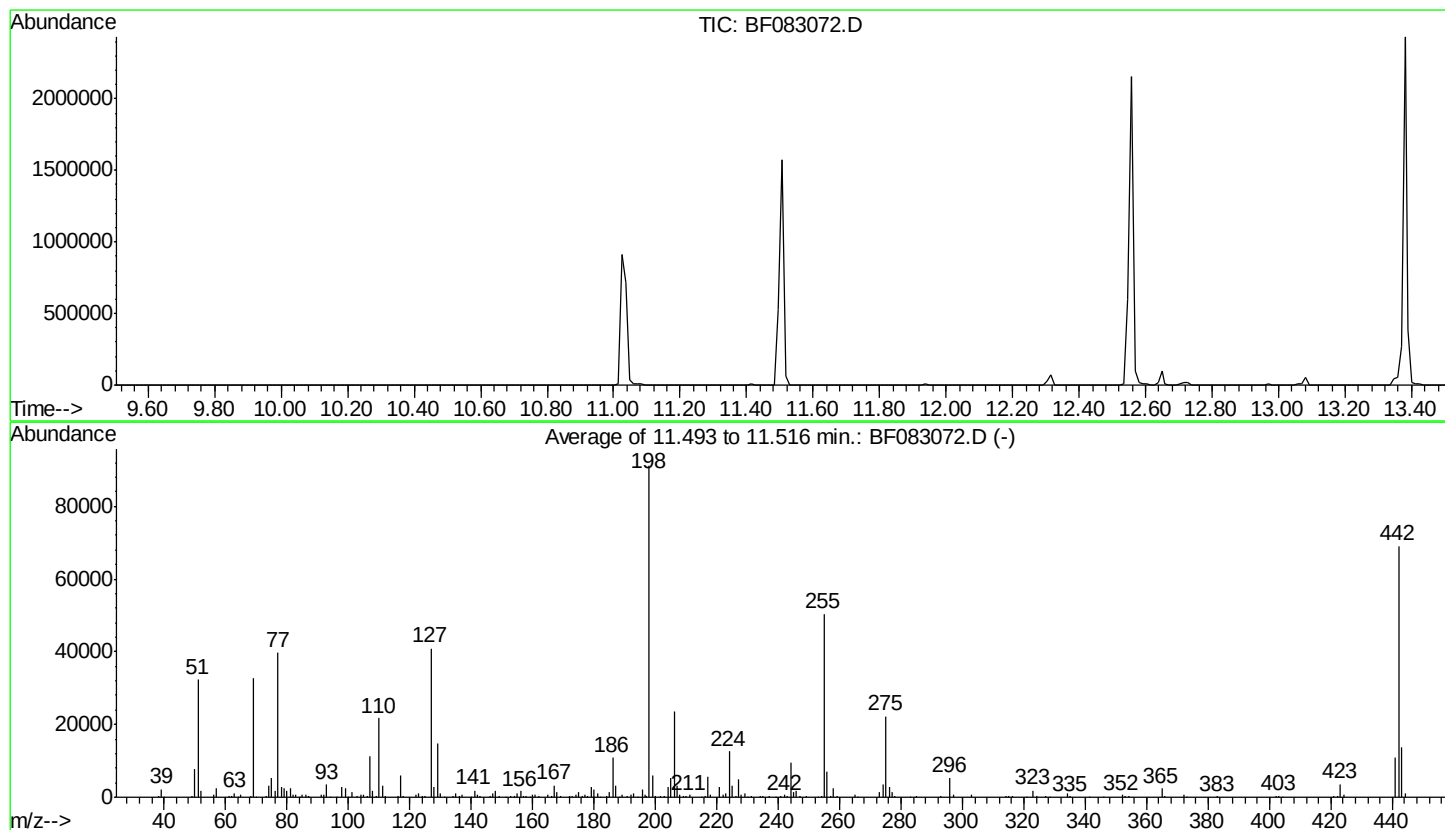

AutoFind: Scans 823, 824, 825; Background Corrected with Scan 819

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.5	32377	PASS
68	69	0.00	2	1.4	466	PASS
69	198	0.00	100	35.8	32658	PASS
70	69	0.00	2	0.3	101	PASS
127	198	10	80	45.0	41014	PASS
197	198	0.00	2	0.6	545	PASS
198	198	100	100	100.0	91191	PASS
199	198	5	9	6.6	5987	PASS
275	198	10	60	24.4	22208	PASS
365	198	1	100	2.6	2391	PASS
441	442	0.01	24	15.8	10951	PASS
442	198	50	100	75.9	69182	PASS
443	442	15	24	19.7	13623	PASS