


Data Path : V:\HPCHEM1\BNA_F\DATA\BF112015\
 Data File : BF083094.D
 Acq On : 21 Nov 2015 00:05
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF111915.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Nov 20 01:33:39 2015

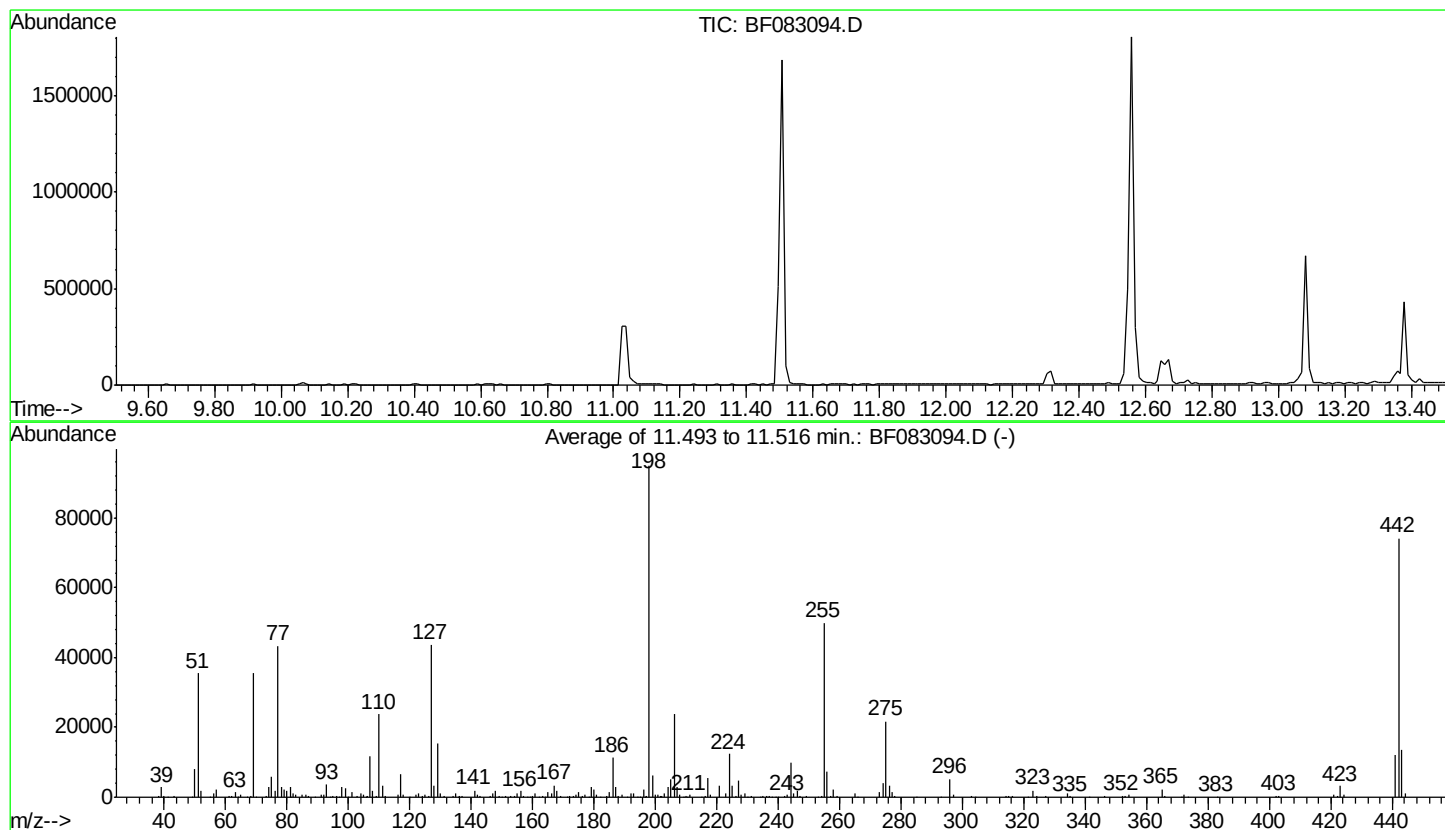

AutoFind: Scans 823, 824, 825; Background Corrected with Scan 820

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.4	35540	PASS
68	69	0.00	2	1.5	535	PASS
69	198	0.00	100	37.3	35418	PASS
70	69	0.00	2	0.3	123	PASS
127	198	10	80	46.0	43687	PASS
197	198	0.00	2	0.5	444	PASS
198	198	100	100	100.0	94989	PASS
199	198	5	9	6.6	6278	PASS
275	198	10	60	23.0	21808	PASS
365	198	1	100	2.5	2346	PASS
441	442	0.01	24	16.3	12098	PASS
442	198	50	100	78.2	74244	PASS
443	442	15	24	18.5	13721	PASS