
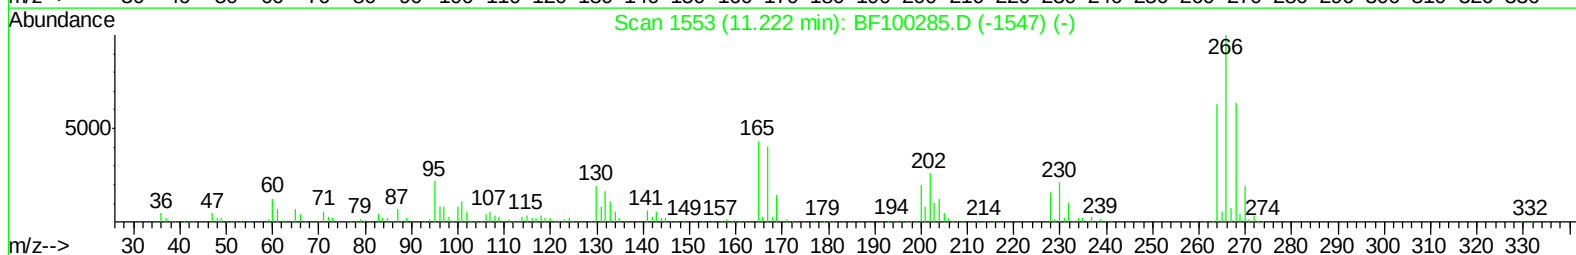
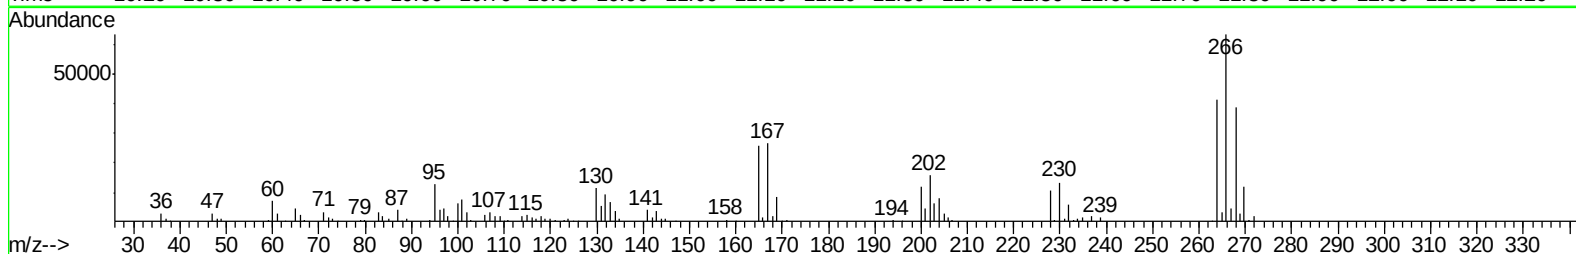


Data File : BF100724.D
Acq On : 20 Nov 2017 12:23
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 21 07:09:39 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 15:22:08 2017
Response via : Initial Calibration

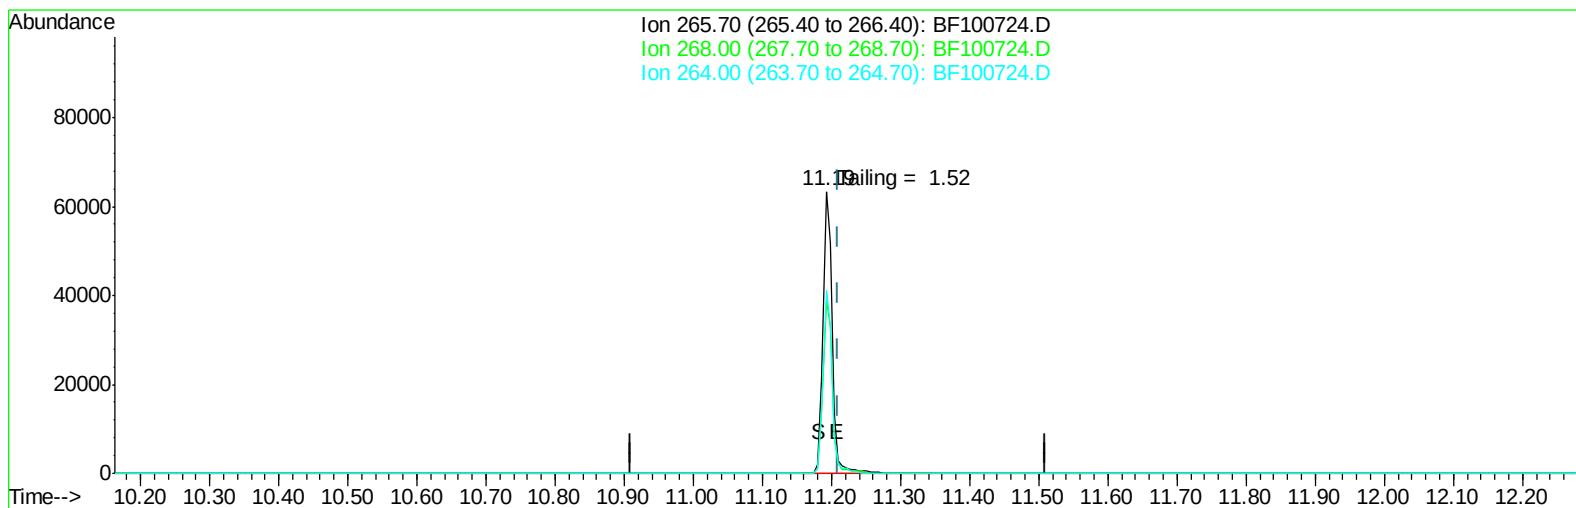

TIC: BF100724.D

(69) Pentachlorophenol (C)




11.192min (-0.018) 48994.81ng

response 57114

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	61.48
264.00	61.90	64.94
0.00	0.00	0.00

Data File : BF100724.D
Acq On : 20 Nov 2017 12:23
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 21 07:09:39 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 15:22:08 2017
Response via : Initial Calibration

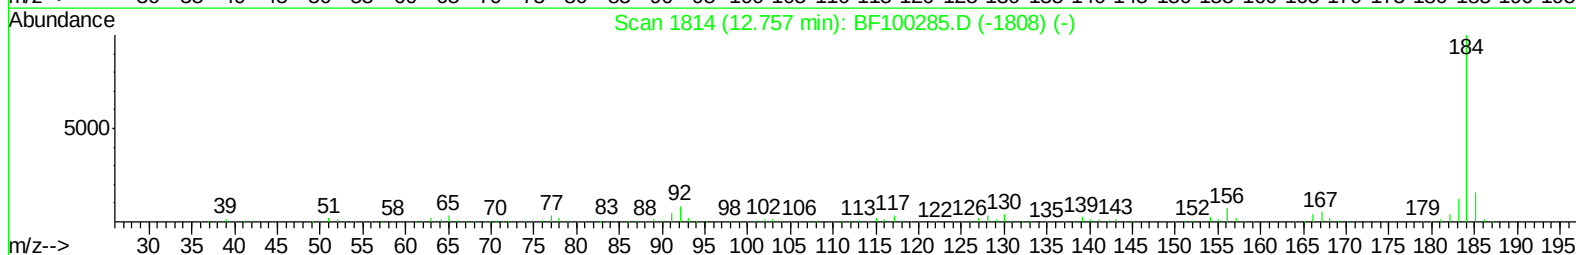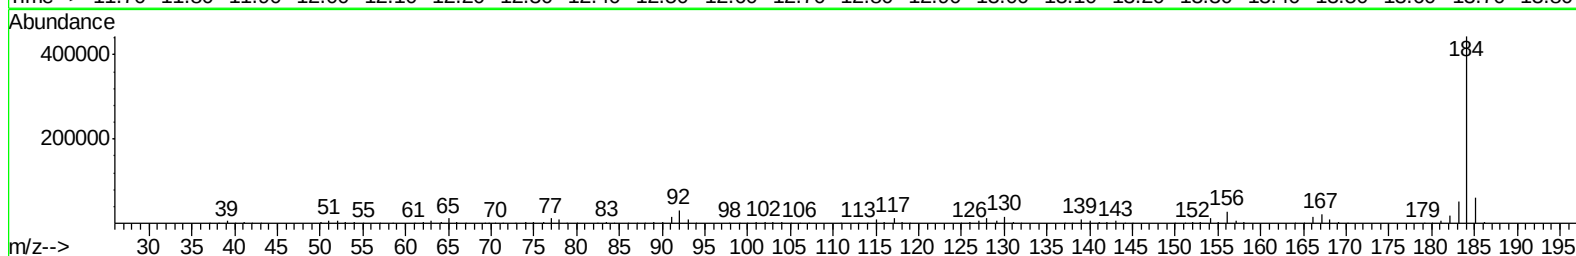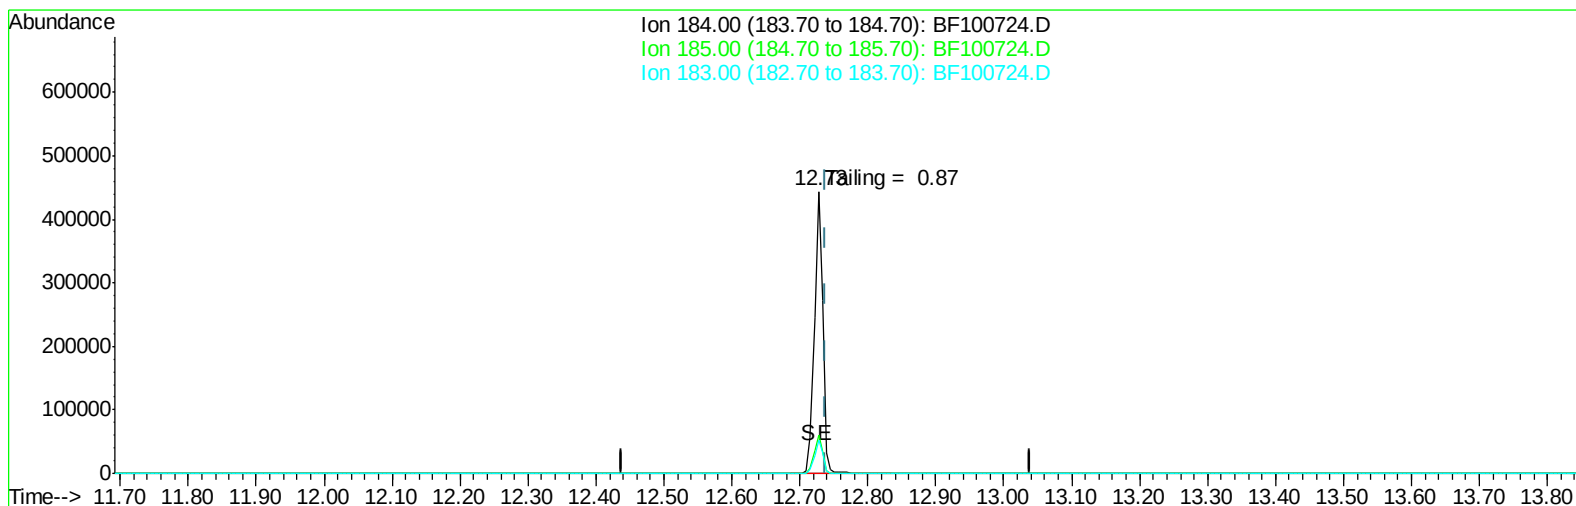

TIC: BF100724.D

(76) Benzidine

12.727min (-0.012) 0.00ng

response 378924

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	13.74
183.00	11.60	11.74
0.00	0.00	0.00