
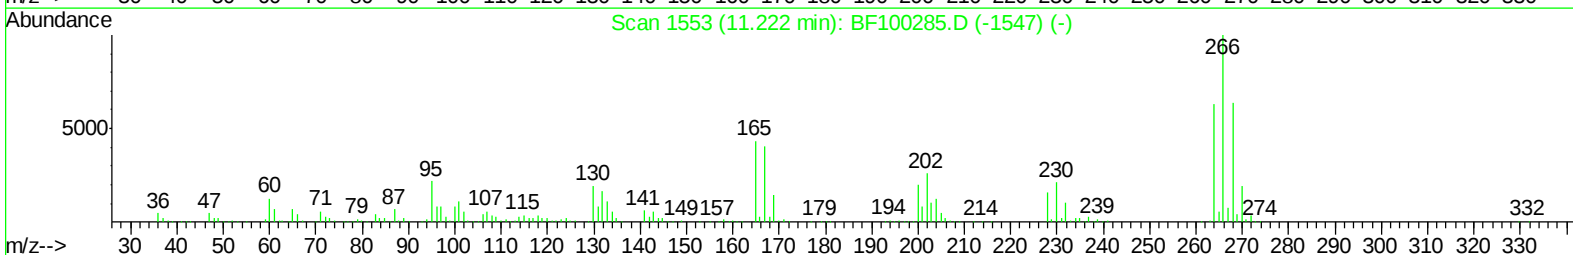
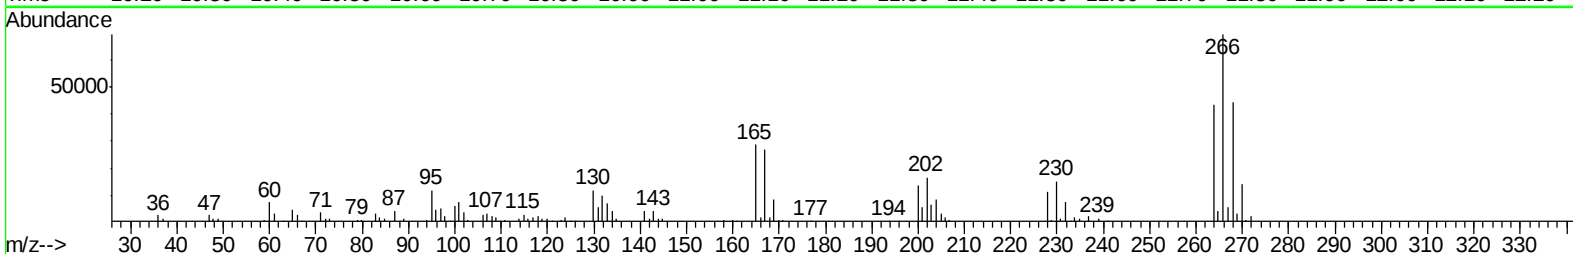


Data File : BF100733.D
Acq On : 20 Nov 2017 16:37
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 21 07:10:26 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 15:22:08 2017
Response via : Initial Calibration

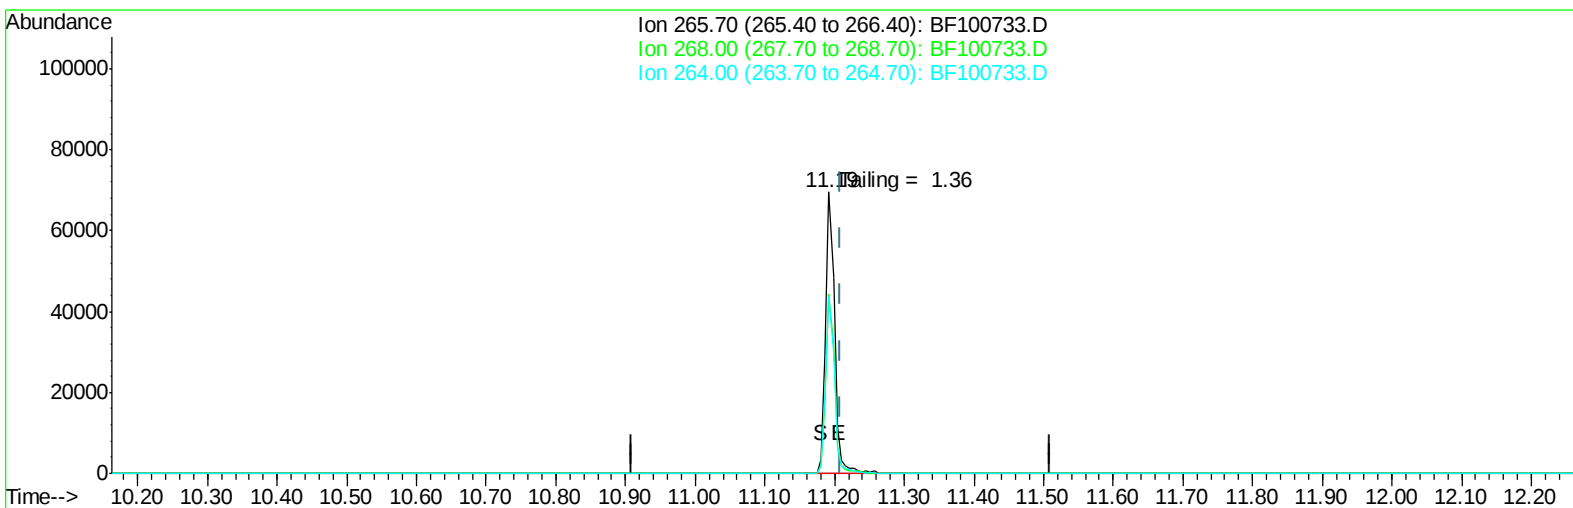

TIC: BF100733.D

(69) Pentachlorophenol (C)




11.192min (-0.018) 67243.02ng

response 60006

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.77
264.00	61.90	62.78
0.00	0.00	0.00

Data File : BF100733.D
Acq On : 20 Nov 2017 16:37
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 21 07:10:26 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 15:22:08 2017
Response via : Initial Calibration

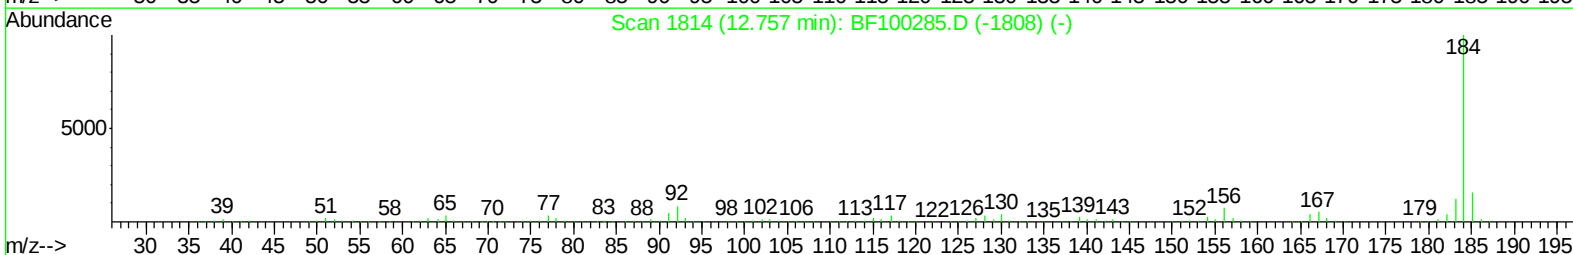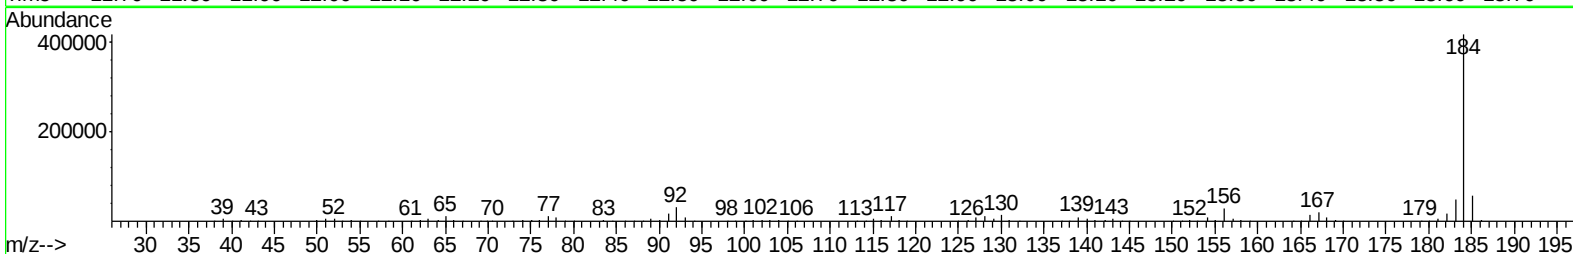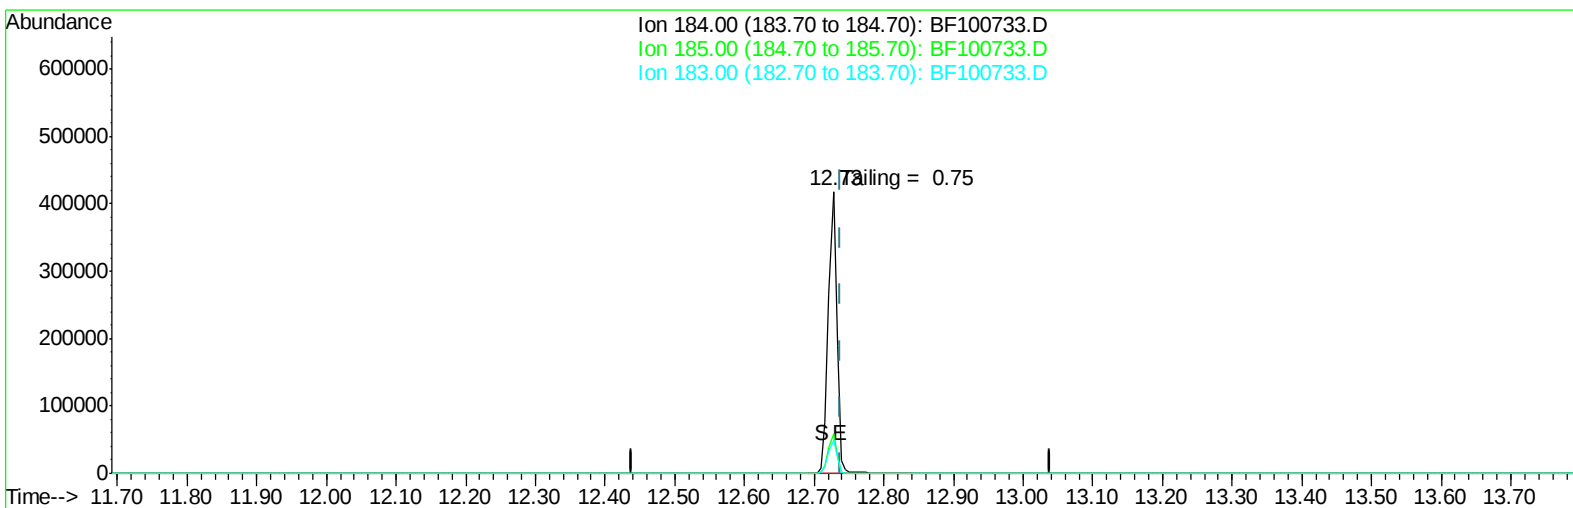

TIC: BF100733.D

(76) Benzidine

12.727min (-0.012) 0.00ng

response 350863

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	13.89
183.00	11.60	11.66
0.00	0.00	0.00