


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF112017\
 Data File : BF100724.D
 Acq On : 20 Nov 2017 12:23
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Nov 17 15:22:08 2017

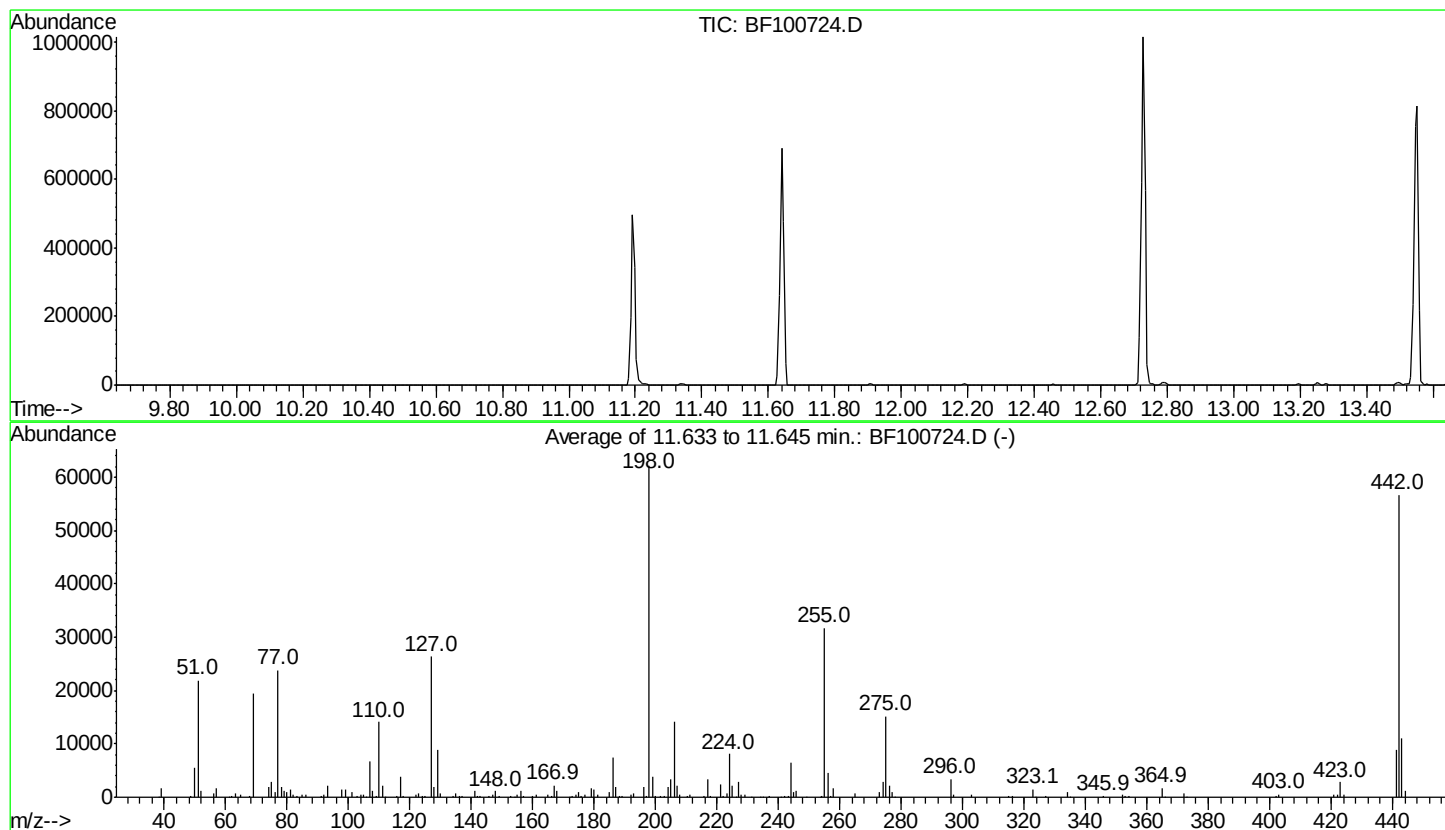

AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.1	21844	PASS
68	69	0.00	2	1.9	364	PASS
69	198	0.00	100	31.3	19466	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.4	26330	PASS
197	198	0.00	2	0.4	239	PASS
198	198	100	100	100.0	62149	PASS
199	198	5	9	6.3	3930	PASS
275	198	10	60	24.5	15237	PASS
365	198	1	100	2.8	1742	PASS
441	443	0.01	100	81.1	8885	PASS
442	198	50	100	91.2	56666	PASS
443	442	15	24	19.3	10952	PASS