


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF112017\
 Data File : BF100759.D
 Acq On : 21 Nov 2017 5:14
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Nov 17 15:22:08 2017

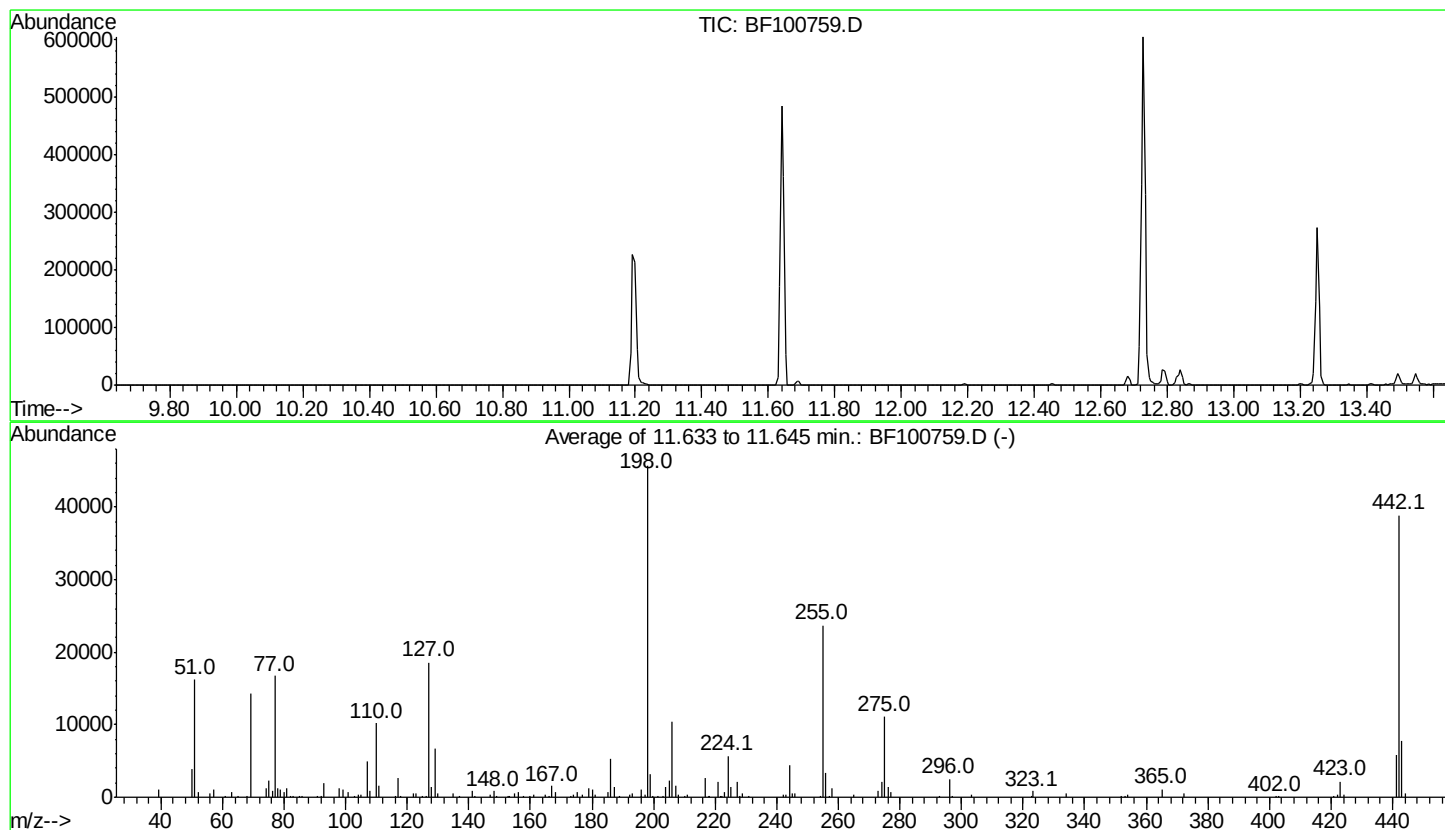

AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.3	16160	PASS
68	69	0.00	2	1.1	158	PASS
69	198	0.00	100	31.1	14223	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	40.7	18594	PASS
197	198	0.00	2	0.7	341	PASS
198	198	100	100	100.0	45736	PASS
199	198	5	9	7.1	3256	PASS
275	198	10	60	24.3	11101	PASS
365	198	1	100	2.4	1100	PASS
441	443	0.01	100	74.8	5826	PASS
442	198	50	100	85.0	38860	PASS
443	442	15	24	20.0	7784	PASS