

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF112018\
 Data File : BF110918.D
 Acq On : 21 Nov 2018 3:30
 Operator : JU/SJ
 Sample : J5996-18
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 NON-UST-06-A

Quant Time: Nov 21 06:19:45 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF110818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 13 12:43:10 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.94	152	58090	20.00	ng	0.00
21) Naphthalene-d8	8.22	136	219581	20.00	ng	0.00
39) Acenaphthene-d10	9.98	164	87291	20.00	ng	-0.01
64) Phenanthrene-d10	11.48	188	137260	20.00	ng	0.00
76) Chrysene-d12	14.13	240	118932	20.00	ng	0.00
87) Perylene-d12	15.67	264	77442	20.00	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.56	112	494467	138.26	ng	0.00
7) Phenol-d6	6.57	99	611940	133.81	ng	0.00
23) Nitrobenzene-d5	7.51	82	381719	100.11	ng	0.00
42) 2,4,6-Tribromophenol	10.78	330	107218	121.90	ng	0.00
45) 2-Fluorobiphenyl	9.30	172	648913	106.17	ng	0.00
79) Terphenyl-d14	13.06	244	524568	82.60	ng	0.00
Target Compounds						
10) Phenol	6.58	94	33126	6.247	ng	Qvalue # 77
50) Dimethylphthalate	9.69	163	60339	9.264	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF112018\
Data File : BF110918.D
Acq On : 21 Nov 2018 3:30
Operator : JU/SJ
Sample : J5996-18
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
NON-UST-06-A

Quant Time: Nov 21 06:19:45 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF110818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 13 12:43:10 2018
Response via : Initial Calibration

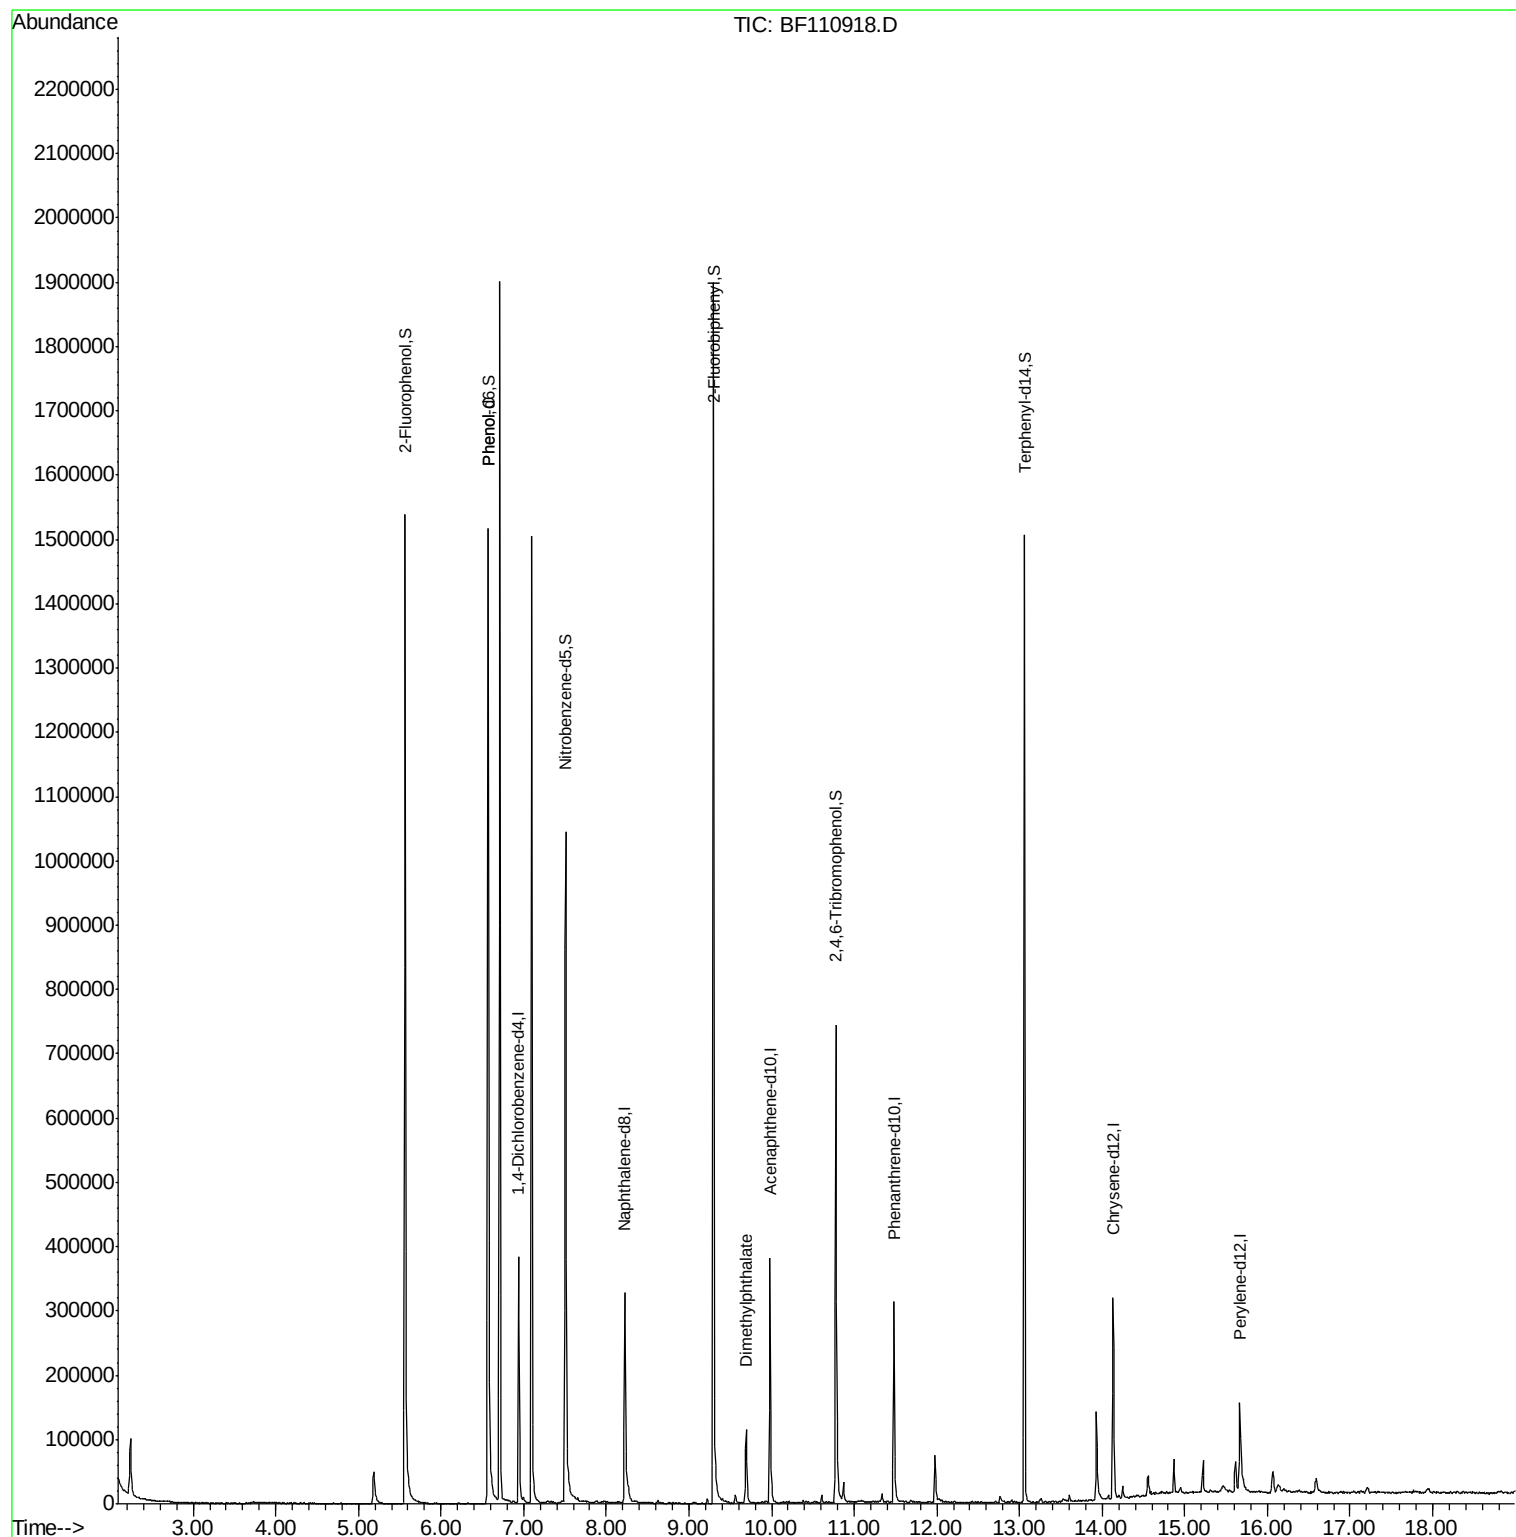

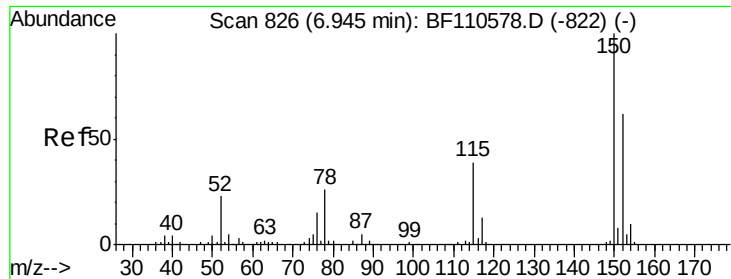


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.94 min Scan# 825
Delta R.T. -0.01 min
Lab File: BF110918.D
Acq: 21 Nov 2018 3:30

Instrument :
BNA_F
ClientSampleId :
NON-UST-06-A

Tot Ion:152 Resp: 58090
Ion Ratio Lower Upper
152 100
150 158.9 122.7 184.1
115 62.8 49.1 73.7

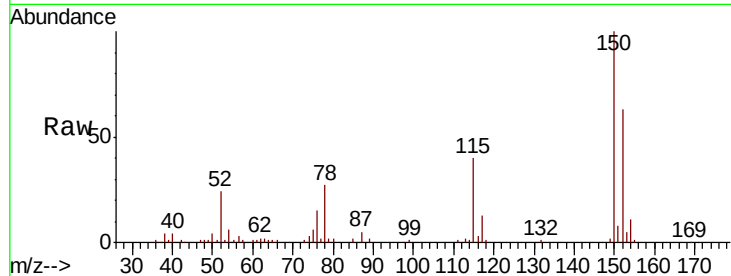


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

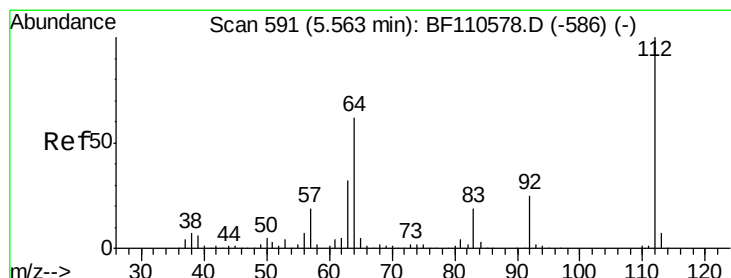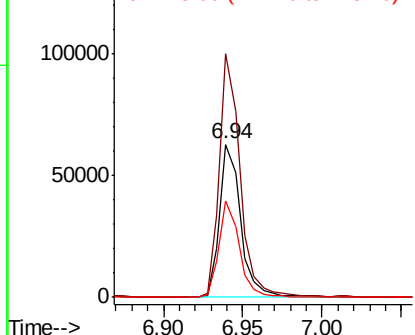



#5


2-Fluorophenol
Concen: 138.263 ng
RT: 5.56 min Scan# 591
Delta R.T. 0.00 min
Lab File: BF110918.D
Acq: 21 Nov 2018 3:30

Tgt Ion:112 Resp: 494467
Ion Ratio Lower Upper
112 100
64 63.5 44.1 66.1
63 33.9 23.7 35.5

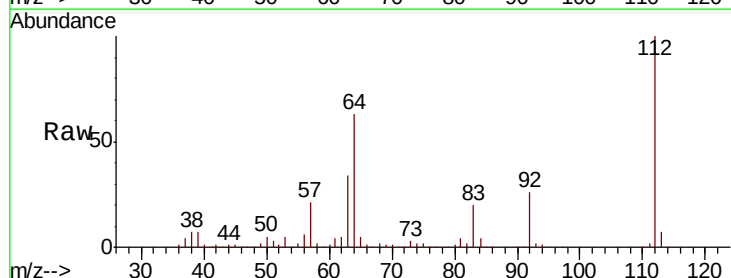

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

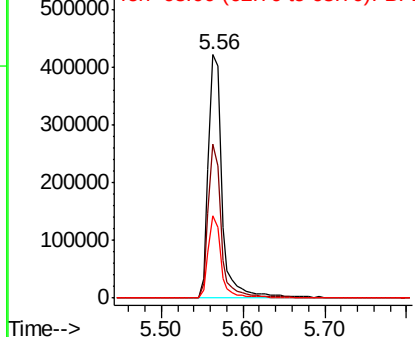

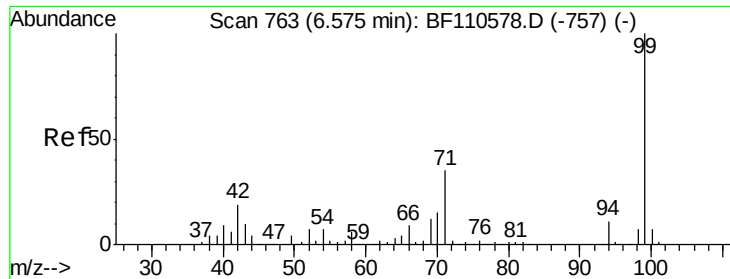

#7

Phenol-d6

Concen: 133.810 ng

RT: 6.57 min Scan# 763

Delta R.T. 0.00 min

Lab File: BF110918.D

Acq: 21 Nov 2018 3:30

Instrument :

BNA_F

ClientSampleId :

NON-UST-06-A


Tot Ion: 99 Resp: 611940

Ion Ratio Lower Upper




99 100

42 18.3 15.8 23.6

71 34.1 28.0 42.0

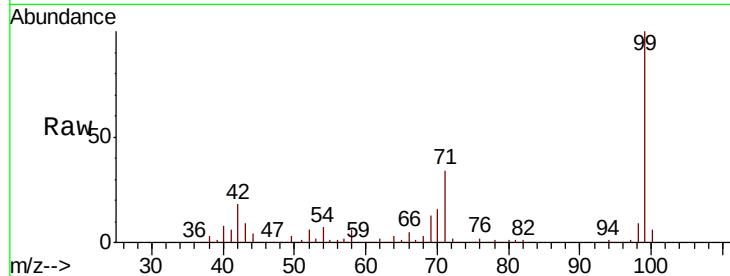

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

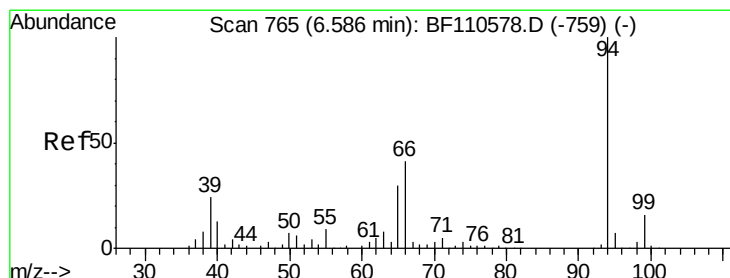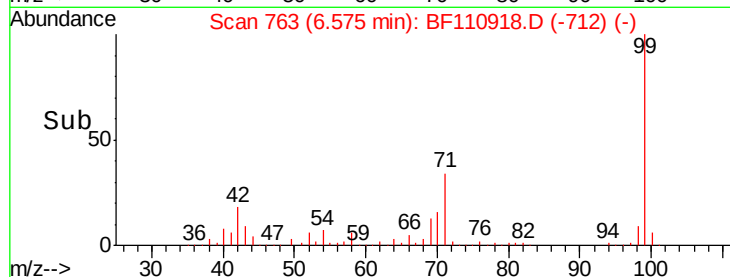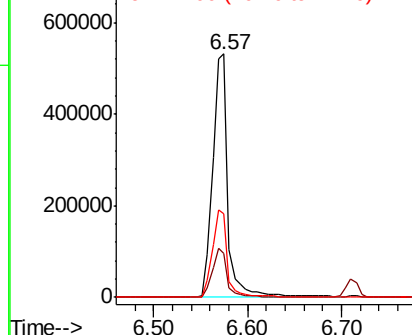

#10

Phenol

Concen: 6.247 ng

RT: 6.58 min Scan# 764

Delta R.T. -0.01 min

Lab File: BF110918.D

Acq: 21 Nov 2018 3:30


Tgt Ion: 94 Resp: 33126

Ion Ratio Lower Upper



94 100


65 32.2 25.3 65.3

66 52.8 54.5 94.5#

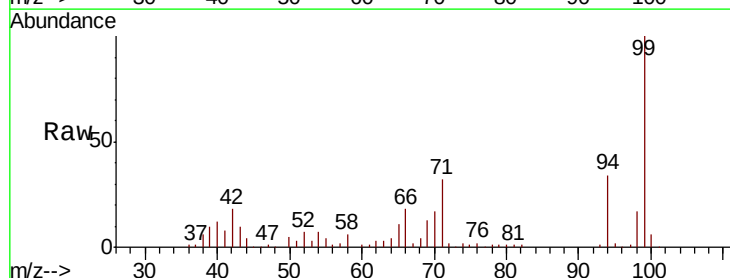

Abundance Ion 94.00 (93.70 to 94.70): BF1
Ion 65.00 (64.70 to 65.70): BF1
Ion 66.00 (65.70 to 66.70): BF1

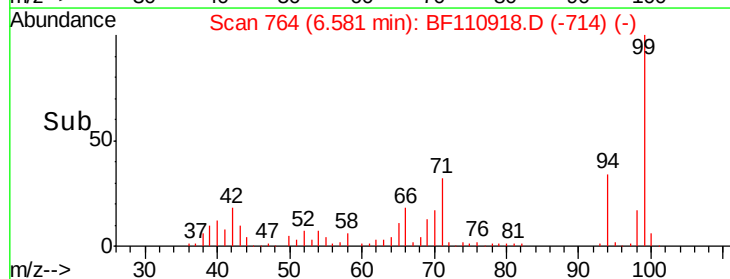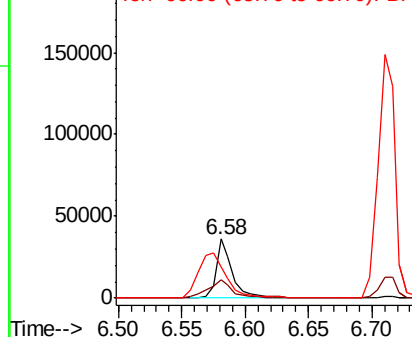


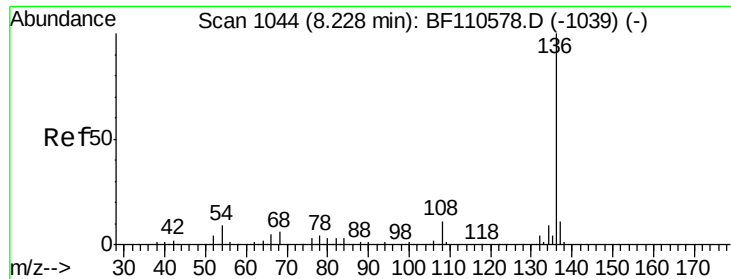




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.22 min Scan# 1043
Delta R.T. -0.01 min
Lab File: BF110918.D
Acq: 21 Nov 2018 3:30

Instrument :
BNA_F
ClientSampleId :
NON-UST-06-A

Tot Ion:136	Resp:	219581
Ion Ratio	Lower	Upper
136	100	
137	11.1	8.8 13.2
54	8.1	5.4 8.2
68	5.2	4.2 6.2

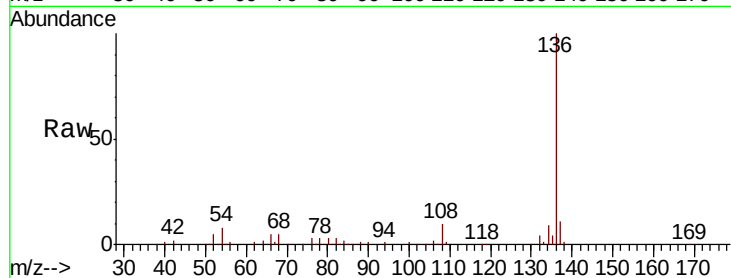


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

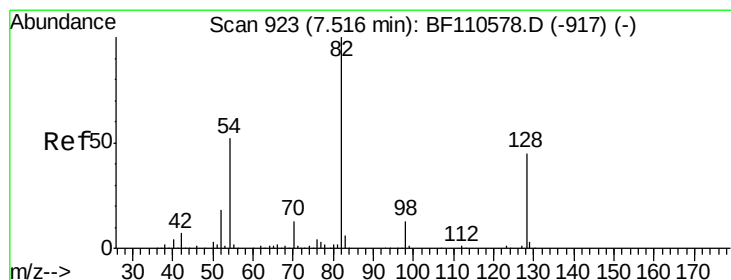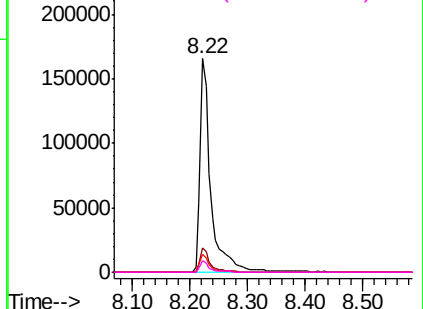




#23
Nitrobenzene-d5
Concen: 100.114 ng
RT: 7.51 min Scan# 922
Delta R.T. -0.01 min
Lab File: BF110918.D
Acq: 21 Nov 2018 3:30

Tgt Ion: 82	Resp:	381719
Ion Ratio	Lower	Upper
82	100	
128	46.1	34.2 51.2
54	53.2	38.6 58.0

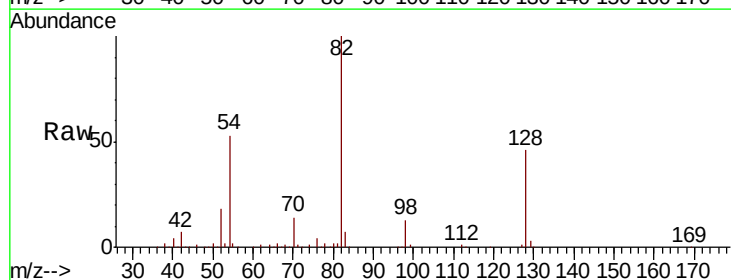

Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF1

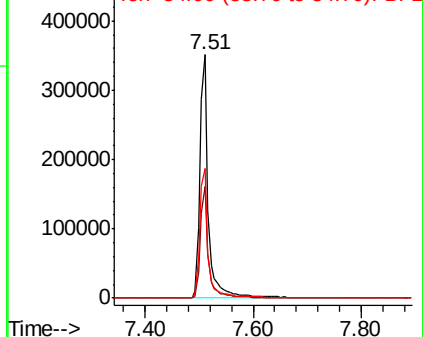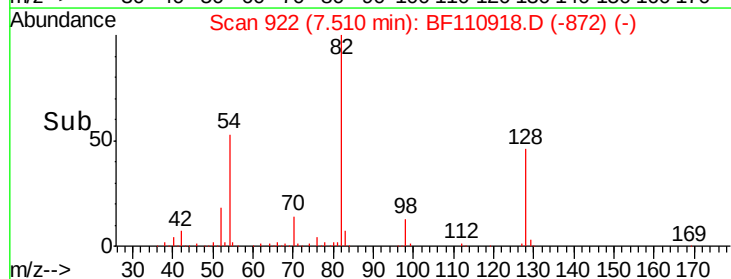



#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.98 min Scan# 1342

Delta R.T. -0.01 min

Lab File: BF110918.D

Acq: 21 Nov 2018 3:30

Instrument :

BNA_F

ClientSampleId :

NON-UST-06-A





Tot Ion:164 Resp: 87291

Ion Ratio Lower Upper

164 100

162 105.4 83.0 124.6

160 45.7 37.0 55.6

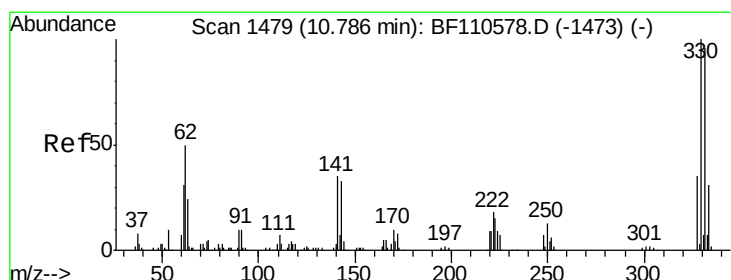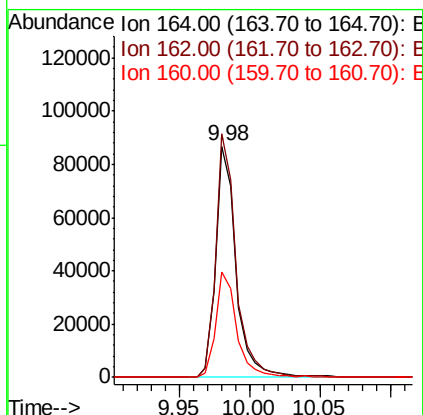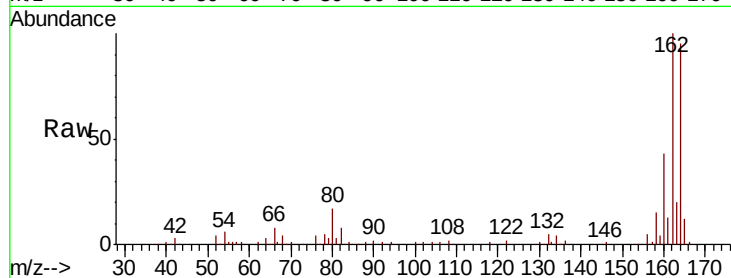

#42

2,4,6-Tribromophenol

Concen: 121.899 ng

RT: 10.78 min Scan# 1478

Delta R.T. -0.01 min

Lab File: BF110918.D

Acq: 21 Nov 2018 3:30




Tgt Ion:330 Resp: 107218


Ion Ratio Lower Upper

330 100

332 96.0 77.1 115.7

141 38.2 27.0 40.4


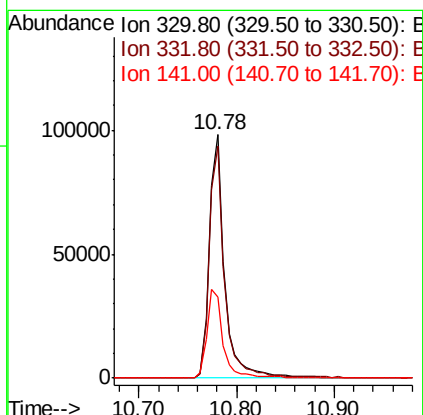

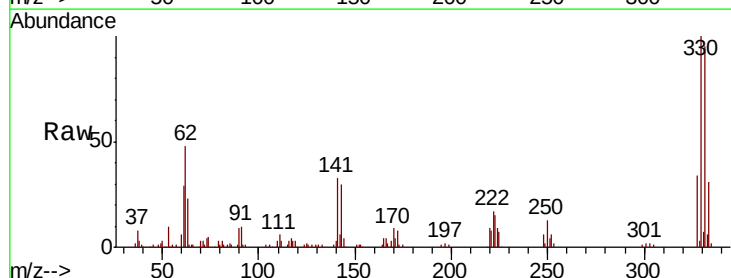




#45
2-Fluorobiphenyl
Concen: 106.170 ng
RT: 9.30 min Scan# 1226
Delta R.T. -0.01 min
Lab File: BF110918.D
Acq: 21 Nov 2018 3:30




Instrument :
BNA_F
ClientSampleId :
NON-UST-06-A


Tot Ion:172 Resp: 648913
Ion Ratio Lower Upper
172 100
171 35.8 28.6 43.0
170 23.0 19.7 29.5

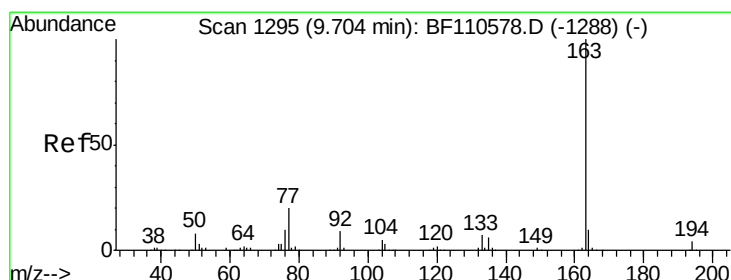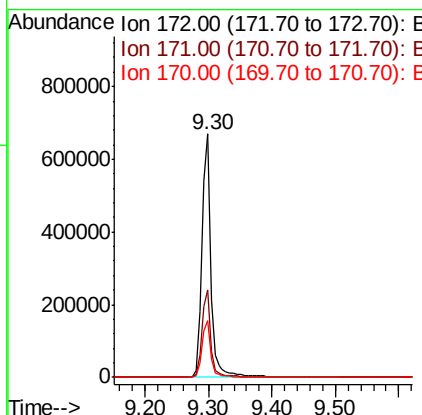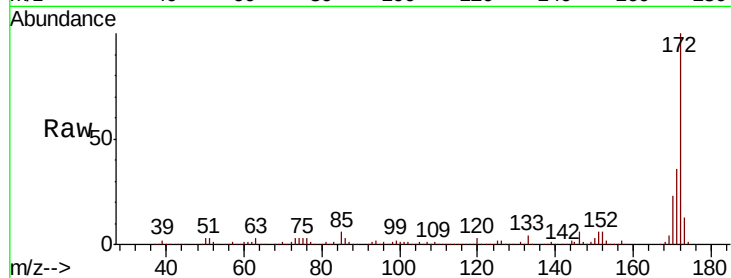

#50
Dimethylphthalate
Concen: 9.264 ng
RT: 9.69 min Scan# 1293
Delta R.T. -0.01 min
Lab File: BF110918.D
Acq: 21 Nov 2018 3:30

Tgt Ion:163 Resp: 60339
Ion Ratio Lower Upper
163 100
194 4.0 3.2 4.8
164 9.7 8.1 12.1

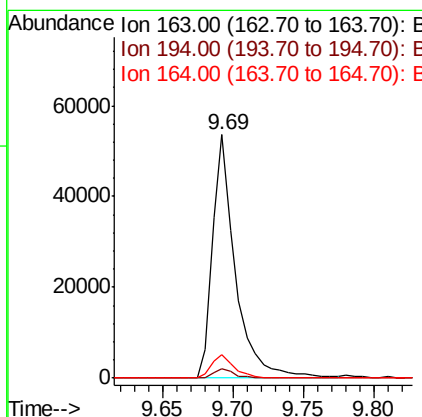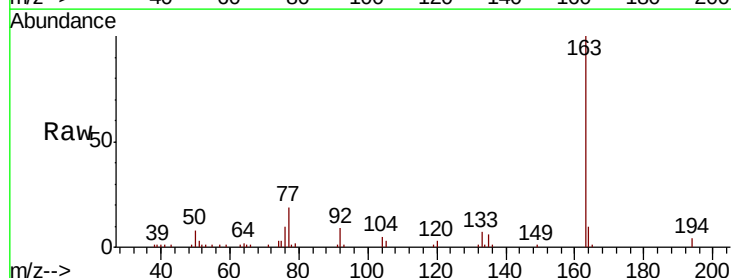


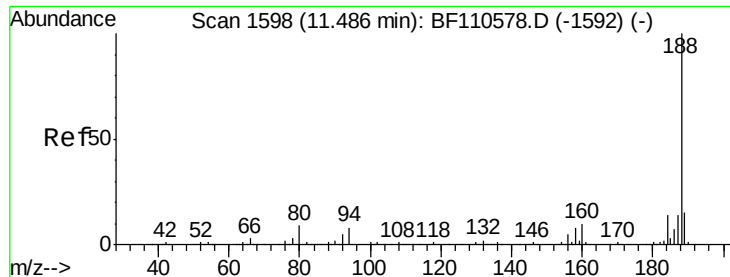




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.48 min Scan# 1597
Delta R.T. -0.01 min
Lab File: BF110918.D
Acq: 21 Nov 2018 3:30

Instrument :
BNA_F
ClientSampleId :
NON-UST-06-A

Tot Ion:188 Resp: 137260
Ion Ratio Lower Upper
188 100
94 7.9 7.2 10.8
80 8.6 7.9 11.9

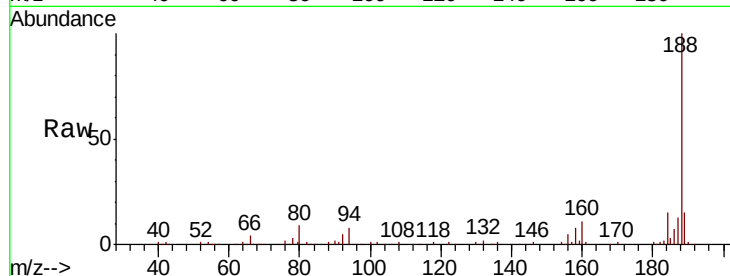


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF1
Ion 80.00 (79.70 to 80.70): BF1

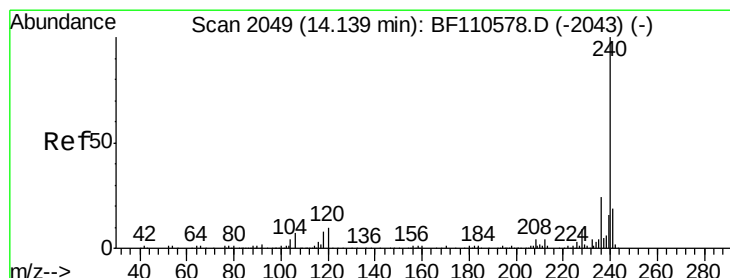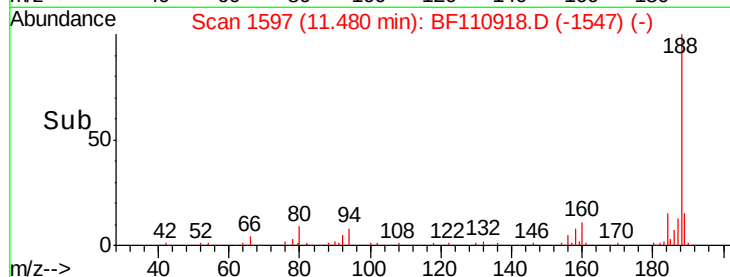
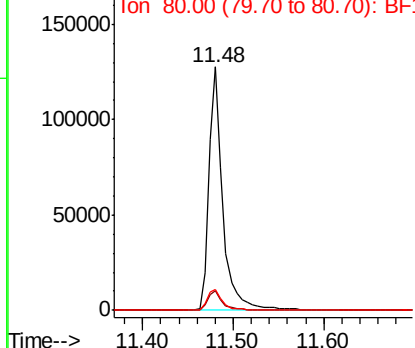



#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.13 min Scan# 2048
Delta R.T. -0.01 min
Lab File: BF110918.D
Acq: 21 Nov 2018 3:30

Tgt Ion:240 Resp: 118932
Ion Ratio Lower Upper
240 100
120 11.9 8.3 12.5
236 25.9 21.2 31.8

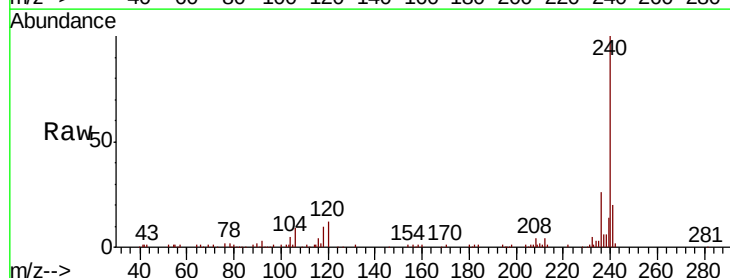

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

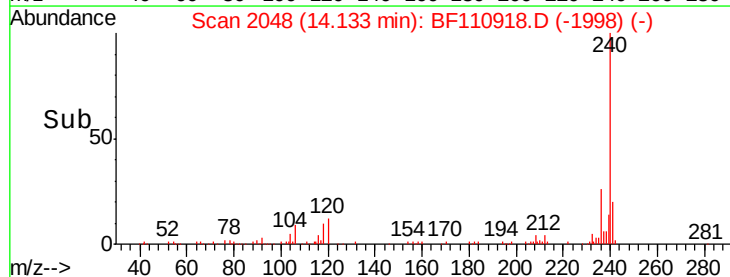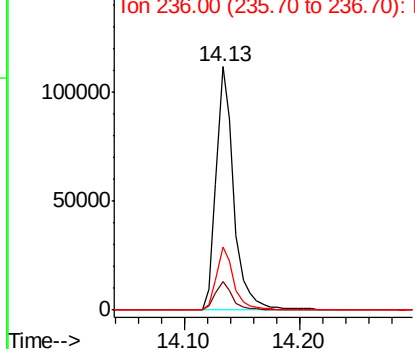

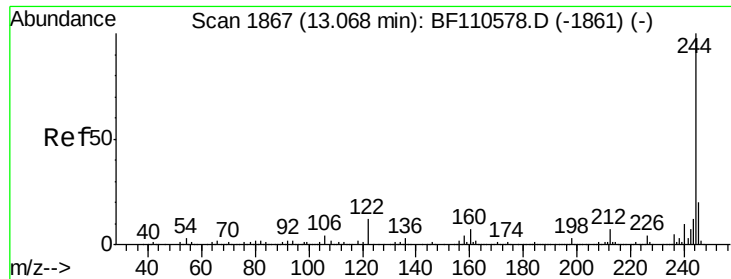

#79

Terphenyl-d14

Concen: 82.601 ng

RT: 13.06 min Scan# 1866

Delta R.T. -0.01 min

Lab File: BF110918.D

Acq: 21 Nov 2018 3:30

Instrument :

BNA_F

ClientSampleId :

NON-UST-06-A


Tot Ion:244 Resp: 524568

Ion Ratio Lower Upper

244 100

212 6.7 5.8 8.8




122 10.5 8.7 13.1

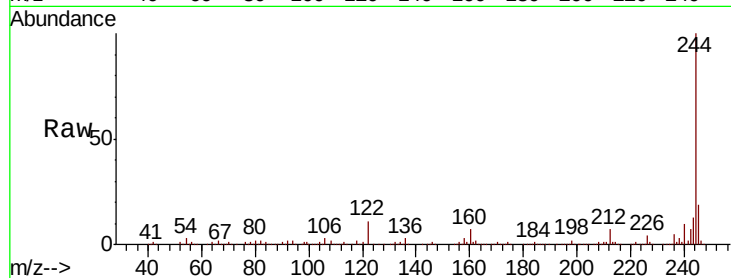

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

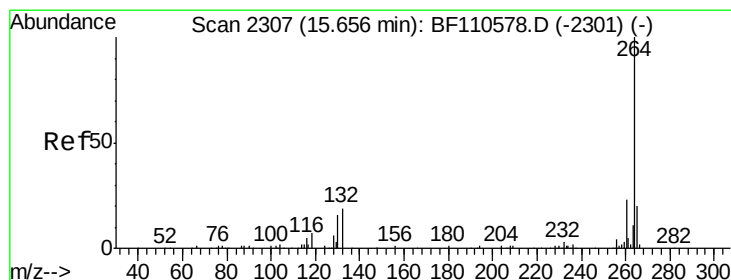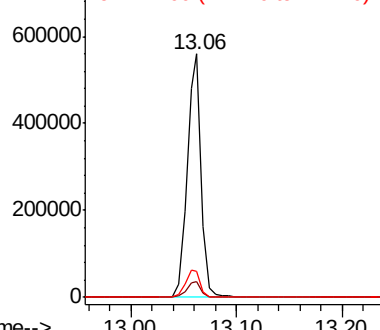

#87

Perylene-d12

Concen: 20.000 ng

RT: 15.67 min Scan# 2309

Delta R.T. 0.01 min

Lab File: BF110918.D

Acq: 21 Nov 2018 3:30


Tgt Ion:264 Resp: 77442

Ion Ratio Lower Upper

264 100

260 24.9 18.7 28.1

265 21.5 16.7 25.1

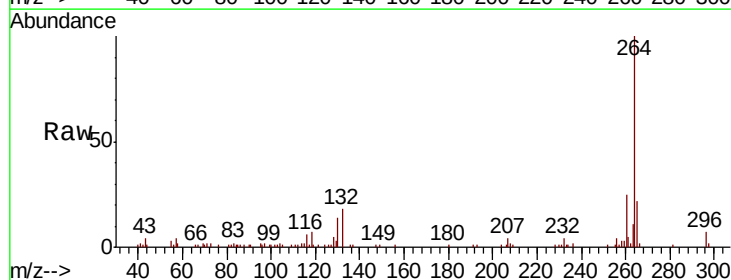

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

