
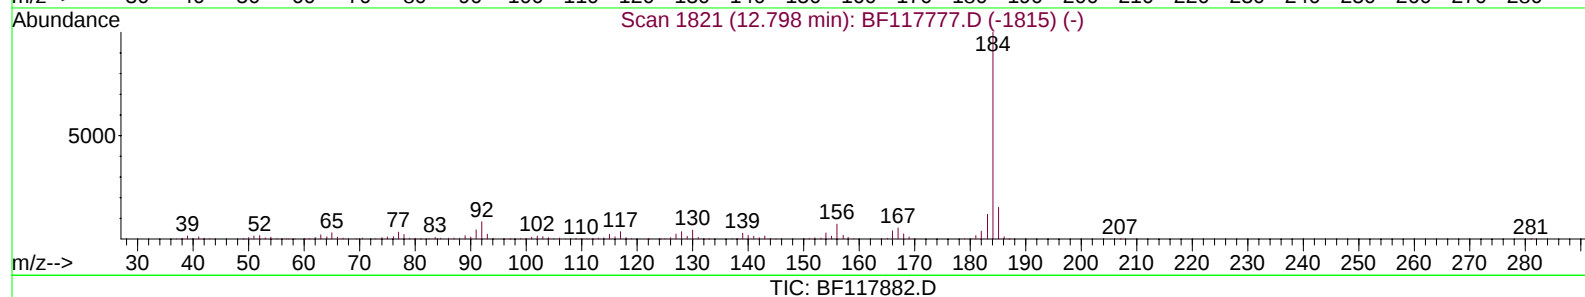
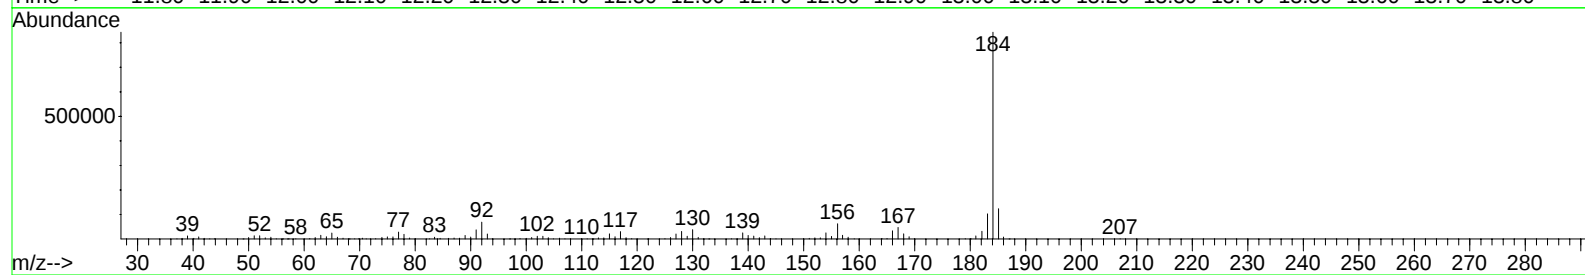


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF112019\
 Data File : BF117882.D
 Acq On : 20 Nov 2019 9:52
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 20 18:35:27 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF111319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 13 18:36:07 2019
 Response via : Initial Calibration

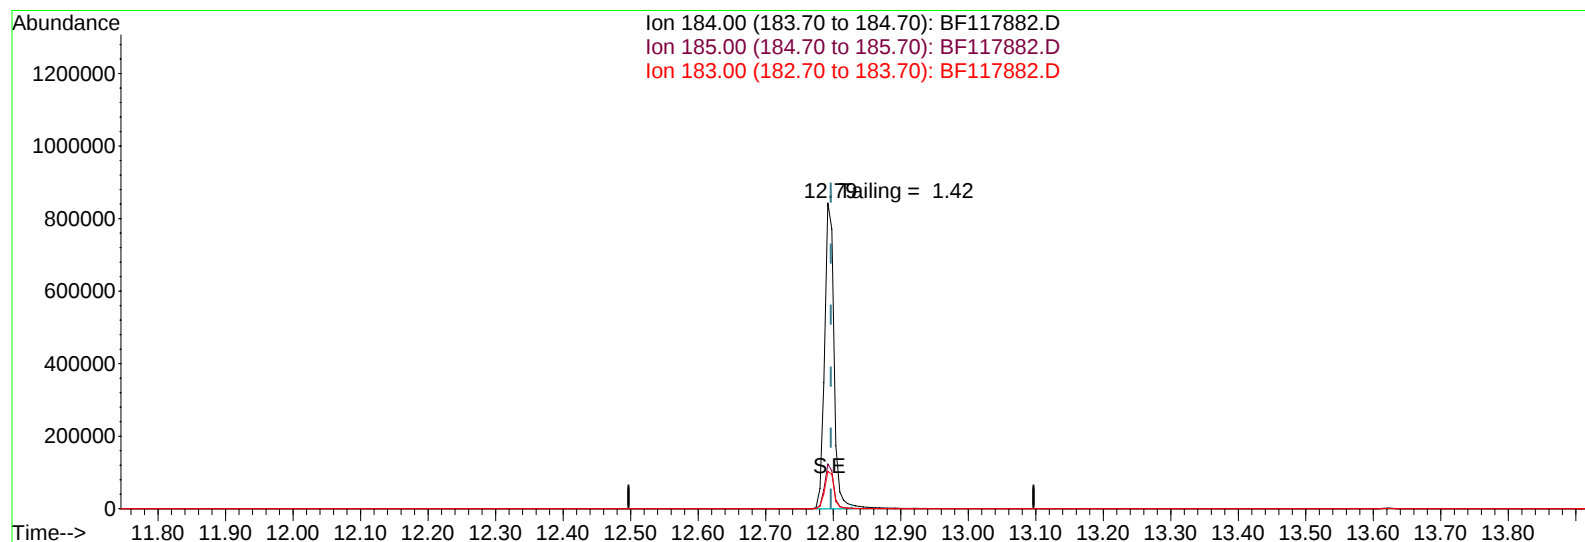

(77) Benzidine




12.792min (-0.005) 0.00ng

response 823305

Ion	Exp%	Act%
184.00	100	100
185.00	15.30	14.66
183.00	11.90	12.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF112019\
Data File : BF117882.D
Acq On : 20 Nov 2019 9:52
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 20 18:35:27 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF111319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 18:36:07 2019
Response via : Initial Calibration

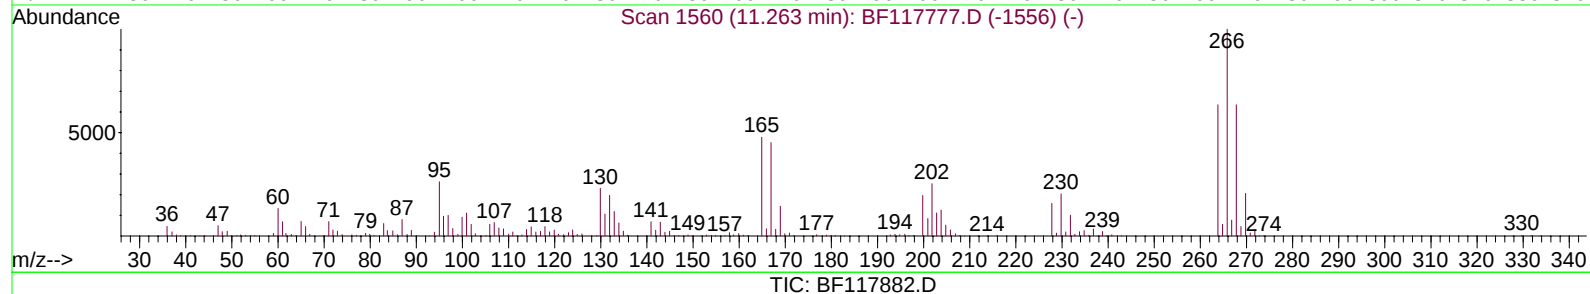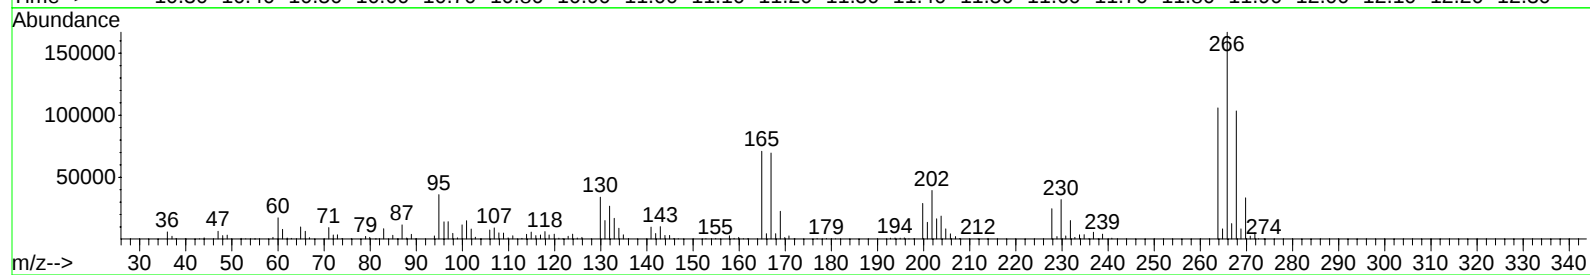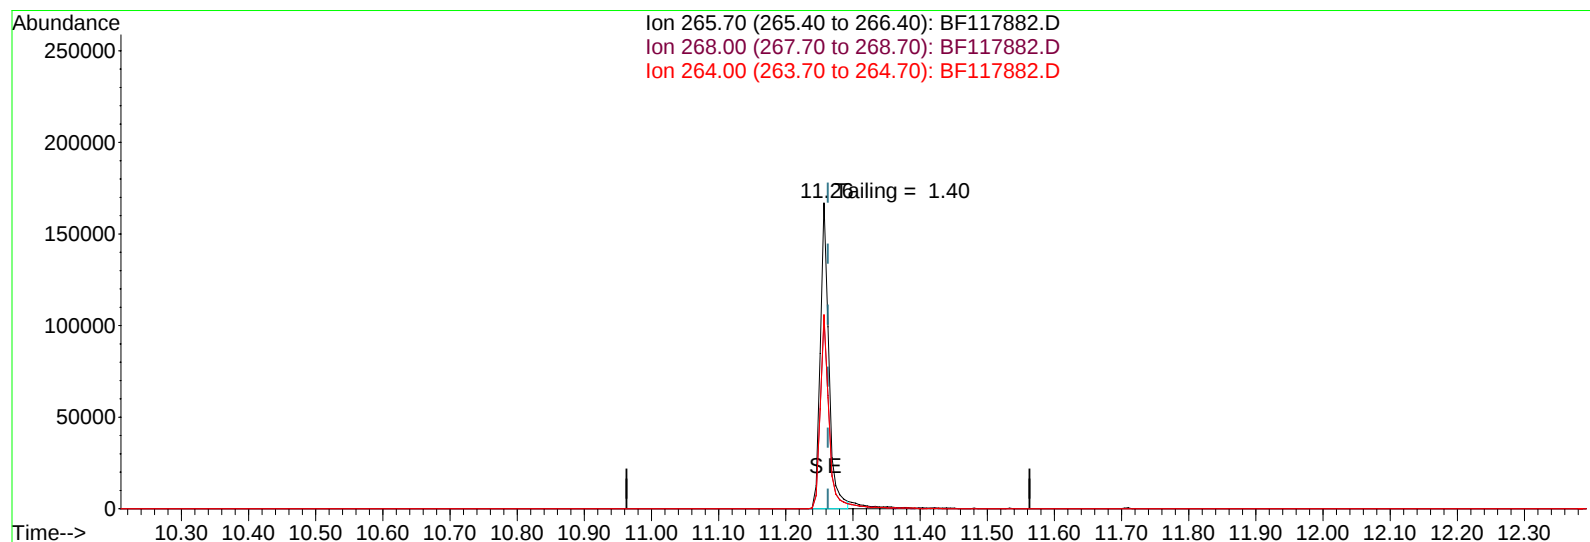

(70) Pentachlorophenol (C)

11.257min (-0.006) 31863.82ng

response 156456

Ion	Exp%	Act%
265.70	100	100
268.00	63.50	61.96
264.00	63.40	63.49
0.00	0.00	0.00