


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF112019\
 Data File : BF117882.D
 Acq On : 20 Nov 2019 9:52
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF111319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 13 18:36:07 2019

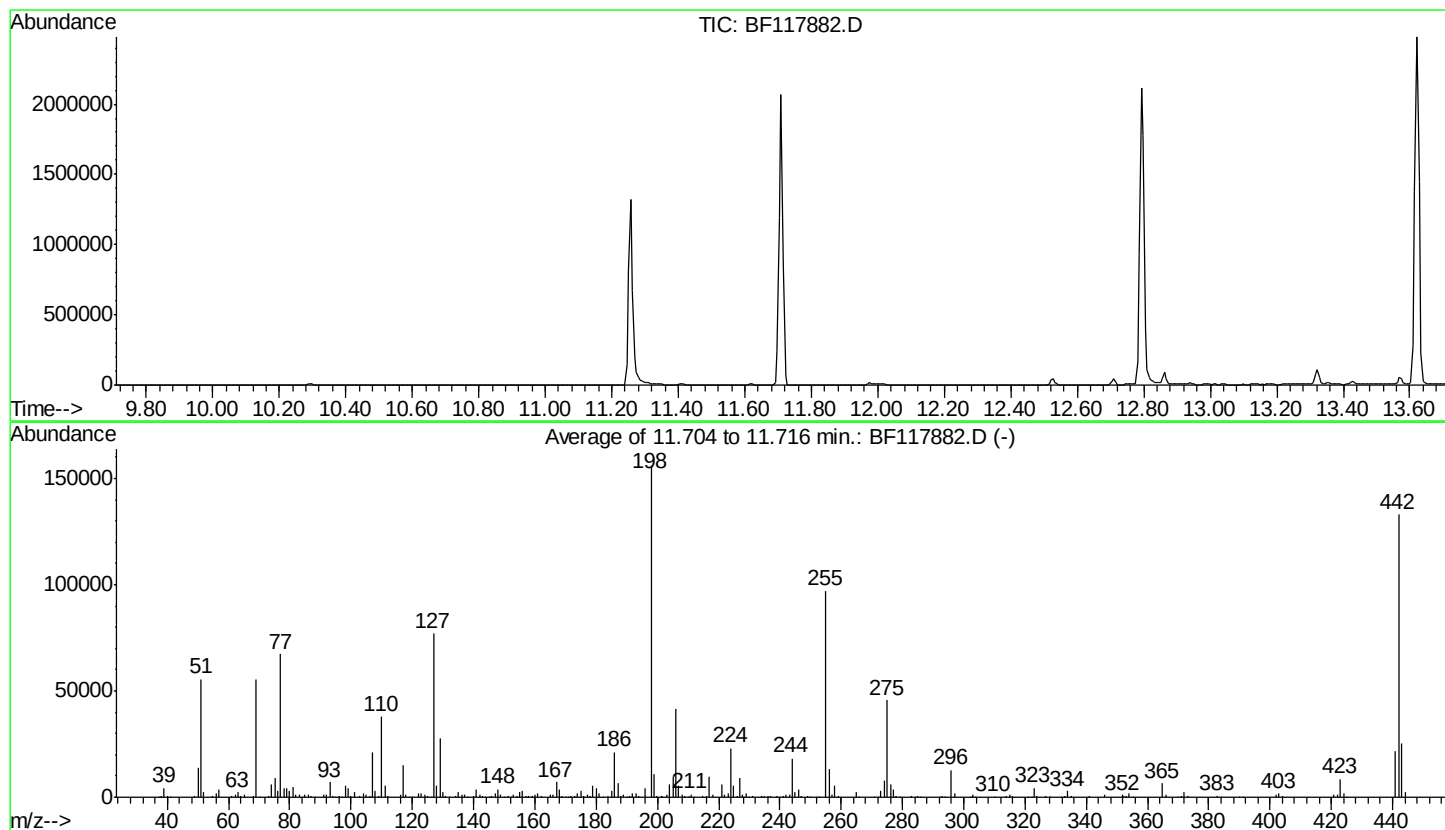

AutoFind: Scans 1635, 1636, 1637; Background Corrected with Scan 1630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.6	55573	PASS
68	69	0.00	2	1.7	915	PASS
69	198	0.00	100	35.3	55138	PASS
70	69	0.00	2	0.5	292	PASS
127	198	10	80	49.3	76970	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	155978	PASS
199	198	5	9	6.8	10662	PASS
275	198	10	60	29.2	45570	PASS
365	198	1	100	4.2	6590	PASS
441	198	0.01	100	13.8	21510	PASS
442	198	50	100	85.2	132882	PASS
443	442	15	24	18.8	25047	PASS