
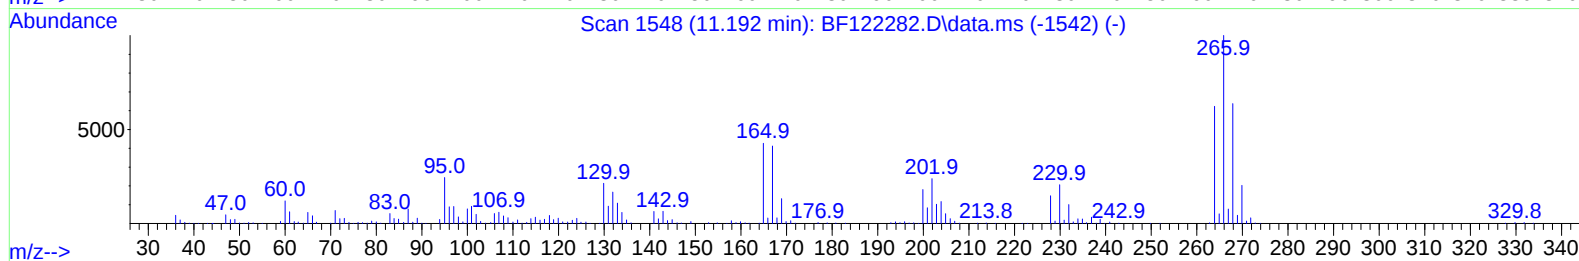
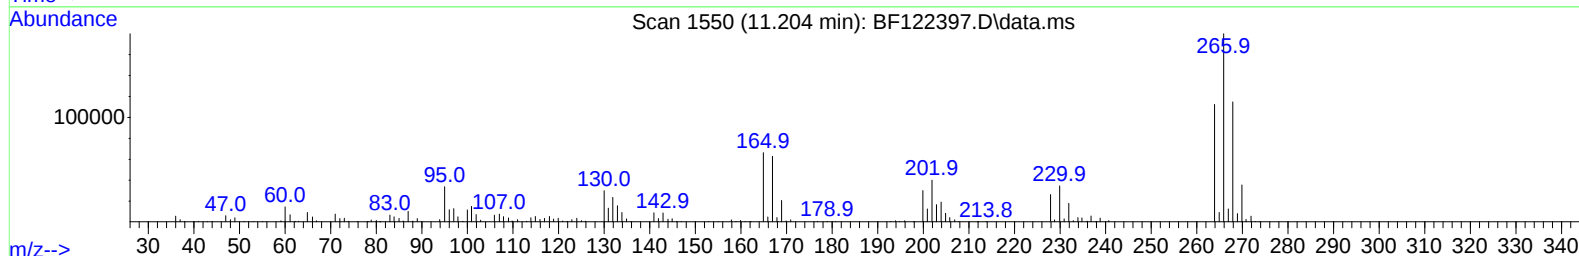


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112020\
Data File : BF122397.D
Acq On : 20 Nov 2020 11:54
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 21 07:52:56 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 20 13:27:02 2020
Response via : Initial Calibration

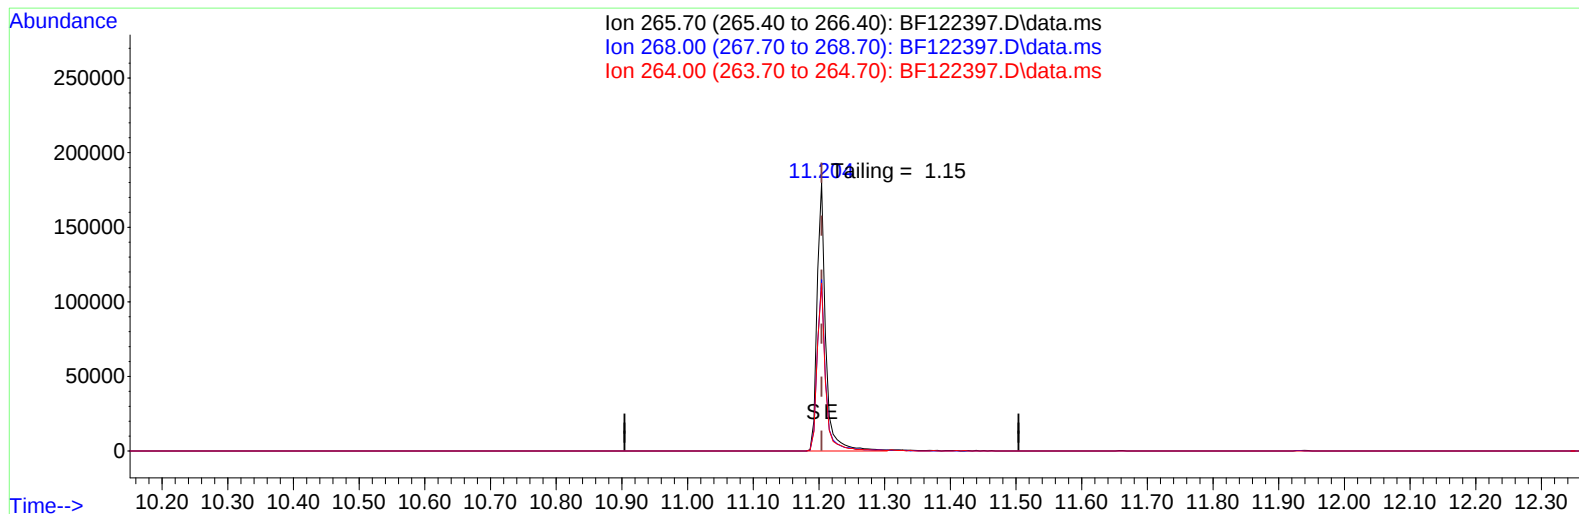

TIC: BF122397.D\data.ms

(70) Pentachlorophenol (C)




11.204min (+ 0.000) 108757.76 ng

response 167062

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.50	63.83
264.00	62.40	62.46
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112020\
Data File : BF122397.D
Acq On : 20 Nov 2020 11:54
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 21 07:52:56 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 20 13:27:02 2020
Response via : Initial Calibration

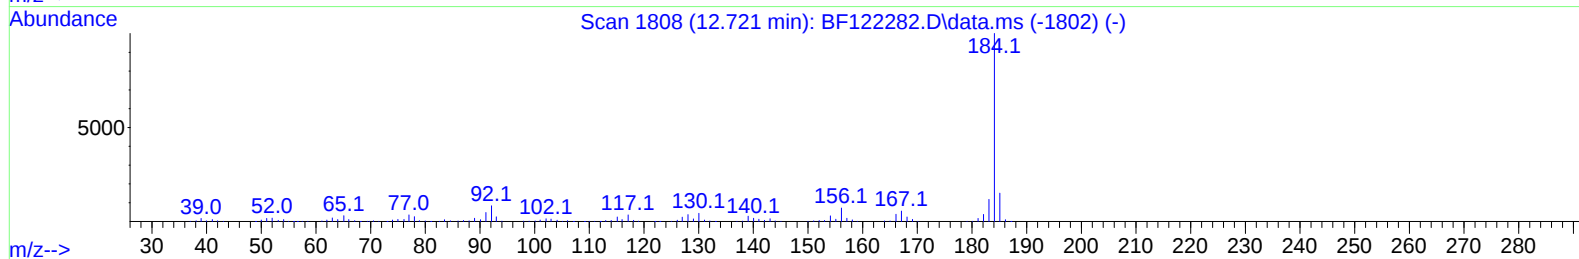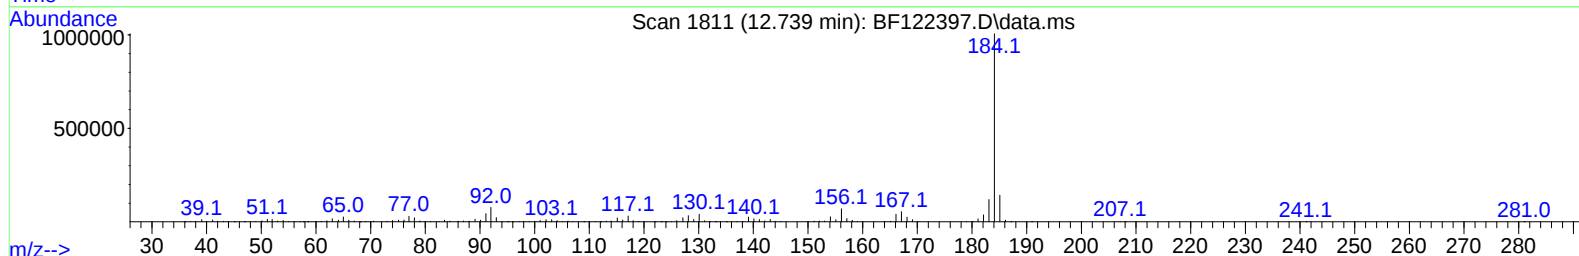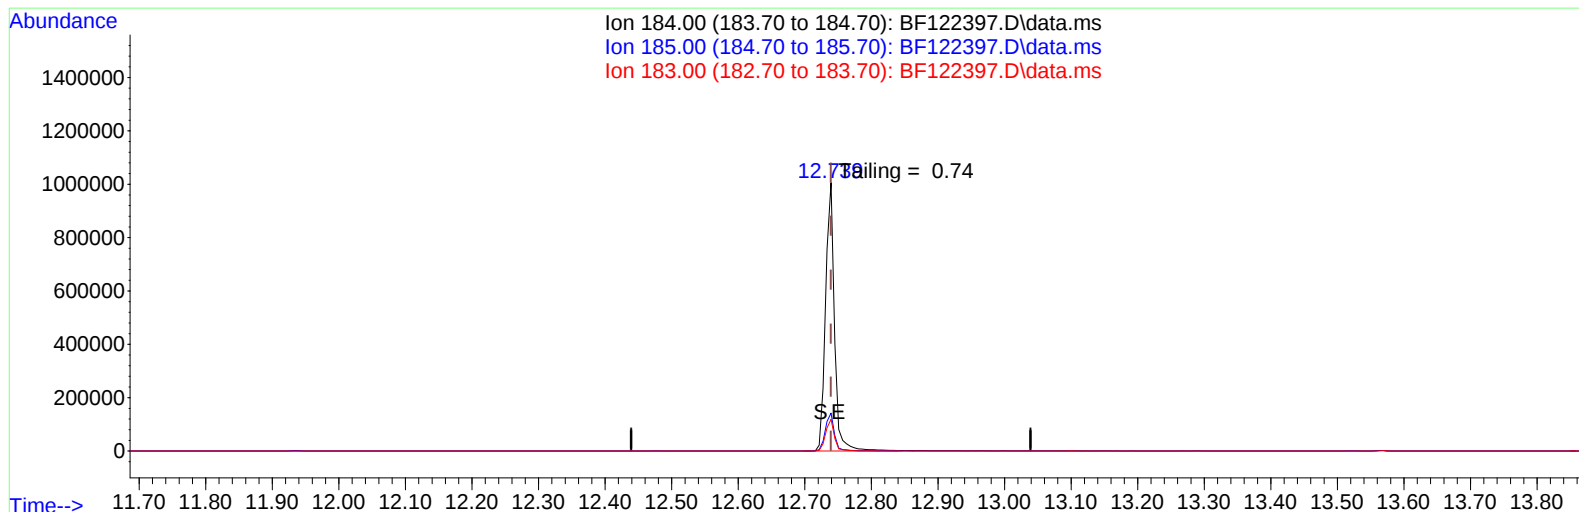

TIC: BF122397.D\data.ms

(77) Benzidine

12.739min (+ 0.000) 47954.47 ng

response 937696

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.14
183.00	11.70	11.82
0.00	0.00	0.00