

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112020\
 Data File : BF122399.D
 Acq On : 20 Nov 2020 12:57
 Operator : JU/CG
 Sample : PB133132BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB133132BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF122399.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.498	575	580	583	rBV	5221936	4876092	61.33%	10.065%
2	6.498	744	750	753	rBV	4596265	5069985	63.77%	10.466%
3	6.863	808	812	815	rBV	2195941	1754487	22.07%	3.622%
4	7.428	902	908	911	rBV	2928084	3296682	41.47%	6.805%
5	8.151	1025	1031	1034	rBV	2342844	2340431	29.44%	4.831%
6	9.227	1208	1214	1217	rBV	6271087	6436431	80.96%	13.286%
7	9.910	1323	1330	1333	rBV	3133919	2908206	36.58%	6.003%
8	10.698	1458	1464	1467	rBV	4550999	4320236	54.34%	8.918%
9	11.398	1577	1583	1586	rBV	3400208	3097322	38.96%	6.394%
10	12.810	1820	1823	1827	rVB	153457	120071	1.51%	0.248%
11	12.992	1846	1854	1857	rBV	8023692	7950093	100.00%	16.411%
12	13.515	1940	1943	1948	rVB	97313	85991	1.08%	0.178%
13	14.045	2028	2033	2036	rBV	3134669	3152800	39.66%	6.508%
14	15.521	2278	2284	2289	rBV	2303031	3035296	38.18%	6.266%




Sum of corrected areas: 48444123

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112020\
Data File : BF122399.D
Acq On : 20 Nov 2020 12:57
Operator : JU/CG
Sample : PB133132BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB133132BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

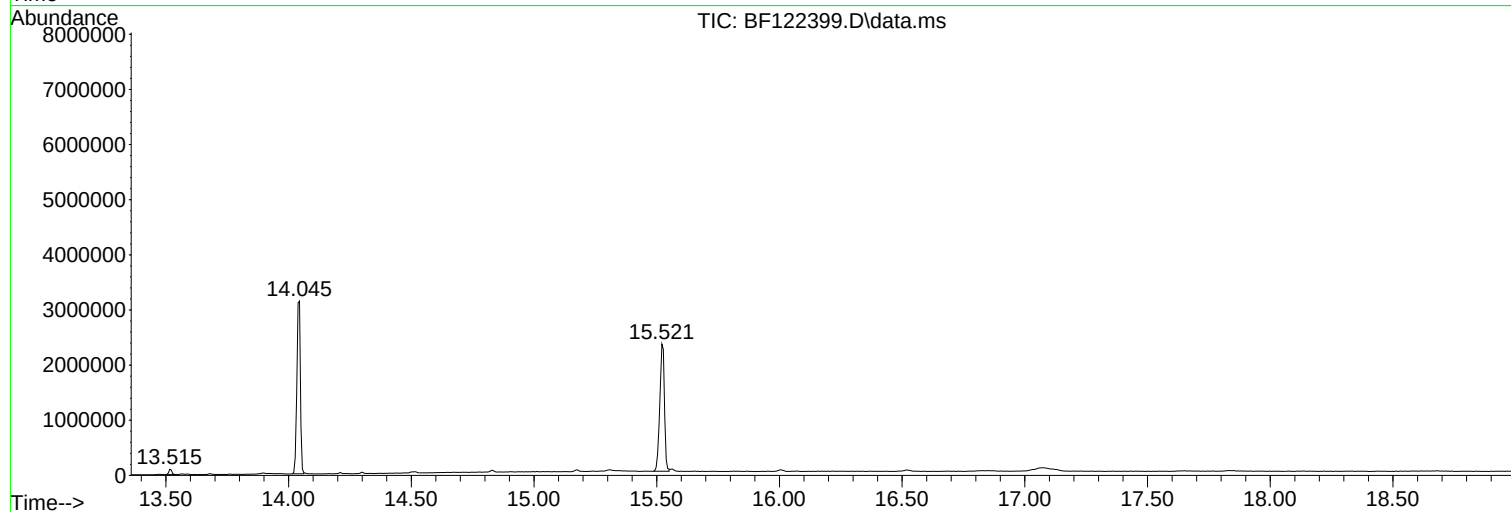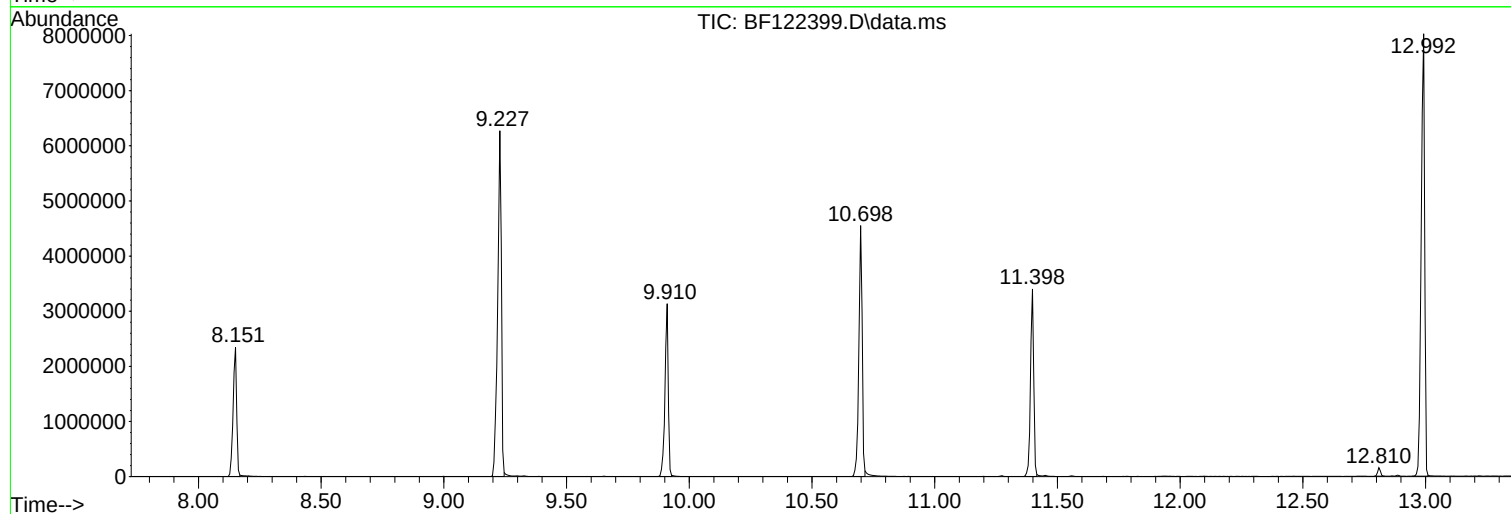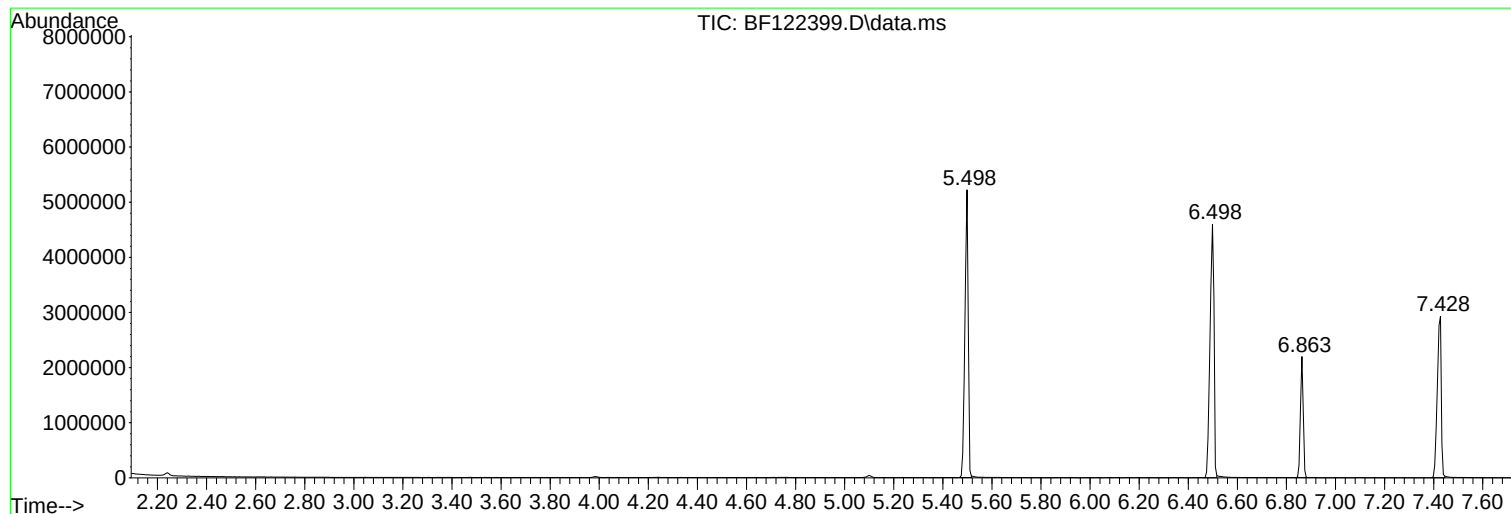

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112020\
Data File : BF122399.D
Acq On : 20 Nov 2020 12:57
Operator : JU/CG
Sample : PB133132BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB133132BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112020\
Data File : BF122399.D
Acq On : 20 Nov 2020 12:57
Operator : JU/CG
Sample : PB133132BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB133132BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------