
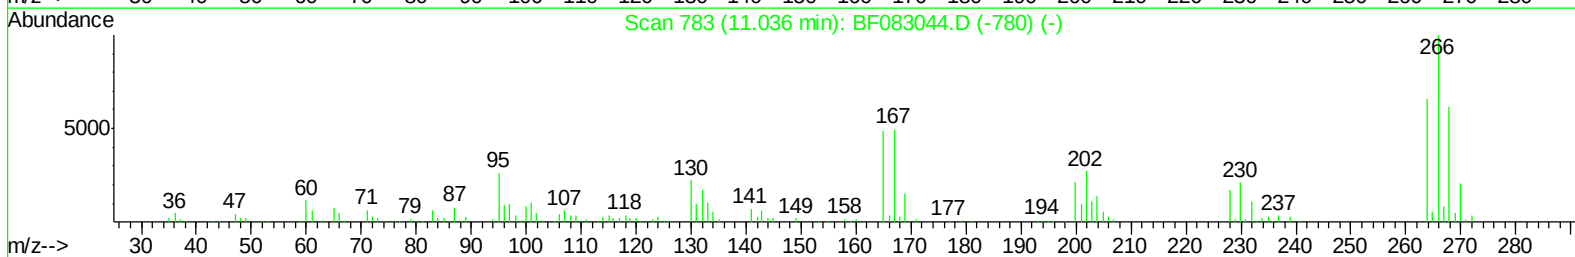
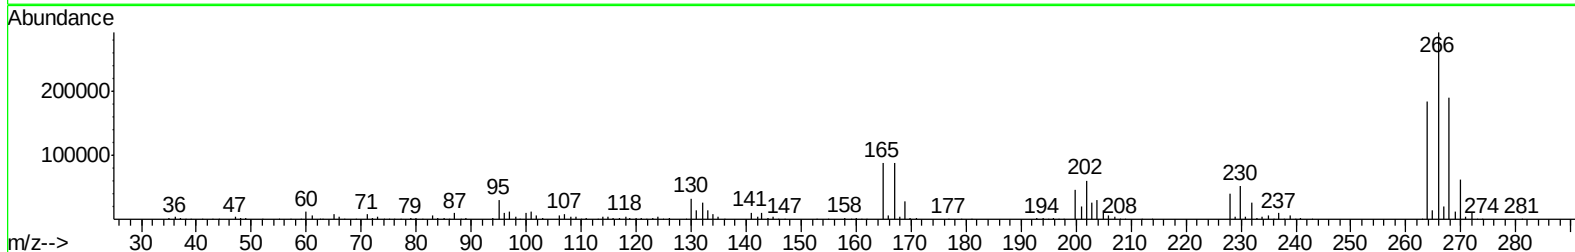


Data Path : Z:\HPCHEM1\BNA_F\Data\BF112115\
Data File : BF083108.D
Acq On : 21 Nov 2015 11:14
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 27 03:28:19 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF111915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 20 01:33:39 2015
Response via : Initial Calibration

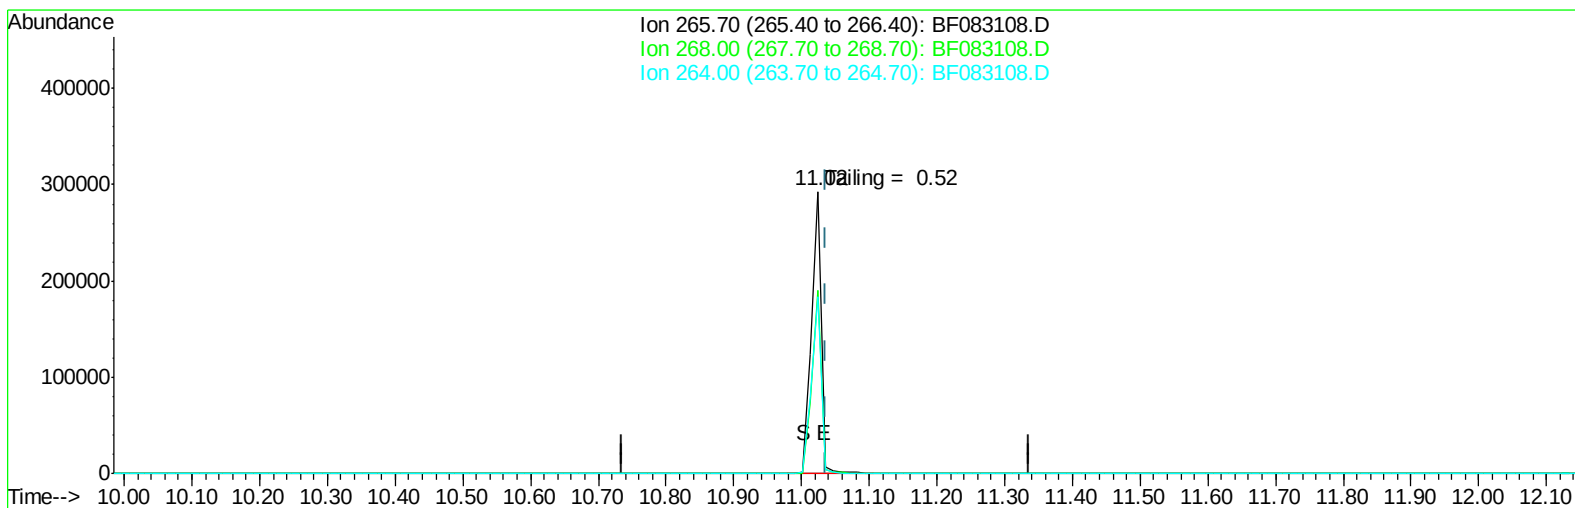

TIC: BF083108.D

(69) Pentachlorophenol (C)




11.025min (-0.011) 55728.42ng

response 296166

Ion	Exp%	Act%
265.70	100	100
268.00	62.00	64.81
264.00	65.90	62.84
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF112115\
 Data File : BF083108.D
 Acq On : 21 Nov 2015 11:14
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 27 03:28:19 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF111915.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 20 01:33:39 2015
 Response via : Initial Calibration

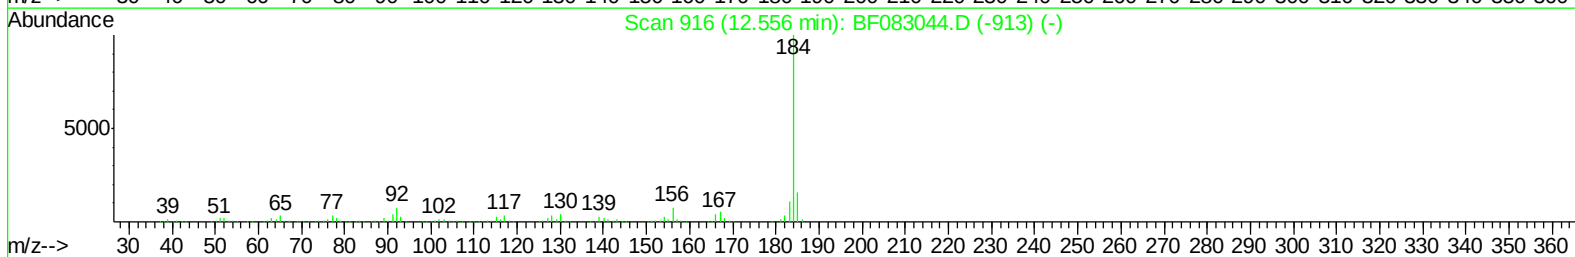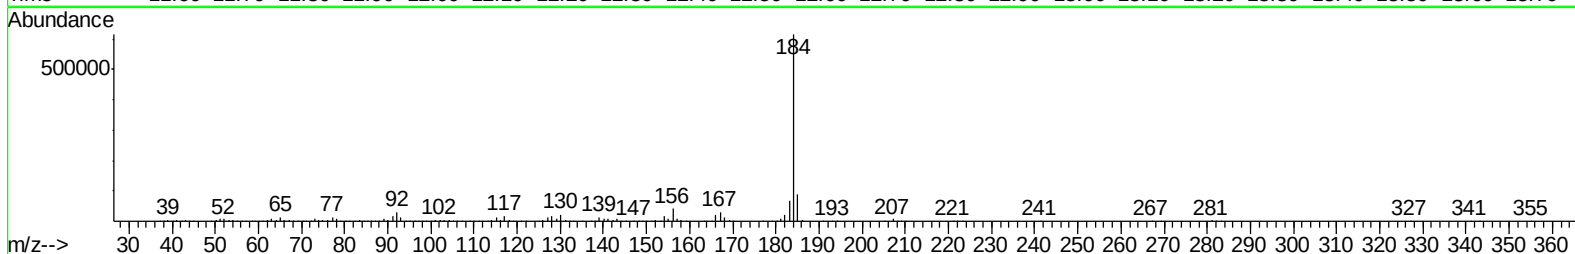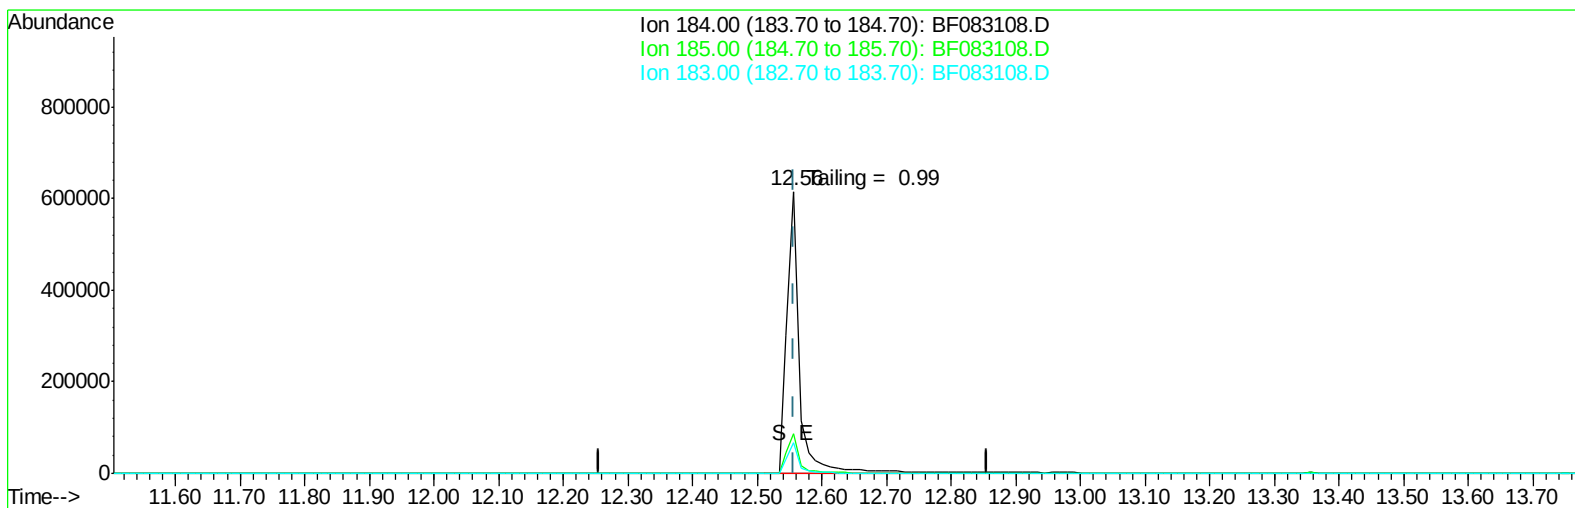

TIC: BF083108.D

(76) Benzidine

12.556min (+0.000) 33238.95ng

response 835286

Ion	Exp%	Act%
184.00	100	100
185.00	15.80	14.31
183.00	11.20	10.96
0.00	0.00	0.00