


Data Path : V:\HPCHEM1\BNA F\DATA\BF112115\
 Data File : BF083108.D
 Acq On : 21 Nov 2015 11:14
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF112115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sun Nov 22 09:22:46 2015

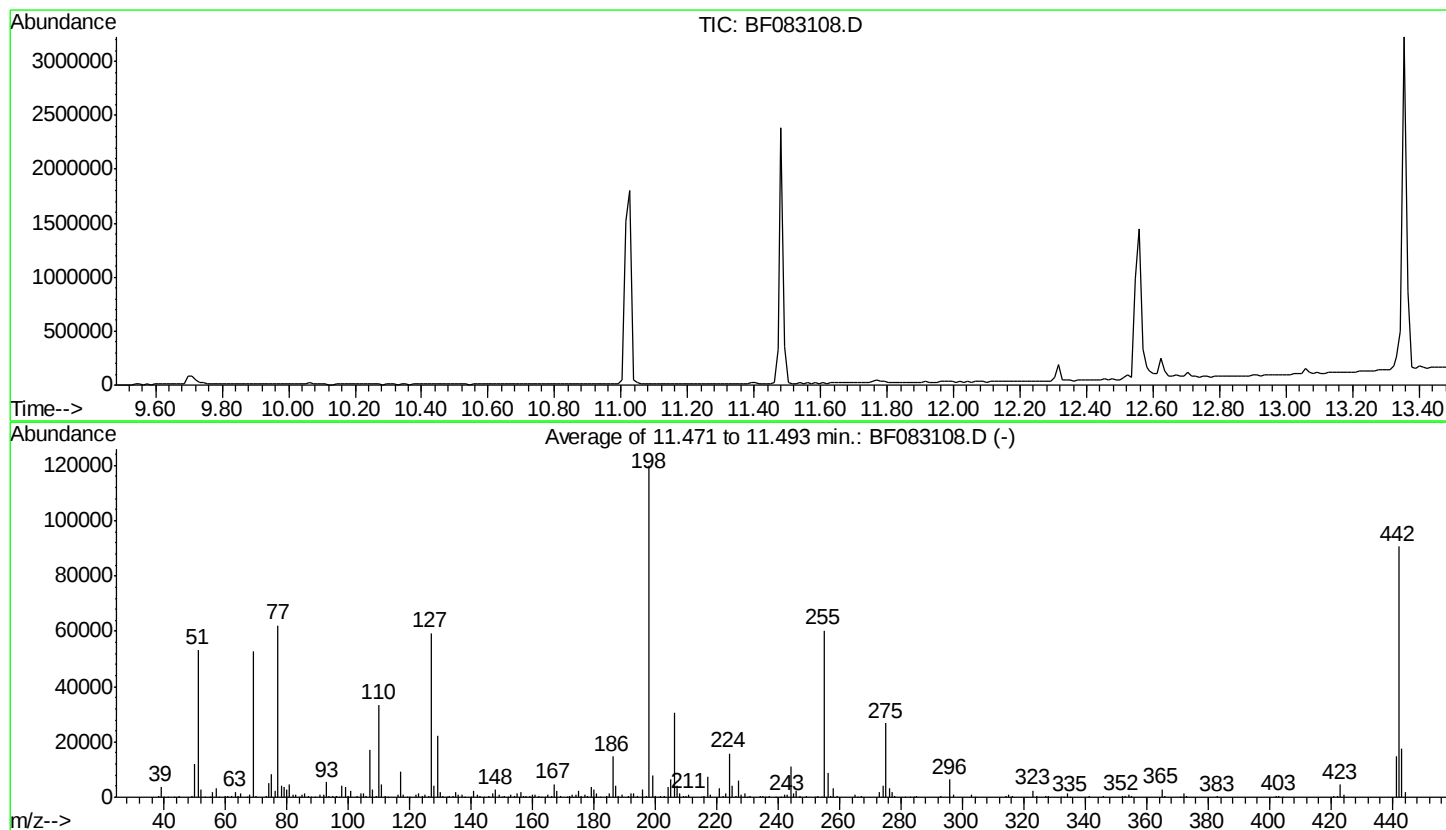

AutoFind: Scans 821, 822, 823; Background Corrected with Scan 817

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.5	53392	PASS
68	69	0.00	2	1.6	857	PASS
69	198	0.00	100	44.1	52901	PASS
70	69	0.00	2	0.5	273	PASS
127	198	10	80	49.5	59410	PASS
197	198	0.00	2	0.4	524	PASS
198	198	100	100	100.0	119944	PASS
199	198	5	9	6.5	7767	PASS
275	198	10	60	22.3	26743	PASS
365	198	1	100	2.4	2841	PASS
441	442	0.01	24	16.3	14816	PASS
442	198	50	100	75.6	90674	PASS
443	442	15	24	19.4	17589	PASS