


Data Path : V:\HPCHEM1\BNA F\DATA\BF112115\
Data File : BF083126.D
Acq On : 21 Nov 2015 22:29
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF112115.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sun Nov 22 09:22:46 2015

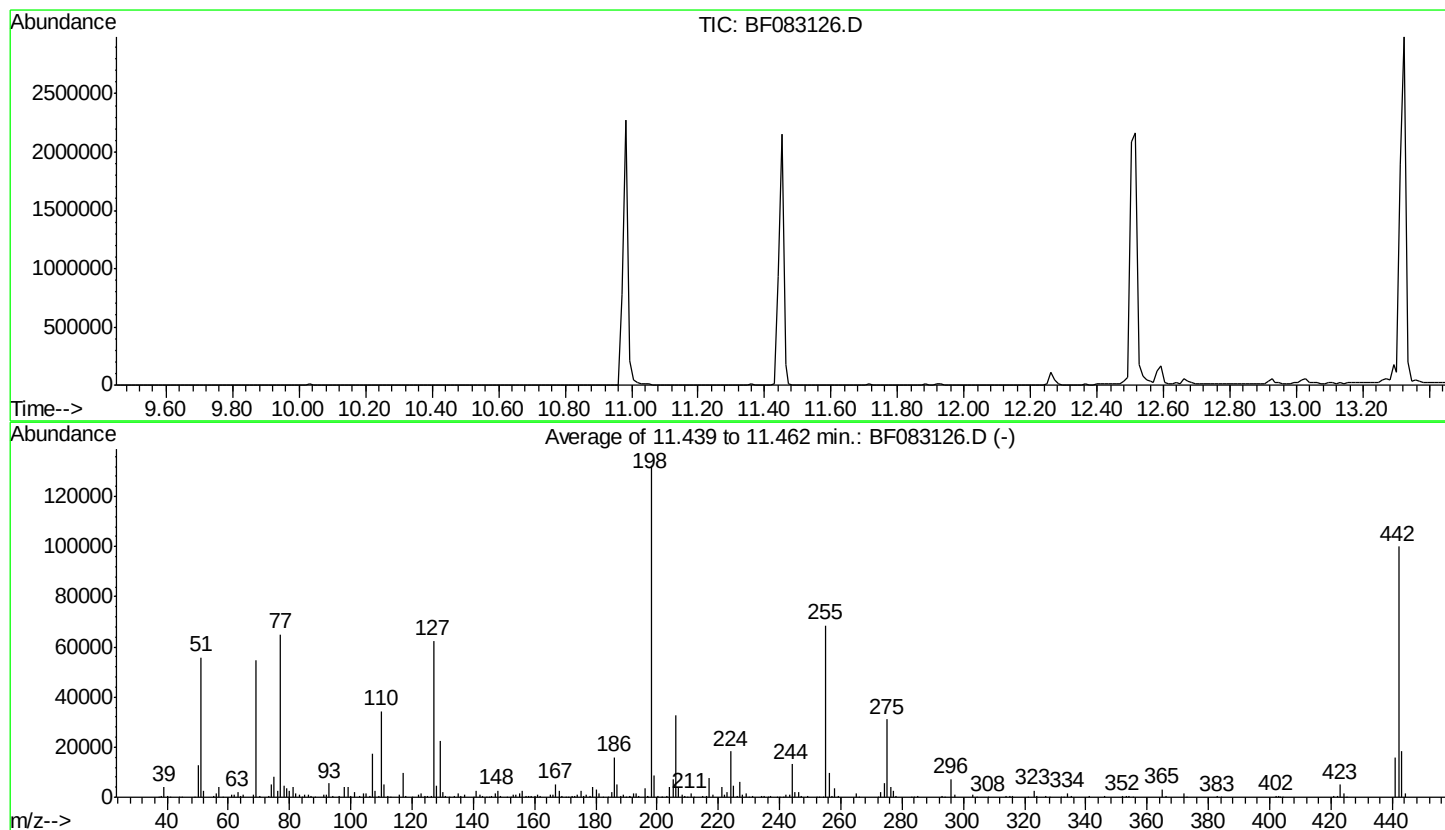

AutoFind: Scans 827, 828, 829; Background Corrected with Scan 823

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.2	55864	PASS
68	69	0.00	2	1.5	793	PASS
69	198	0.00	100	41.3	54616	PASS
70	69	0.00	2	0.6	340	PASS
127	198	10	80	47.2	62509	PASS
197	198	0.00	2	0.5	604	PASS
198	198	100	100	100.0	132357	PASS
199	198	5	9	6.6	8693	PASS
275	198	10	60	23.5	31126	PASS
365	198	1	100	2.3	3105	PASS
441	442	0.01	24	15.7	15675	PASS
442	198	50	100	75.6	100057	PASS
443	442	15	24	18.3	18323	PASS