



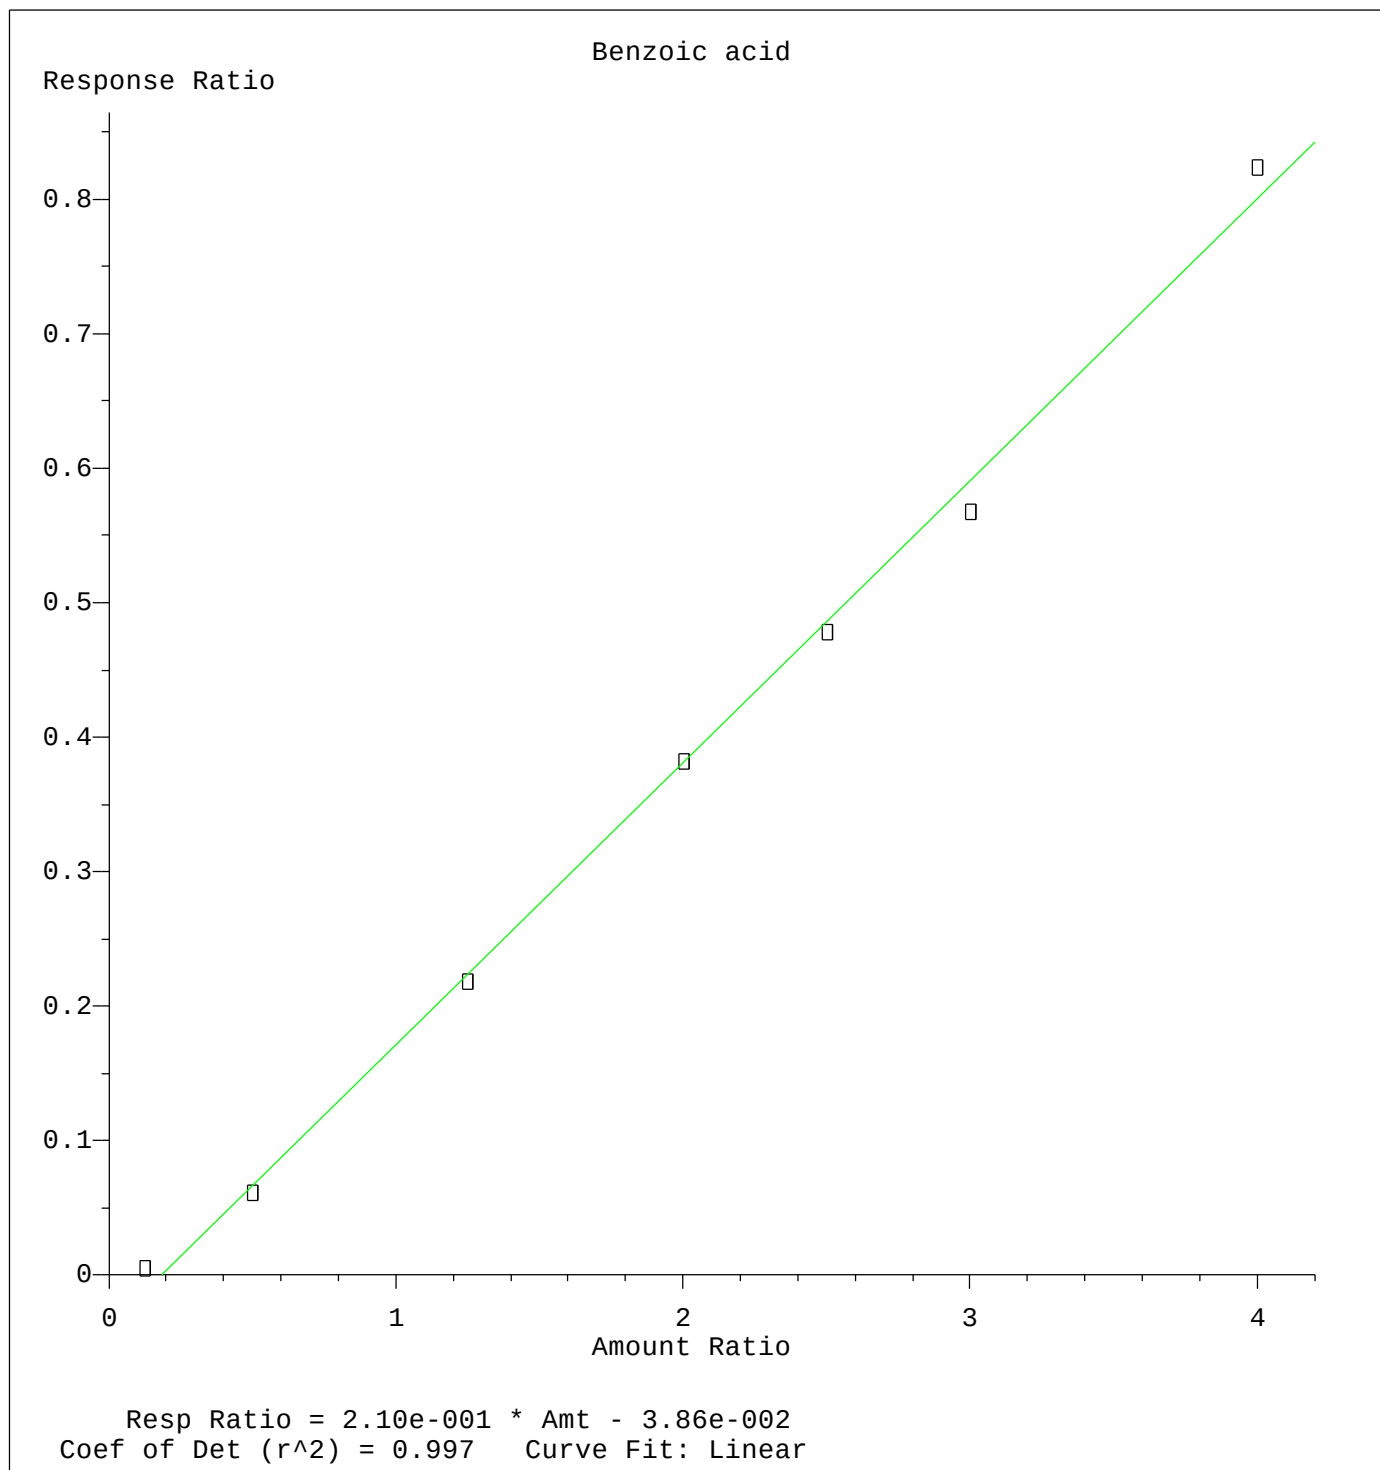

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF112116.M
Calibration Table Last Updated: Tue Nov 22 10:25:16 2016


Hexachlorocyclopentadiene

Response Ratio

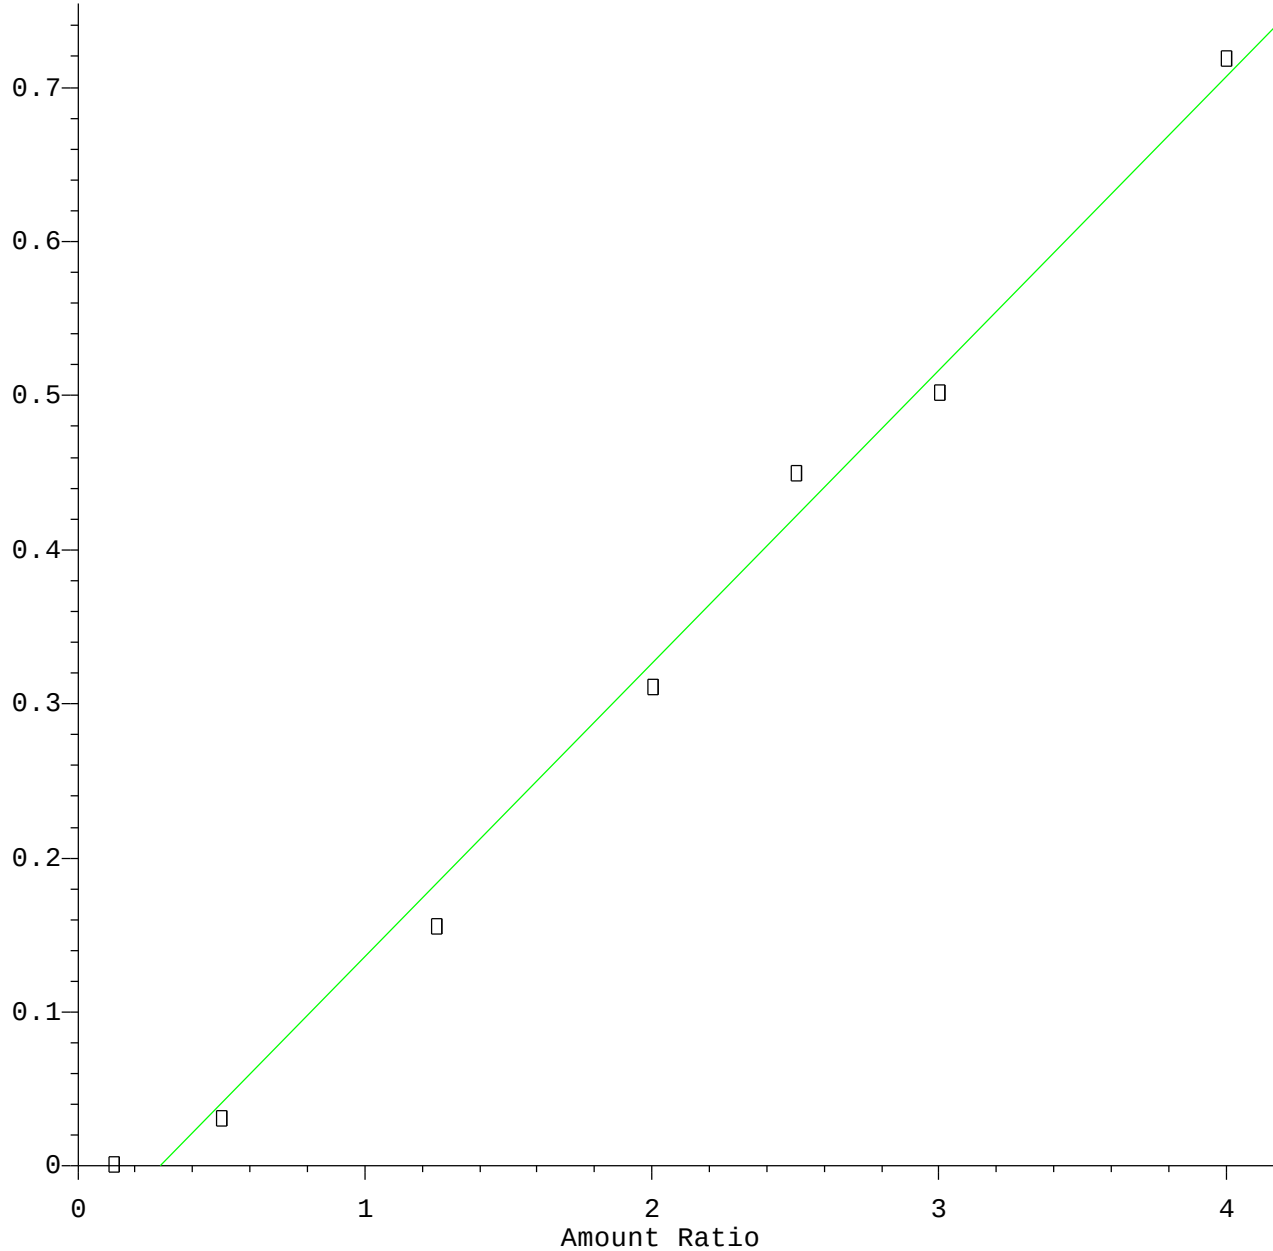


Resp Ratio = $1.90 \times 10^{-1} \times \text{Amt} - 5.38 \times 10^{-2}$
Coef of Det (r^2) = 0.992 Curve Fit: Linear


Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF112116.M
Calibration Table Last Updated: Tue Nov 22 10:25:16 2016

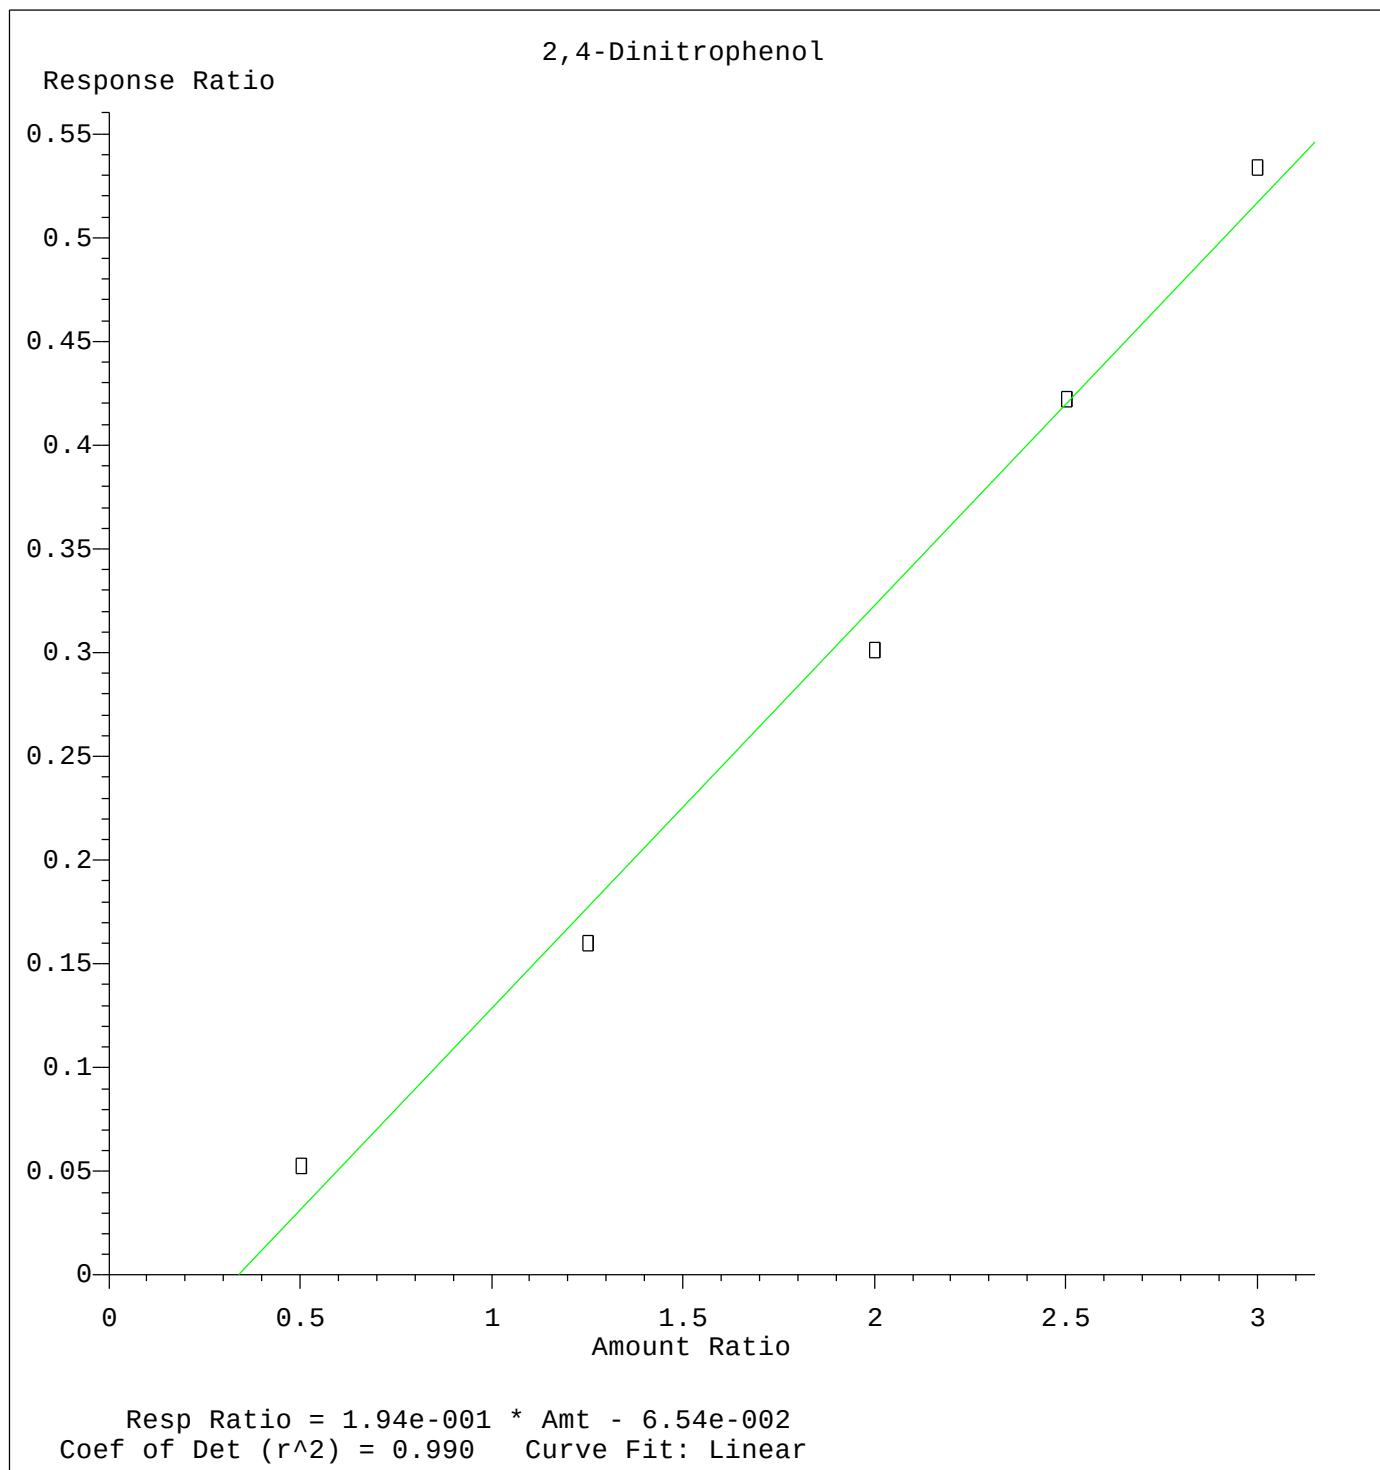

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF112116.M
Calibration Table Last Updated: Tue Nov 22 10:25:16 2016

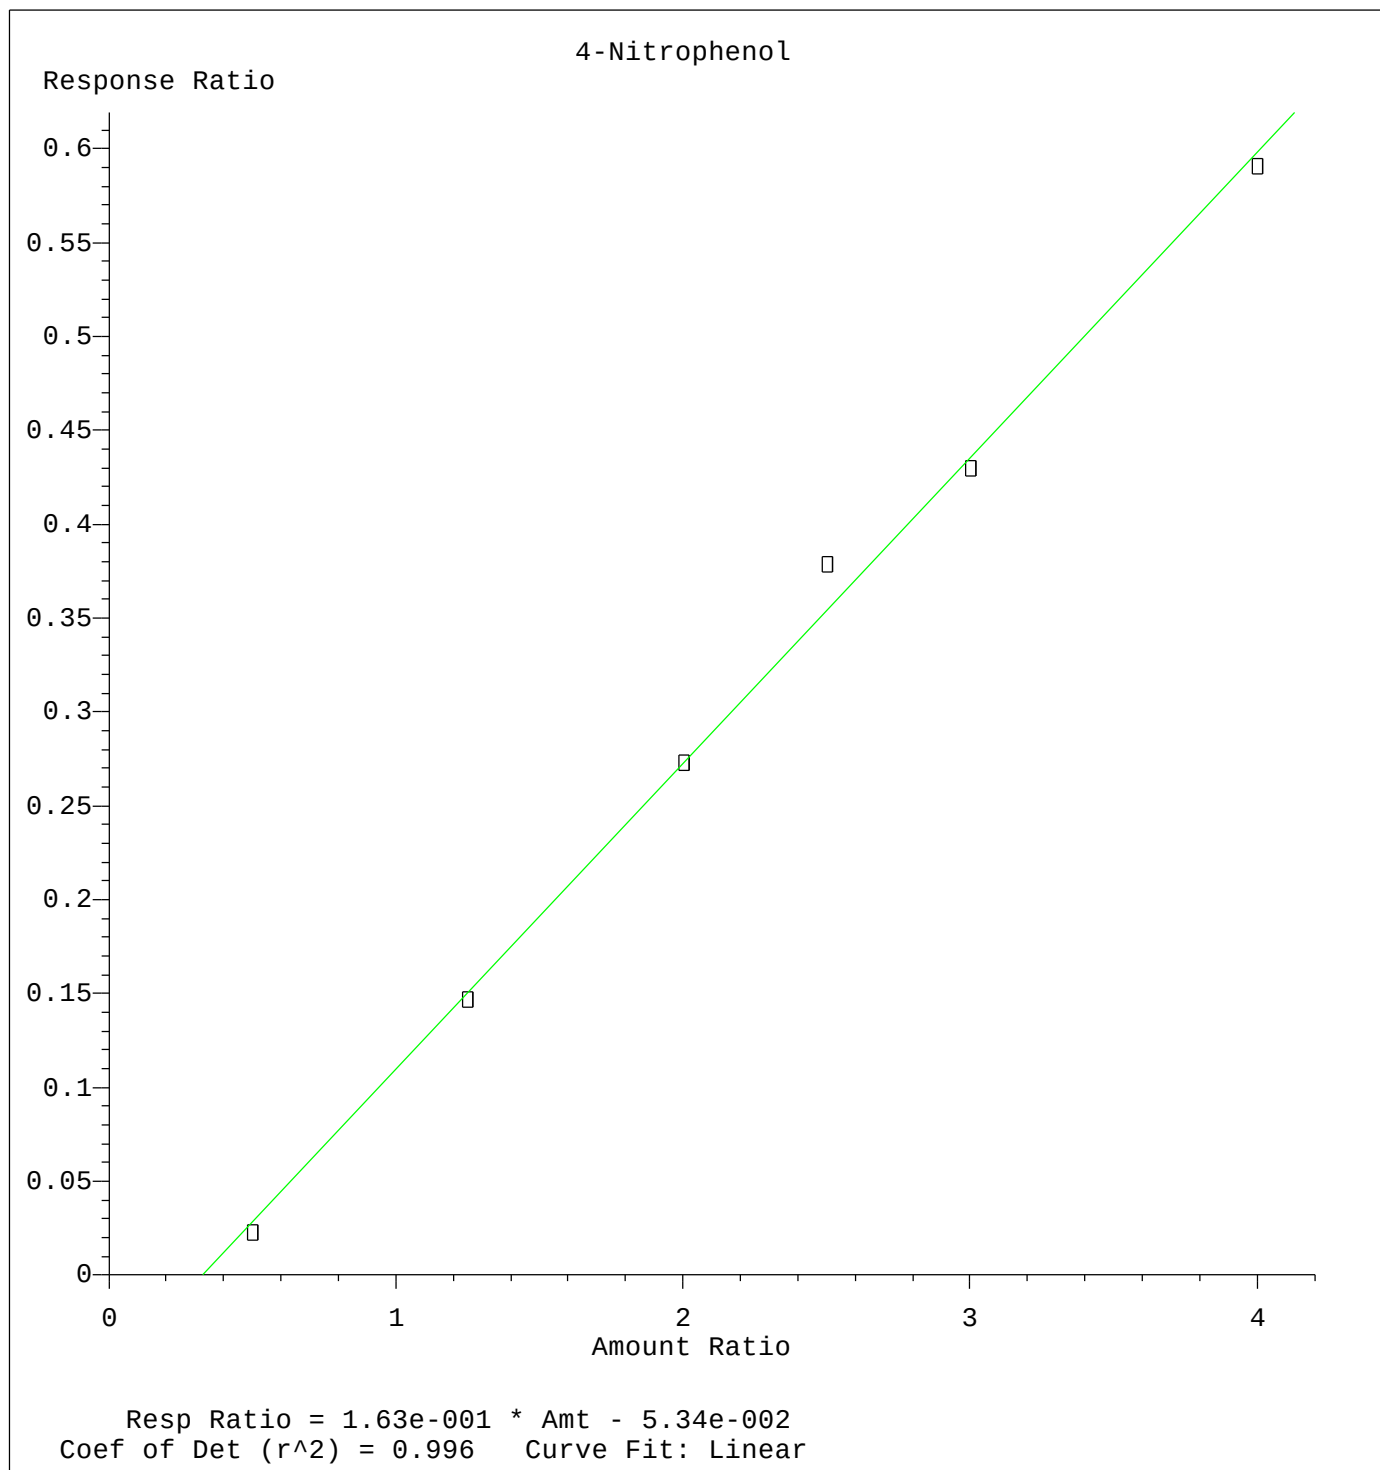

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF112116.M
Calibration Table Last Updated: Tue Nov 22 10:25:16 2016

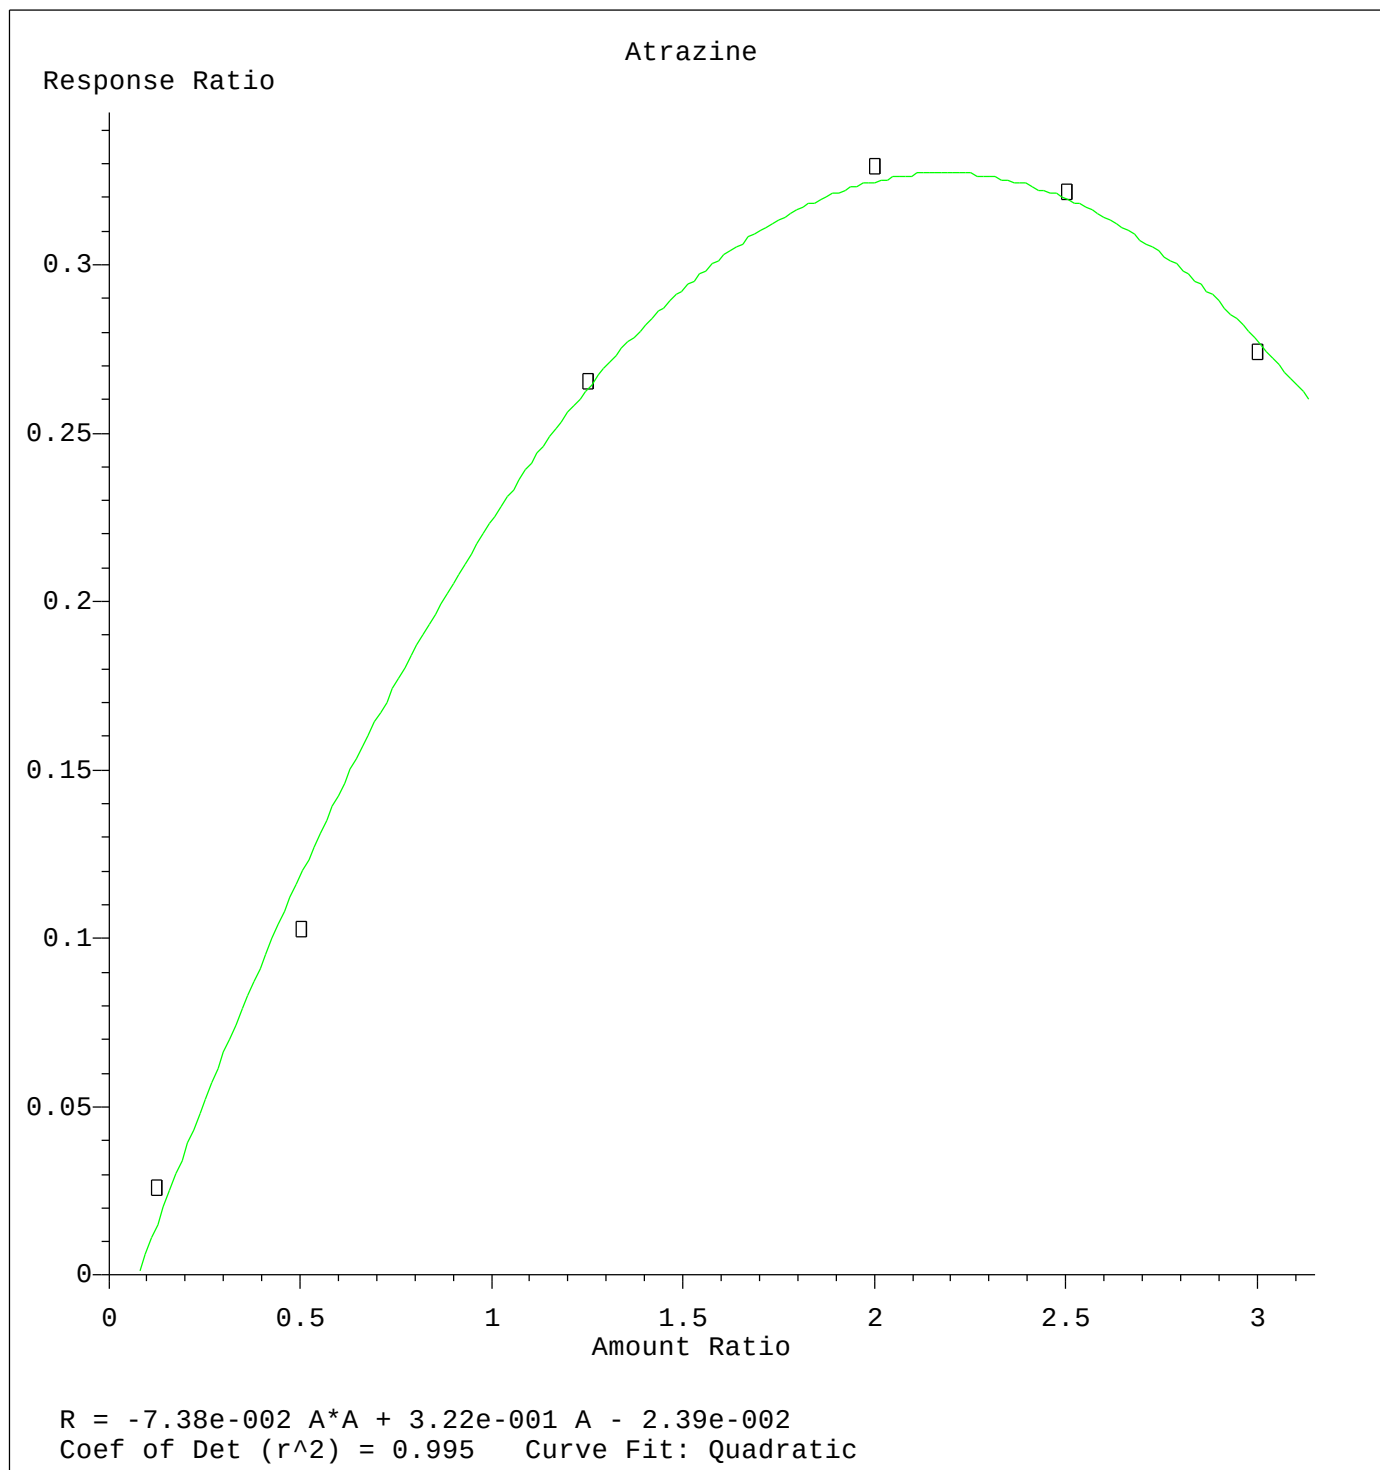

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF112116.M
Calibration Table Last Updated: Tue Nov 22 10:25:16 2016