
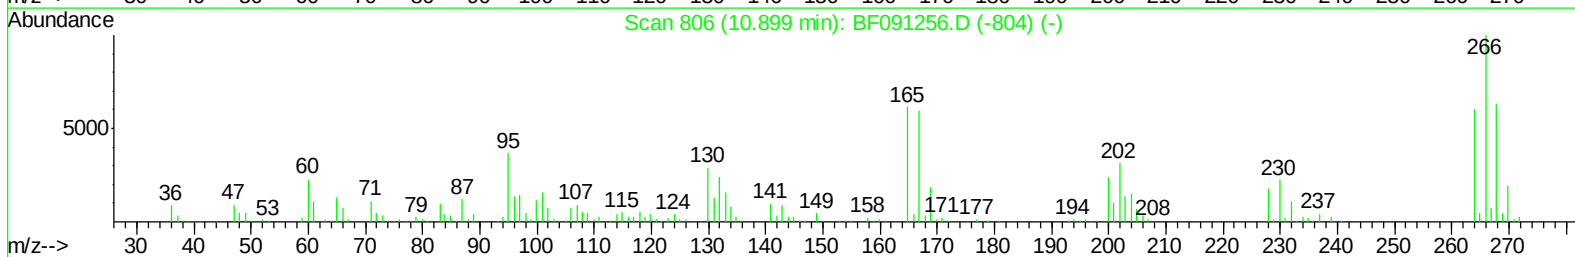
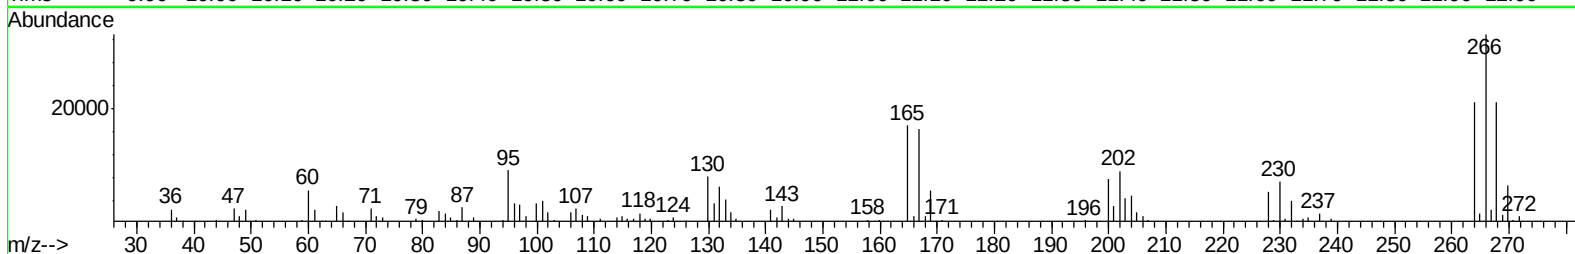


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF112116\
Data File : BF091252.D
Acq On : 21 Nov 2016 19:29
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 22 08:01:18 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF112116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 22 00:44:52 2016
Response via : Initial Calibration

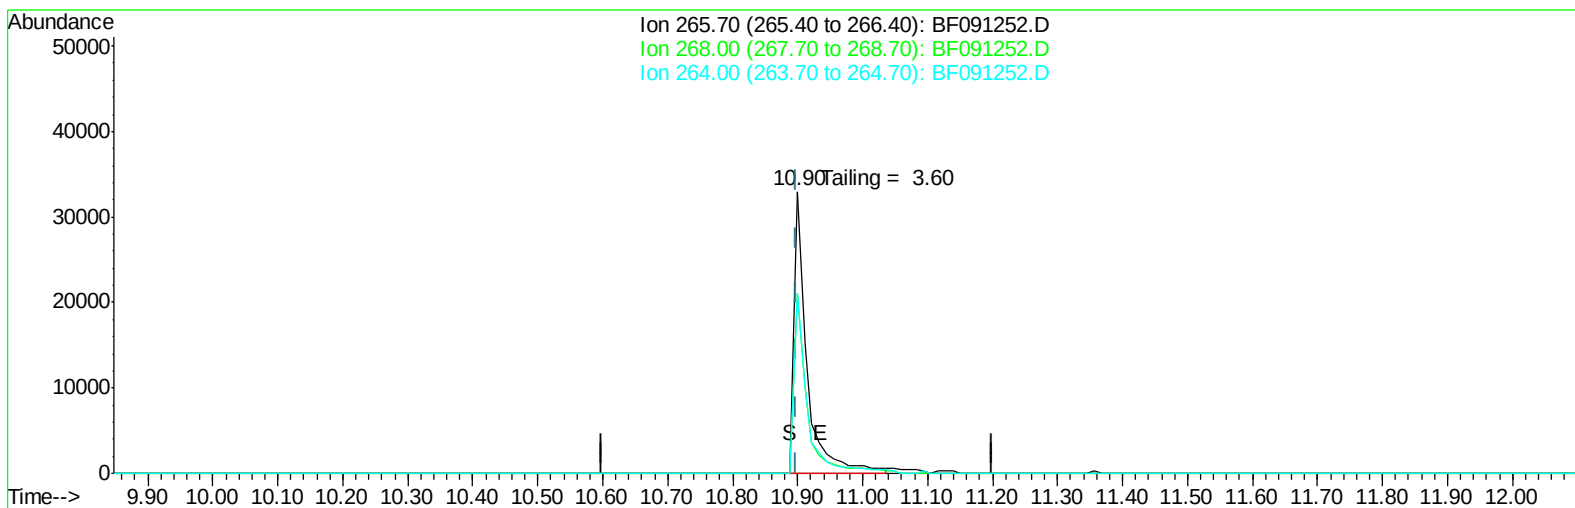

TIC: BF091252.D

(69) Pentachlorophenol (C)




10.899min (+0.000) 0.00ng

response 47760

Ion	Exp%	Act%
265.70	100	100
268.00	62.90	63.72
264.00	60.20	64.08
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF112116\
Data File : BF091252.D
Acq On : 21 Nov 2016 19:29
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 22 08:01:18 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF112116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 22 00:44:52 2016
Response via : Initial Calibration

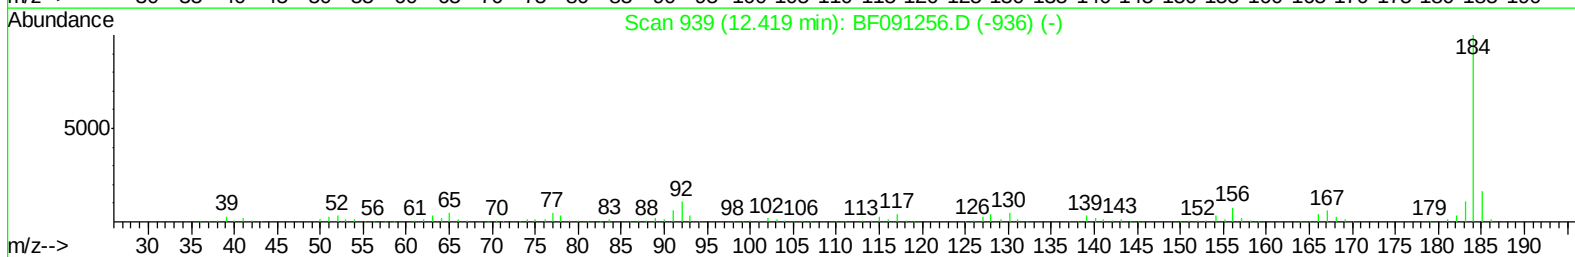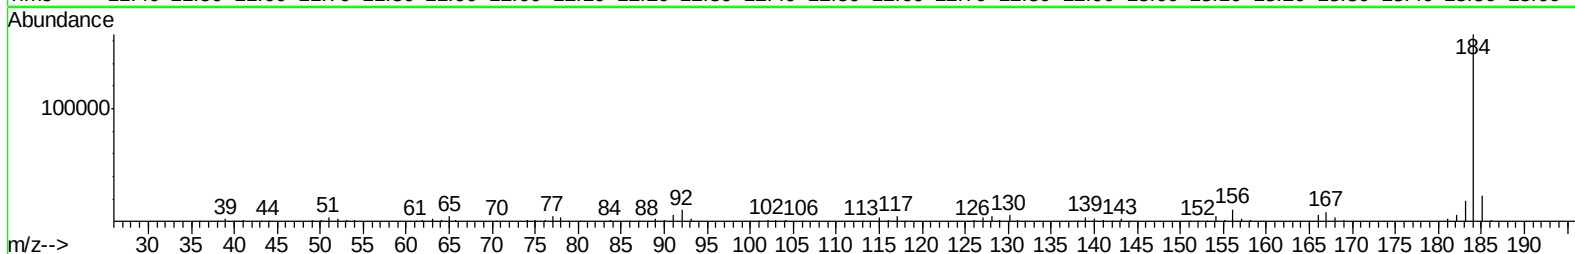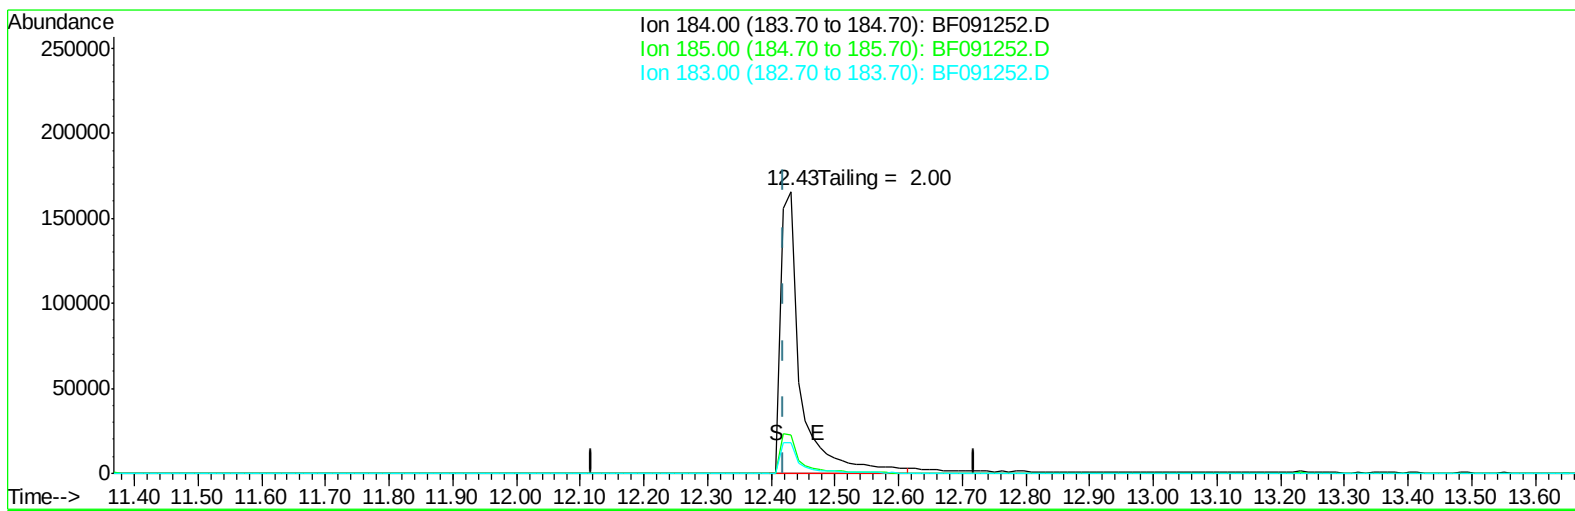

TIC: BF091252.D

(76) Benzidine

12.431min (+0.011) 0.00ng

response 355791

Ion	Exp%	Act%
184.00	100	100
185.00	16.40	13.65
183.00	11.10	11.08
0.00	0.00	0.00