


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF112116\
 Data File : BF091252.D
 Acq On : 21 Nov 2016 19:29
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF112116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 22 10:25:16 2016

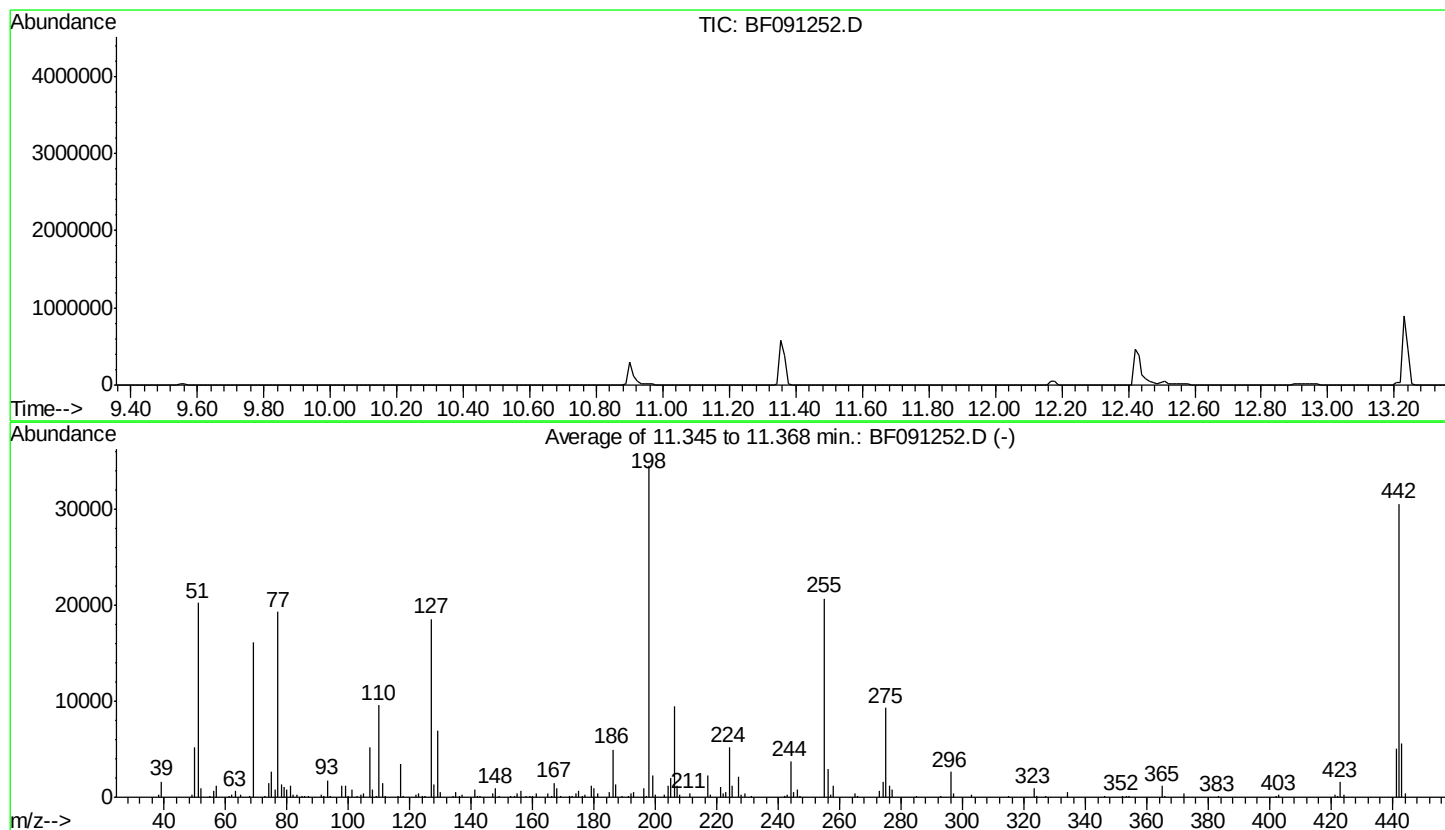

AutoFind: Scans 845, 846, 847; Background Corrected with Scan 842

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	58.6	20227	PASS
68	69	0.00	2	1.2	197	PASS
69	198	0.00	100	46.6	16082	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.7	18521	PASS
197	198	0.00	2	0.4	126	PASS
198	198	100	100	100.0	34509	PASS
199	198	5	9	6.6	2262	PASS
275	198	10	60	27.0	9323	PASS
365	198	1	100	3.4	1190	PASS
441	442	0.01	24	16.7	5086	PASS
442	198	50	100	88.4	30513	PASS
443	442	15	24	18.2	5543	PASS