

Data Path : Z:\HPCHEM1\BNA F\DATA\BF112117\
 Data File : BF100808.D
 Acq On : 22 Nov 2017 4:39
 Operator : SJ/JU
 Sample : I6542-01
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Nov 22 07:36:41 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110817.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 17 15:22:08 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.87	152	89883	20.00	ng	0.00
21) Naphthalene-d8	8.15	136	338687	20.00	ng	-0.02
38) Acenaphthene-d10	9.91	164	150324	20.00	ng	-0.01
63) Phenanthrene-d10	11.40	188	235328	20.00	ng	0.00
75) Chrysene-d12	14.03	240	176628	20.00	ng	-0.01
86) Perylene-d12	15.51	264	155652	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.49	112	225560	40.23	ng	0.00
7) Phenol-d6	6.49	99	168521	24.37	ng	-0.02
23) Nitrobenzene-d5	7.44	82	545964	106.57	ng	-0.01
41) 2,4,6-Tribromophenol	10.70	330	129307	84.41	ng	-0.01
44) 2-Fluorobiphenyl	9.23	172	1034035	104.74	ng	0.00
78) Terphenyl-d14	12.98	244	654258	85.11	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propylamine	7.44	70	70351	14.67	ng	# 80
25) Isophorone	7.44	82	545959	50.72	ng	# 64
47) 2-Nitroaniline	9.23	65	1656	3.34	ng	# 11
50) 2,6-Dinitrotoluene	9.91	165	18994	8.36	ng	# 25
56) 2,4-Dinitrotoluene	9.91	165	18994	6.63	ng	# 22
64) 4,6-Dinitro-2-methylphenol	10.70	198	140	8.67	ng	# 3
66) 4-Bromophenyl-phenylether	10.70	248	7965	3.16	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF112117\
Data File : BF100808.D
Acq On : 22 Nov 2017 4:39
Operator : SJ/JU
Sample : I6542-01
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Nov 22 07:36:41 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 15:22:08 2017
Response via : Initial Calibration

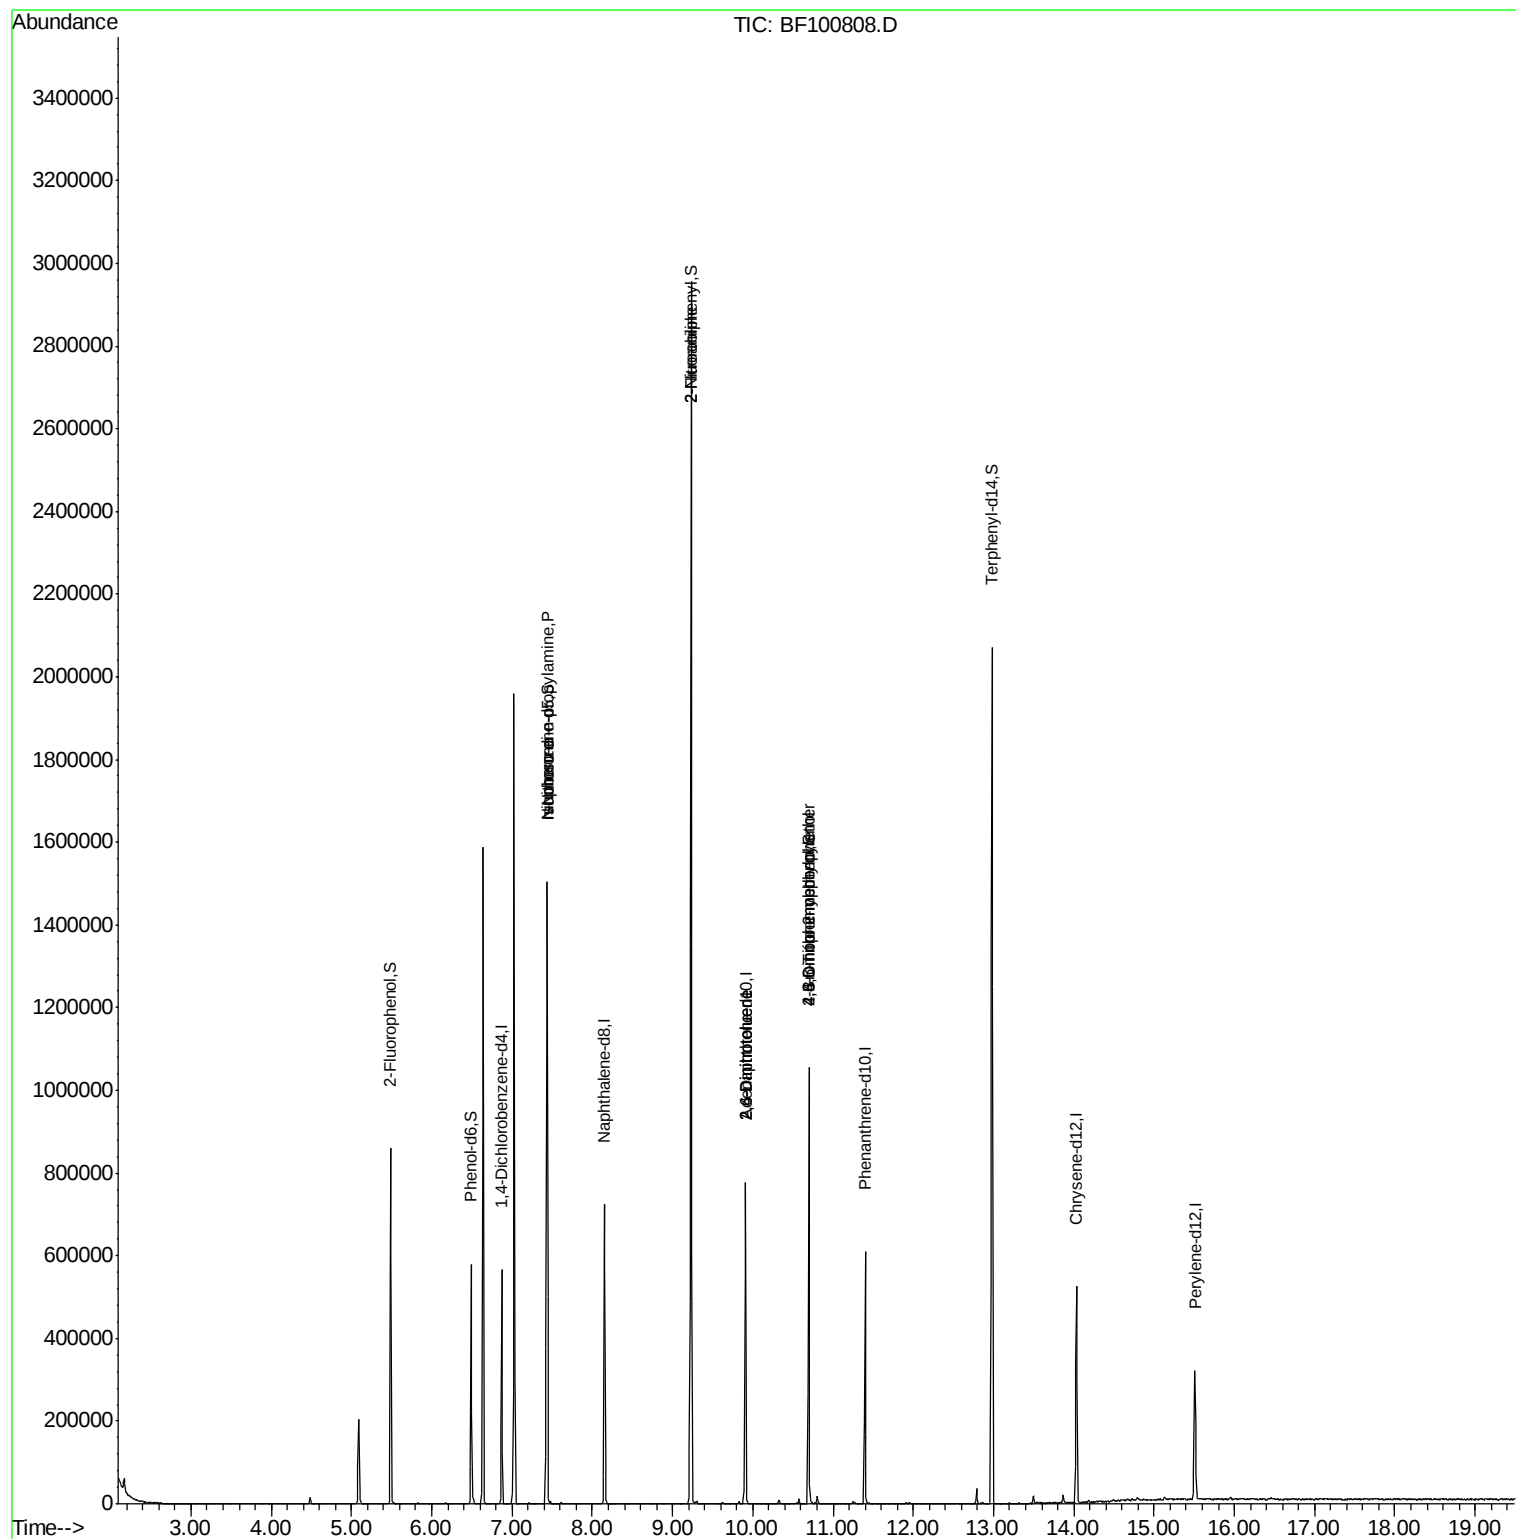

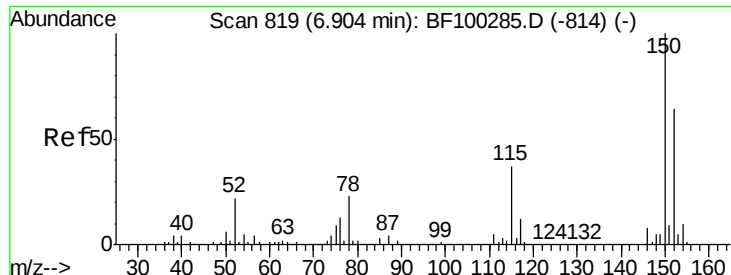


#1



1,4-Dichlorobenzene-d4
 Concen: 20.00 ng
 RT: 6.87 min Scan# 814
 Delta R.T. -0.01 min
 Lab File: BF100808.D
 Acq: 22 Nov 2017 4:39

Instrument :
 BNA_F
 ClientSampled :

Tot Ion	Ratio	Lower	Upper
152	100		
150	153.3	124.6	186.8
115	53.2	50.1	75.1

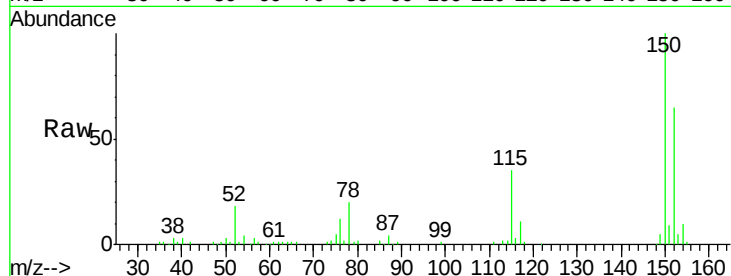


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

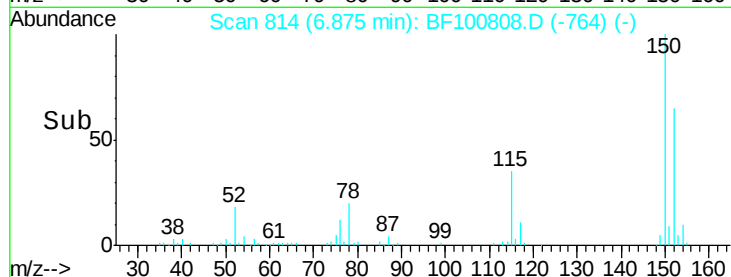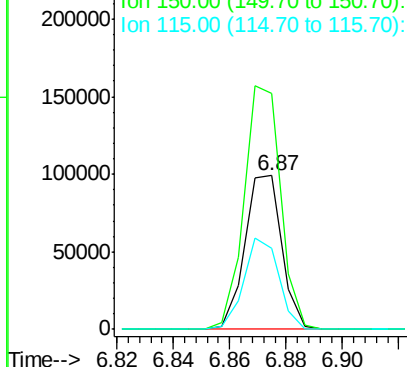



#5



2-Fluorophenol
 Concen: 40.23 ng
 RT: 5.49 min Scan# 578
 Delta R.T. -0.01 min
 Lab File: BF100808.D
 Acq: 22 Nov 2017 4:39

Tgt Ion	Ratio	Lower	Upper
112	100		
64	59.7	47.9	71.9
63	30.8	23.7	35.5

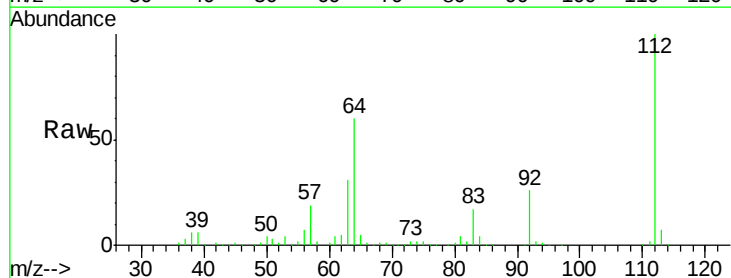

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF1
 Ion 63.00 (62.70 to 63.70): BF1

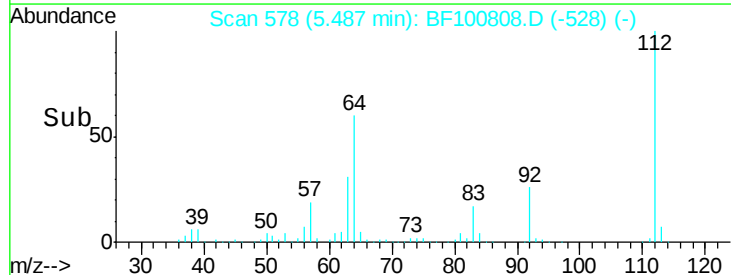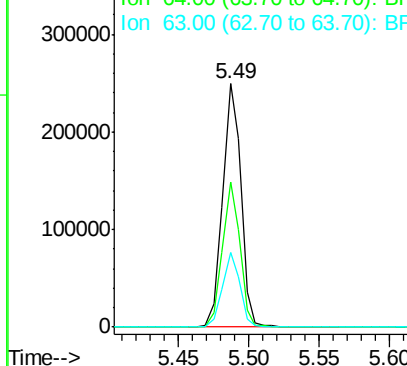

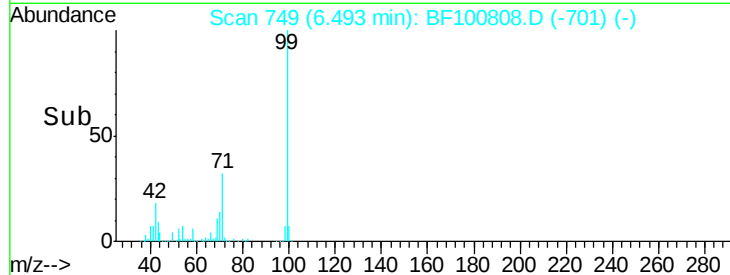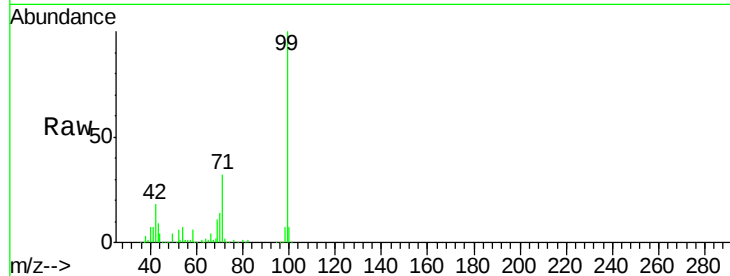

#7

Phenol-d6

Concen: 24.37 ng

RT: 6.49 min Scan# 749

Delta R.T. -0.02 min

Lab File: BF100808.D

Acq: 22 Nov 2017 4:39

Instrument :

BNA_F

ClientSampleId :





Tot Ion: 99 Resp: 168521

Ion Ratio Lower Upper

99 100

42 18.4 14.5 21.7

71 31.5 25.4 38.0

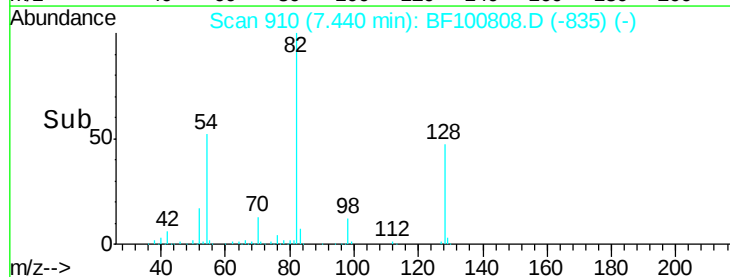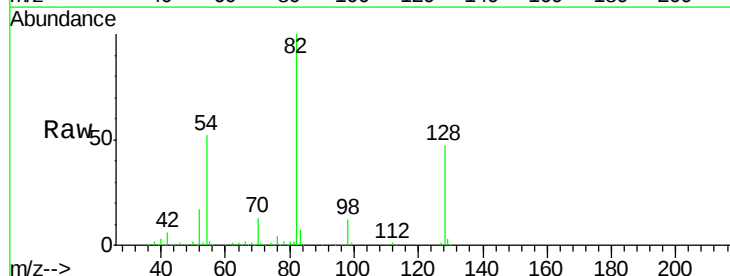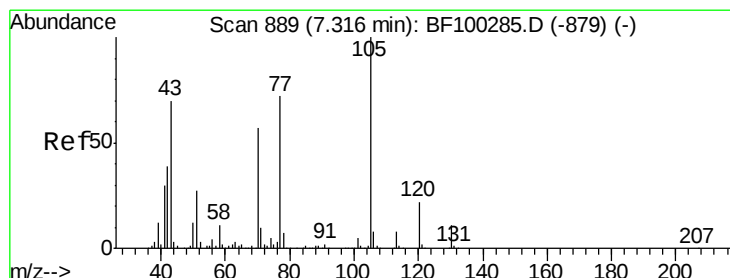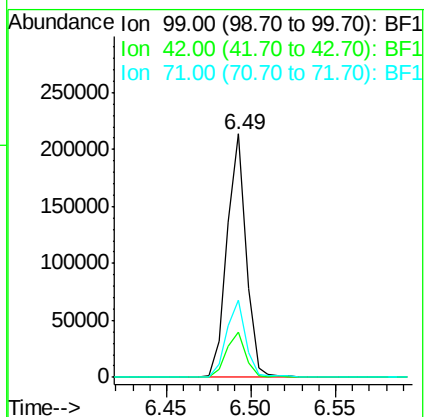

#19

n-Nitroso-di-n-propylamine

Concen: 14.67 ng

RT: 7.44 min Scan# 910

Delta R.T. 0.14 min

Lab File: BF100808.D

Acq: 22 Nov 2017 4:39

Tgt Ion: 70 Resp: 70351


Ion Ratio Lower Upper

70 100

42 50.4 47.5 71.3

101 0.0 7.4 11.2#

130 2.1 16.6 25.0#




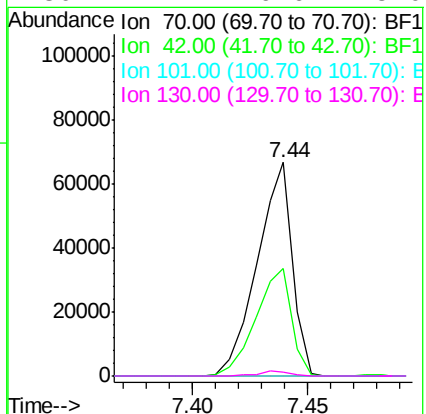




#21
Naphthalene-d8
Concen: 20.00 ng
RT: 8.15 min Scan# 1031
Delta R.T. -0.02 min
Lab File: BF100808.D
Acq: 22 Nov 2017 4:39




Instrument :
BNA_F
ClientSampleId :

Tot Ion:136	Resp:	338687
Ion Ratio	Lower	Upper
136	100	
137	11.2	8.9 13.3
54	8.3	6.6 9.8
68	5.8	5.0 7.4

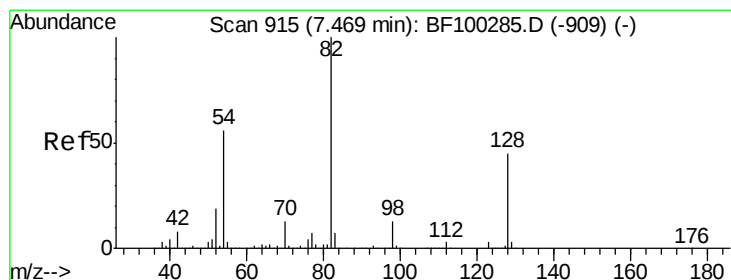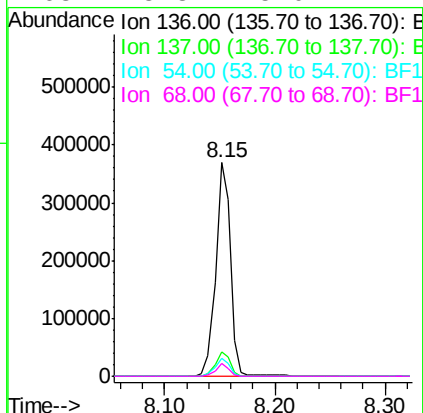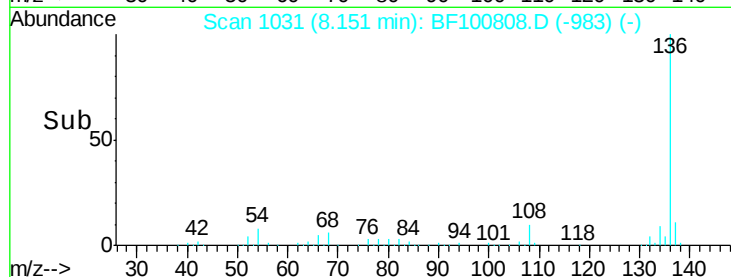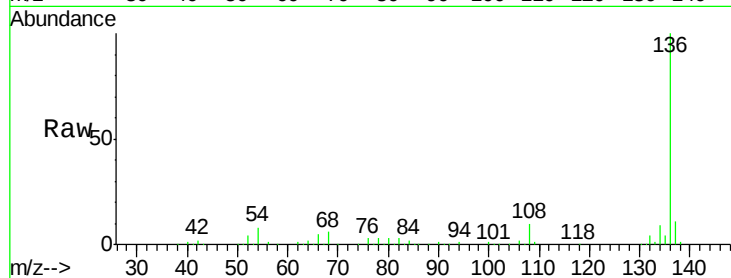

#23
Nitrobenzene-d5
Concen: 106.57 ng
RT: 7.44 min Scan# 910
Delta R.T. -0.01 min
Lab File: BF100808.D
Acq: 22 Nov 2017 4:39

Tgt Ion: 82	Resp:	545964
Ion Ratio	Lower	Upper
82	100	
128	47.0	36.1 54.1
54	52.1	41.4 62.2

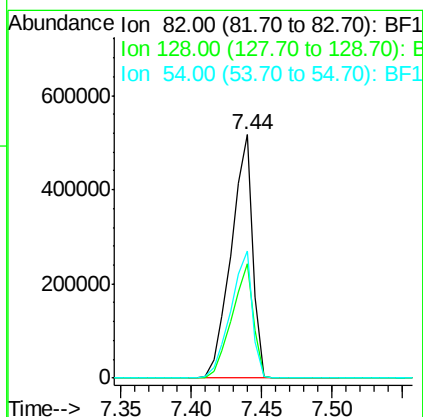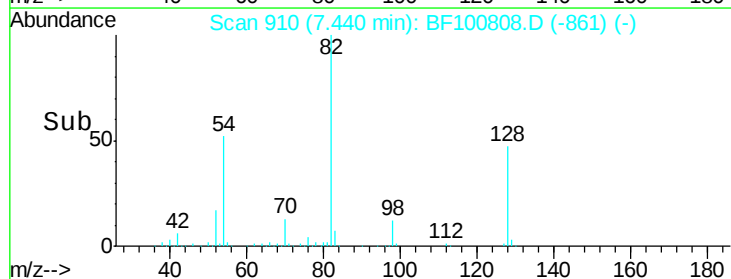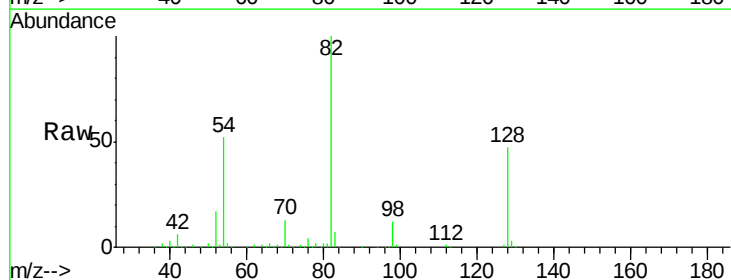



#25

Isophorone

Concen: 50.72 ng

RT: 7.44 min Scan# 910

Delta R.T. -0.26 min

Lab File: BF100808.D

Acq: 22 Nov 2017 4:39

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 82 Resp: 545959

Ion Ratio Lower Upper




82 100

95 0.0 5.2 7.8#

138 0.0 14.9 22.3#

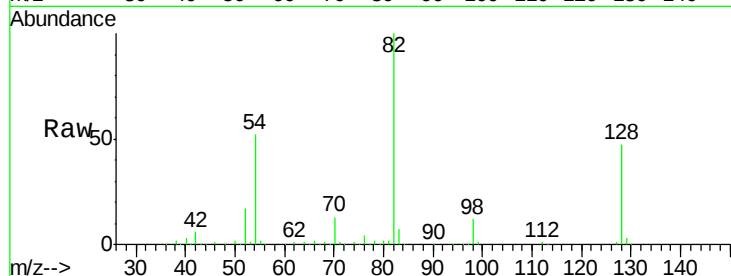

Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 95.00 (94.70 to 95.70): BF1
Ion 138.00 (137.70 to 138.70): BF1

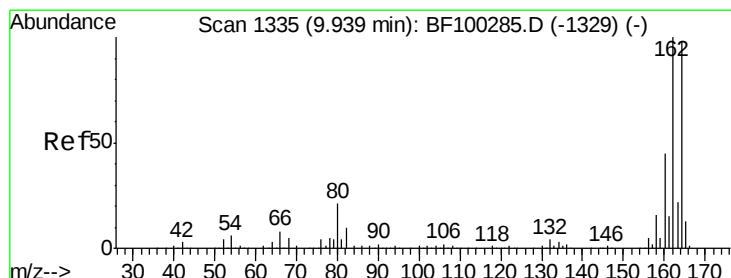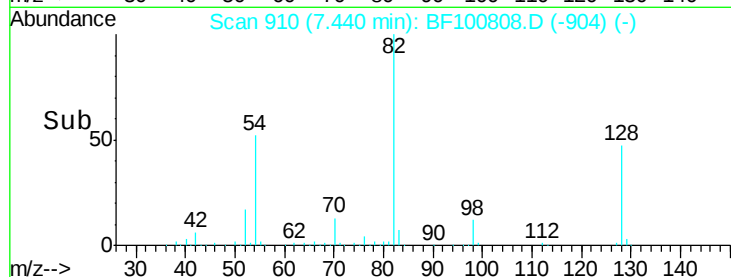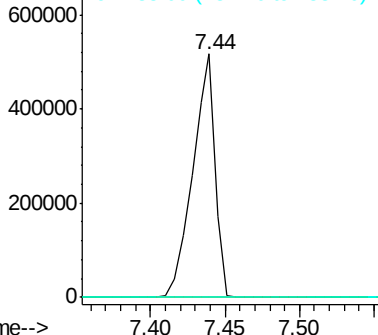

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.91 min Scan# 1330

Delta R.T. -0.01 min

Lab File: BF100808.D

Acq: 22 Nov 2017 4:39


Tgt Ion: 164 Resp: 150324

Ion Ratio Lower Upper



164 100


162 103.2 86.1 129.1

160 46.8 38.3 57.5

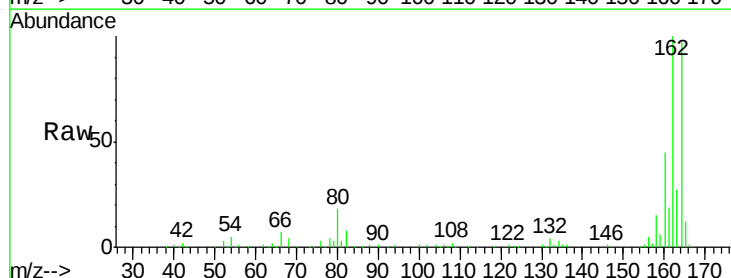

Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E



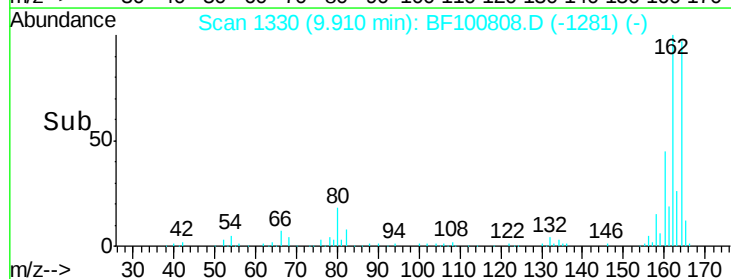
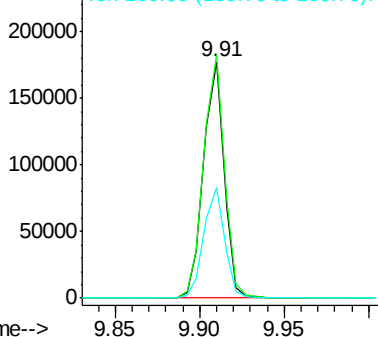


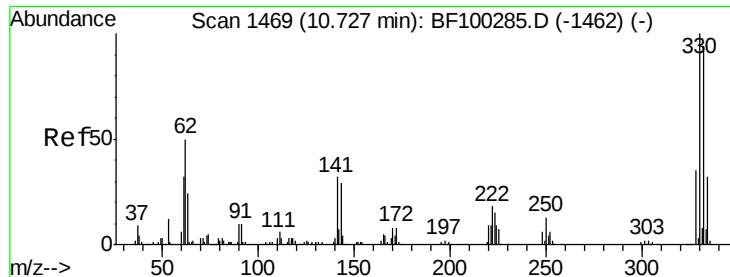

#41
 2,4,6-Tribromophenol
 Concen: 84.41 ng
 RT: 10.70 min Scan# 1464
 Delta R.T. -0.01 min
 Lab File: BF100808.D
 Acq: 22 Nov 2017 4:39




Instrument :
 BNA_F
 ClientSampled :

Tot Ion	Ratio	Lower	Upper
330	100		
332	94.2	77.0	115.6
141	28.8	29.9	44.9#

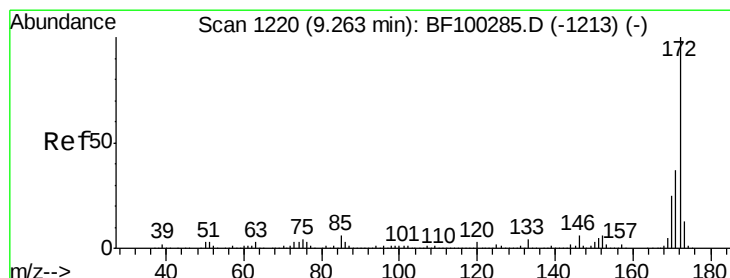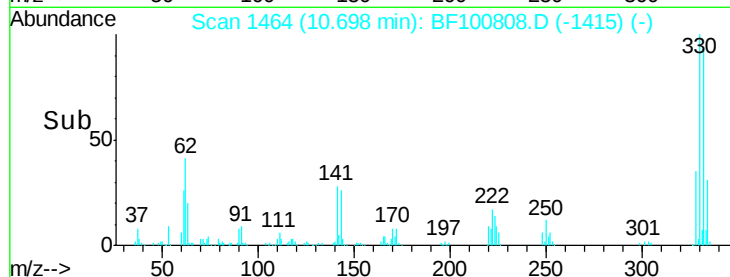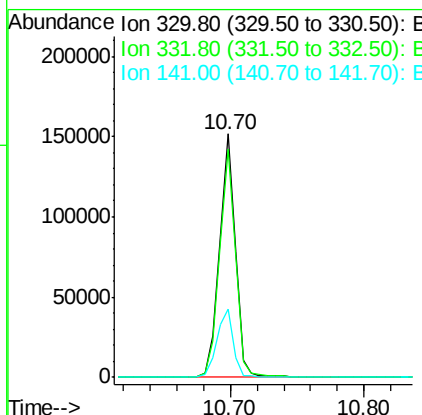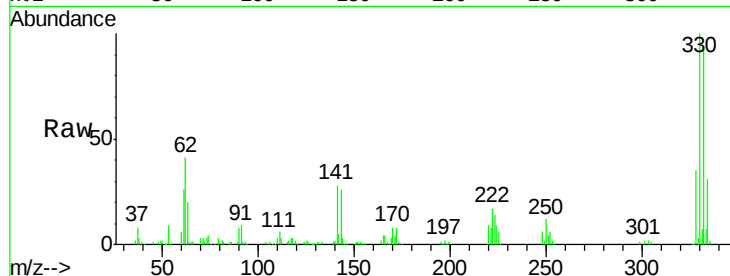

#44
 2-Fluorobiphenyl
 Concen: 104.74 ng
 RT: 9.23 min Scan# 1215
 Delta R.T. -0.01 min
 Lab File: BF100808.D
 Acq: 22 Nov 2017 4:39

Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.1	29.7	44.5
170	23.7	19.6	29.4

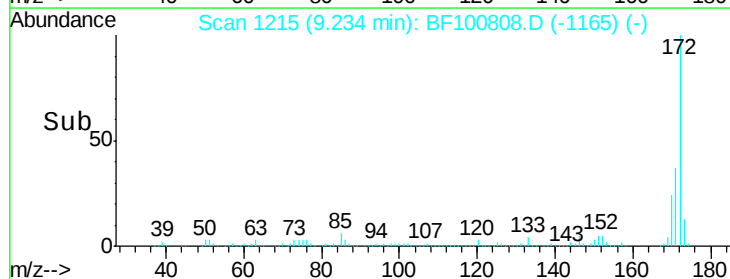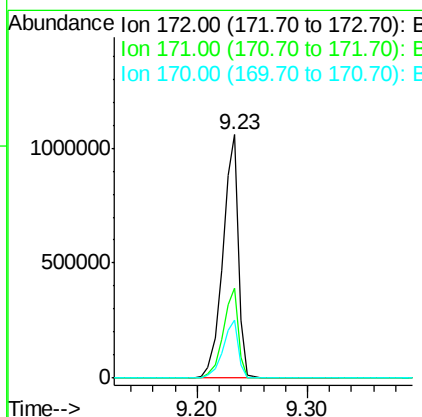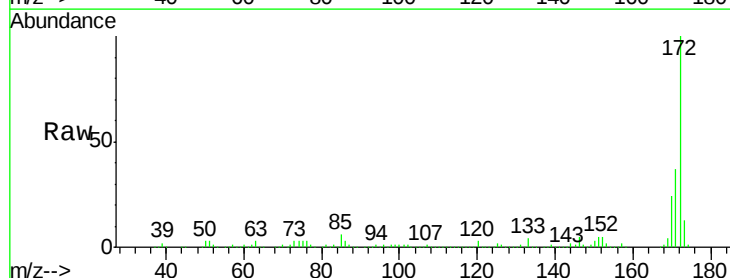



#47

2-Nitroaniline

Concen: 3.34 ng

RT: 9.23 min Scan# 1215

Delta R.T. -0.23 min

Lab File: BF100808.D

Acq: 22 Nov 2017 4:39

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 65 Resp: 1656

Ion Ratio Lower Upper




65 100

92 162.5 55.8 83.6#

138 33.5 91.2 136.8#

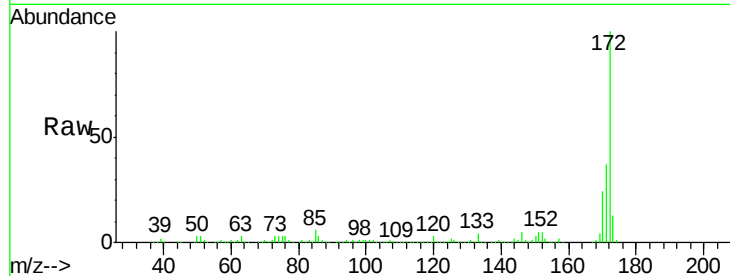

Abundance Ion 65.00 (64.70 to 65.70): BF1
Ion 92.00 (91.70 to 92.70): BF1
Ion 138.00 (137.70 to 138.70): BF1

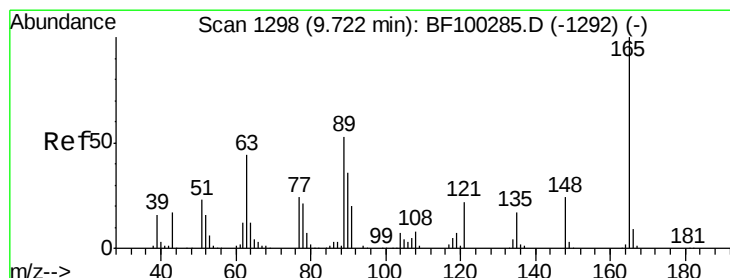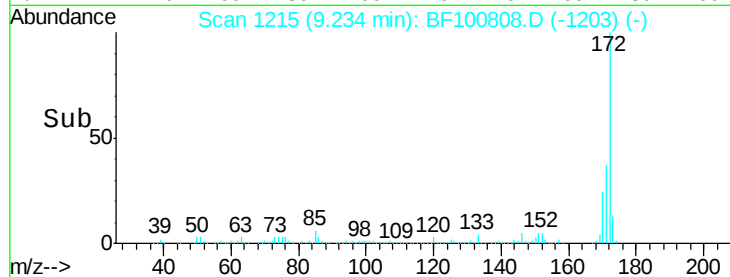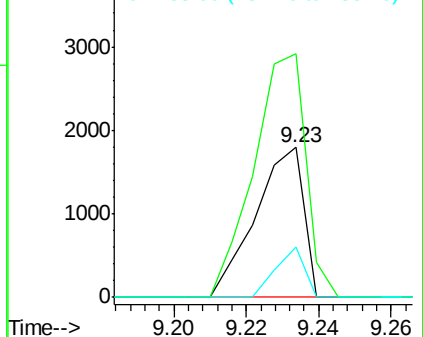

#50

2,6-Dinitrotoluene

Concen: 8.36 ng

RT: 9.91 min Scan# 1330

Delta R.T. 0.21 min

Lab File: BF100808.D

Acq: 22 Nov 2017 4:39


Tgt Ion:165 Resp: 18994

Ion Ratio Lower Upper



165 100


63 1.4 44.7 67.1#

89 0.0 44.0 66.0#

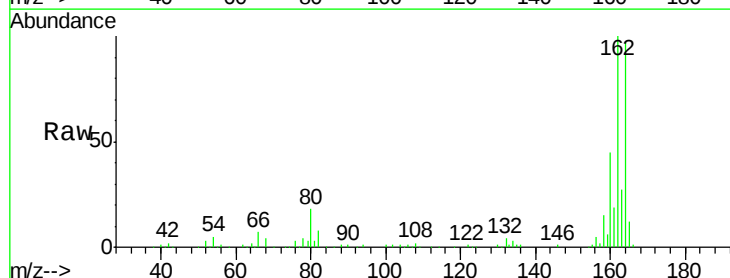

Abundance Ion 165.00 (164.70 to 165.70): BF1
Ion 63.00 (62.70 to 63.70): BF1
Ion 89.00 (88.70 to 89.70): BF1



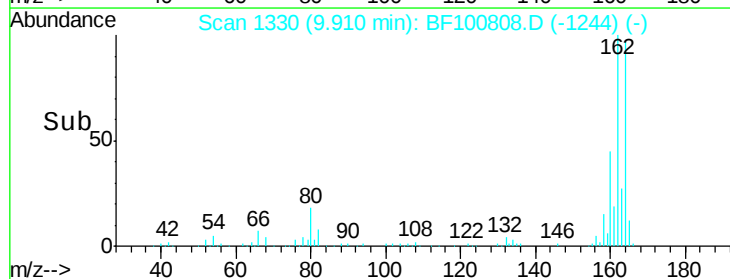
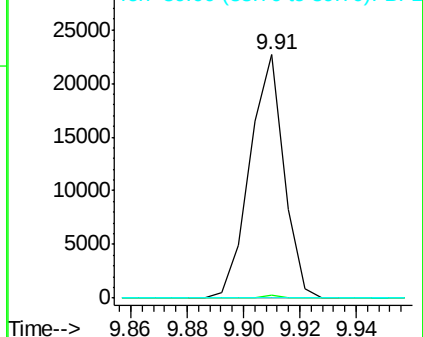


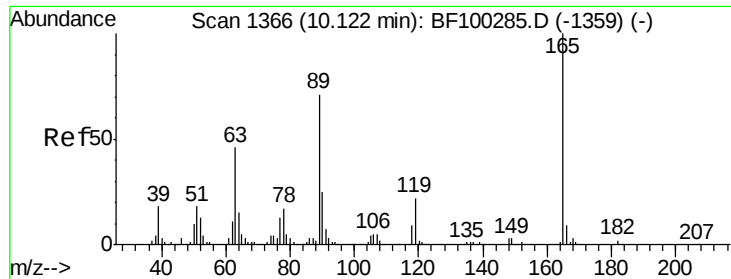

#56
 2,4-Dinitrotoluene
 Concen: 6.63 ng
 RT: 9.91 min Scan# 1330
 Delta R.T. -0.20 min
 Lab File: BF100808.D
 Acq: 22 Nov 2017 4:39




Instrument :
 BNA_F
 ClientSampleId :


Tot Ion	Ratio	Lower	Upper
165	100		
63	1.4	36.4	54.6#
89	0.0	57.8	86.6#
182	0.0	1.6	2.4#

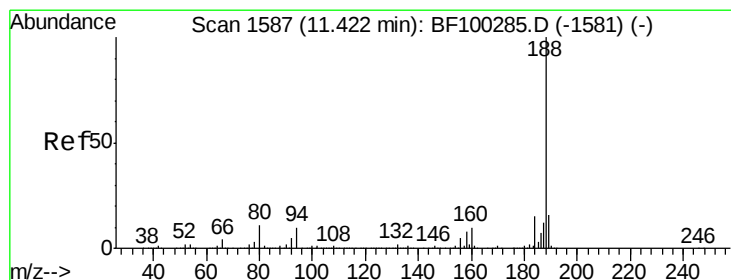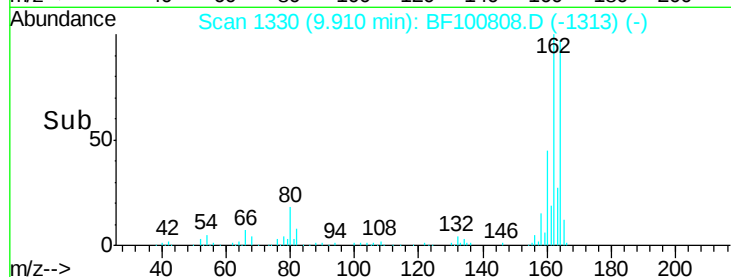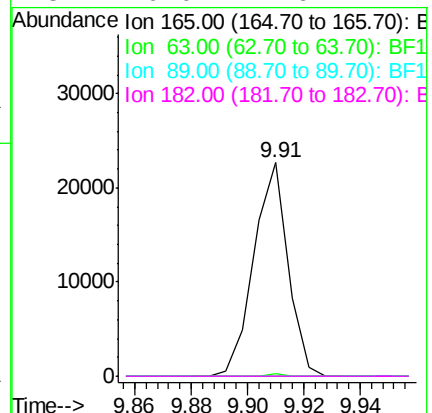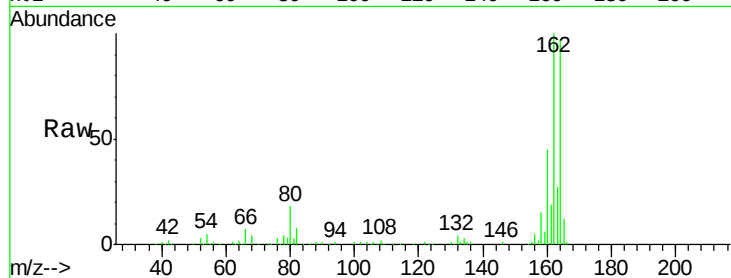

#63
 Phenanthrene-d10
 Concen: 20.00 ng
 RT: 11.40 min Scan# 1583
 Delta R.T. -0.01 min
 Lab File: BF100808.D
 Acq: 22 Nov 2017 4:39

Tgt Ion	Ratio	Lower	Upper
188	100		
94	8.2	8.5	12.7#
80	8.3	9.2	13.8#

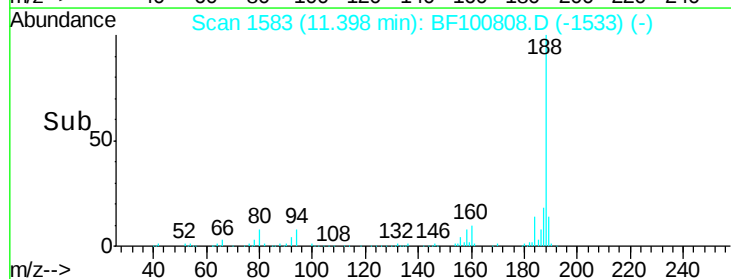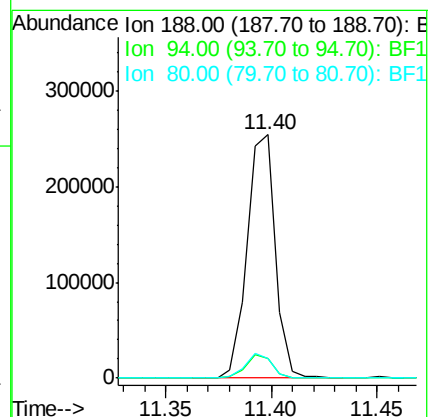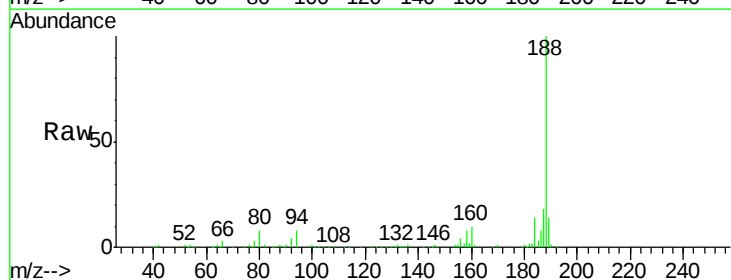


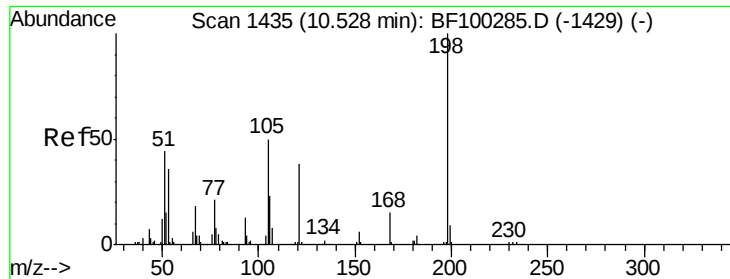




#64
4,6-Dinitro-2-methylphenol
Concen: 8.67 ng
RT: 10.70 min Scan# 1464
Delta R.T. 0.18 min
Lab File: BF100808.D
Acq: 22 Nov 2017 4:39

Instrument :
BNA_F
ClientSampleId :

Tot Ion:198 Resp: 140
Ion Ratio Lower Upper
198 100
51 134.1 37.7 77.7#
105 122.2 36.3 76.3#

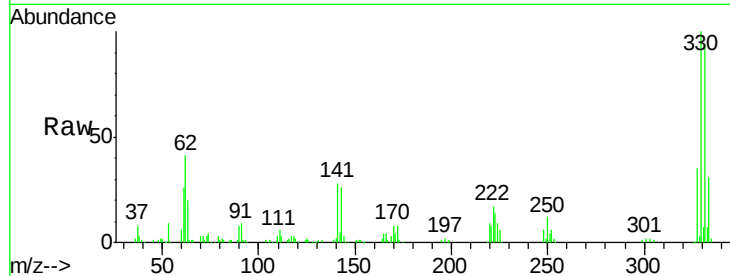


Abundance Ion 198.00 (197.70 to 198.70): E
Ion 51.00 (50.70 to 51.70): BF1
Ion 105.00 (104.70 to 105.70): E

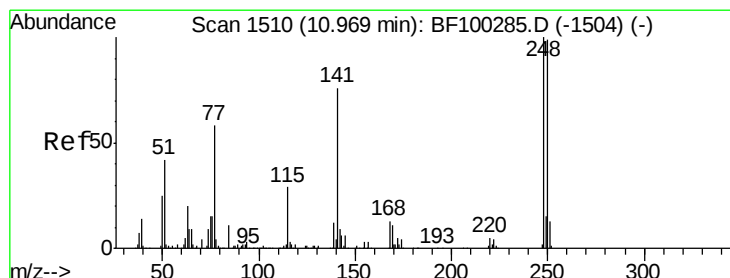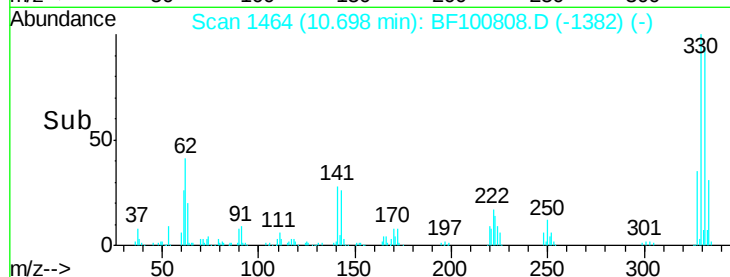
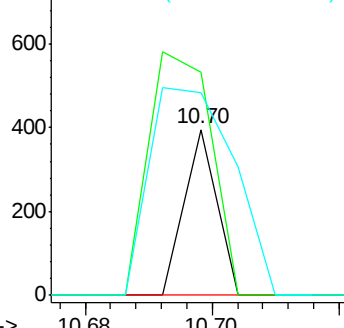



#66
4-Bromophenyl-phenylether
Concen: 3.16 ng
RT: 10.70 min Scan# 1464
Delta R.T. -0.25 min
Lab File: BF100808.D
Acq: 22 Nov 2017 4:39

Tgt Ion:248 Resp: 7965
Ion Ratio Lower Upper
248 100
250 194.2 76.9 115.3#
141 447.1 74.4 111.6#

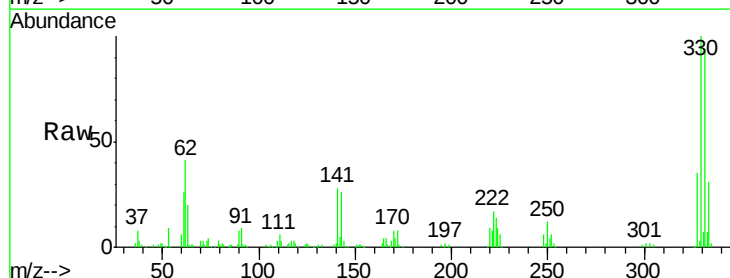

Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E



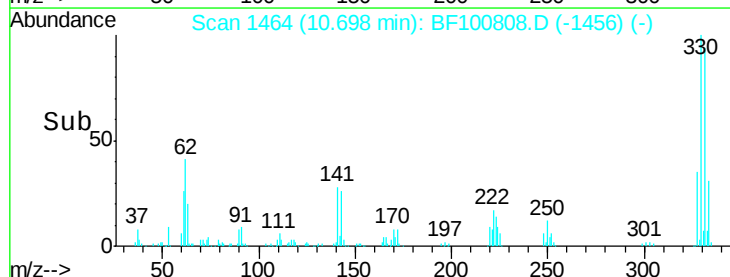
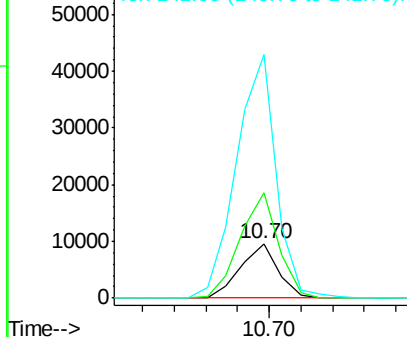


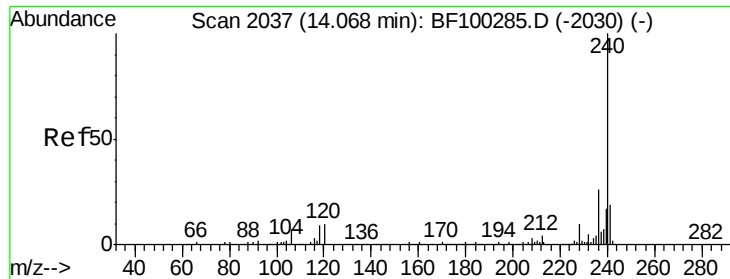

#75
Chrysene-d12
Concen: 20.00 ng
RT: 14.03 min Scan# 2031
Delta R.T. -0.01 min
Lab File: BF100808.D
Acq: 22 Nov 2017 4:39




Instrument :
BNA_F
ClientSampleId :


Tot Ion:240 Resp: 176628
Ion Ratio Lower Upper
240 100
120 10.8 9.5 14.3
236 25.6 20.7 31.1

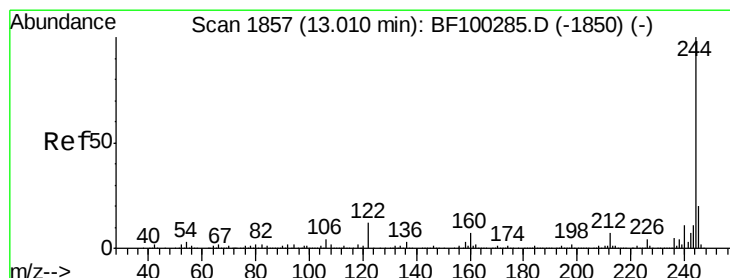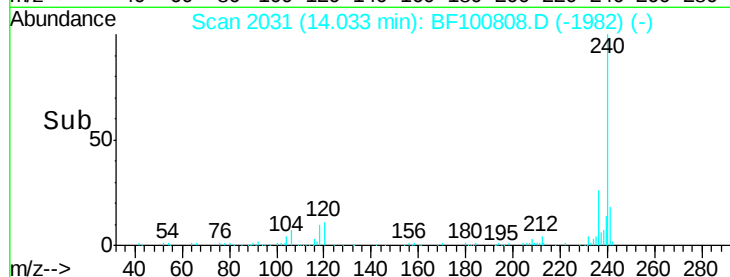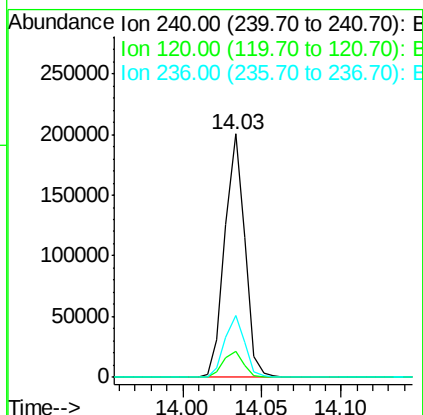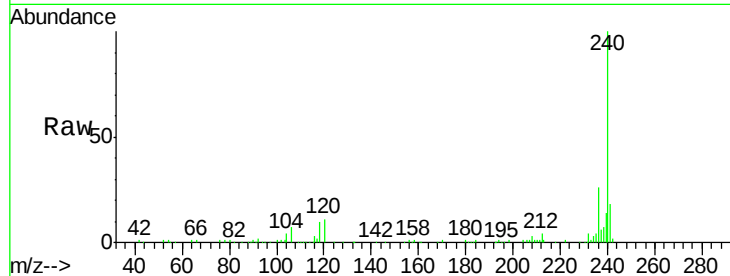

#78
Terphenyl-d14
Concen: 85.11 ng
RT: 12.98 min Scan# 1852
Delta R.T. -0.01 min
Lab File: BF100808.D
Acq: 22 Nov 2017 4:39

Tgt Ion:244 Resp: 654258
Ion Ratio Lower Upper
244 100
212 7.2 5.4 8.0
122 11.8 11.0 16.4

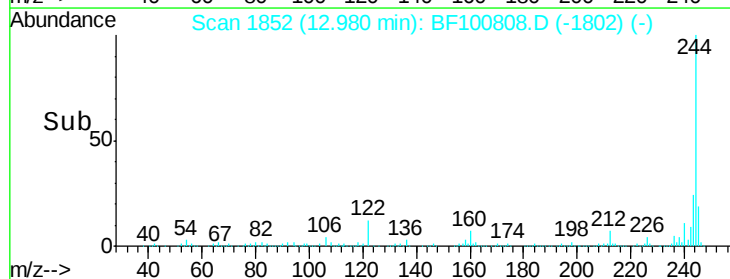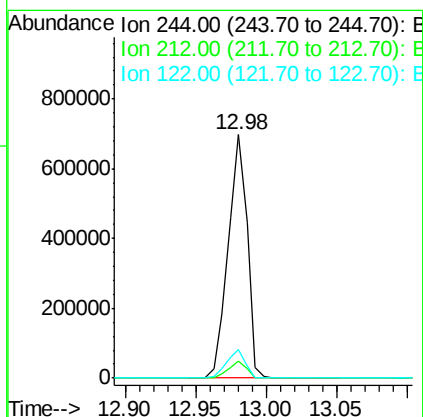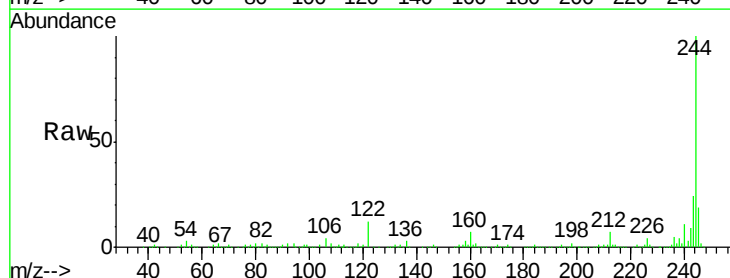


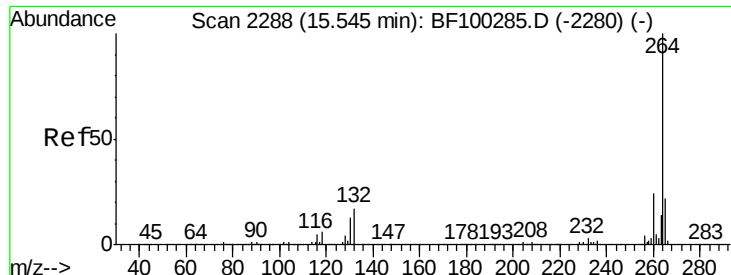

#86
 Pervlene-d12
 Concen: 20.00 ng
 RT: 15.51 min Scan# 2282
 Delta R.T. -0.01 min
 Lab File: BF100808.D
 Acq: 22 Nov 2017 4:39

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
264	100		
260	22.9	19.2	28.8
265	21.7	17.5	26.3

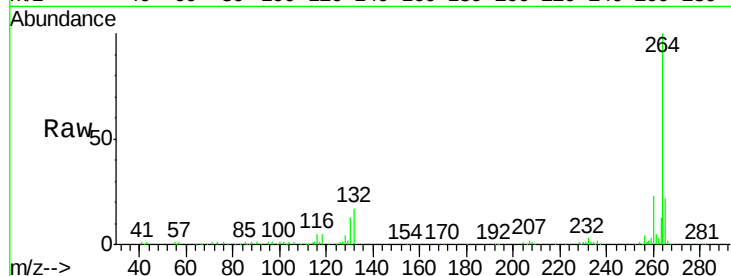

Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

