
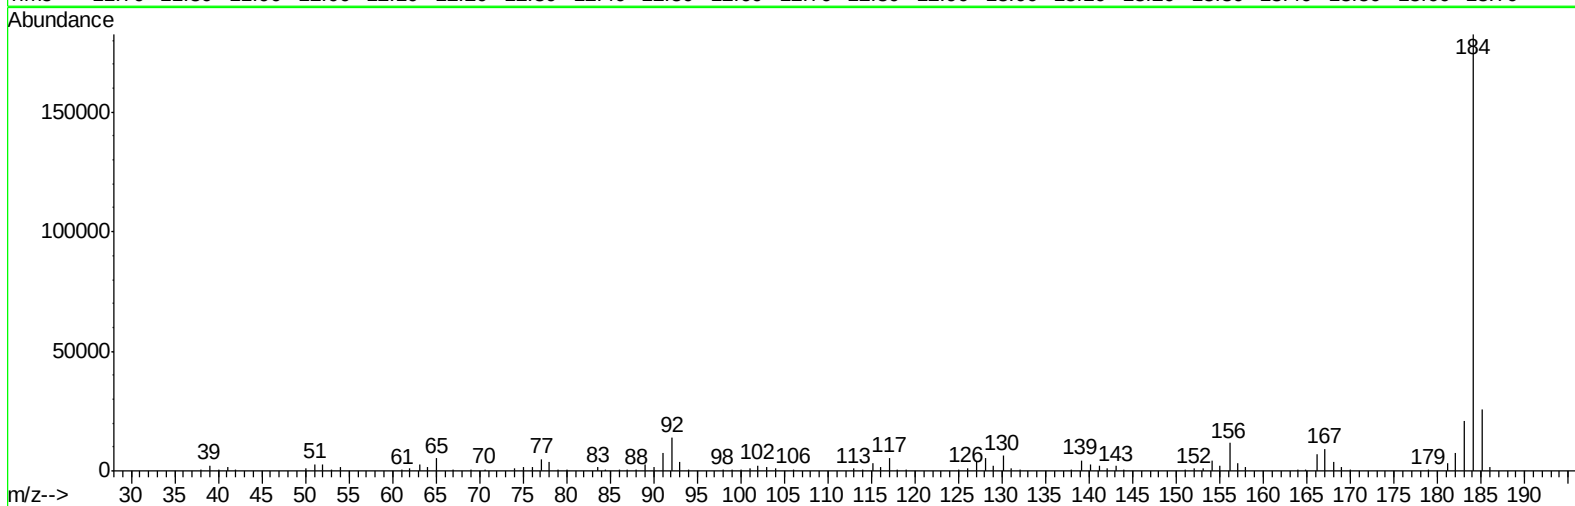


Data Path : Z:\HPCHEM1\BNA F\DATA\BF112117\
Data File : BF100797.D
Acq On : 21 Nov 2017 23:41
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 22 08:30:50 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 15:22:08 2017
Response via : Initial Calibration

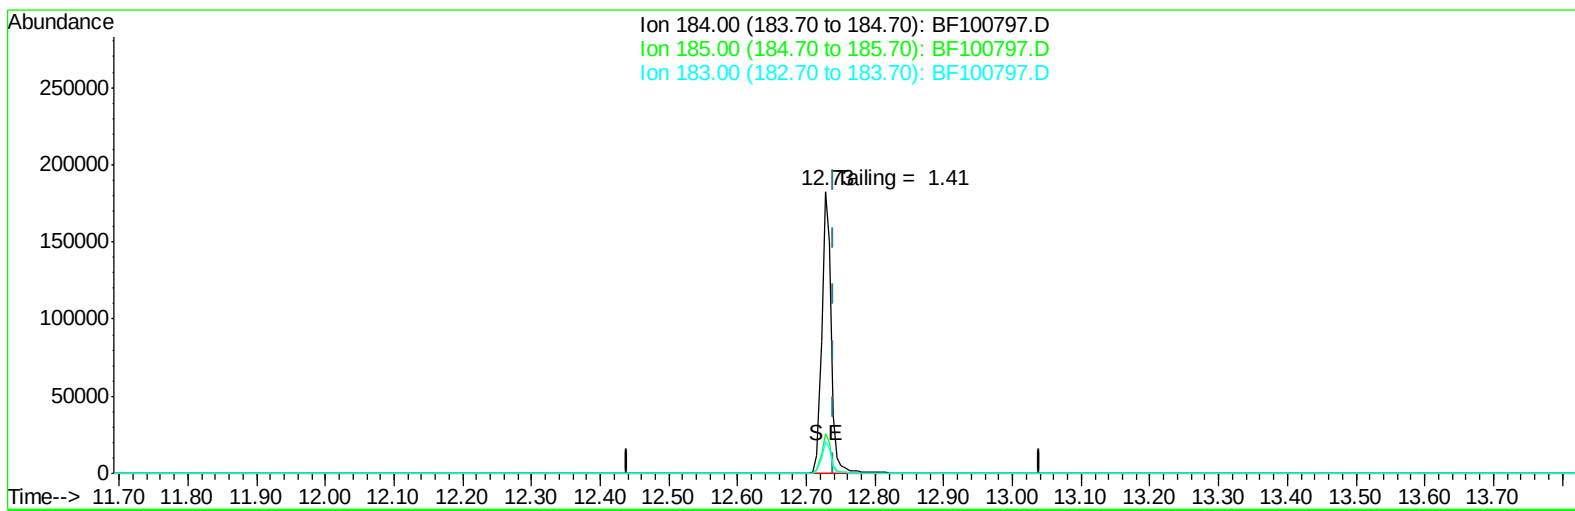

TIC: BF100797.D

(76) Benzidine



12.727min (-0.012) 15191.66ng

response 175217

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.08
183.00	11.60	11.47
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF112117\
Data File : BF100797.D
Acq On : 21 Nov 2017 23:41
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 22 08:30:50 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 15:22:08 2017
Response via : Initial Calibration

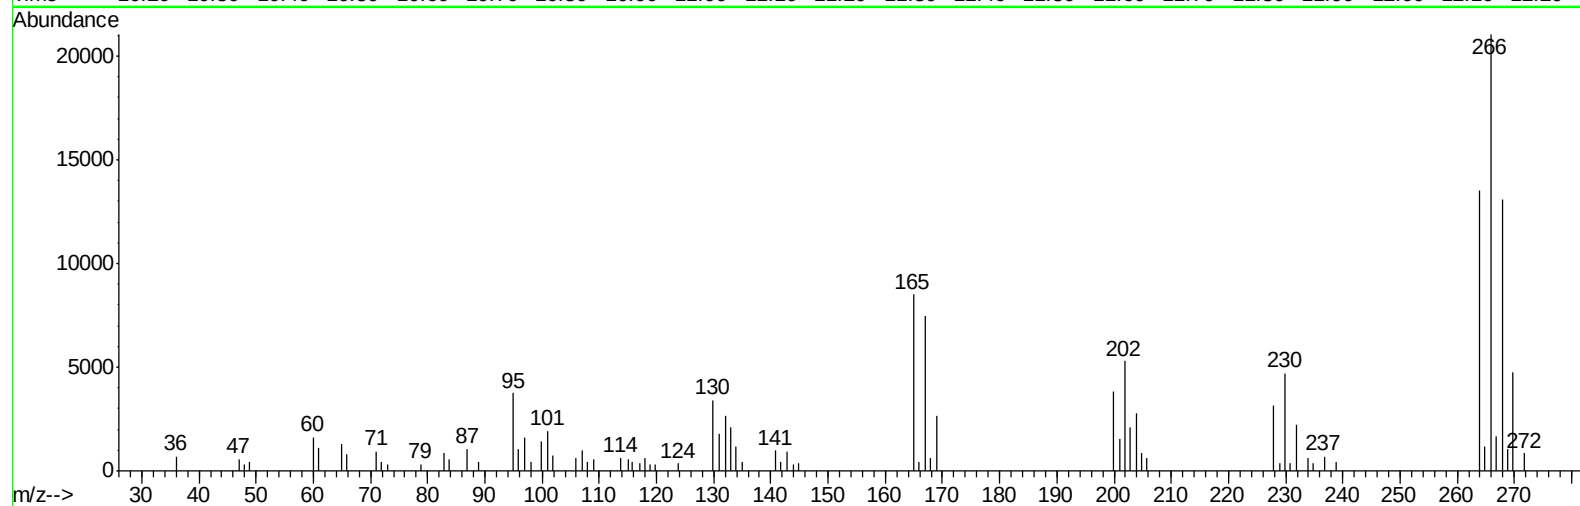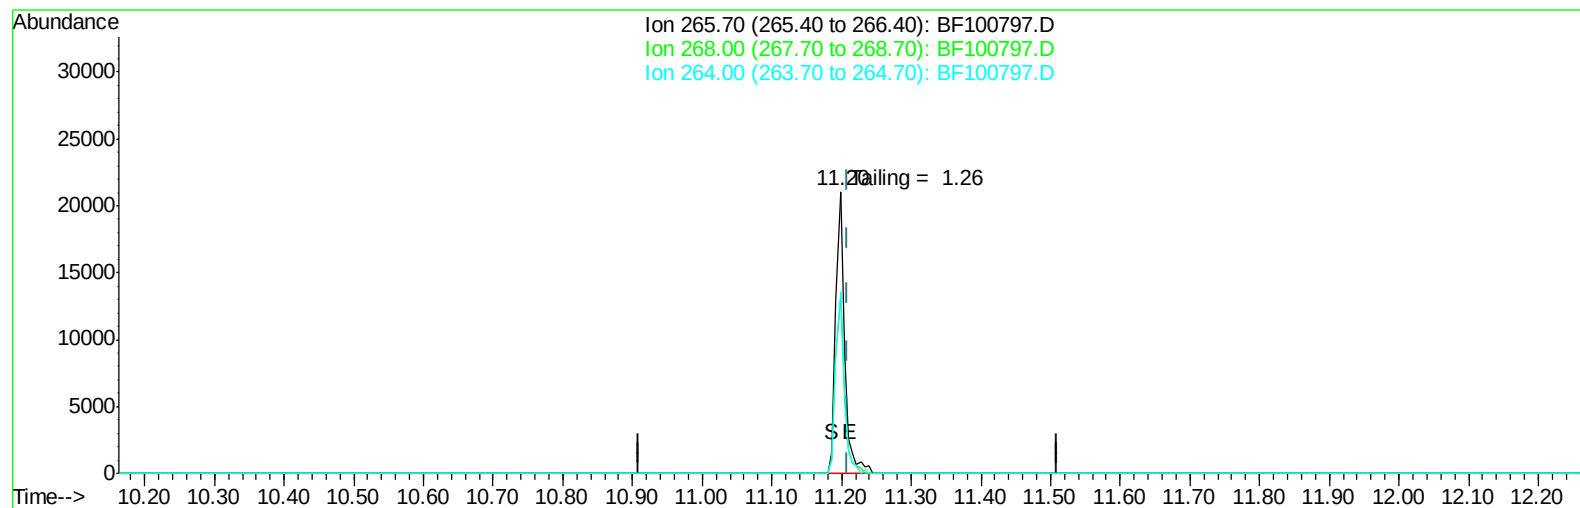

TIC: BF100797.D

(69) Pentachlorophenol (C)

11.198min (-0.012) 0.00ng

response 18209

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.07
264.00	61.90	64.37
0.00	0.00	0.00