
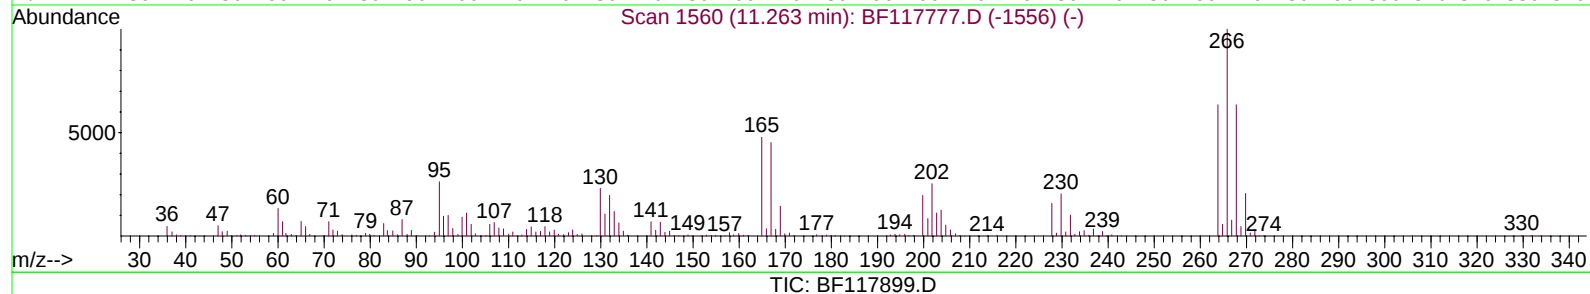
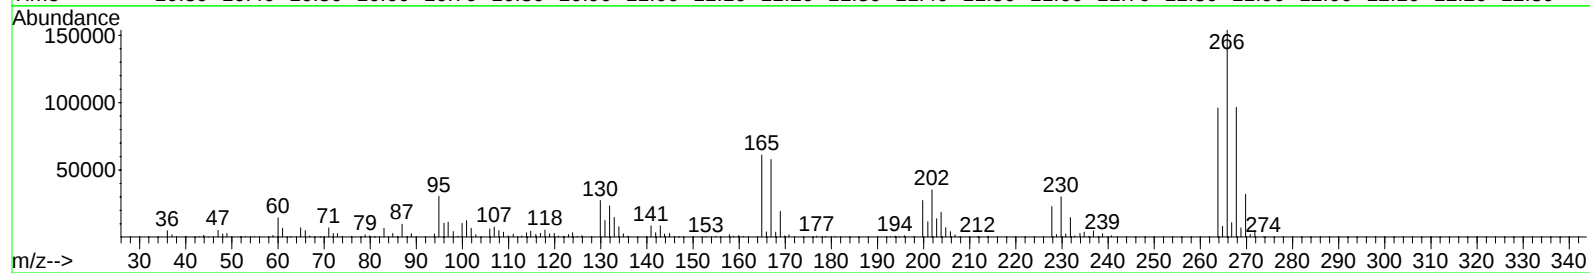


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF112119\
Data File : BF117899.D
Acq On : 21 Nov 2019 9:19
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 21 17:36:56 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF111319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 18:36:07 2019
Response via : Initial Calibration

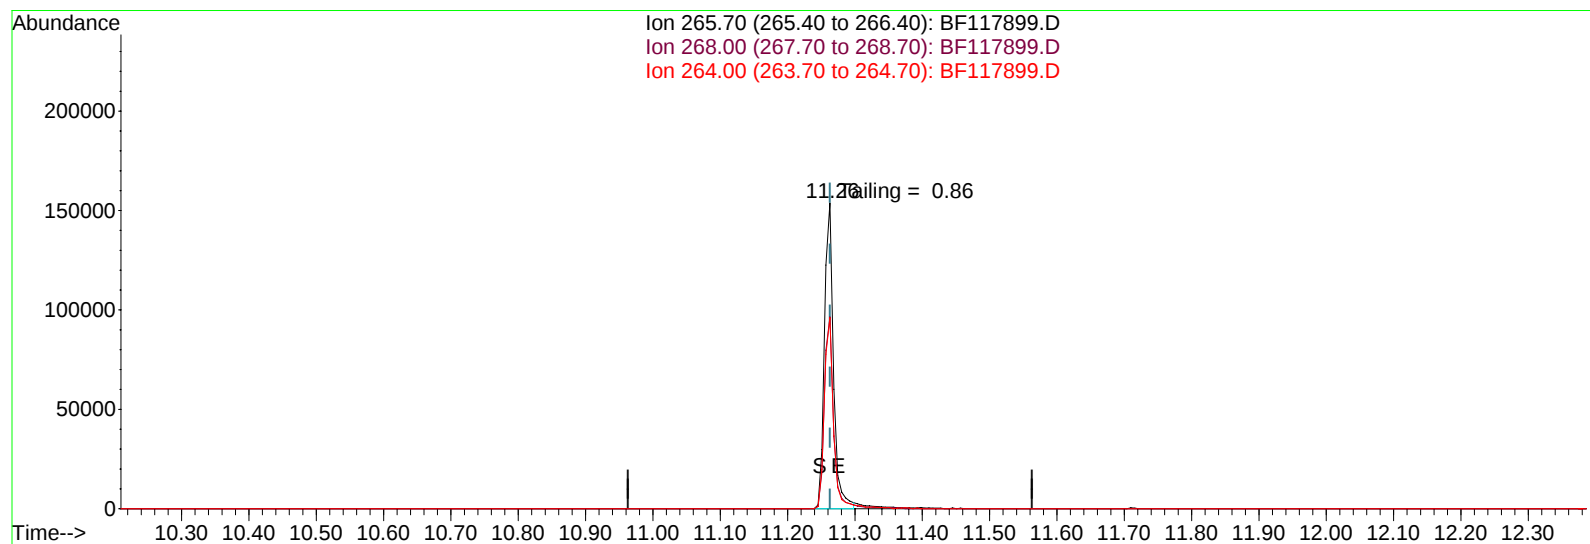

(70) Pentachlorophenol (C)




11.263min (0.000) 31780.37ng

response 148571

Ion	Exp%	Act%
265.70	100	100
268.00	63.50	62.73
264.00	63.40	62.46
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF112119\
Data File : BF117899.D
Acq On : 21 Nov 2019 9:19
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 21 17:36:56 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF111319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 18:36:07 2019
Response via : Initial Calibration

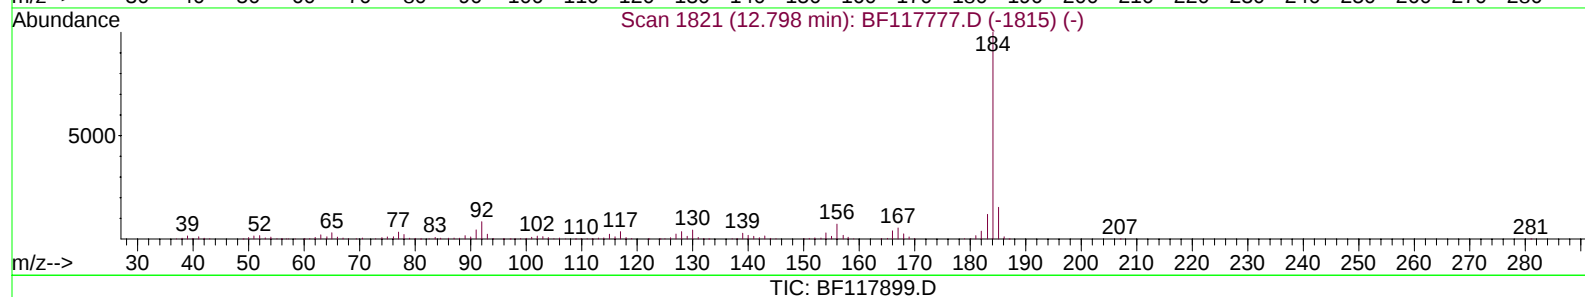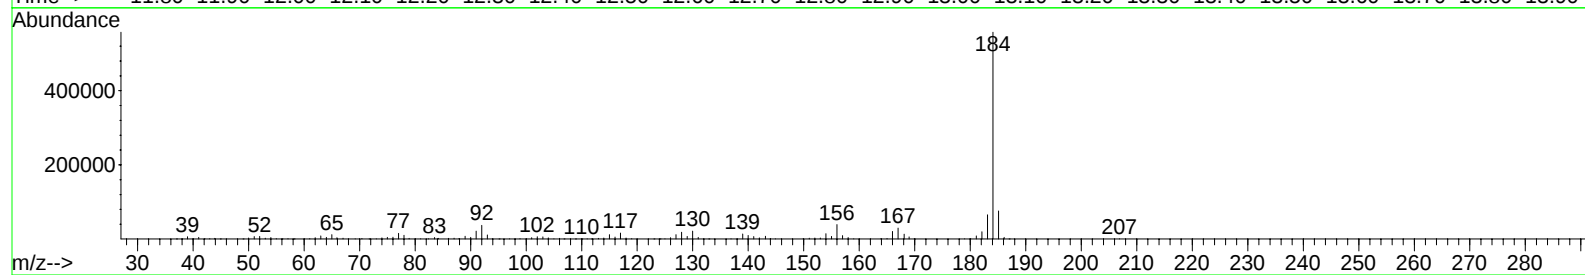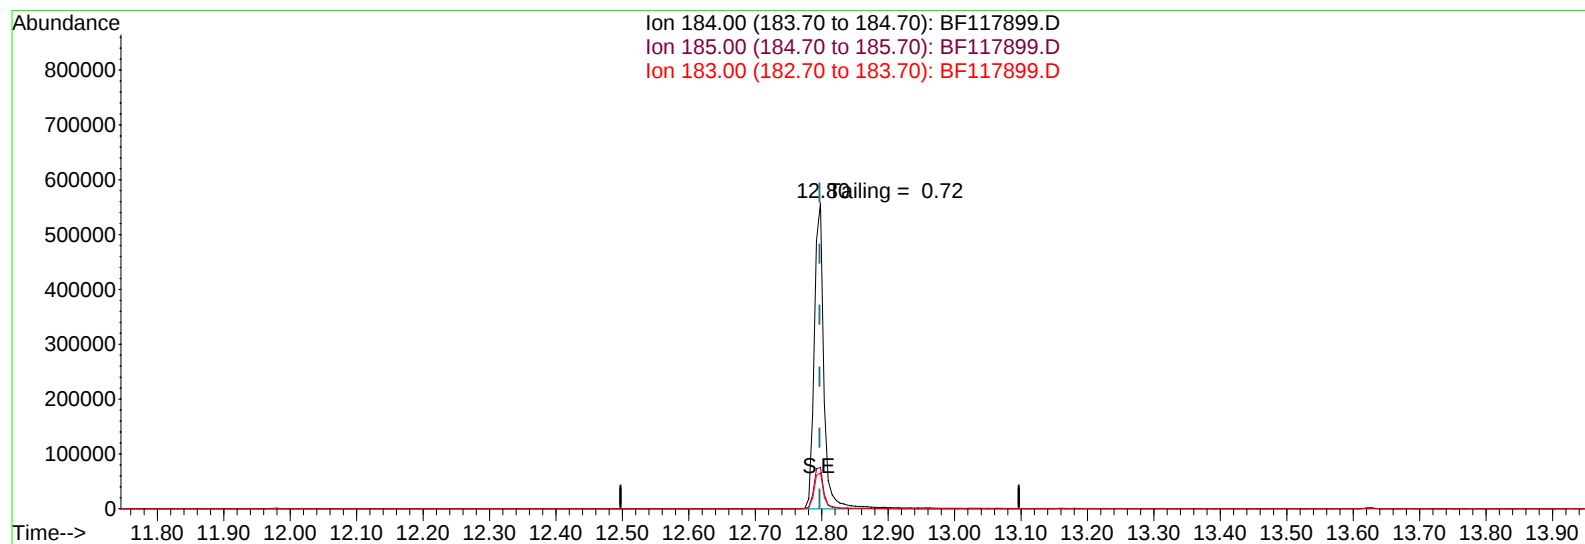

(77) Benzidine

12.798min (+0.001) 0.00ng

response 562858

Ion	Exp%	Act%
184.00	100	100
185.00	15.30	13.57
183.00	11.90	11.73
0.00	0.00	0.00