
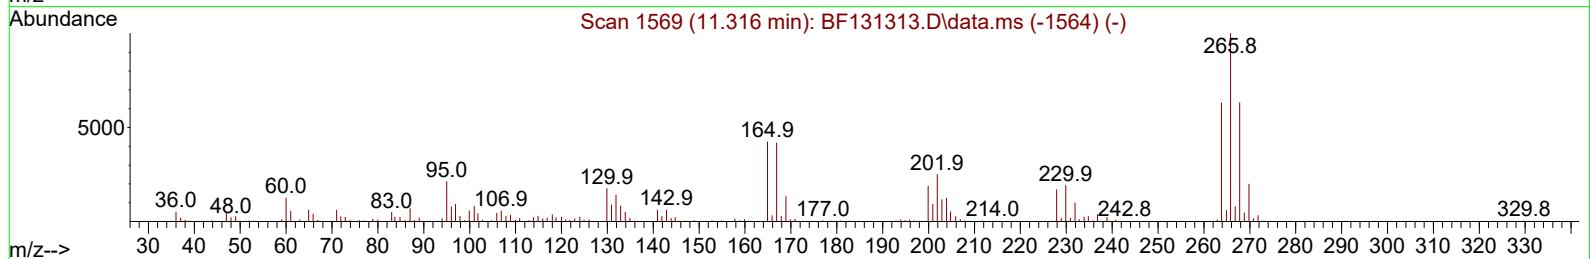
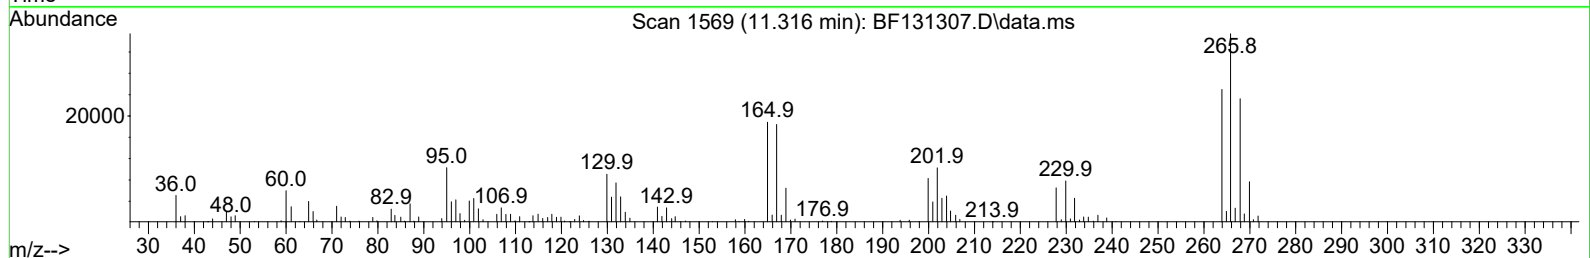


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112122\
Data File : BF131307.D
Acq On : 21 Nov 2022 08:57
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 22 06:05:00 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 22 01:17:52 2022
Response via : Initial Calibration

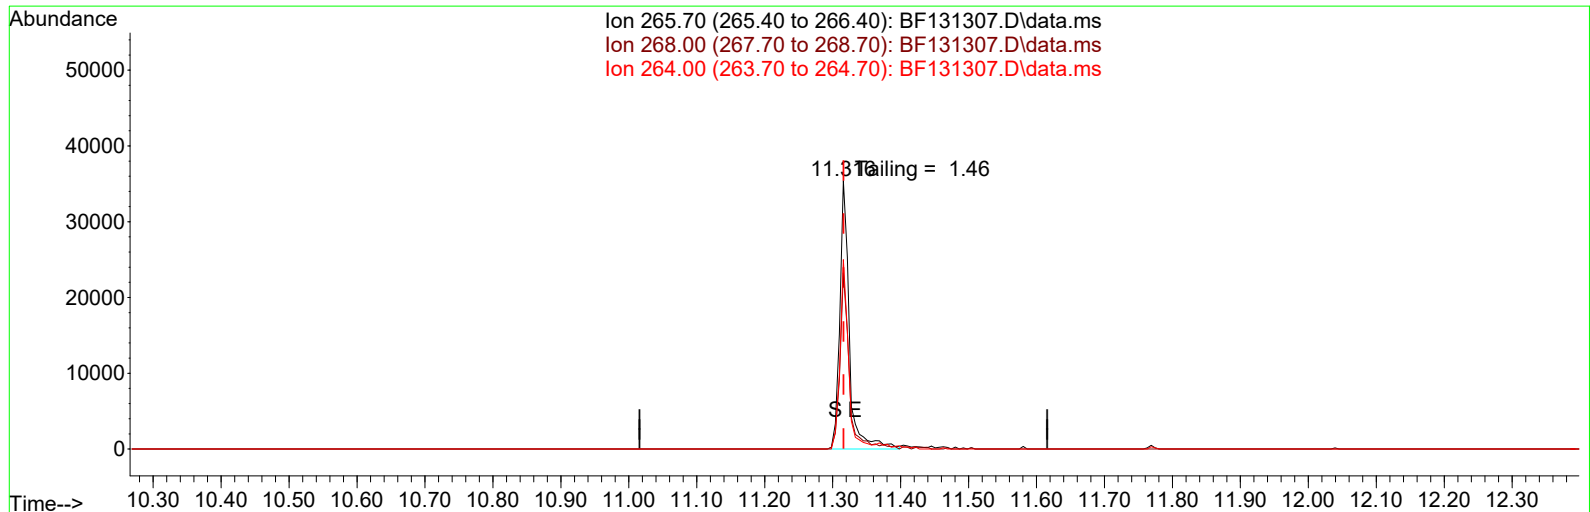

TIC: BF131307.D\data.ms

(70) Pentachlorophenol (C)




11.316min (-0.000) 7989.25 ng

response 34834

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.20	65.63
264.00	63.00	70.51
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112122\
Data File : BF131307.D
Acq On : 21 Nov 2022 08:57
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 22 06:05:00 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 22 01:17:52 2022
Response via : Initial Calibration

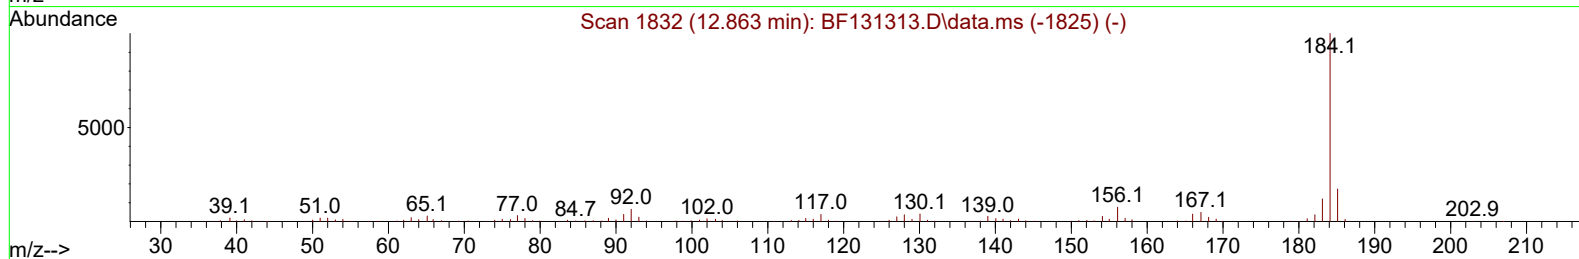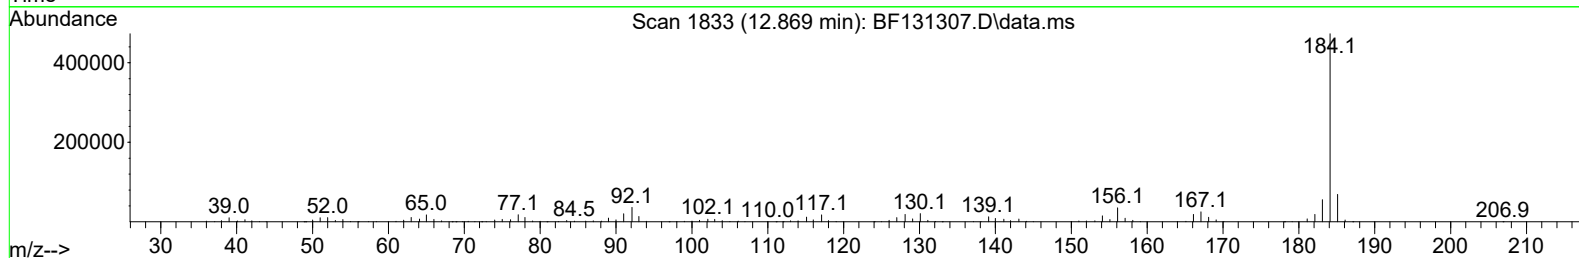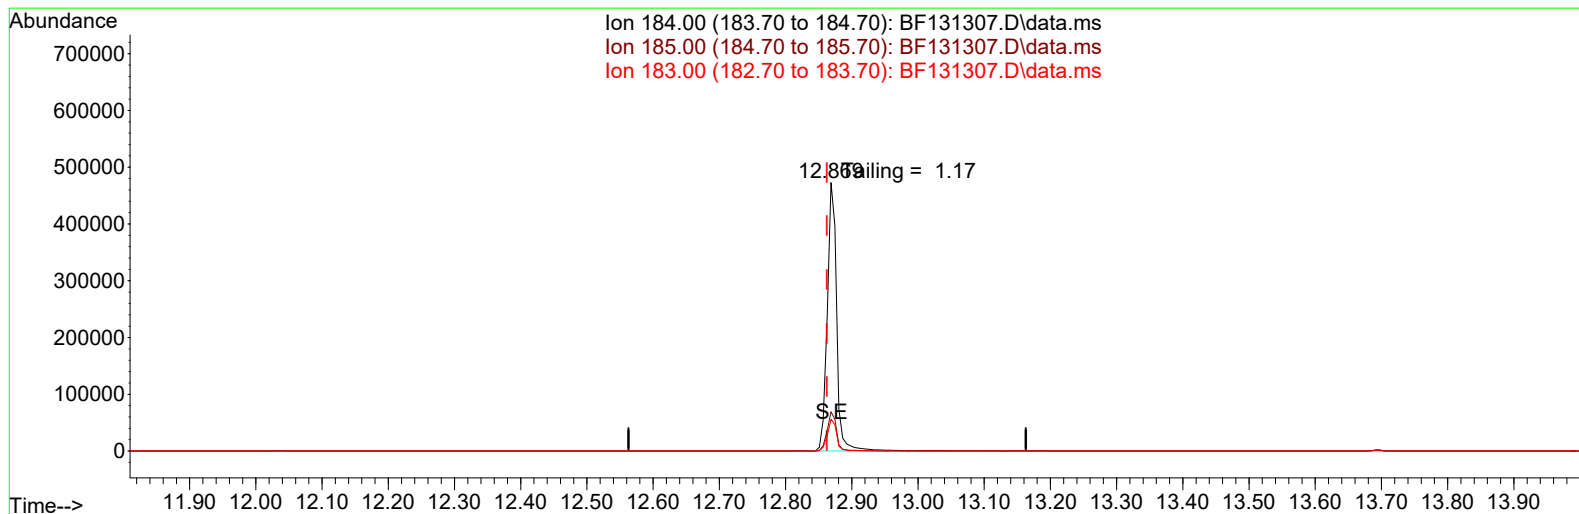

TIC: BF131307.D\data.ms

(77) Benzidine

12.869min (+ 0.006) 0.00 ng

response 467344

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	17.30	14.61
183.00	12.00	11.80
0.00	0.00	0.00